


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD081018\
Data File : VD059731.D
Acq On : 10 Aug 2018 15:38
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampled :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D081018S.M
Title : SW846 8260
Last Update : Sat Aug 11 05:42:24 2018

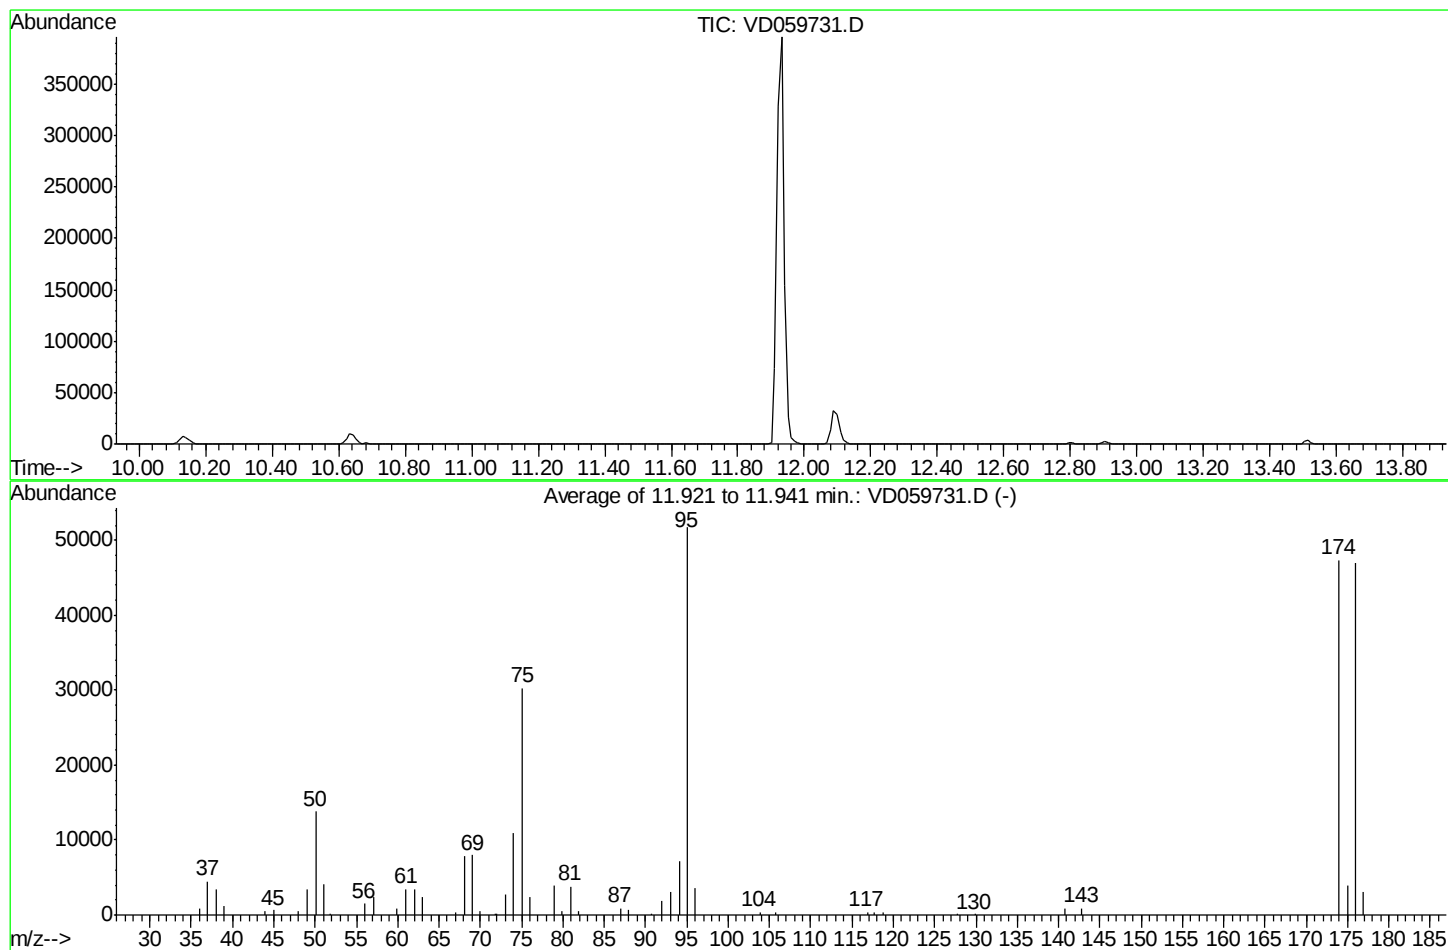

AutoFind: Scans 1189, 1190, 1191; Background Corrected with Scan 1184

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.6	13765	PASS
75	95	30	60	58.6	30310	PASS
95	95	100	100	100.0	51722	PASS
96	95	5	9	7.1	3656	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	91.6	47397	PASS
175	174	5	9	8.3	3919	PASS
176	174	95	101	99.0	46904	PASS
177	176	5	9	6.6	3117	PASS