
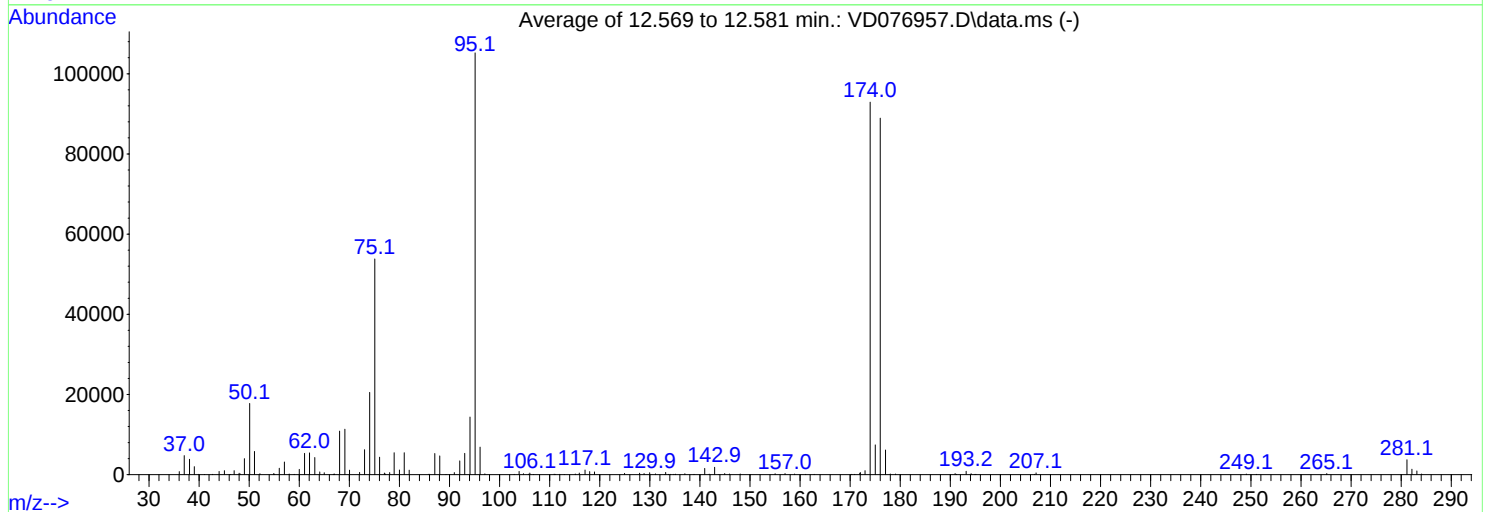


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD081023\
 Data File : VD076957.D
 Acq On : 10 Aug 2023 11:21
 Operator : JC/SY
 Sample : BFB155
 Misc : 5.00G/10.0ml/MSVOA_D/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB155

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM080323SMA.M
 Title : SFAM01.0
 Last Update : Sat Aug 12 02:16:48 2023

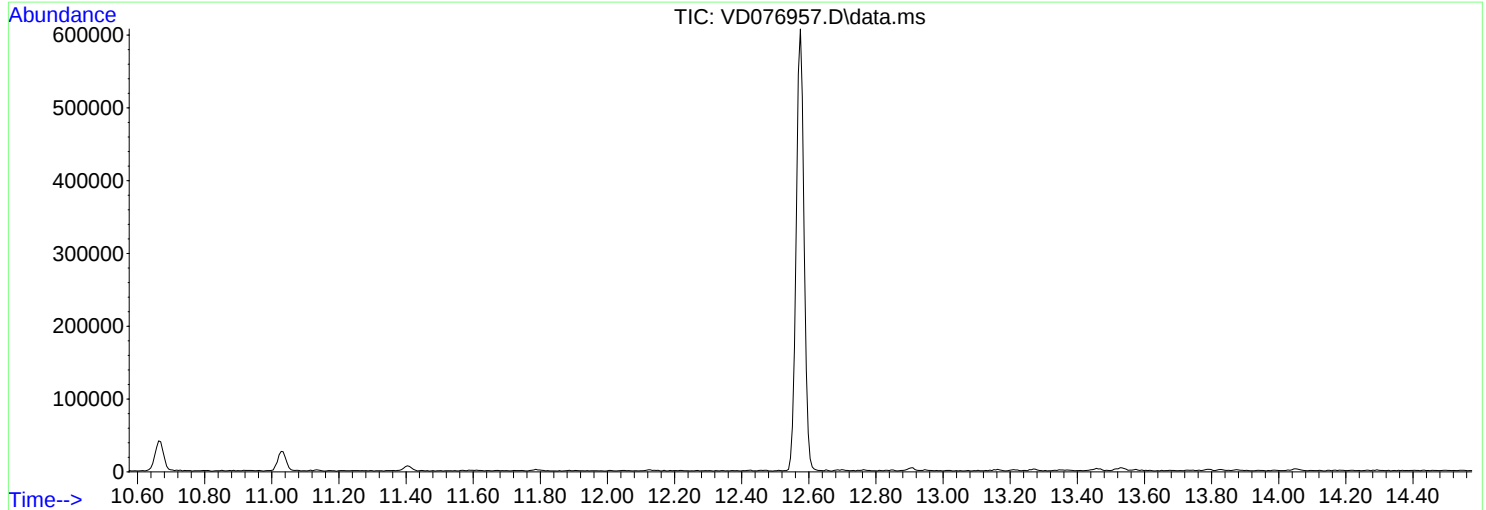

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	17756	PASS
75	95	30	80	51.2	53824	PASS
95	95	100	100	100.0	105219	PASS
96	95	5	9	6.5	6876	PASS
173	174	0.00	2	1.1	1019	PASS
174	95	50	120	88.3	92907	PASS
175	174	5	9	8.0	7415	PASS
176	174	95	105	95.7	88936	PASS
177	176	5	10	6.9	6160	PASS

m/z	Abundance
39.90	786.0
44.00	664.0

Instrument :
MSVOA_D
ClientSampleId :
BFB155

m/z	Abundance
36.00	593.0
37.10	4944.0
38.10	4033.0
39.00	2468.0
40.00	836.0
41.10	177.0
44.10	1462.0
45.00	878.0
47.00	1365.0
48.00	540.0
49.10	4077.0
50.10	19048.0
51.10	5683.0
54.80	312.0
56.00	1983.0
57.10	3008.0
58.00	198.0
60.00	1410.0
61.00	5631.0
62.00	5255.0
63.20	4633.0
64.20	845.0
65.00	603.0
67.10	220.0
68.00	11446.0
69.10	10485.0
70.10	1193.0
72.00	528.0
73.10	5841.0
74.10	20544.0
75.10	54784.0
76.00	4072.0
77.00	565.0
78.00	266.0
79.00	5351.0
80.10	787.0
81.00	5641.0
82.00	1313.0
87.10	5074.0
88.00	4249.0
90.90	517.0
92.00	2893.0
93.10	5707.0
94.10	13124.0
95.10	106392.0
96.10	6973.0
97.10	232.0
103.90	713.0
104.70	195.0
106.10	672.0
110.90	156.0
112.90	181.0
115.10	163.0
115.90	401.0
117.10	1285.0
118.00	845.0
119.10	577.0
125.00	359.0
127.90	337.0
128.80	355.0
129.90	483.0
133.00	176.0
133.70	205.0
137.00	370.0
141.00	1103.0
141.90	225.0
142.90	1392.0
144.90	445.0
155.10	227.0
157.10	331.0
159.00	270.0
170.30	192.0
171.90	1118.0
173.00	974.0
174.00	89904.0
175.00	7094.0
176.00	84992.0
177.00	6376.0
178.10	240.0
191.20	307.0
193.20	578.0
194.10	203.0
206.80	225.0
249.20	150.0
265.30	165.0
281.30	2354.0
282.10	881.0
283.10	944.0
284.10	167.0

Instrument :
MSVOA_D
ClientSampleId :
BFB155

m/z	Abundance
36.10	902.0
37.10	5536.0
38.10	3802.0
39.10	1889.0
40.10	1075.0
42.70	196.0
44.00	1434.0
45.10	1438.0
46.10	165.0
47.00	1081.0
48.00	516.0
49.00	4143.0
50.10	18488.0
51.10	6398.0
52.10	509.0
54.90	361.0
56.00	1589.0
57.00	3058.0
58.00	238.0
60.00	1261.0
61.10	5951.0
62.10	6167.0
63.10	3892.0
64.00	772.0
65.00	373.0
66.80	413.0
68.00	12652.0
69.10	13994.0
70.10	1268.0
72.10	501.0
73.00	7380.0
74.00	22208.0
75.10	58712.0
76.10	4604.0
77.20	467.0
78.00	716.0
79.00	6074.0
80.00	1697.0
80.90	5190.0
81.90	1183.0
85.90	153.0
87.10	5606.0
88.00	4608.0
89.30	156.0
90.90	576.0
92.00	3855.0
93.10	5337.0
94.10	16648.0
95.10	114032.0
96.10	7184.0
97.10	232.0
102.90	233.0
103.80	937.0
104.80	369.0
106.00	597.0
111.10	299.0
112.00	248.0
115.10	269.0
116.00	502.0
116.90	768.0
117.90	720.0
118.90	922.0
125.00	197.0
127.90	455.0
128.90	274.0
130.00	586.0
131.20	388.0
133.20	552.0
135.10	394.0
137.00	416.0
138.80	284.0
140.90	1636.0
141.80	172.0
142.90	1942.0
144.90	169.0
146.00	293.0
148.10	319.0
150.00	150.0
155.00	252.0
157.00	299.0
161.10	260.0
162.80	233.0
172.10	769.0
173.00	1159.0
174.00	101952.0
175.00	7474.0
176.00	98456.0
177.10	6298.0
177.90	191.0
179.00	192.0
190.90	408.0
193.00	881.0

Instrument :
MSVOA_D
ClientSampleId :
BFB155

194.20	208.0
194.90	264.0
207.10	593.0
249.10	175.0
265.10	381.0
281.10	4130.0
282.20	1672.0
283.20	907.0
284.10	314.0

Instrument :
MSVOA_D
ClientSampleId :
BFB155

m/z	Abundance
36.00	836.0
37.00	3826.0
38.10	3682.0
39.00	1585.0
40.00	748.0
44.00	1513.0
45.10	672.0
46.30	185.0
47.10	587.0
48.20	655.0
49.10	3734.0
50.10	15731.0
51.00	5242.0
52.20	227.0
55.10	462.0
56.00	1262.0
57.00	3362.0
59.00	294.0
60.00	1258.0
61.00	4330.0
62.10	4813.0
63.00	4325.0
64.10	476.0
65.00	463.0
67.00	231.0
68.10	8470.0
69.10	9574.0
70.00	868.0
72.00	618.0
73.00	5468.0
74.00	18760.0
75.10	47976.0
76.10	4339.0
77.00	600.0
78.10	594.0
78.90	5009.0
79.90	964.0
81.00	5578.0
81.90	877.0
85.90	222.0
87.00	5100.0
88.10	5108.0
91.00	503.0
92.10	3562.0
93.00	4919.0
94.10	13332.0
95.10	95232.0
96.10	6472.0
97.00	185.0
104.00	750.0
104.80	170.0
105.80	345.0
106.80	151.0
110.90	165.0
115.80	312.0
117.00	1460.0
118.10	768.0
118.90	520.0
124.90	415.0
128.00	267.0
128.90	278.0
130.00	361.0
131.00	259.0
133.10	1118.0
134.10	196.0
134.80	214.0
141.00	1895.0
143.00	2177.0
143.80	155.0
145.00	262.0
145.80	216.0
147.90	191.0
154.90	198.0
156.90	196.0
158.80	222.0
170.90	237.0
172.00	816.0
172.90	925.0
174.00	86864.0
175.00	7676.0
176.00	83360.0
177.00	5805.0
179.10	280.0
191.00	415.0
193.20	1052.0
194.10	275.0
195.10	228.0
207.10	711.0
249.00	199.0
251.10	231.0
265.10	341.0
281.20	4703.0

Instrument :
MSVOA_D
ClientSampleId :
BFB155

282.201525.0

283.10867.0

Instrument :
MSVOA_D
ClientSampleId :
BFB155