

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD081121\
 Data File : VD070027.D
 Acq On : 11 Aug 2021 17:01
 Operator : VA/SY
 Sample : M3340-01
 Misc : 5.05G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 205-239-929

Quant Time: Aug 12 05:30:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D072221S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 23 04:51:13 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	741368	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	1514930	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	1433534	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.567	152	625244	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	391840	45.956	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	91.920%
35) Dibromofluoromethane	7.914	113	439574	46.028	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	92.060%
50) Toluene-d8	10.338	98	2002910	54.390	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	108.780%
62) 4-Bromofluorobenzene	12.626	95	666796	54.181	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	108.360%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD081121\
Data File : VD070027.D
Acq On : 11 Aug 2021 17:01
Operator : VA/SY
Sample : M3340-01
Misc : 5.05G/5.00ml/MSVOA_D/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
205-239-929

Quant Time: Aug 12 05:30:47 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D072221S.M
Quant Title : SW846 8260
QLast Update : Fri Jul 23 04:51:13 2021
Response via : Initial Calibration




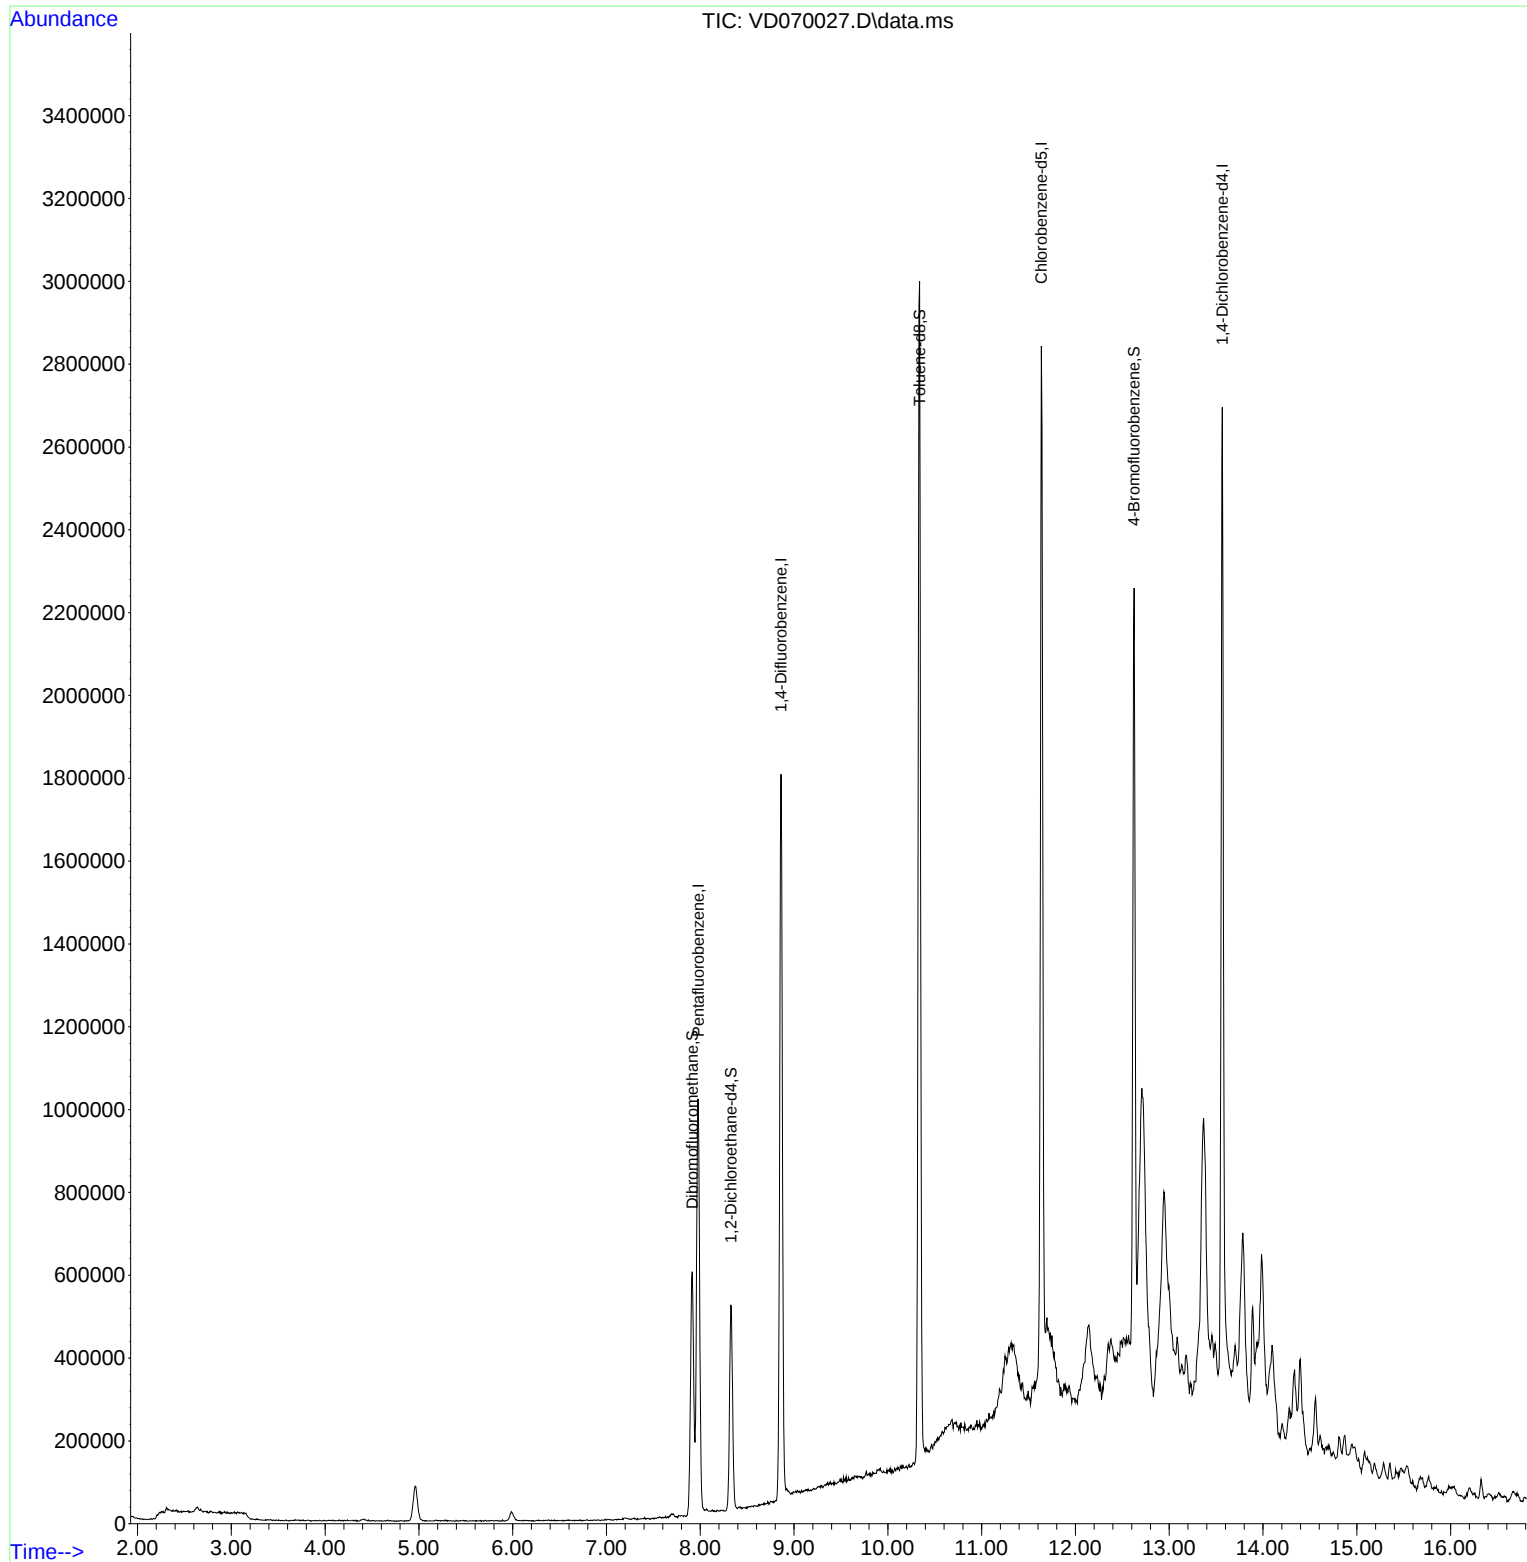


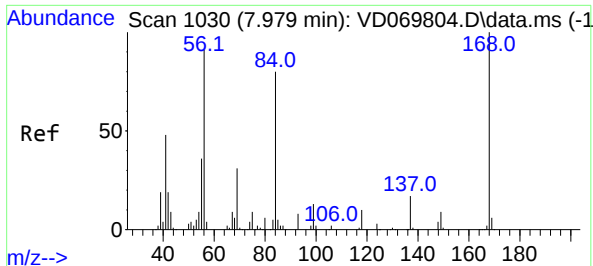

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.000 min
Lab File: VD070027.D
Acq: 11 Aug 2021 17:01




Instrument :
MSVOA_D
ClientSampleId :
205-239-929

Tgt Ion:168 Resp: 741368
Ion Ratio Lower Upper
168 100
99 60.4 51.1 76.7

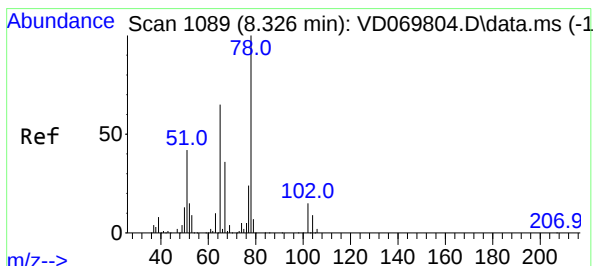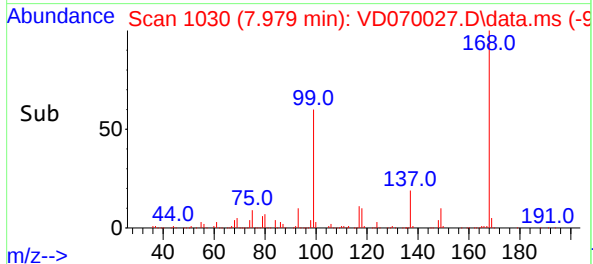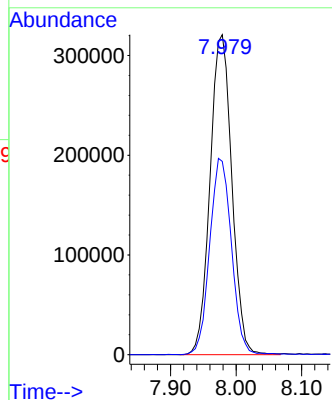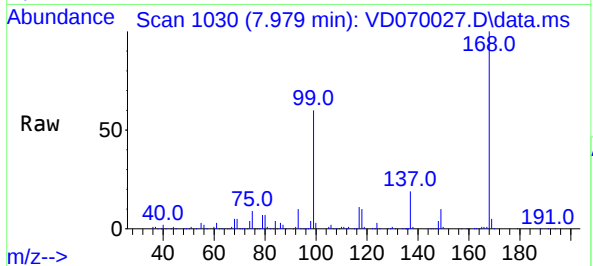

#33
1,2-Dichloroethane-d4
Concen: 45.956 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. -0.000 min
Lab File: VD070027.D
Acq: 11 Aug 2021 17:01

Tgt Ion: 65 Resp: 391840
Ion Ratio Lower Upper
65 100
67 55.3 0.0 111.2

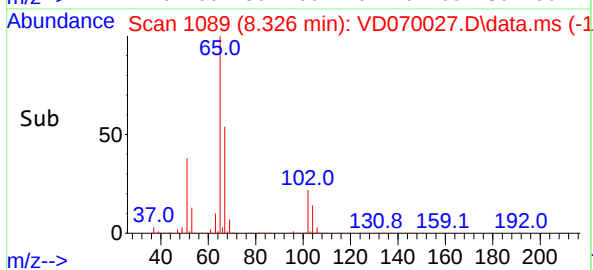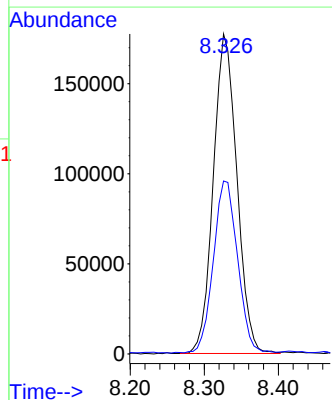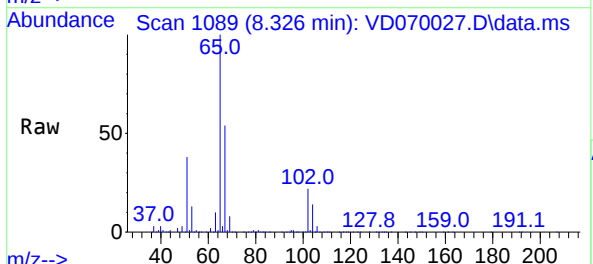







#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. 0.000 min
Lab File: VD070027.D
Acq: 11 Aug 2021 17:01

Instrument :
MSVOA_D
ClientSampleId :
205-239-929




Tgt Ion:114 Resp: 1514930
Ion Ratio Lower Upper
114 100
63 19.6 0.0 41.6
88 15.7 0.0 31.4

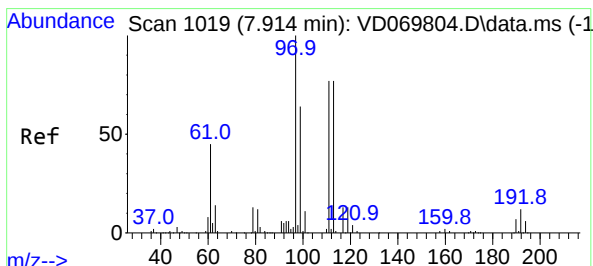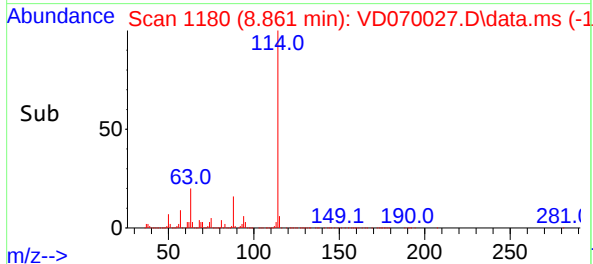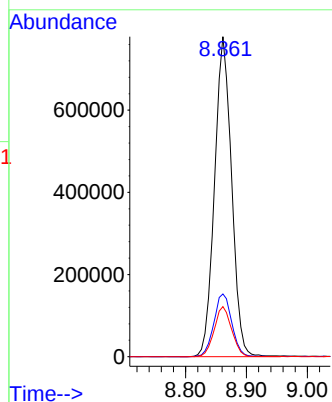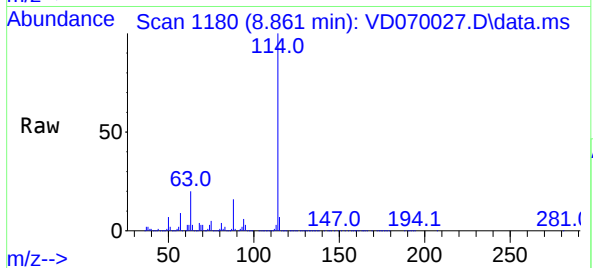

#35

Dibromofluoromethane
Concen: 46.028 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. -0.000 min
Lab File: VD070027.D
Acq: 11 Aug 2021 17:01

Tgt Ion:113 Resp: 439574
Ion Ratio Lower Upper
113 100
111 103.7 80.5 120.7
192 17.3 12.6 19.0


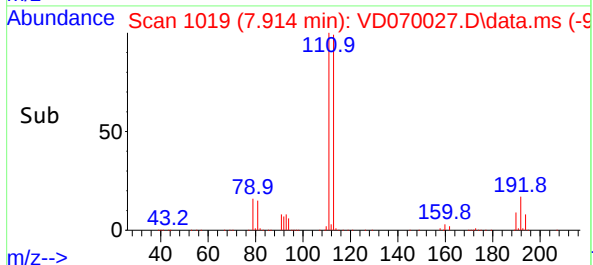
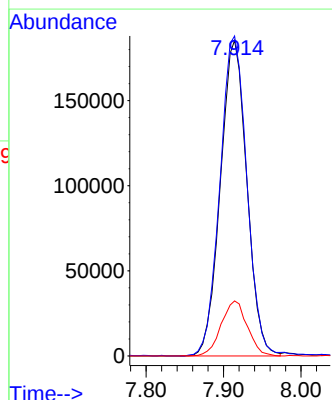
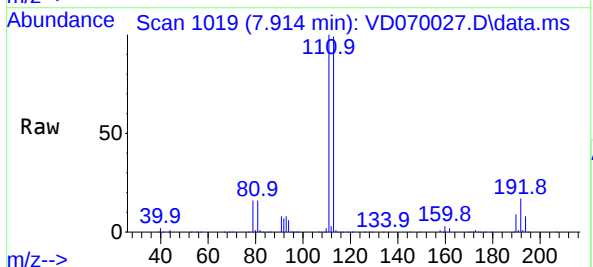




#50
Toluene-d8
Concen: 54.390 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. -0.000 min
Lab File: VD070027.D
Acq: 11 Aug 2021 17:01




Instrument :
MSVOA_D
ClientSampleId :
205-239-929


Tgt Ion: 98 Resp: 2002910
Ion Ratio Lower Upper
98 100
100 65.0 51.9 77.9

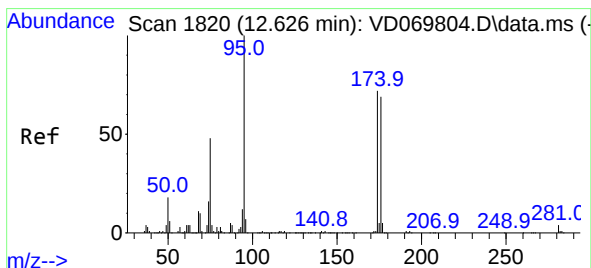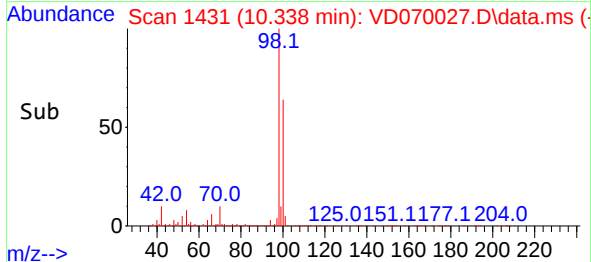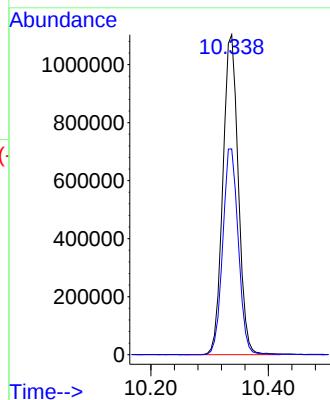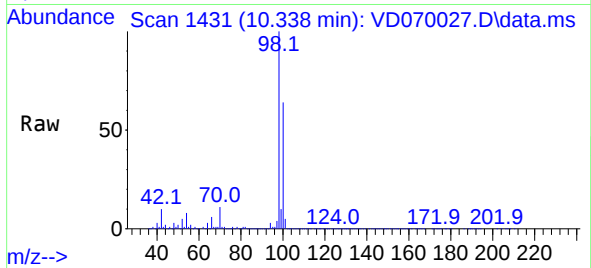

#62
4-Bromofluorobenzene
Concen: 54.181 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. -0.000 min
Lab File: VD070027.D
Acq: 11 Aug 2021 17:01

Tgt Ion: 95 Resp: 666796
Ion Ratio Lower Upper
95 100
174 70.5 0.0 142.6
176 68.8 0.0 134.2


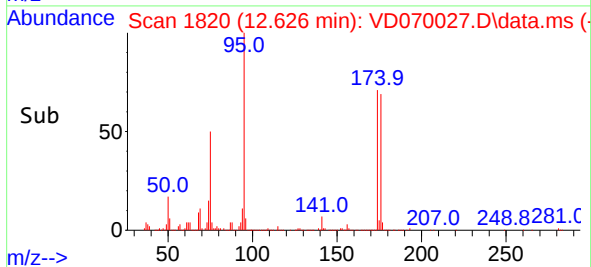
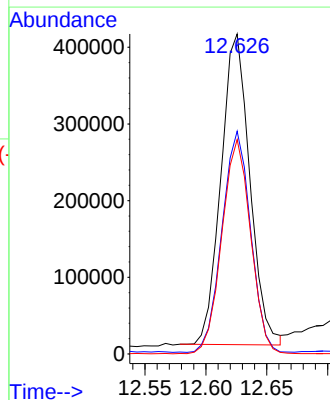
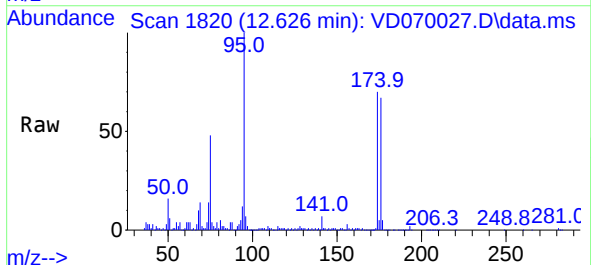


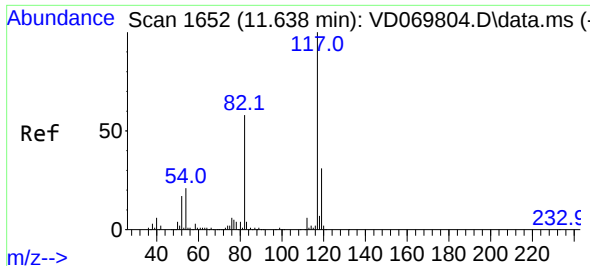

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1652
Delta R.T. -0.000 min
Lab File: VD070027.D
Acq: 11 Aug 2021 17:01

Instrument :
MSVOA_D
ClientSampleId :
205-239-929

Tgt Ion:117 Resp: 1433534
Ion Ratio Lower Upper
117 100
82 57.4 46.3 69.5
119 31.5 24.7 37.1

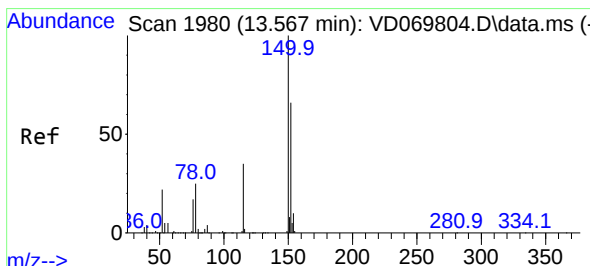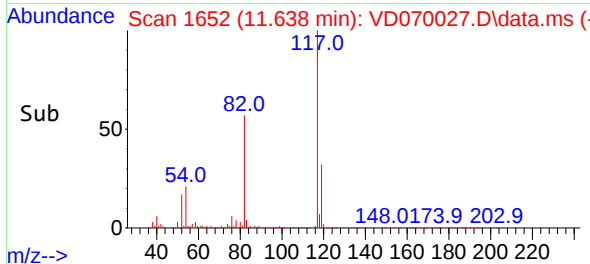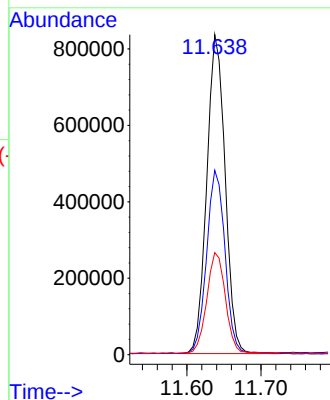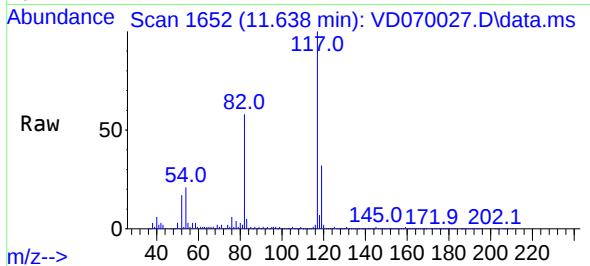

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.567 min Scan# 1980
Delta R.T. -0.000 min
Lab File: VD070027.D
Acq: 11 Aug 2021 17:01

Tgt Ion:152 Resp: 625244
Ion Ratio Lower Upper
152 100
115 60.3 31.1 93.3
150 155.9 0.0 343.0

