




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD081123\
 Data File : VD076982.D
 Acq On : 11 Aug 2023 11:36
 Operator : JC/SY
 Sample : 03965-07RE
 Misc : 5.24G/10.0ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 A48H7RE

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/15/2023
 Supervised By :Mahesh Dadoda 08/15/2023

Quant Time: Aug 12 02:21:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM080323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 12 02:16:48 2023
 Response via : Initial Calibration

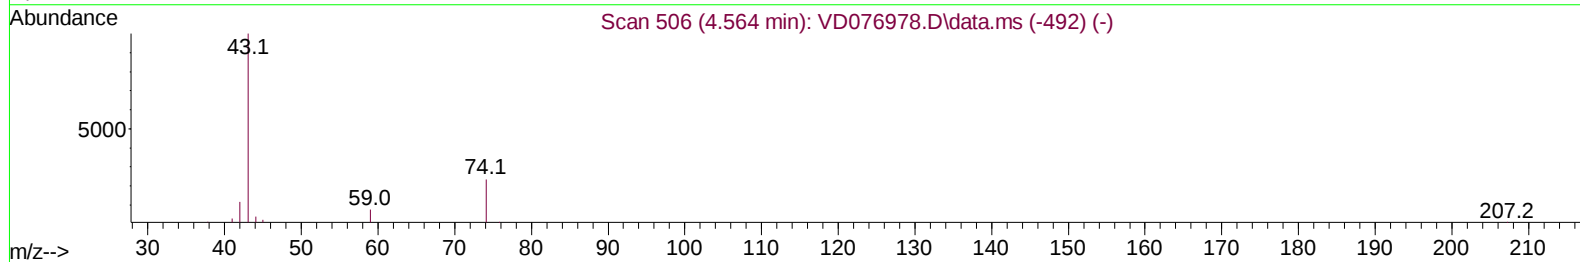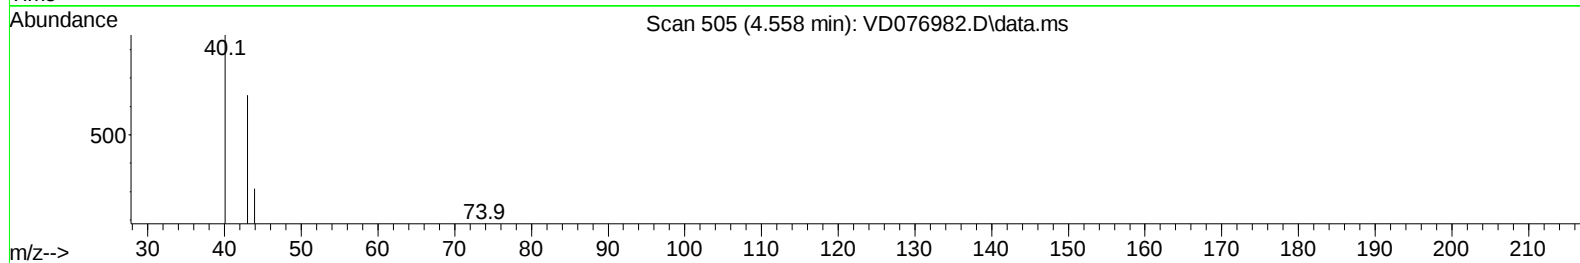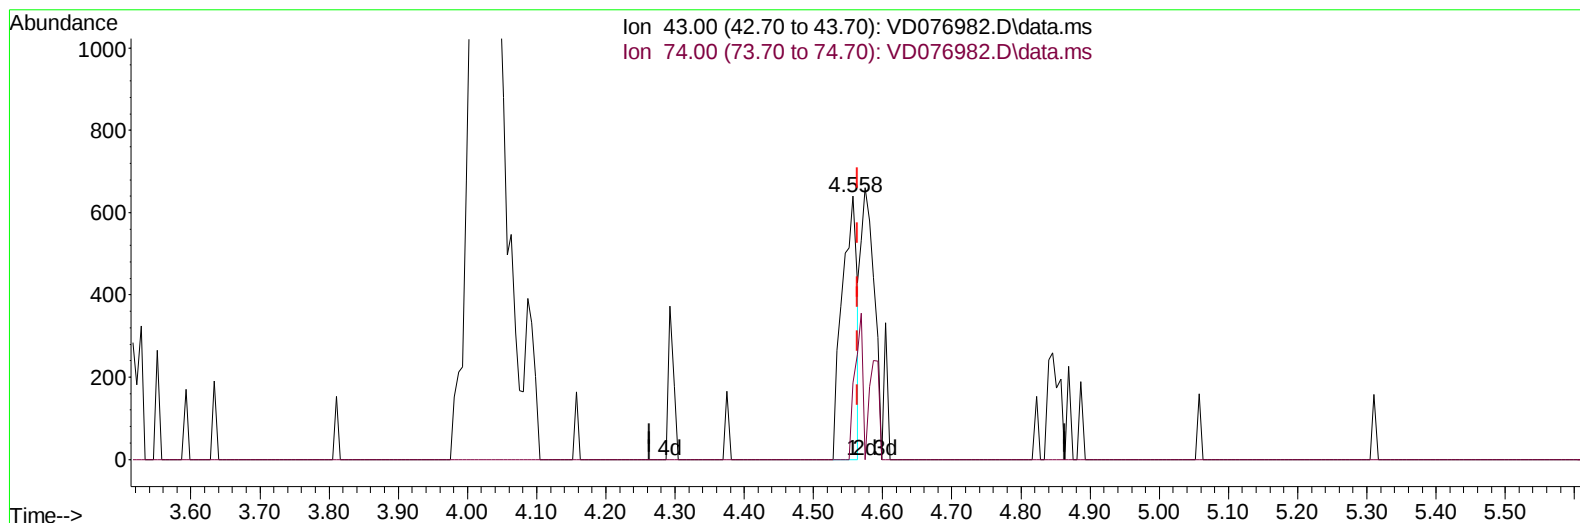

TIC: VD076982.D\data.ms

(15) Methyl Acetate (T)

4.558min (-0.006) 1.46 ug/L

response 961

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	22.70	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD081123\
 Data File : VD076982.D
 Acq On : 11 Aug 2023 11:36
 Operator : JC/SY
 Sample : 03965-07RE
 Misc : 5.24G/10.0ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 A48H7RE

Manual IntegrationsAPPROVED

Quant Time: Aug 12 02:21:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM080323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 12 02:16:48 2023
 Response via : Initial Calibration

Reviewed By :Romaben Patel 08/15/2023
 Supervised By :Mahesh Dadoda 08/15/2023

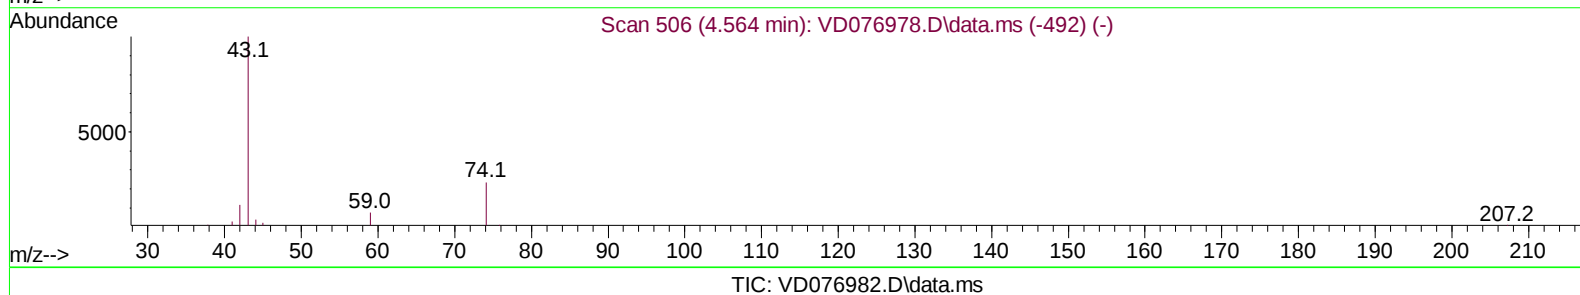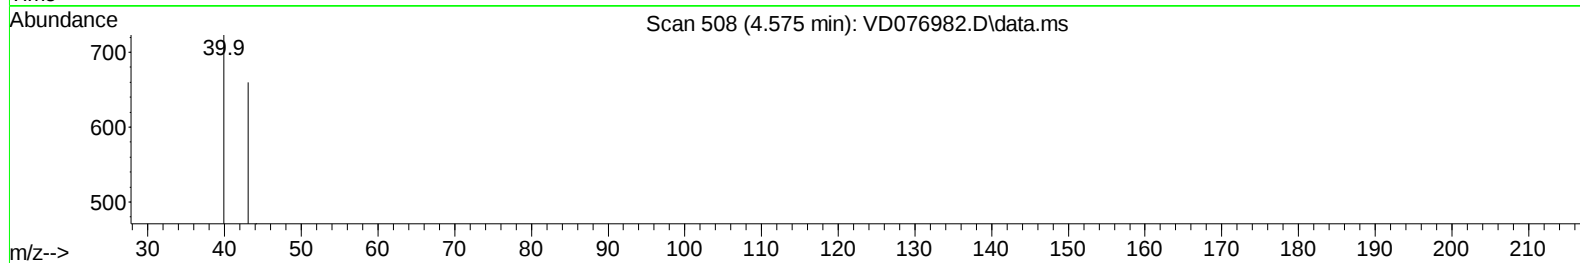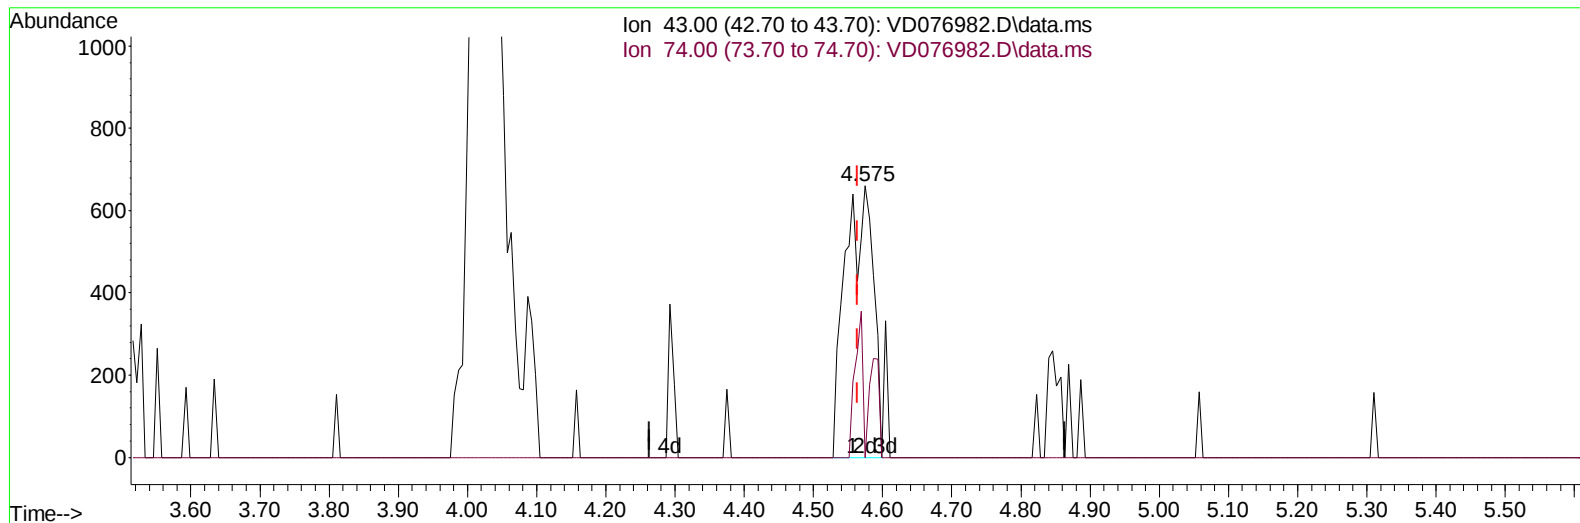

(15) Methyl Acetate (T)

4.575min (+ 0.012) 2.81 ug/L m

response 1847

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	22.70	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD081123\
 Data File : VD076982.D
 Acq On : 11 Aug 2023 11:36
 Operator : JC/SY
 Sample : 03965-07RE
 Misc : 5.24G/10.0ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 A48H7RE

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/15/2023
 Supervised By :Mahesh Dadoda 08/15/2023

Quant Time: Aug 12 02:21:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM080323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Aug 12 02:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	86253	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	40004	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	6512	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.269	65	113536	47.865	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 191.440%#			
7) Chloroethane-d5	2.799	69	112860	51.468	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 205.880%#			
11) 1,1-Dichloroethene-d2	3.916	65	23246	41.360	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 165.440%#			
21) 2-Butanone-d5	6.981	46	31751	83.374	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 166.740%#			
24) Chloroform-d	7.563	84	122534	43.627	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 174.520%#			
26) 1,2-Dichloroethane-d4	8.228	65	68773	49.119	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 196.480%#			
32) Benzene-d6	8.204	84	223368	88.809	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 355.240%#			
36) 1,2-Dichloropropane-d6	9.210	67	71454	92.400	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 369.600%#			
41) Toluene-d8	10.269	98	132638	57.519	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 230.080%#			
43) trans-1,3-Dichloroprop...	10.528	79	20930	59.865	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 239.480%#			
47) 2-Hexanone-d5	10.881	63	15595	105.573	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 211.140%#			
56) 1,1,2,2-Tetrachloroeth...	12.651	84	30443	40.740	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 162.960%#			
66) 1,2-Dichlorobenzene-d4	13.816	152	9657	40.563	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 162.240%#			
Target Compounds						
13) Acetone	4.028	43	5035	12.929	ug/L	77
15) Methyl Acetate	4.575	43	1847m	2.806	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD081123\
Data File : VD076982.D
Acq On : 11 Aug 2023 11:36
Operator : JC/SY
Sample : 03965-07RE
Misc : 5.24G/10.0ml/MSVOA_D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
A48H7RE

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 08/15/2023
Supervised By :Mahesh Dadoda 08/15/2023

Quant Time: Aug 12 02:21:37 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM080323SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Aug 12 02:16:48 2023
Response via : Initial Calibration

