


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD081219\
 Data File : VD063501.D
 Acq On : 12 Aug 2019 21:54
 Operator : JC/SY
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D080919S.M
 Title : SW846 8260
 Last Update : Sat Aug 10 06:42:47 2019

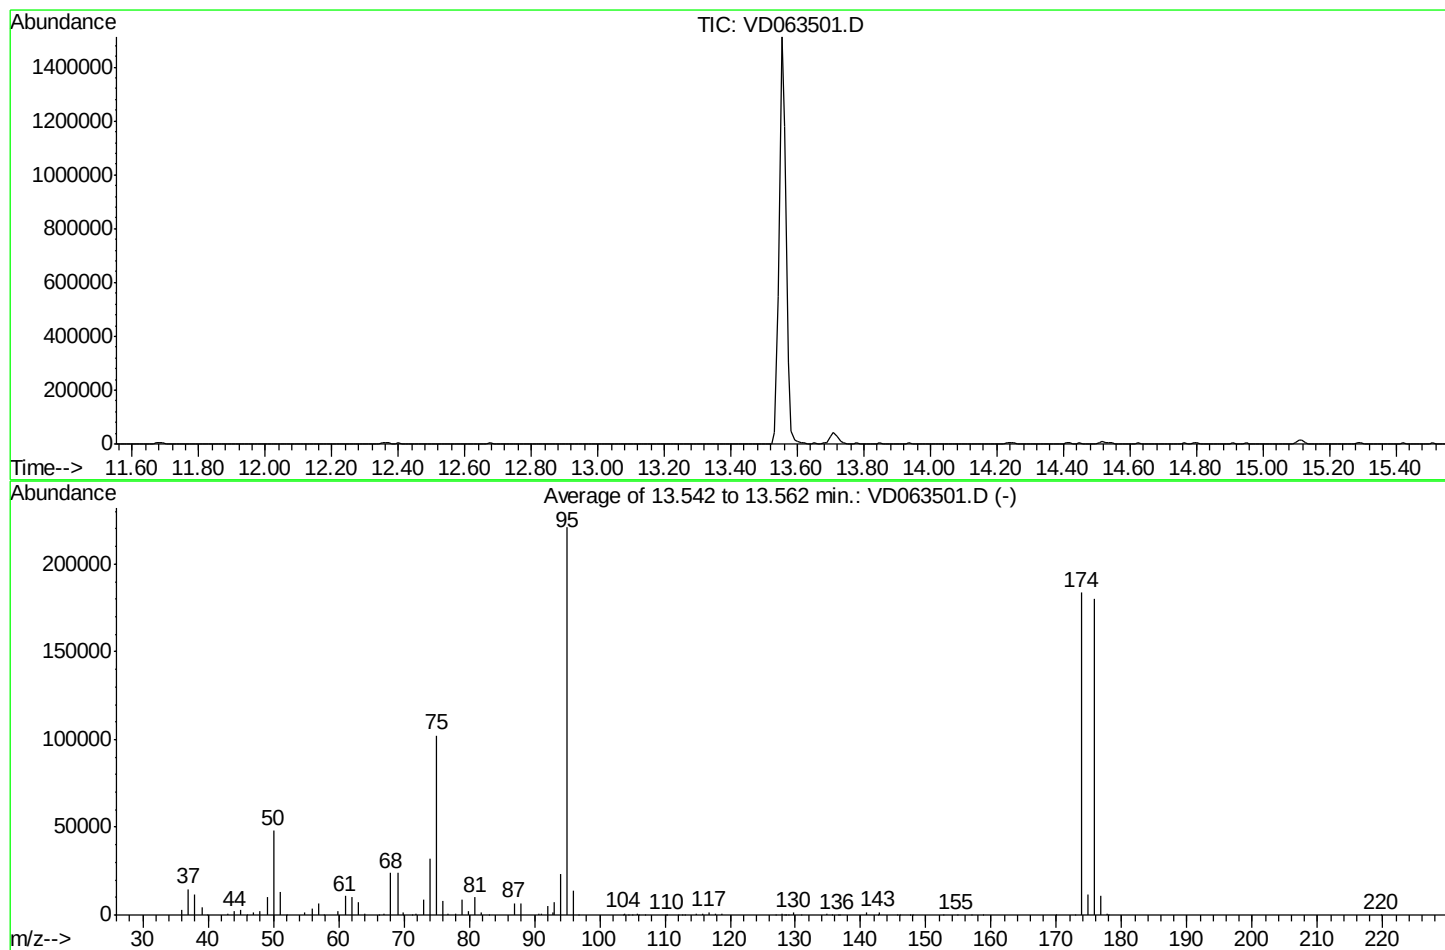

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	47994	PASS
75	95	30	60	46.3	102210	PASS
95	95	100	100	100.0	220914	PASS
96	95	5	9	6.2	13776	PASS
173	174	0.00	2	0.1	241	PASS
174	95	50	100	83.1	183541	PASS
175	174	5	9	6.4	11762	PASS
176	174	95	101	98.2	180152	PASS
177	176	5	9	6.0	10888	PASS