
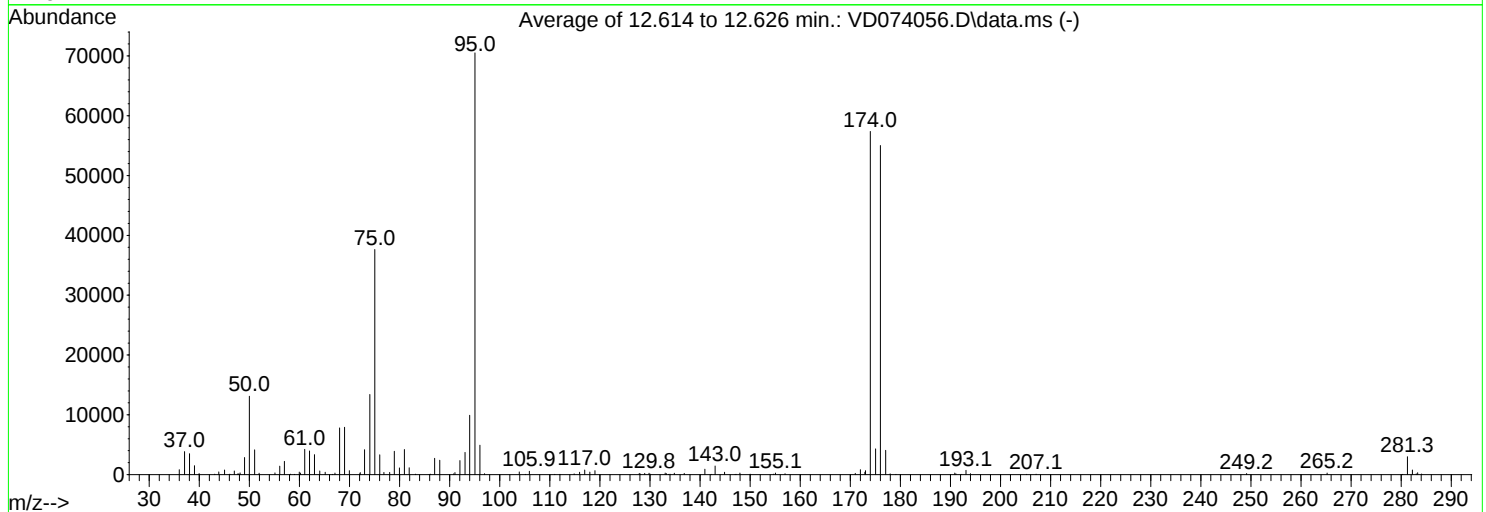


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD081222\
Data File : VD074056.D
Acq On : 12 Aug 2022 09:43
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D081022S.M
Title : SW846 8260
Last Update : Sat Aug 13 01:47:26 2022

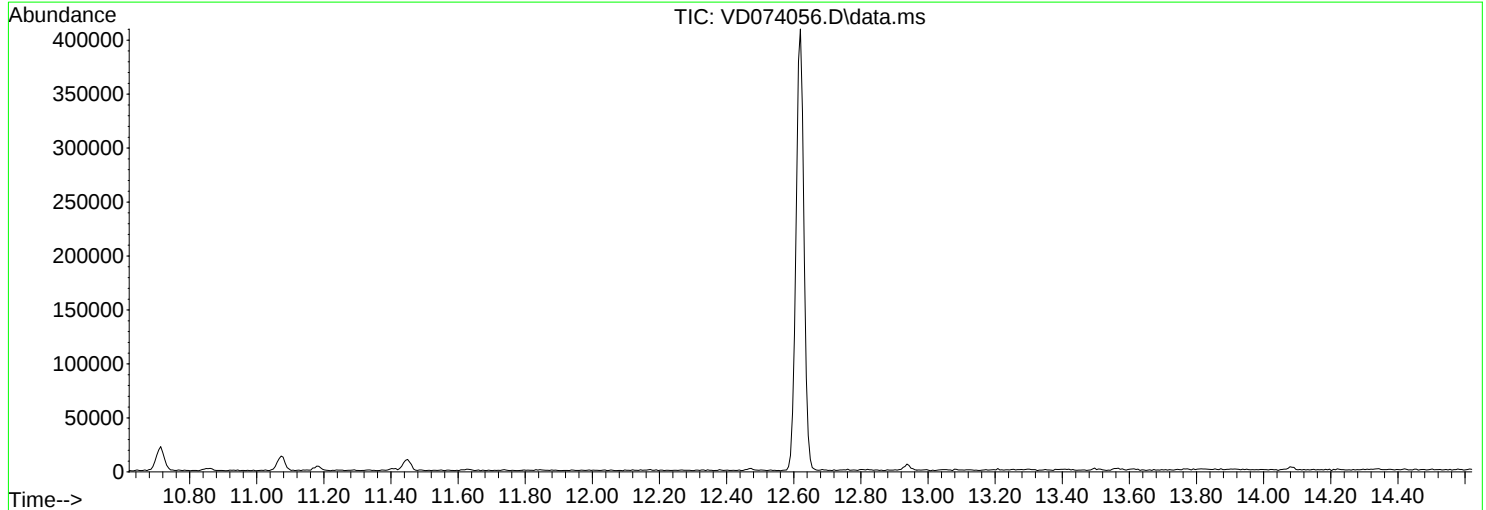

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1810

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	13107	PASS
75	95	30	60	53.4	37648	PASS
95	95	100	100	100.0	70515	PASS
96	95	5	9	7.0	4916	PASS
173	174	0.00	2	1.2	674	PASS
174	95	50	100	81.4	57373	PASS
175	174	5	9	7.5	4318	PASS
176	174	95	101	95.9	55021	PASS
177	176	5	9	7.4	4059	PASS