

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD081318\
 Data File : VD059754.D
 Acq On : 14 Aug 2018 00:56
 Operator : VA/AP
 Sample : J4442-51
 Misc : 6.01g/5ml/MSVOA D/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SP-1-6

Quant Time: Aug 14 04:41:02 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D081018S.M
 Quant Title : SW846 8260
 QLast Update : Sat Aug 11 05:42:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.64	168	18544	50.00	ug/l	0.02
34) 1,4-Difluorobenzene	6.69	114	30313	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.69	117	28503	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.90	152	14186	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.02	65	27456	94.59	ug/l	0.02
Spiked Amount 50.000			Recovery	=	189.18%	
35) Dibromofluoromethane	5.54	113	16845	53.96	ug/l	0.00
Spiked Amount 50.000			Recovery	=	107.92%	
50) Toluene-d8	8.70	98	27034	43.67	ug/l	0.00
Spiked Amount 50.000			Recovery	=	87.34%	
62) 4-Bromofluorobenzene	11.93	95	13487	43.43	ug/l	0.00
Spiked Amount 50.000			Recovery	=	86.86%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD081318\
Data File : VD059754.D
Acq On : 14 Aug 2018 00:56
Operator : VA/AP
Sample : J4442-51
Misc : 6.01a/5ml/MSVOA D/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SP-1-6

Quant Time: Aug 14 04:41:02 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D081018S.M
Quant Title : SW846 8260
QLast Update : Sat Aug 11 05:42:24 2018
Response via : Initial Calibration




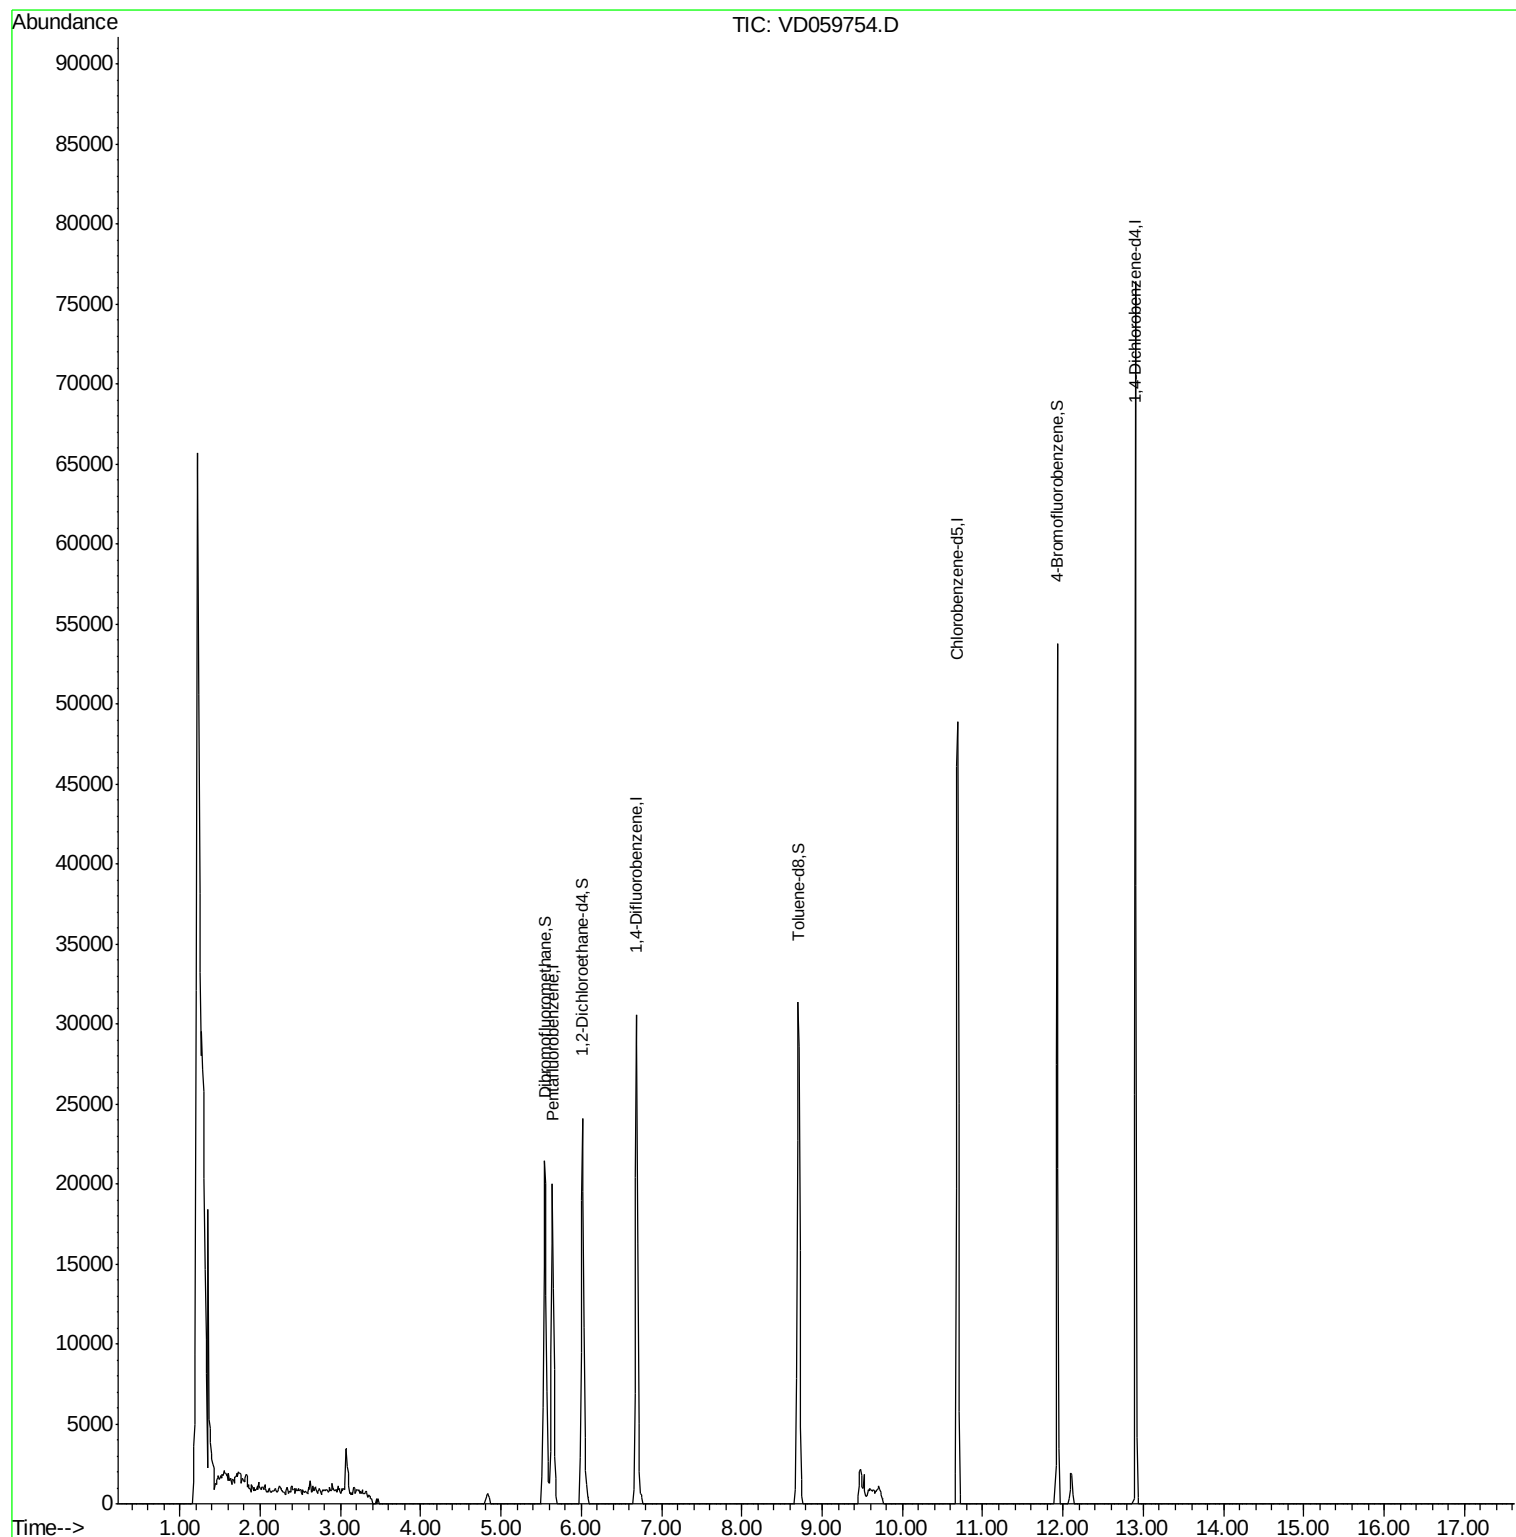


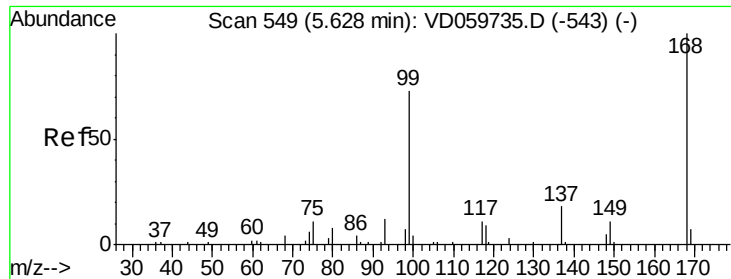

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.64 min Scan# 551
Delta R.T. 0.02 min
Lab File: VD059754.D
Acq: 14 Aug 2018 00:56




Instrument :
MSVOA_D
ClientSampleId :
SP-1-6


Tot Ion:168 Resp: 18544
Ion Ratio Lower Upper
168 100
99 64.0 61.4 92.2

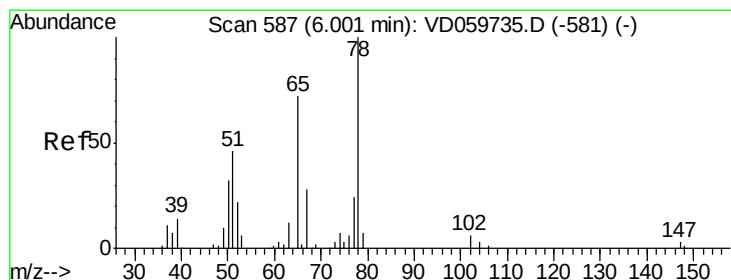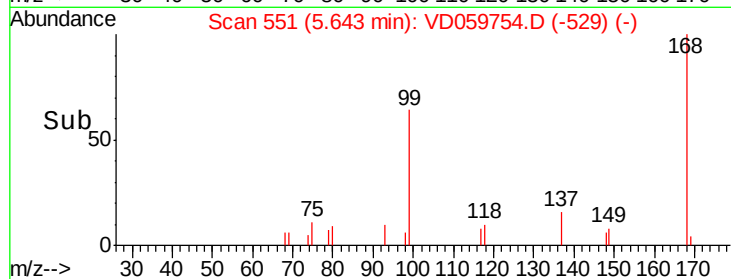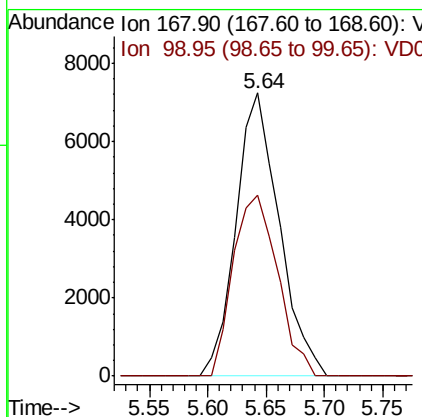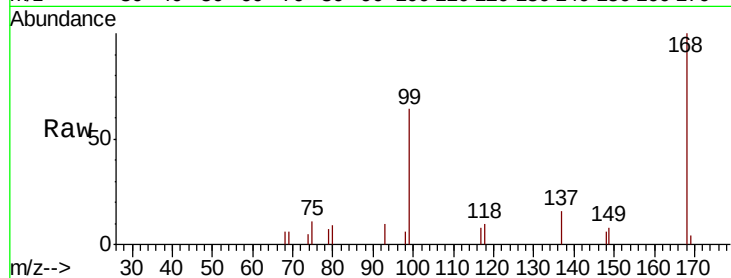

#33
1,2-Dichloroethane-d4
Concen: N.D. ug/l
RT: 6.02 min Scan# 589
Delta R.T. 0.02 min
Lab File: VD059754.D
Acq: 14 Aug 2018 00:56

Tgt Ion: 65 Resp: 27456
Ion Ratio Lower Upper
65 100
67 42.4 0.0 77.4

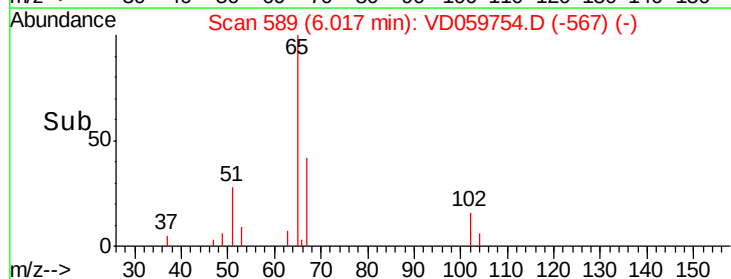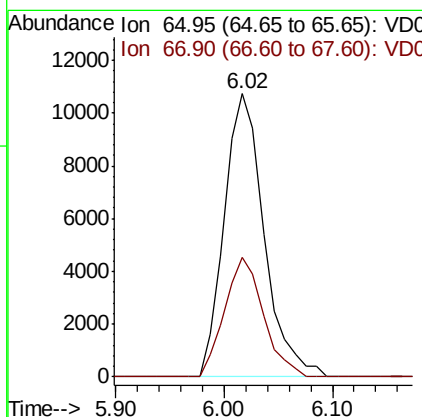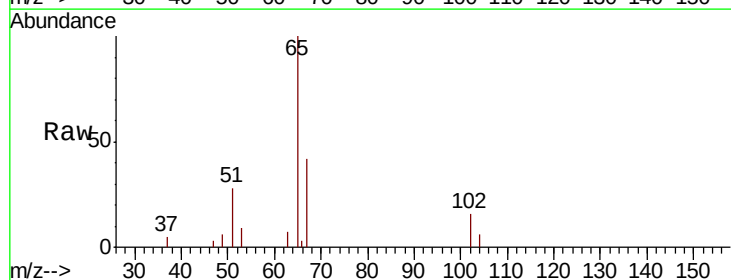

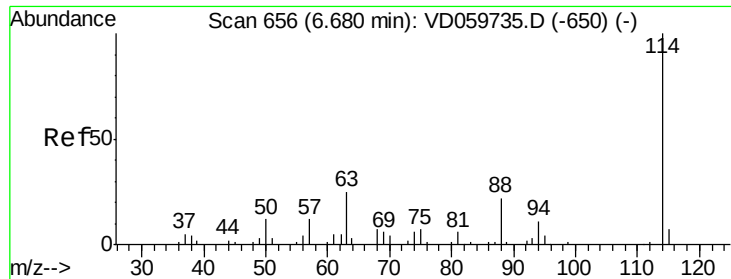

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.69 min Scan# 657

Delta R.T. 0.01 min

Lab File: VD059754.D

Acq: 14 Aug 2018 00:56

Instrument :

MSVOA_D

ClientSampleId :

SP-1-6


Tot Ion:114 Resp: 30313

Ion Ratio Lower Upper

114 100

63 24.0 0.0 50.6




88 22.8 0.0 43.4

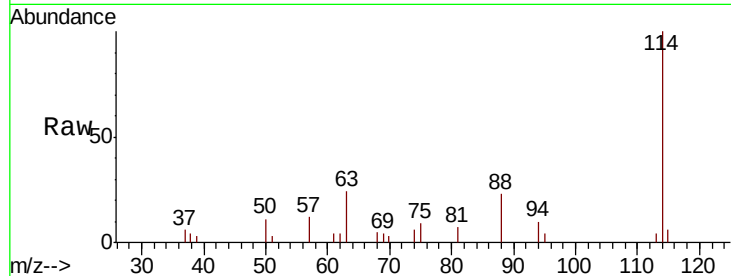

Abundance Ion 114.00 (113.70 to 114.70): V

Ion 62.95 (62.65 to 63.65): V

Ion 87.90 (87.60 to 88.60): V

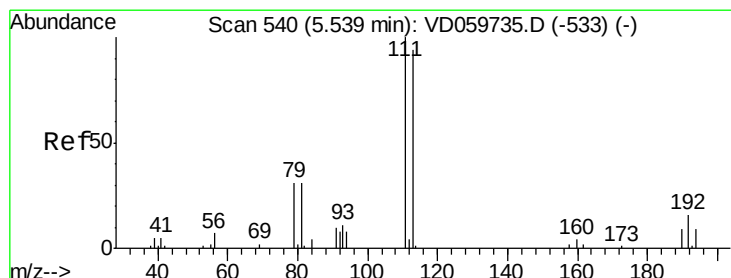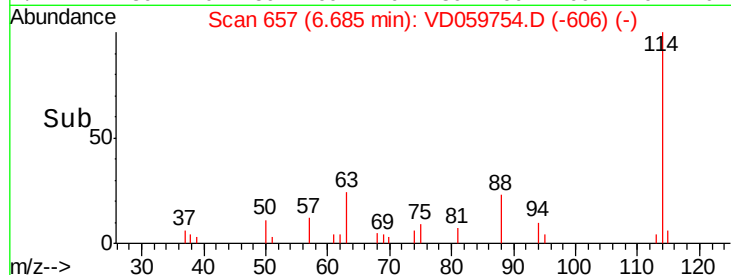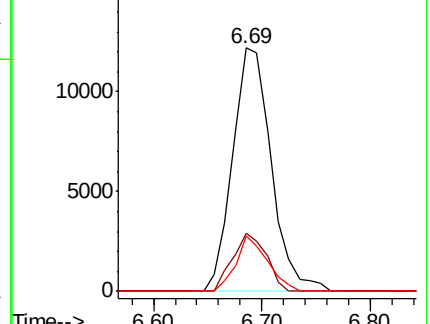

#35

Dibromofluoromethane

Concen: 50.00 ug/l

RT: 5.54 min Scan# 541

Delta R.T. 0.01 min

Lab File: VD059754.D

Acq: 14 Aug 2018 00:56


Tgt Ion:113 Resp: 16845

Ion Ratio Lower Upper

113 100

111 89.8 85.3 127.9



192 18.5 13.9 20.9

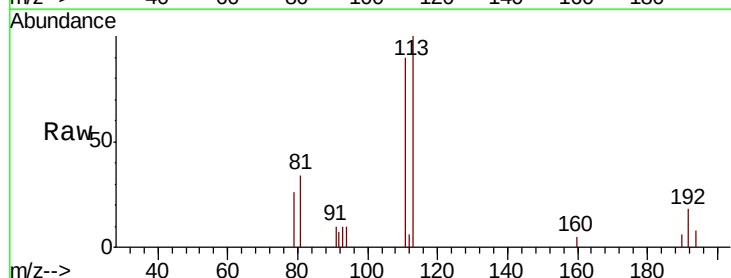


Abundance Ion 112.90 (112.60 to 113.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 191.80 (191.50 to 192.50): V

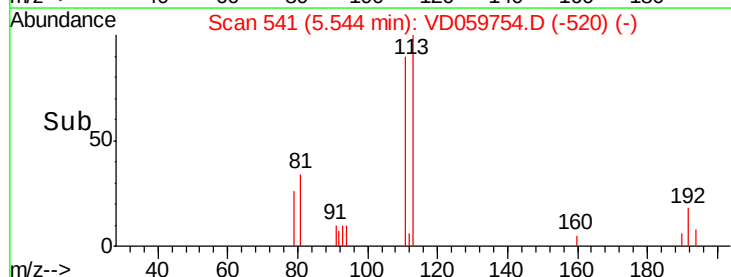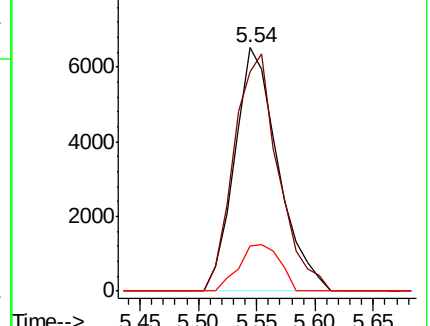


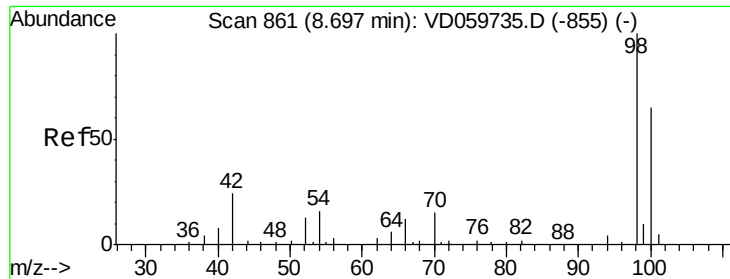




#50
Toluene-d8
Concen: N.D. ug/l
RT: 8.70 min Scan# 862
Delta R.T. 0.01 min
Lab File: VD059754.D
Acq: 14 Aug 2018 00:56

Instrument :
MSVOA_D
ClientSampleId :
SP-1-6

Tot Ion: 98 Resp: 27034
Ion Ratio Lower Upper
98 100
100 65.2 52.2 78.2

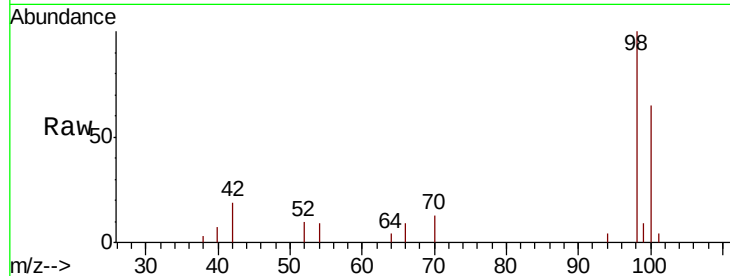


Abundance Ion 98.05 (97.75 to 98.75): VD0
Ion 100.05 (99.75 to 100.75): VD

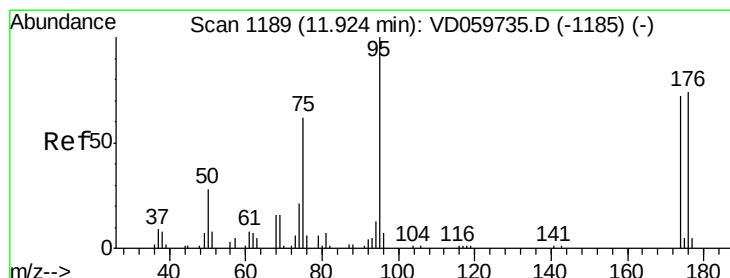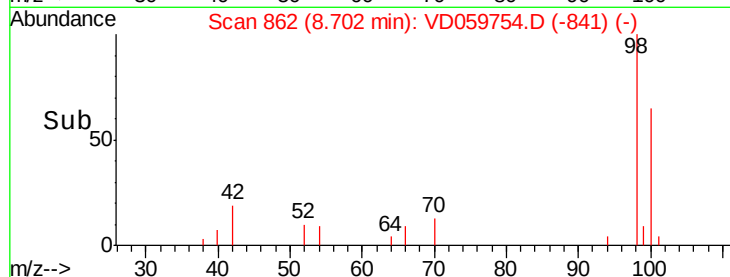
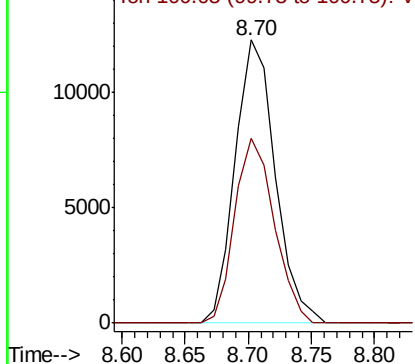



#62
4-Bromofluorobenzene
Concen: N.D. ug/l
RT: 11.93 min Scan# 1190
Delta R.T. 0.01 min
Lab File: VD059754.D
Acq: 14 Aug 2018 00:56

Tgt Ion: 95 Resp: 13487
Ion Ratio Lower Upper
95 100
174 92.0 0.0 143.2
176 99.9 0.0 147.2

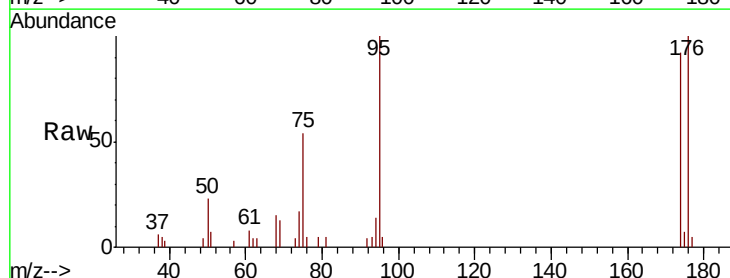

Abundance Ion 95.00 (94.70 to 95.70): VD0
Ion 173.90 (173.60 to 174.60): V
Ion 175.90 (175.60 to 176.60): V

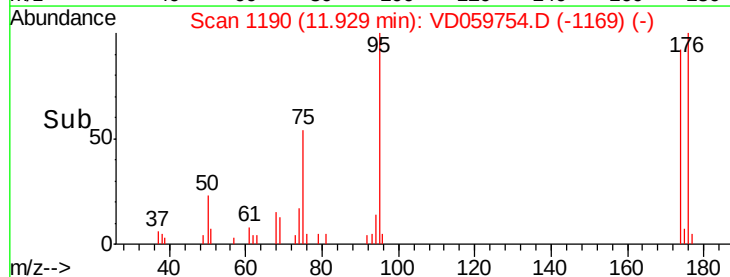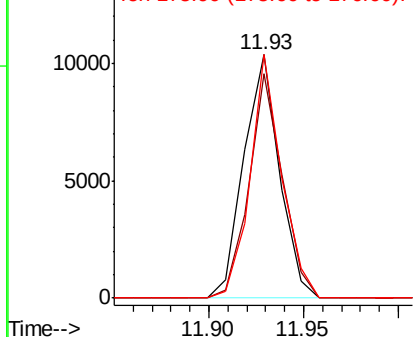


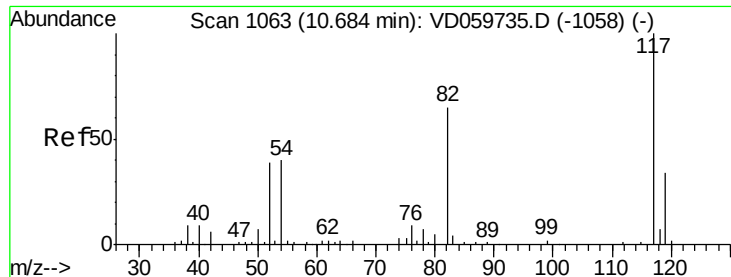




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.69 min Scan# 1064
Delta R.T. 0.01 min
Lab File: VD059754.D
Acq: 14 Aug 2018 00:56

Instrument :
MSVOA_D
ClientSampleId :
SP-1-6

Tot Ion:117 Resp: 28503
Ion Ratio Lower Upper
117 100
82 60.6 51.9 77.9
119 31.3 27.4 41.0

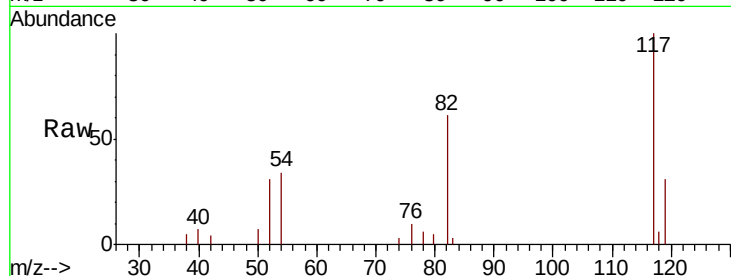


Abundance Ion 116.95 (116.65 to 117.65): V
Ion 82.05 (81.75 to 82.75): V
Ion 118.95 (118.65 to 119.65): V

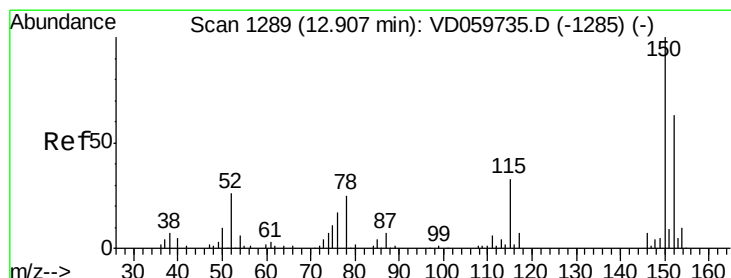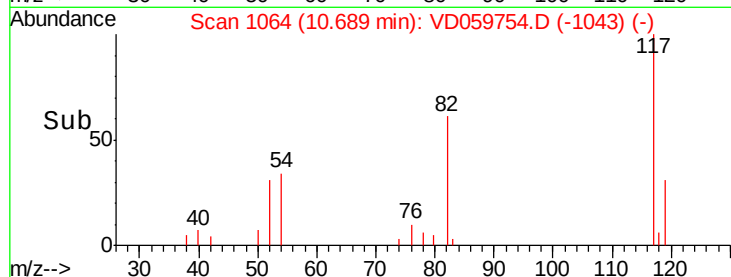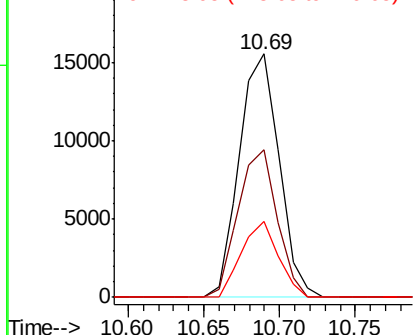

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.90 min Scan# 1289
Delta R.T. -0.00 min
Lab File: VD059754.D
Acq: 14 Aug 2018 00:56

Tgt Ion:152 Resp: 14186
Ion Ratio Lower Upper
152 100
115 61.3 29.8 89.3
150 158.6 0.0 320.4

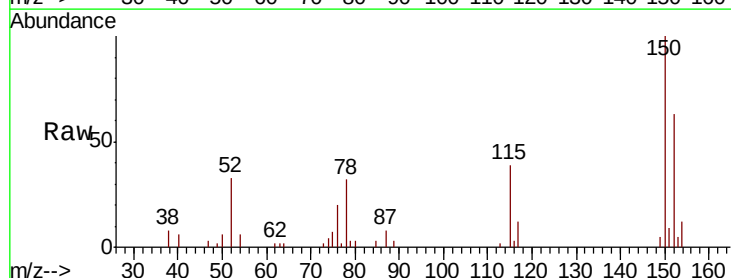

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 115.00 (114.70 to 115.70): V
Ion 149.90 (149.60 to 150.60): V

