
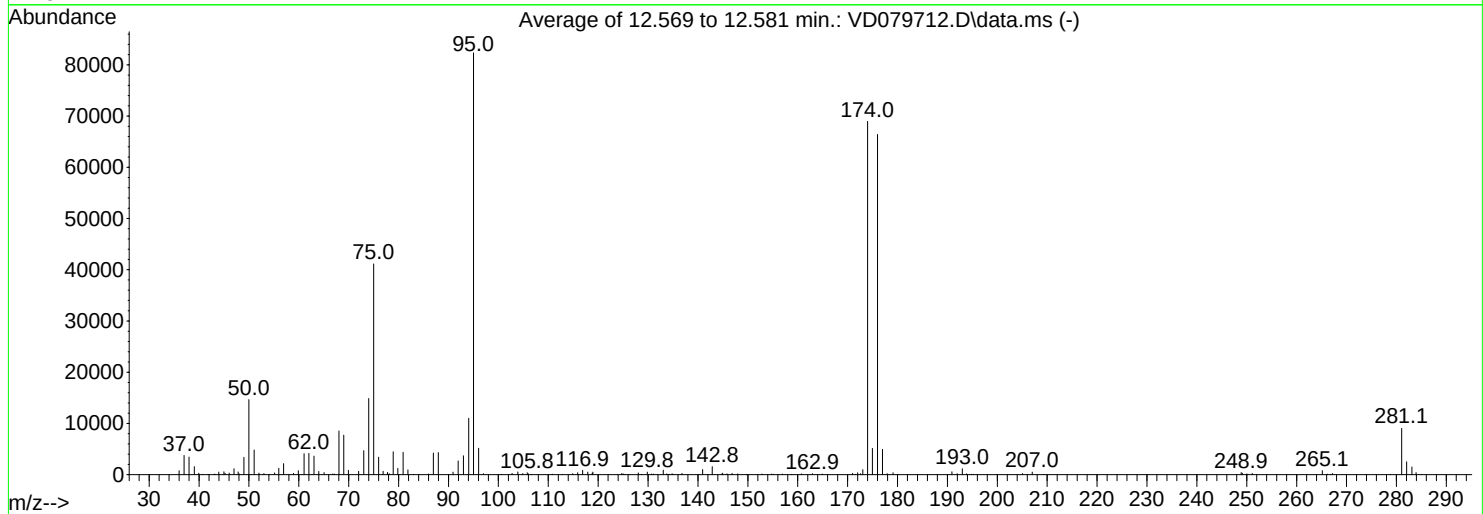


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD081324\
Data File : VD079712.D
Acq On : 13 Aug 2024 08:47
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D081224S.M
Title : SW846 8260
Last Update : Tue Aug 13 01:06:11 2024

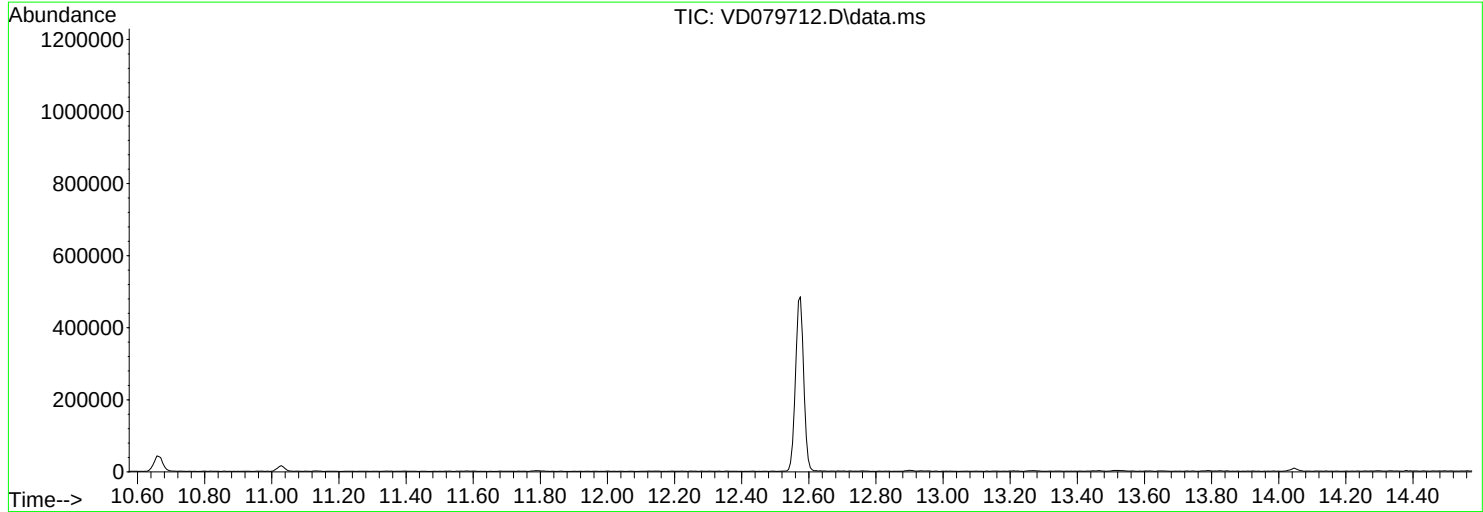

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.8	14637	PASS
75	95	30	60	49.9	41125	PASS
95	95	100	100	100.0	82339	PASS
96	95	5	9	6.3	5148	PASS
173	174	0.00	2	1.4	975	PASS
174	95	50	100	83.7	68955	PASS
175	174	5	9	7.4	5121	PASS
176	174	95	101	96.3	66416	PASS
177	176	5	9	7.4	4932	PASS