


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD081418\
Data File : VD059762.D
Acq On : 14 Aug 2018 11:40
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D081018S.M
Title : SW846 8260
Last Update : Sat Aug 11 05:42:24 2018

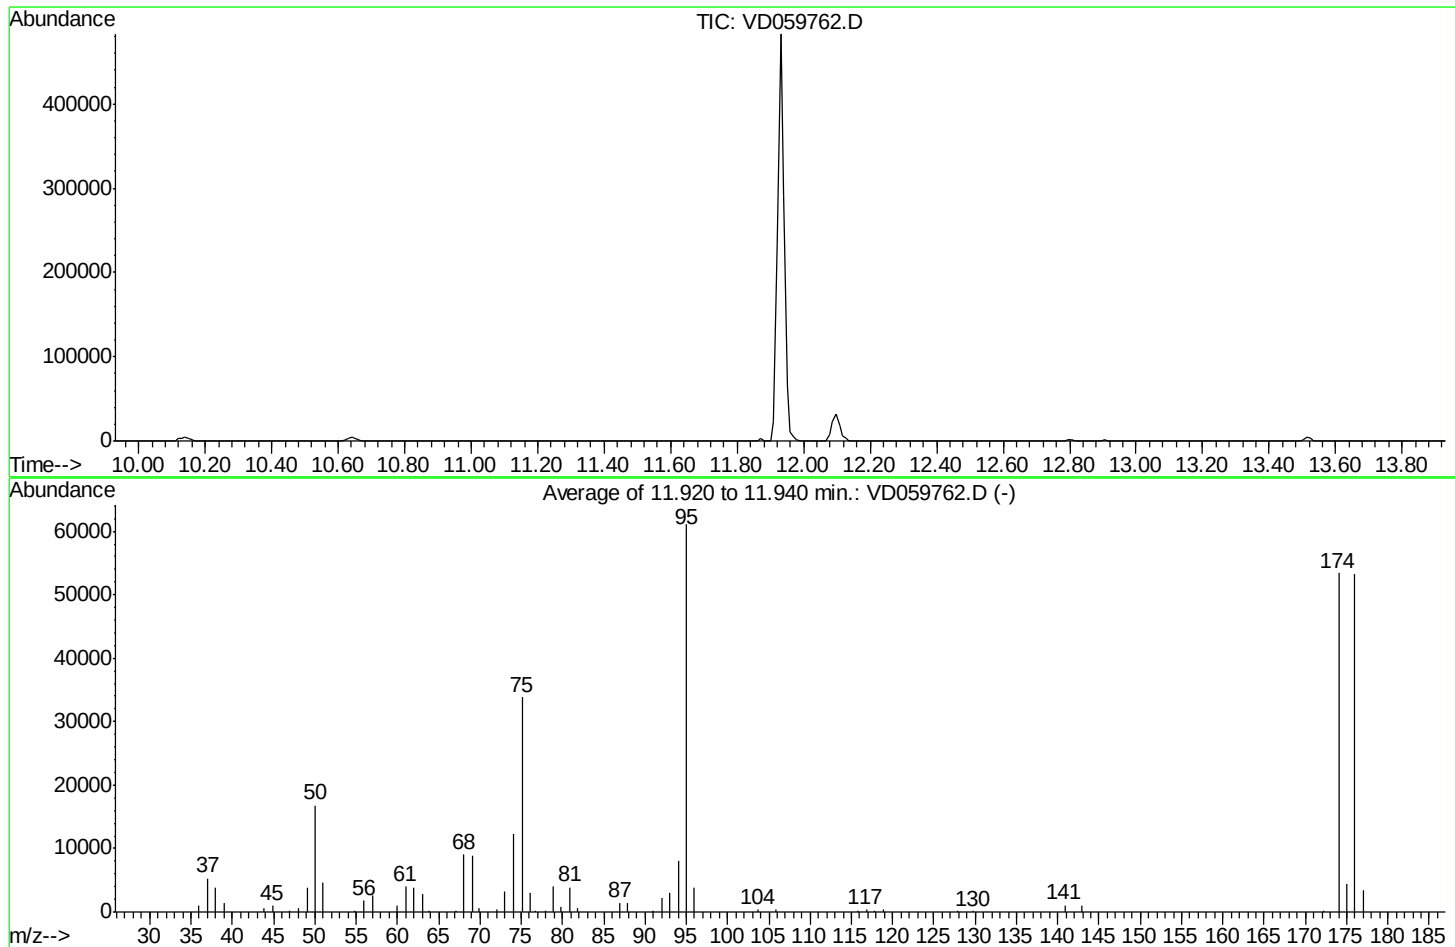

AutoFind: Scans 1189, 1190, 1191; Background Corrected with Scan 1185

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	27.6	16846	PASS
75	95	30	60	55.4	33869	PASS
95	95	100	100	100.0	61098	PASS
96	95	5	9	6.3	3826	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.4	53418	PASS
175	174	5	9	8.3	4407	PASS
176	174	95	101	99.7	53232	PASS
177	176	5	9	6.3	3374	PASS