


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD081419\
Data File : VD063570.D
Acq On : 14 Aug 2019 12:32
Operator : JC/SY
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D080919S.M
Title : SW846 8260
Last Update : Sat Aug 10 06:42:47 2019

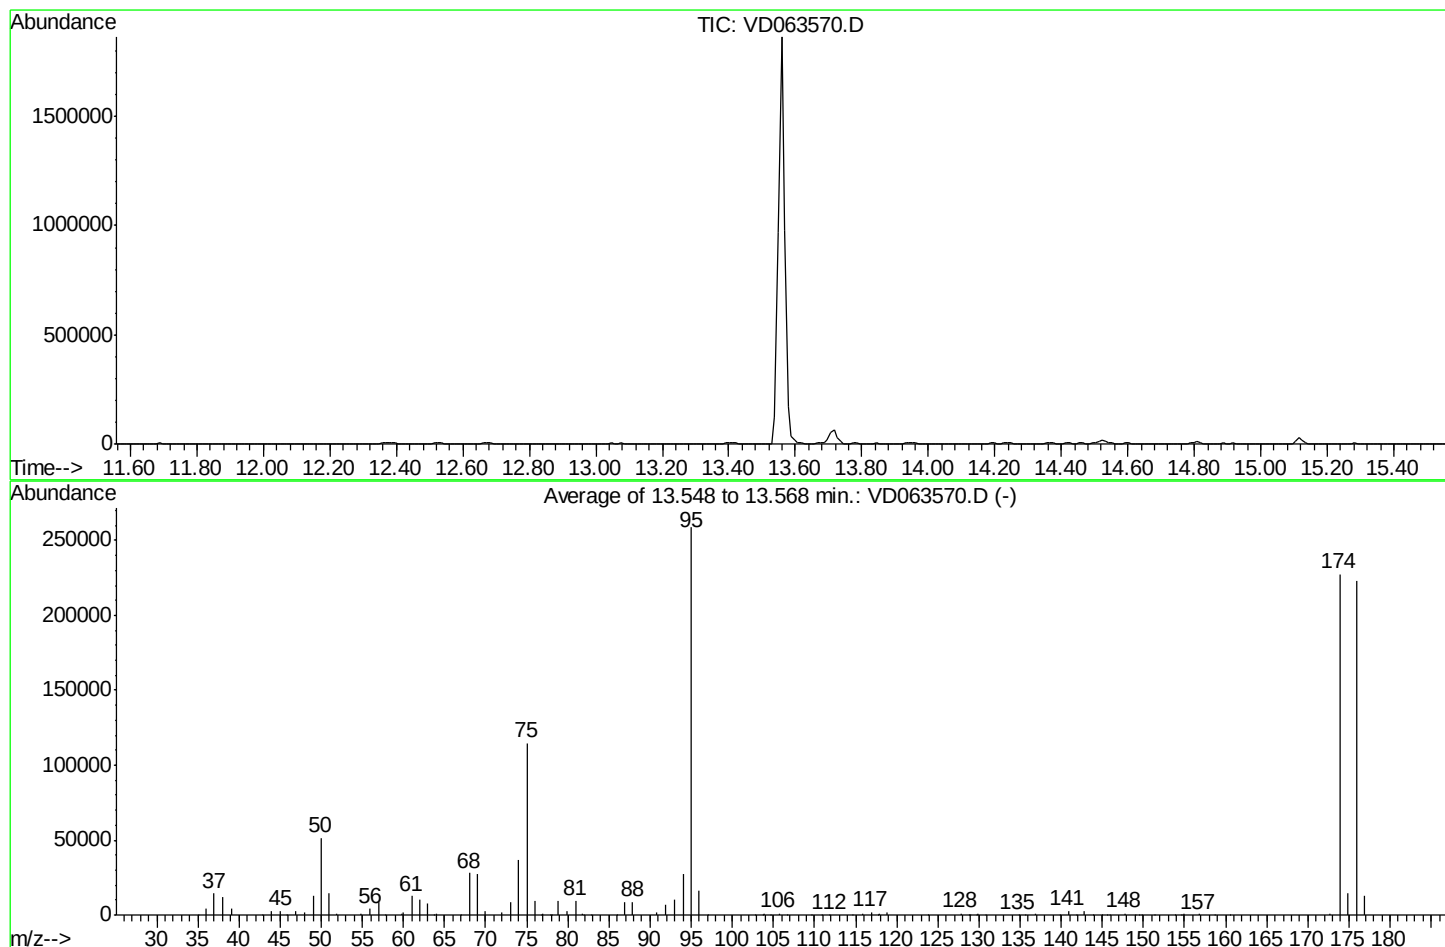

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1226

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	51466	PASS
75	95	30	60	44.4	114874	PASS
95	95	100	100	100.0	258752	PASS
96	95	5	9	6.2	15938	PASS
173	174	0.00	2	0.2	529	PASS
174	95	50	100	87.9	227509	PASS
175	174	5	9	6.5	14799	PASS
176	174	95	101	98.0	222920	PASS
177	176	5	9	5.9	13235	PASS