


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD081423\
Data File : VD076989.D
Acq On : 14 Aug 2023 09:15
Operator : JC/SY
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D080823S.M
Title : SW846 8260
Last Update : Wed Aug 09 07:25:36 2023

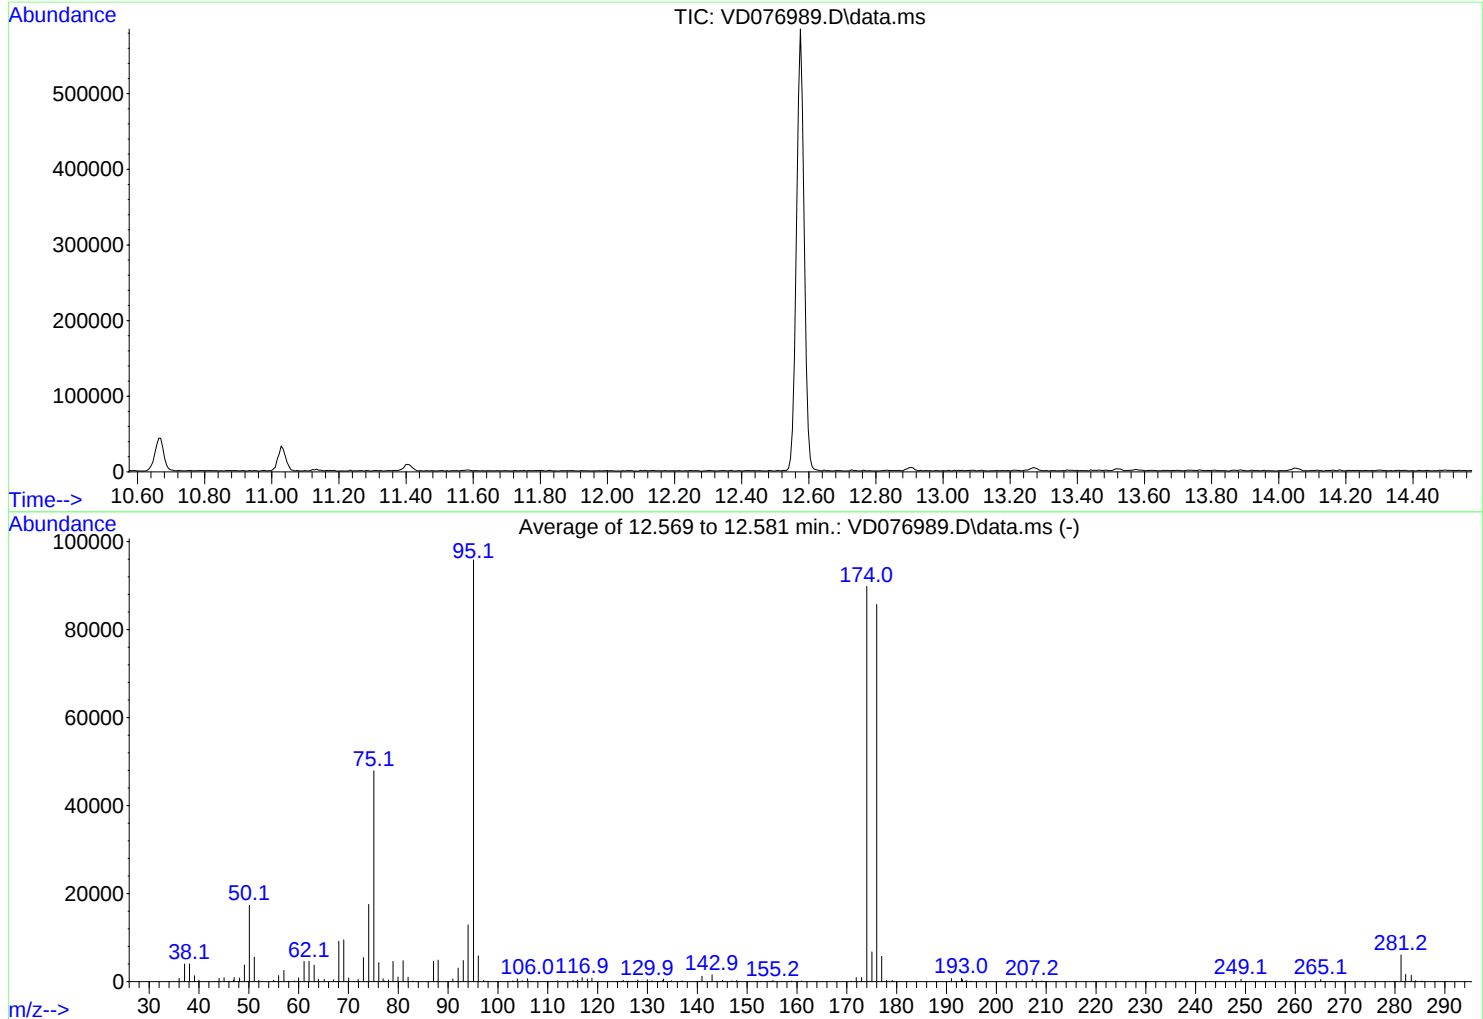

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	17346	PASS
75	95	30	60	50.0	47909	PASS
95	95	100	100	100.0	95851	PASS
96	95	5	9	6.1	5845	PASS
173	174	0.00	2	1.0	926	PASS
174	95	50	100	93.7	89800	PASS
175	174	5	9	7.5	6776	PASS
176	174	95	101	95.4	85691	PASS
177	176	5	9	6.7	5761	PASS