


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD081518\
Data File : VD059795.D
Acq On : 15 Aug 2018 12:49
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D081518S.M
Title : SW846 8260
Last Update : Wed Aug 15 16:08:23 2018

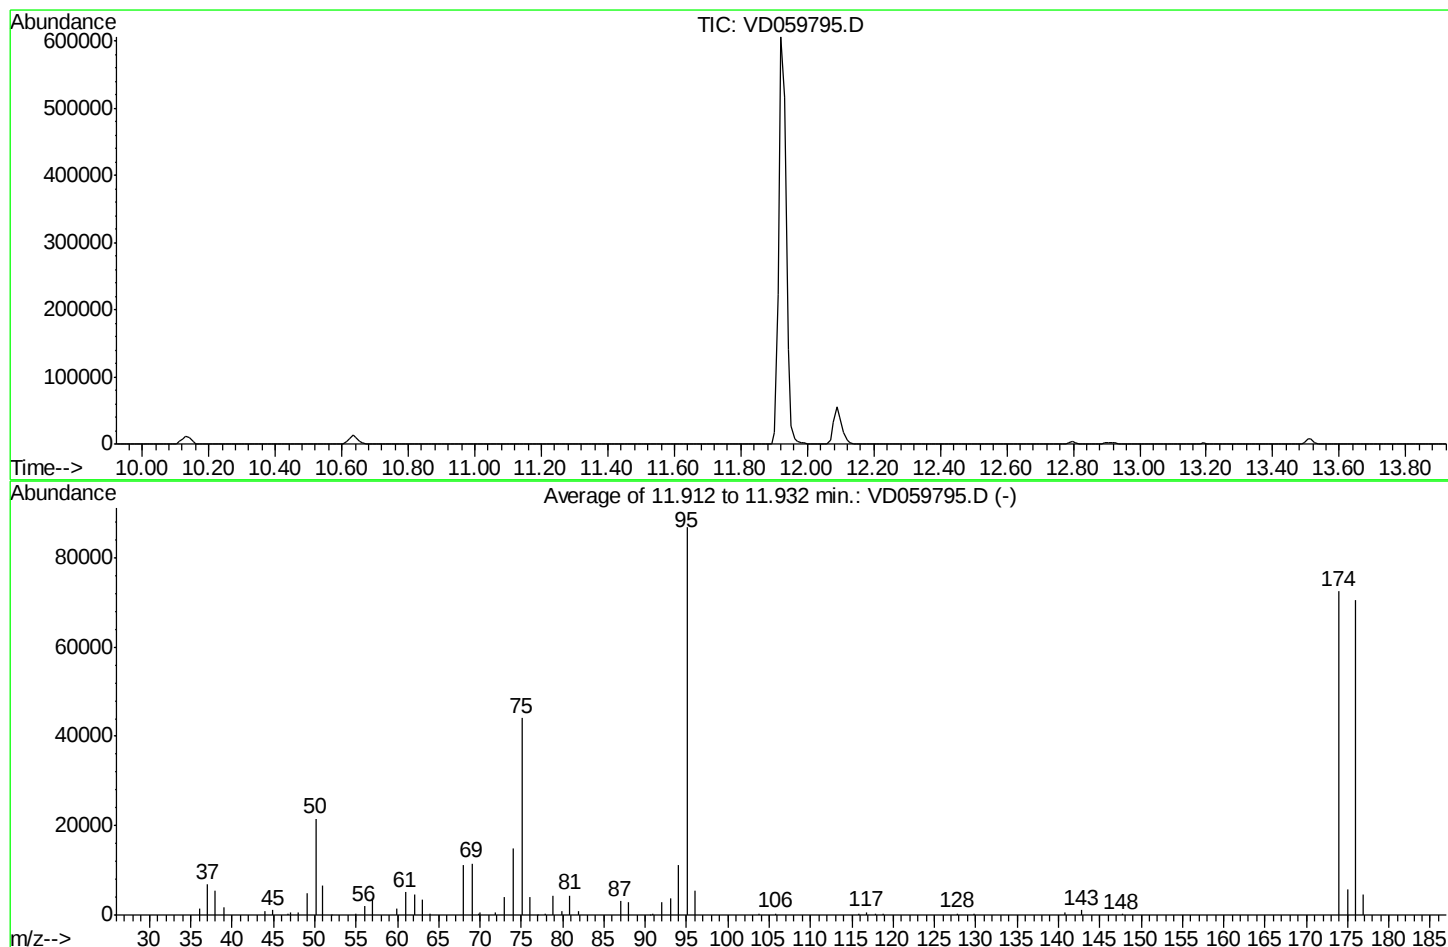

AutoFind: Scans 1188, 1189, 1190; Background Corrected with Scan 1184

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.8	21534	PASS
75	95	30	60	50.7	44024	PASS
95	95	100	100	100.0	86797	PASS
96	95	5	9	6.4	5593	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	83.4	72416	PASS
175	174	5	9	8.0	5809	PASS
176	174	95	101	97.4	70533	PASS
177	176	5	9	6.5	4571	PASS