
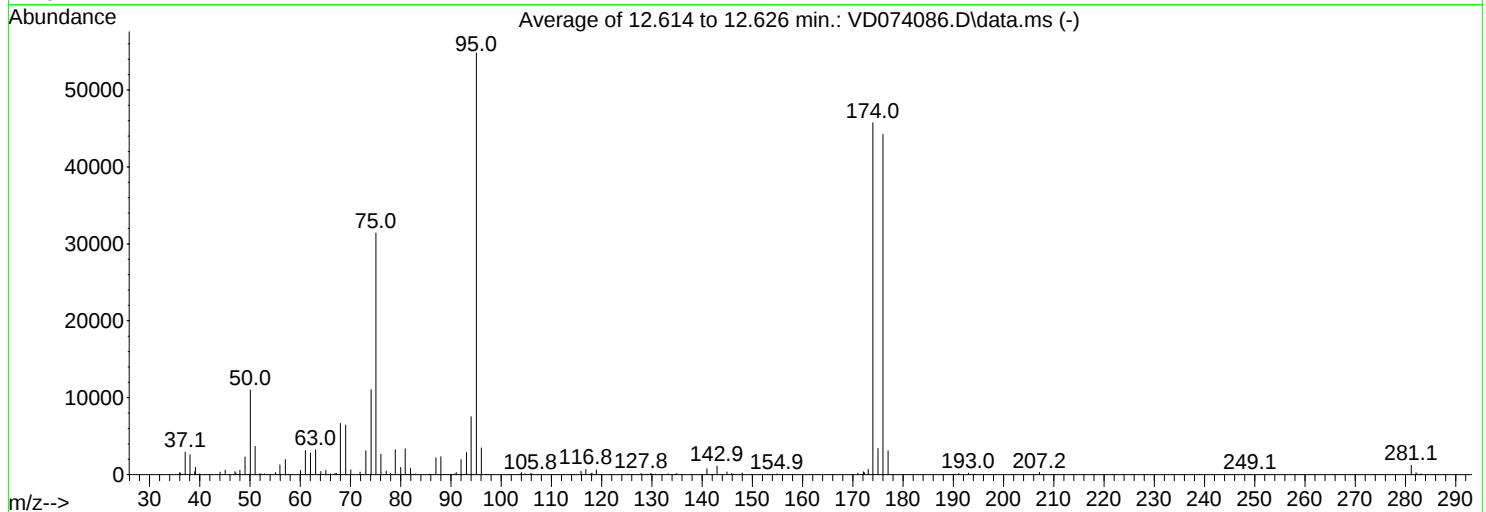


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD081522\
 Data File : VD074086.D
 Acq On : 15 Aug 2022 08:42
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D081522S.M
 Title : SW846 8260
 Last Update : Tue Aug 16 01:41:25 2022

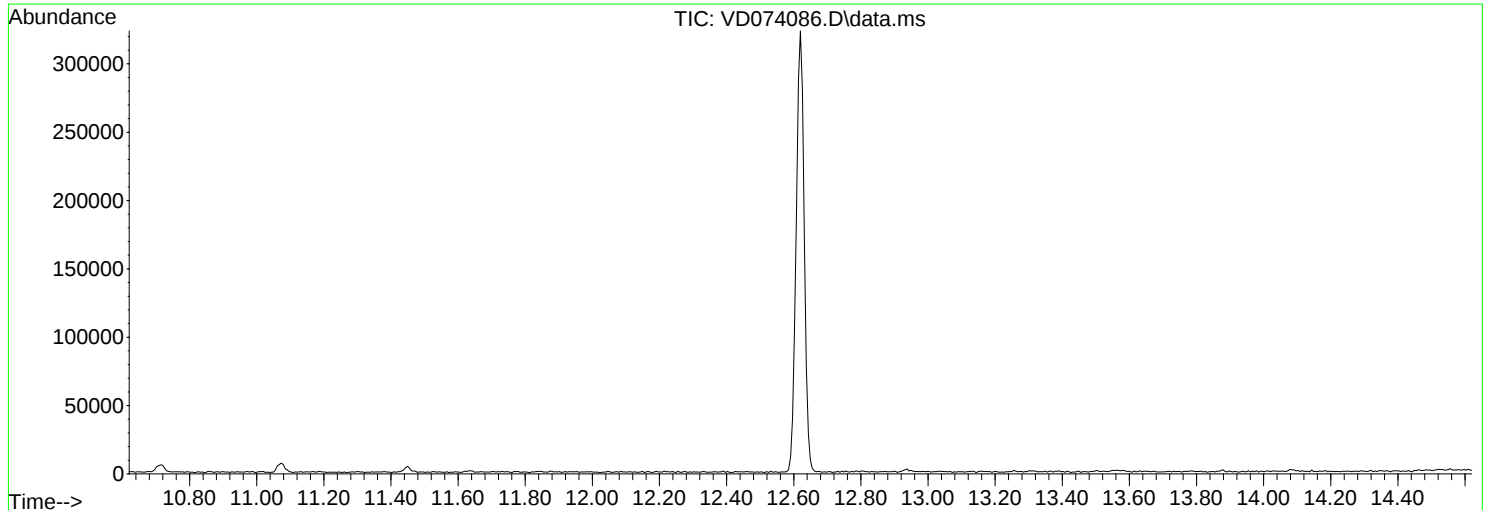

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1809

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	10999	PASS
75	95	30	60	57.3	31405	PASS
95	95	100	100	100.0	54827	PASS
96	95	5	9	6.3	3480	PASS
173	174	0.00	2	1.5	682	PASS
174	95	50	100	83.4	45752	PASS
175	174	5	9	7.5	3412	PASS
176	174	95	101	96.6	44208	PASS
177	176	5	9	7.0	3093	PASS