


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD081618\
Data File : VD059806.D
Acq On : 16 Aug 2018 10:38
Operator : VA/AP
Sample : BFB
Misc : 5.00g/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D081518S.M
Title : SW846 8260
Last Update : Wed Aug 15 16:08:23 2018

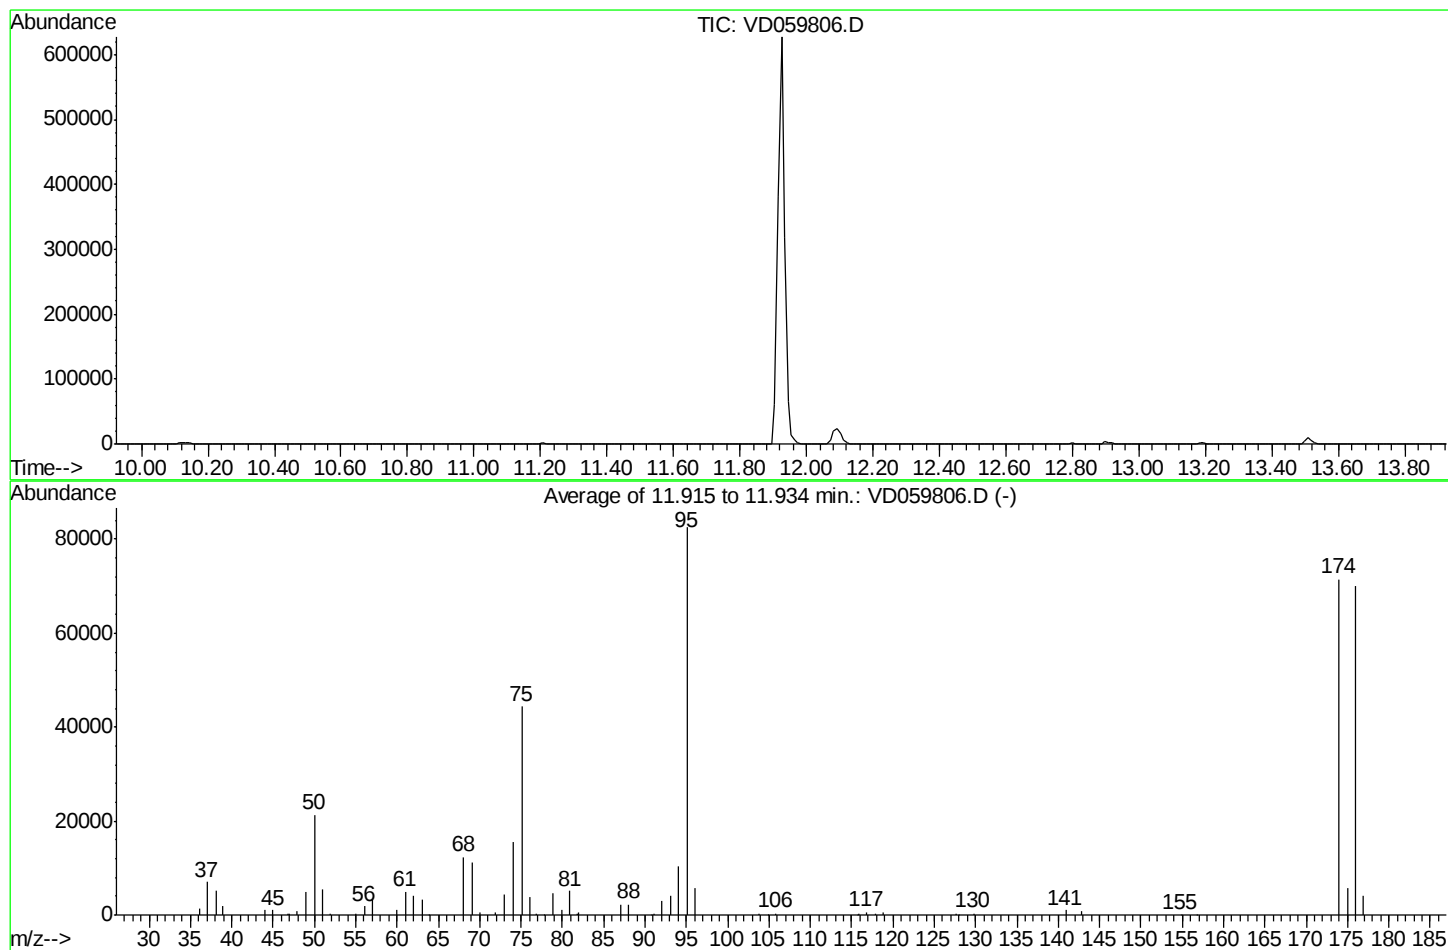

AutoFind: Scans 1188, 1189, 1190; Background Corrected with Scan 1183

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.9	21358	PASS
75	95	30	60	53.8	44365	PASS
95	95	100	100	100.0	82530	PASS
96	95	5	9	6.8	5633	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.6	71480	PASS
175	174	5	9	8.0	5699	PASS
176	174	95	101	97.8	69938	PASS
177	176	5	9	5.9	4096	PASS