


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD081619\
 Data File : VD063625.D
 Acq On : 16 Aug 2019 8:26
 Operator : JC/SY
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D080919S.M
 Title : SW846 8260
 Last Update : Sat Aug 10 06:42:47 2019

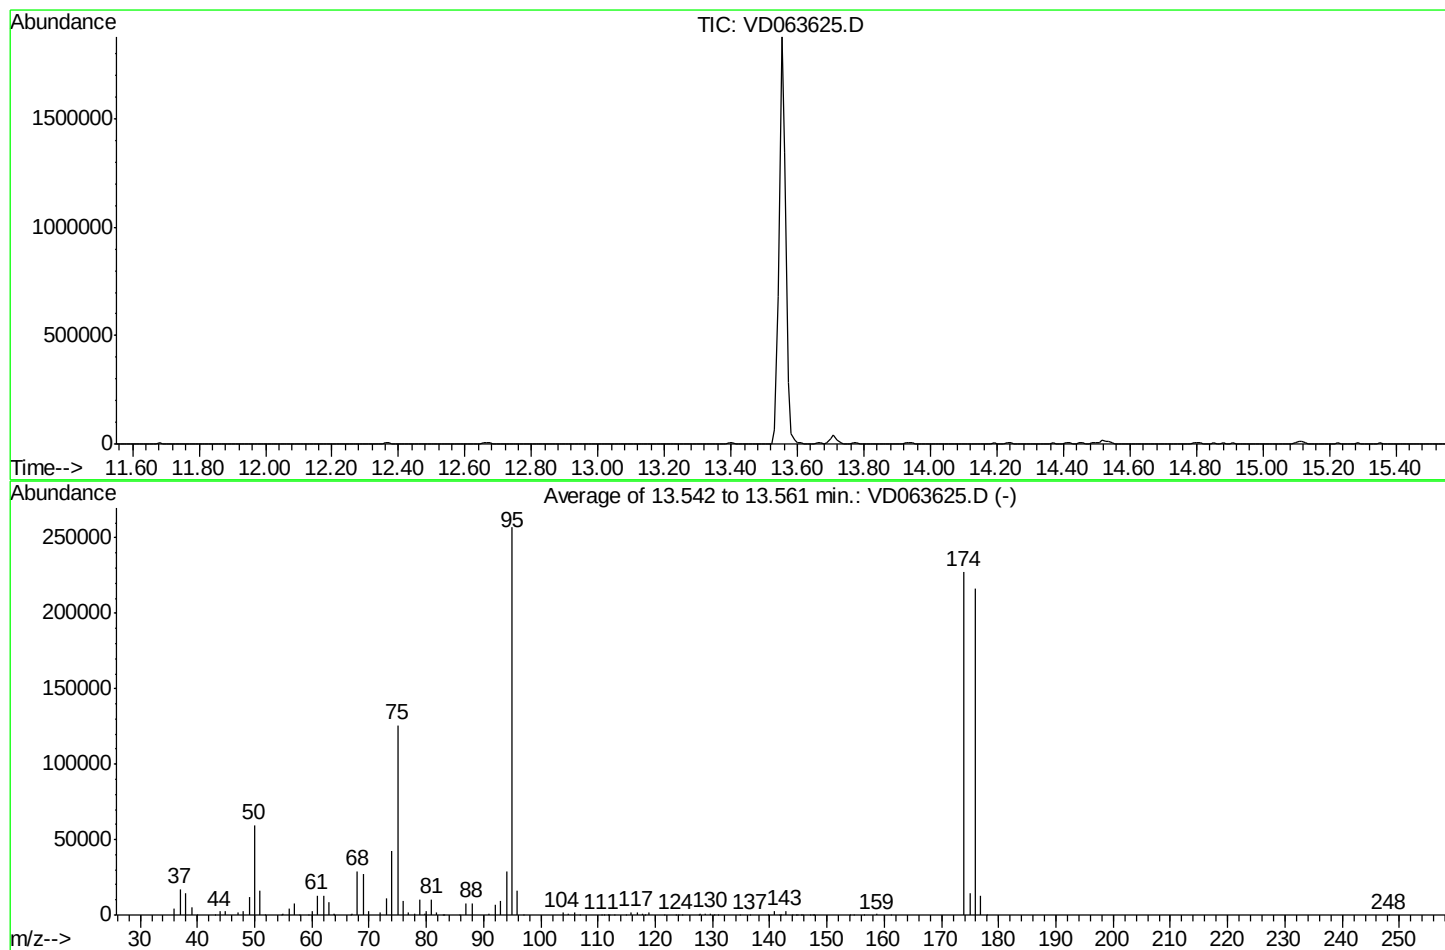

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	59429	PASS
75	95	30	60	48.9	125736	PASS
95	95	100	100	100.0	257066	PASS
96	95	5	9	6.3	16089	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	88.5	227509	PASS
175	174	5	9	6.5	14855	PASS
176	174	95	101	95.0	216141	PASS
177	176	5	9	5.8	12616	PASS