

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD081721\
 Data File : VD070102.D
 Acq On : 17 Aug 2021 23:46
 Operator : VA/SY
 Sample : VD0817SBL02
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD0817SBL02

Quant Time: Aug 18 04:32:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D081321S.M
 Quant Title : SW846 8260
 QLast Update : Sat Aug 14 02:33:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	371777	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	781952	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	766754	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	319588	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	297148	67.956	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	135.920%
35) Dibromofluoromethane	7.914	113	272152	53.871	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	107.740%
50) Toluene-d8	10.338	98	968295	49.279	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	98.560%
62) 4-Bromofluorobenzene	12.626	95	306080	47.293	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	94.580%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD081721\
Data File : VD070102.D
Acq On : 17 Aug 2021 23:46
Operator : VA/SY
Sample : VD0817SBL02
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD0817SBL02

Quant Time: Aug 18 04:32:52 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D081321S.M
Quant Title : SW846 8260
QLast Update : Sat Aug 14 02:33:51 2021
Response via : Initial Calibration




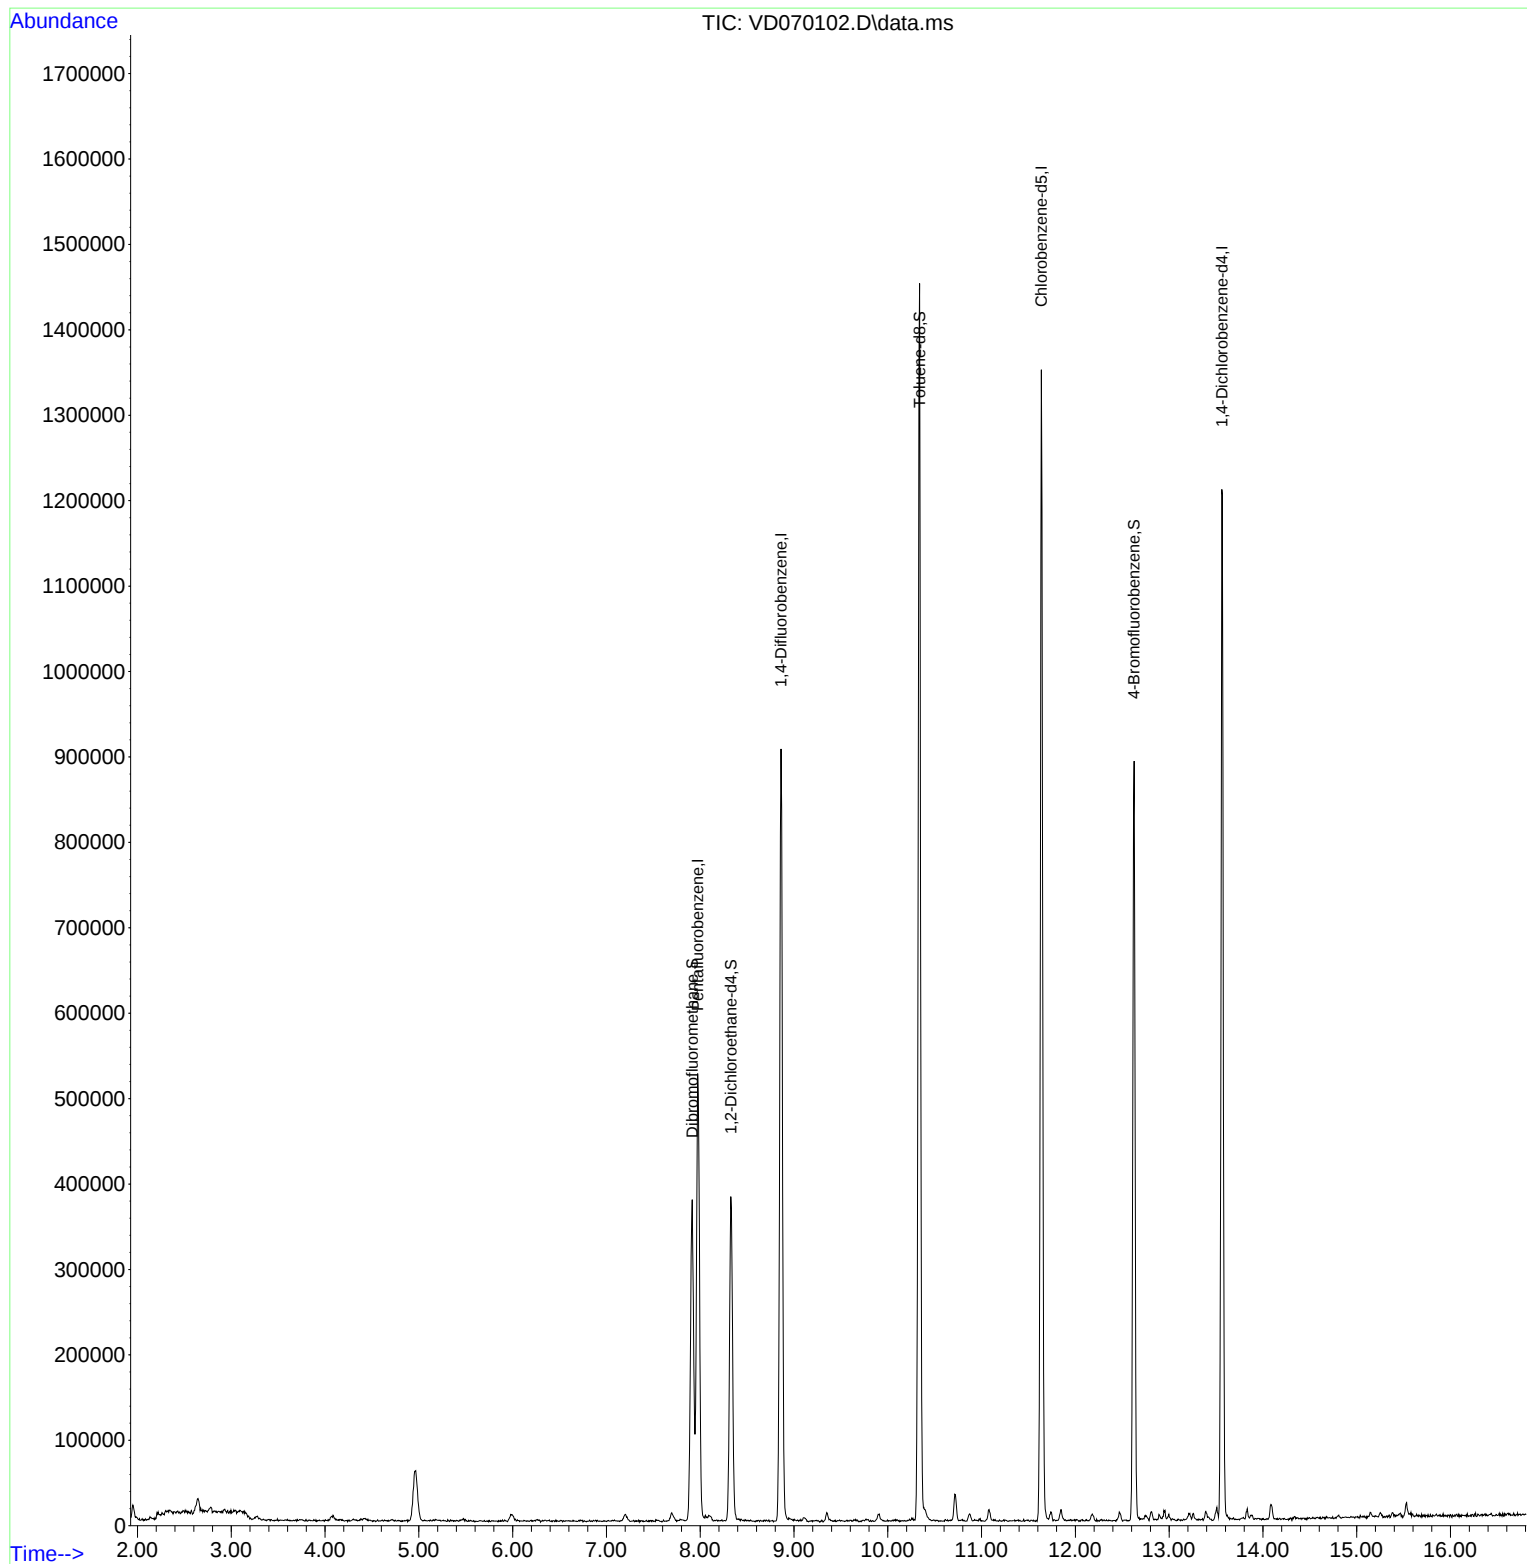


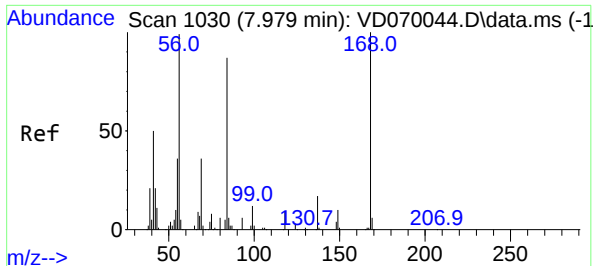

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.973 min Scan# 1029
Delta R.T. -0.006 min
Lab File: VD070102.D
Acq: 17 Aug 2021 23:46




Instrument :
MSVOA_D
ClientSampleId :
VD0817SBL02


Tgt Ion:168 Resp: 371777
Ion Ratio Lower Upper
168 100
99 57.3 50.3 75.5

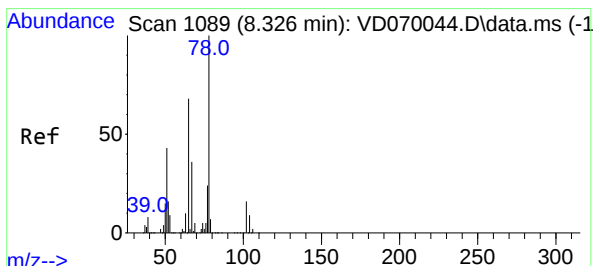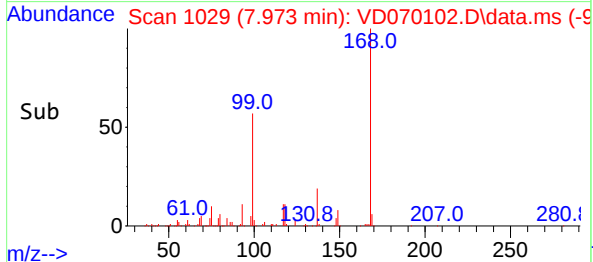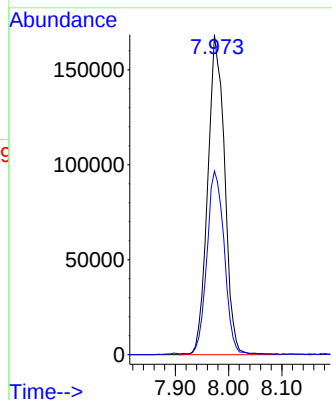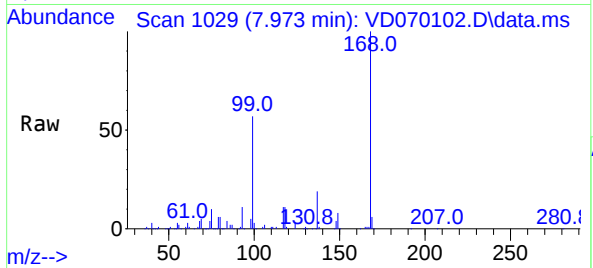

#33
1,2-Dichloroethane-d4
Concen: 67.956 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. 0.000 min
Lab File: VD070102.D
Acq: 17 Aug 2021 23:46

Tgt Ion: 65 Resp: 297148
Ion Ratio Lower Upper
65 100
67 54.2 0.0 107.8

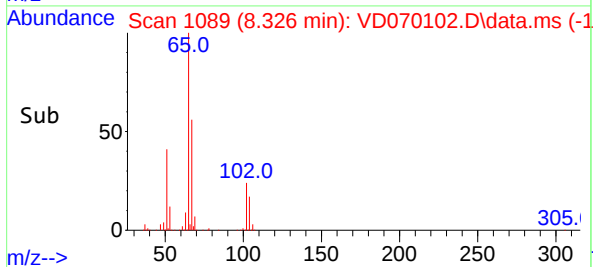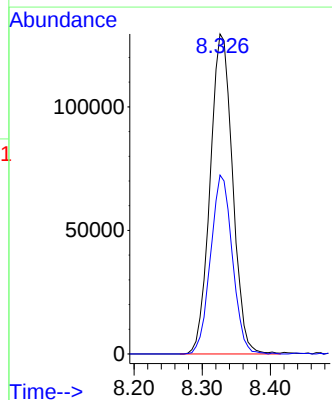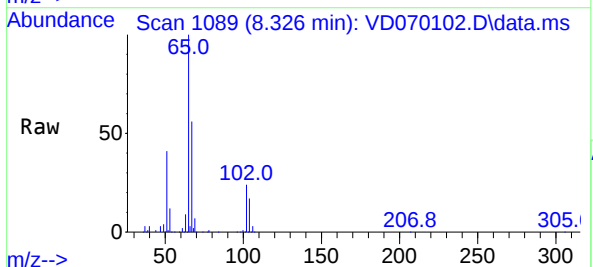




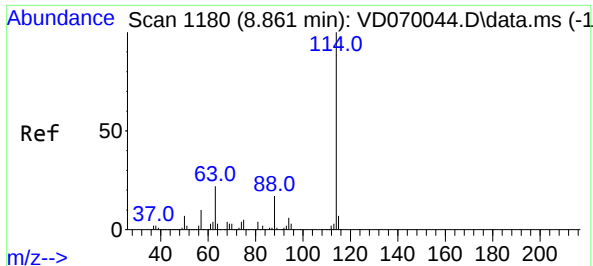


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. 0.000 min
Lab File: VD070102.D
Acq: 17 Aug 2021 23:46

Instrument :
MSVOA_D
ClientSampleId :
VD0817SBL02




Tgt Ion:114 Resp: 781952
Ion Ratio Lower Upper
114 100
63 20.0 0.0 43.6
88 15.8 0.0 33.4

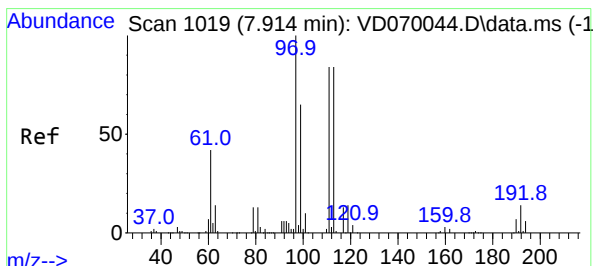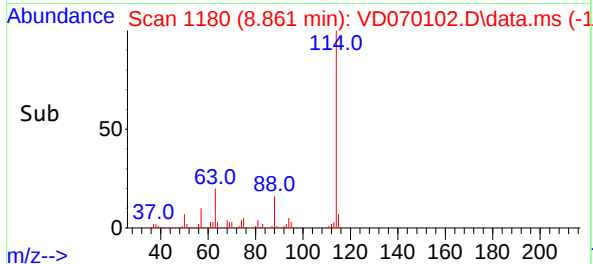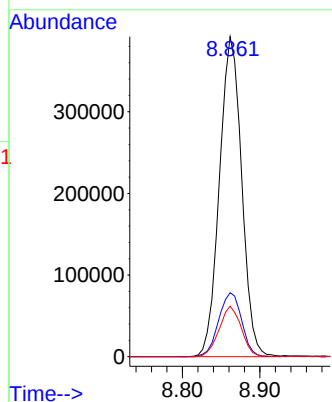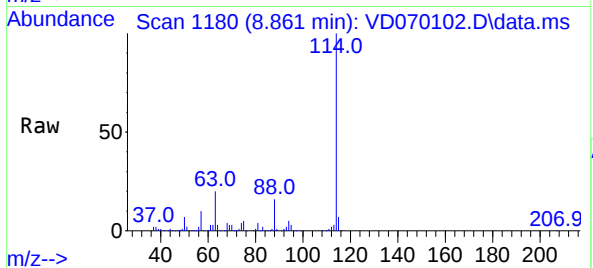


#35

Dibromofluoromethane
Concen: 53.871 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. 0.000 min
Lab File: VD070102.D
Acq: 17 Aug 2021 23:46

Tgt Ion:113 Resp: 272152
Ion Ratio Lower Upper
113 100
111 104.2 81.8 122.6
192 17.2 13.2 19.8


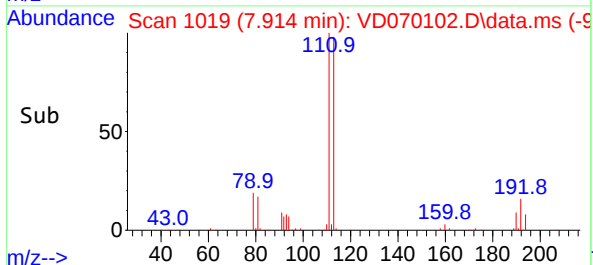
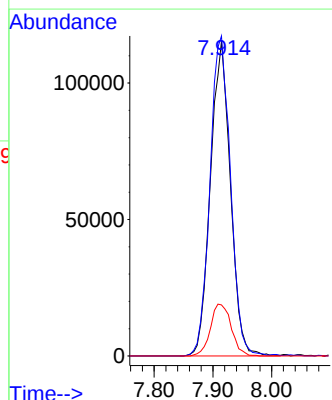
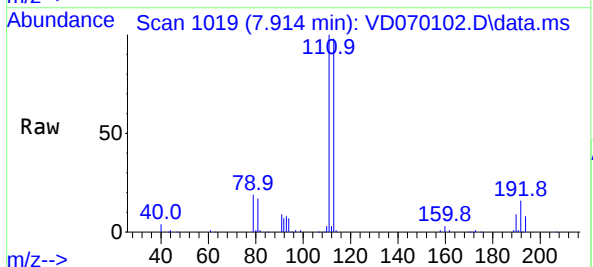


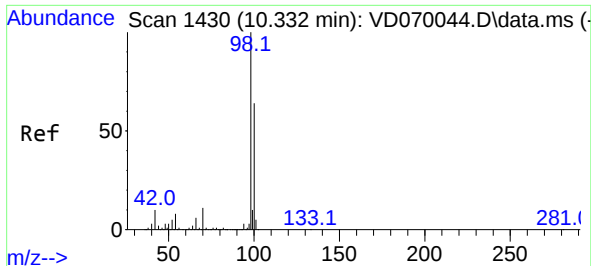

#50
Toluene-d8
Concen: 49.279 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. 0.006 min
Lab File: VD070102.D
Acq: 17 Aug 2021 23:46




Instrument :
MSVOA_D
ClientSampleId :
VD0817SBL02


Tgt Ion: 98 Resp: 968295
Ion Ratio Lower Upper
98 100
100 64.8 52.6 78.8

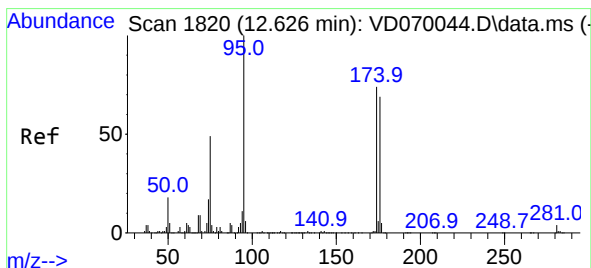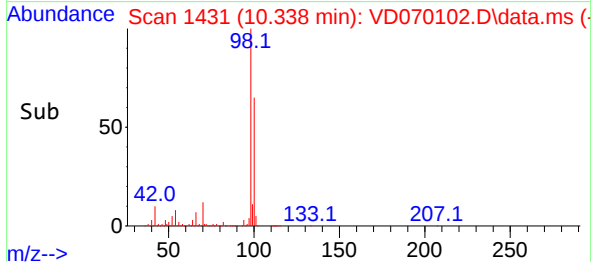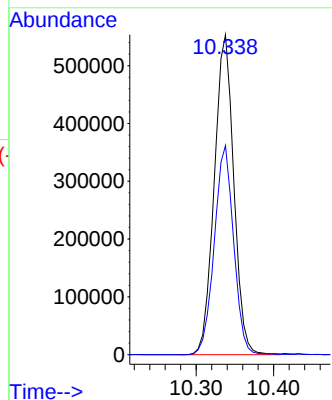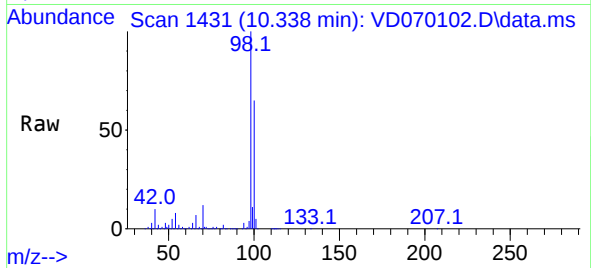

#62
4-Bromofluorobenzene
Concen: 47.293 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. 0.000 min
Lab File: VD070102.D
Acq: 17 Aug 2021 23:46

Tgt Ion: 95 Resp: 306080
Ion Ratio Lower Upper
95 100
174 74.1 0.0 141.6
176 71.3 0.0 138.2

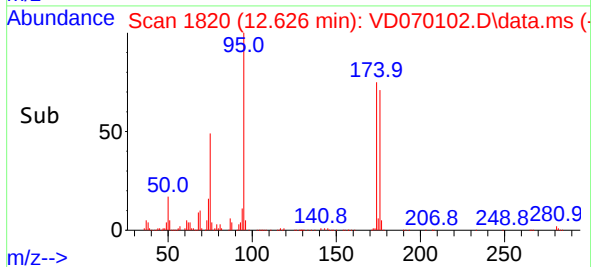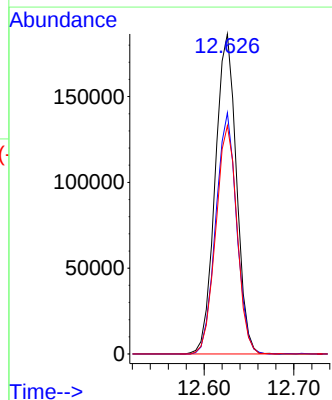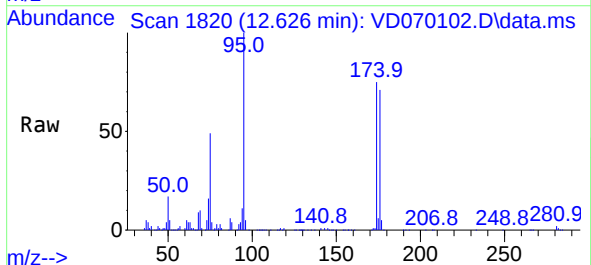




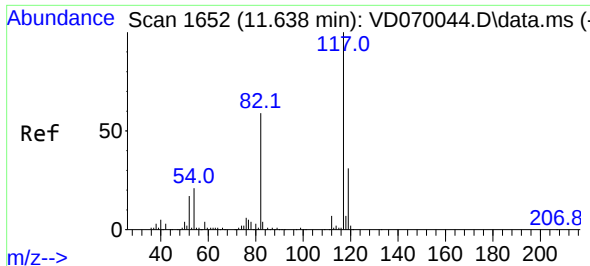


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1652
Delta R.T. 0.000 min
Lab File: VD070102.D
Acq: 17 Aug 2021 23:46

Instrument :
MSVOA_D
ClientSampleId :
VD0817SBL02

Tgt Ion:117 Resp: 766754

Ion	Ratio	Lower	Upper
117	100		
82	57.2	47.5	71.3
119	31.9	25.1	37.7

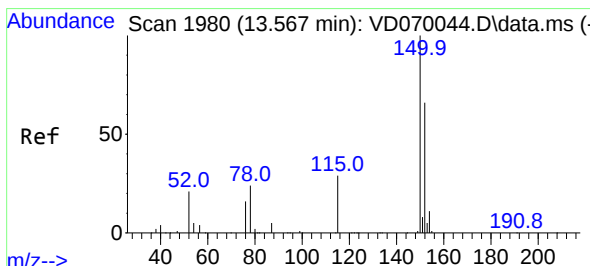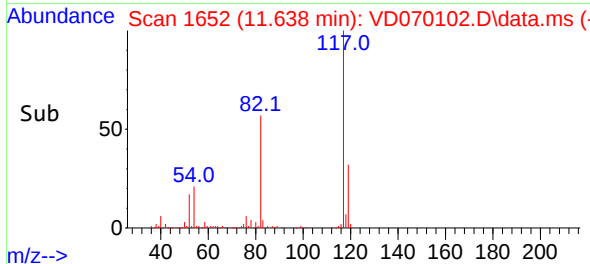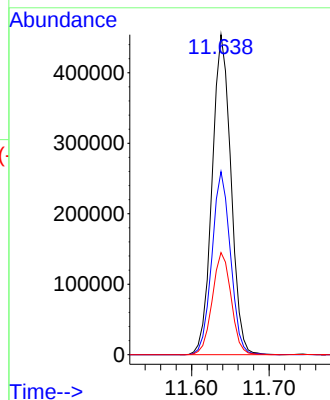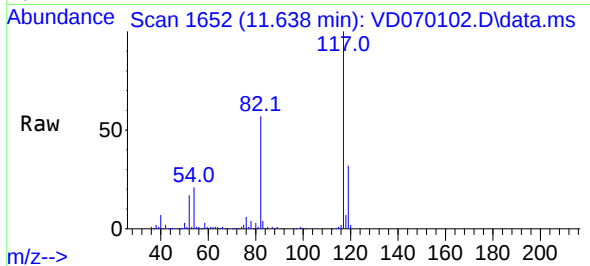

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. -0.006 min
Lab File: VD070102.D
Acq: 17 Aug 2021 23:46

Tgt Ion:152 Resp: 319588

Ion	Ratio	Lower	Upper
152	100		
115	62.4	31.2	93.6
150	159.9	0.0	352.0

