
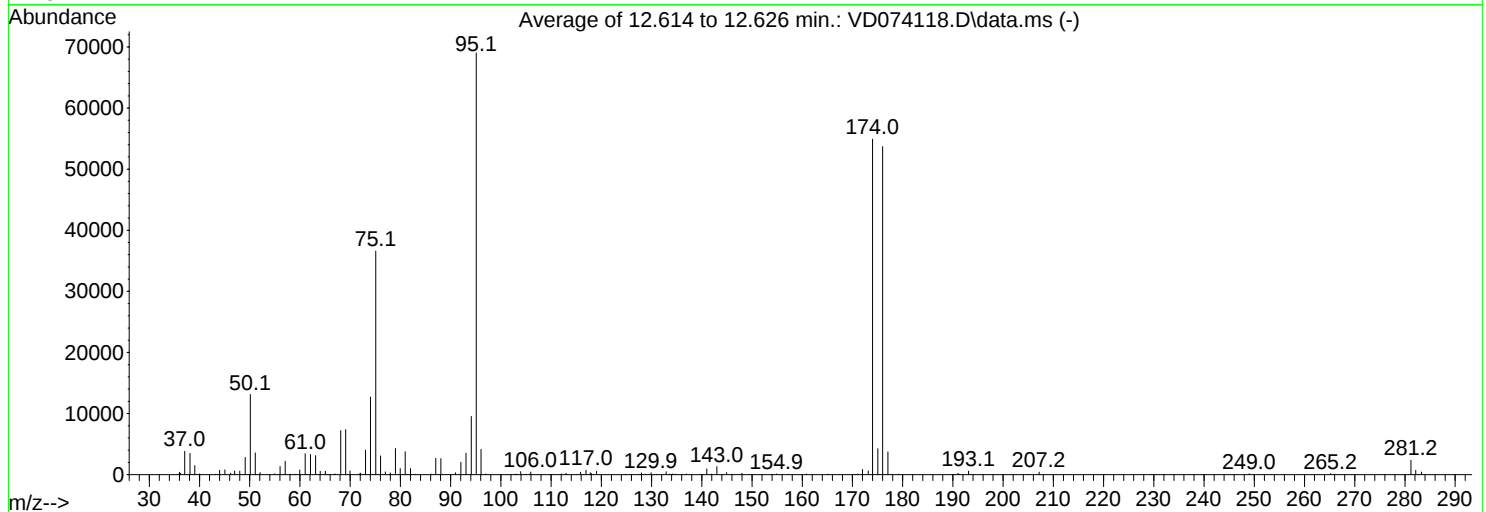


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD081722\
Data File : VD074118.D
Acq On : 17 Aug 2022 09:48
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D081522S.M
Title : SW846 8260
Last Update : Tue Aug 16 01:41:25 2022

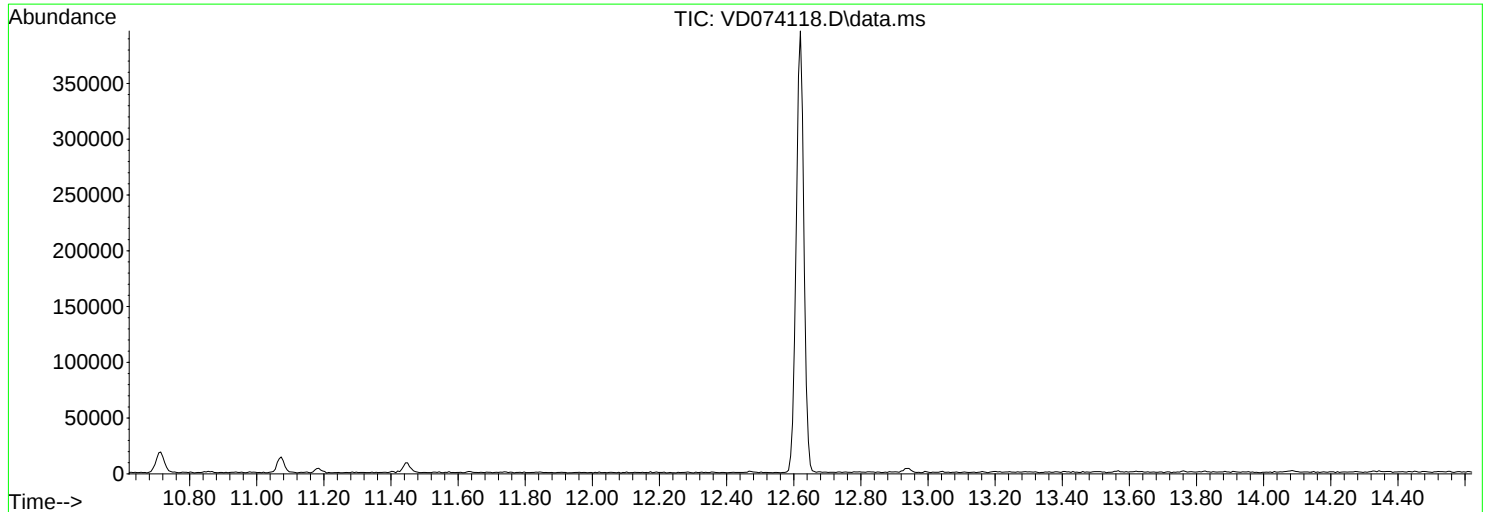

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1809

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	13122	PASS
75	95	30	60	53.0	36576	PASS
95	95	100	100	100.0	69037	PASS
96	95	5	9	6.0	4131	PASS
173	174	0.00	2	1.1	602	PASS
174	95	50	100	79.6	54931	PASS
175	174	5	9	7.7	4249	PASS
176	174	95	101	97.7	53683	PASS
177	176	5	9	6.9	3710	PASS