
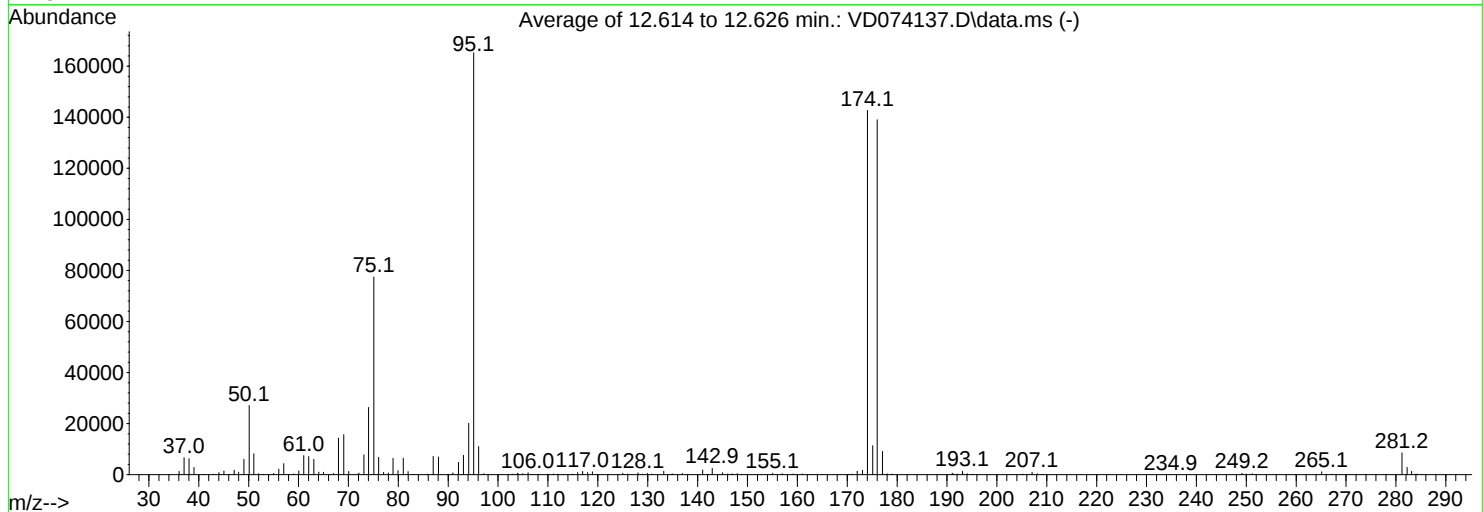


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD081822\
 Data File : VD074137.D
 Acq On : 18 Aug 2022 14:04
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D081822S.M
 Title : SW846 8260
 Last Update : Mon Aug 22 18:40:04 2022

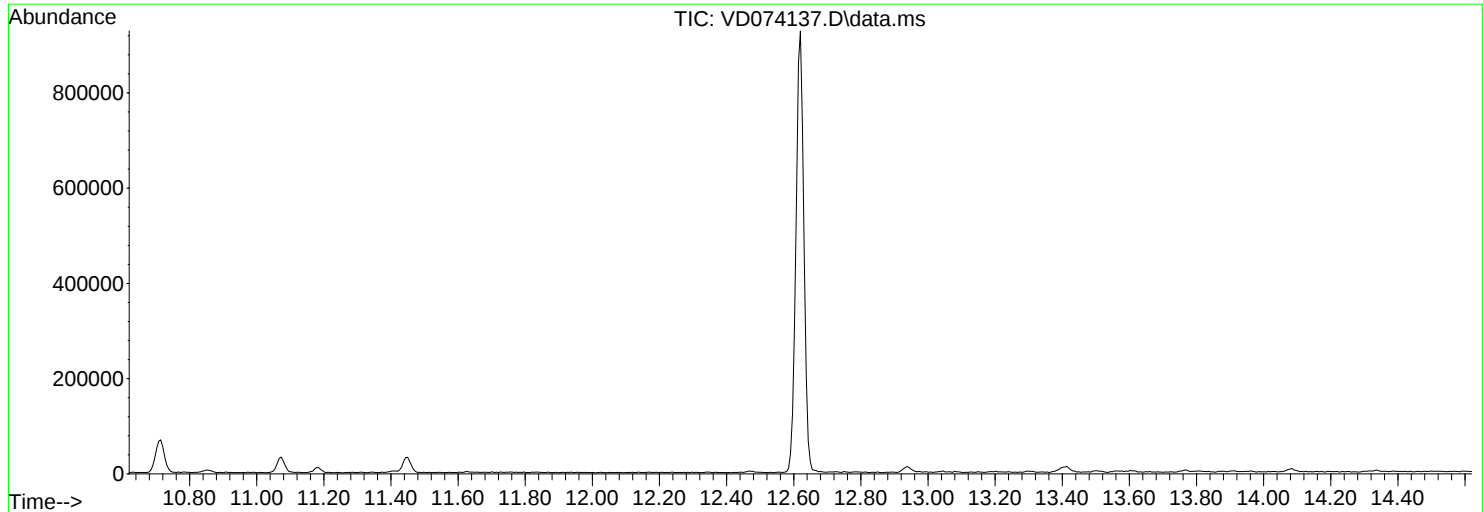

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1809

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	27104	PASS
75	95	30	60	46.8	77397	PASS
95	95	100	100	100.0	165227	PASS
96	95	5	9	6.7	11068	PASS
173	174	0.00	2	1.2	1676	PASS
174	95	50	100	86.4	142675	PASS
175	174	5	9	7.9	11327	PASS
176	174	95	101	97.4	139013	PASS
177	176	5	9	6.5	9087	PASS