

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD081921\
 Data File : VD070175.D
 Acq On : 19 Aug 2021 18:41
 Operator : VA/SY
 Sample : M3418-11
 Misc : 8.81G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SWCS-11-0002

Quant Time: Aug 20 05:48:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D081321S.M
 Quant Title : SW846 8260
 QLast Update : Sat Aug 14 02:33:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	499916	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	970334	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	943557	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.567	152	372000	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	333562	56.730	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	113.460%
35) Dibromofluoromethane	7.908	113	324686	51.792	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	103.580%
50) Toluene-d8	10.338	98	1258550	51.616	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	103.240%
62) 4-Bromofluorobenzene	12.626	95	382484	47.625	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	95.260%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD081921\
Data File : VD070175.D
Acq On : 19 Aug 2021 18:41
Operator : VA/SY
Sample : M3418-11
Misc : 8.81G/5.00ml/MSVOA_D/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SWCS-11-0002

Quant Time: Aug 20 05:48:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D081321S.M
Quant Title : SW846 8260
QLast Update : Sat Aug 14 02:33:51 2021
Response via : Initial Calibration




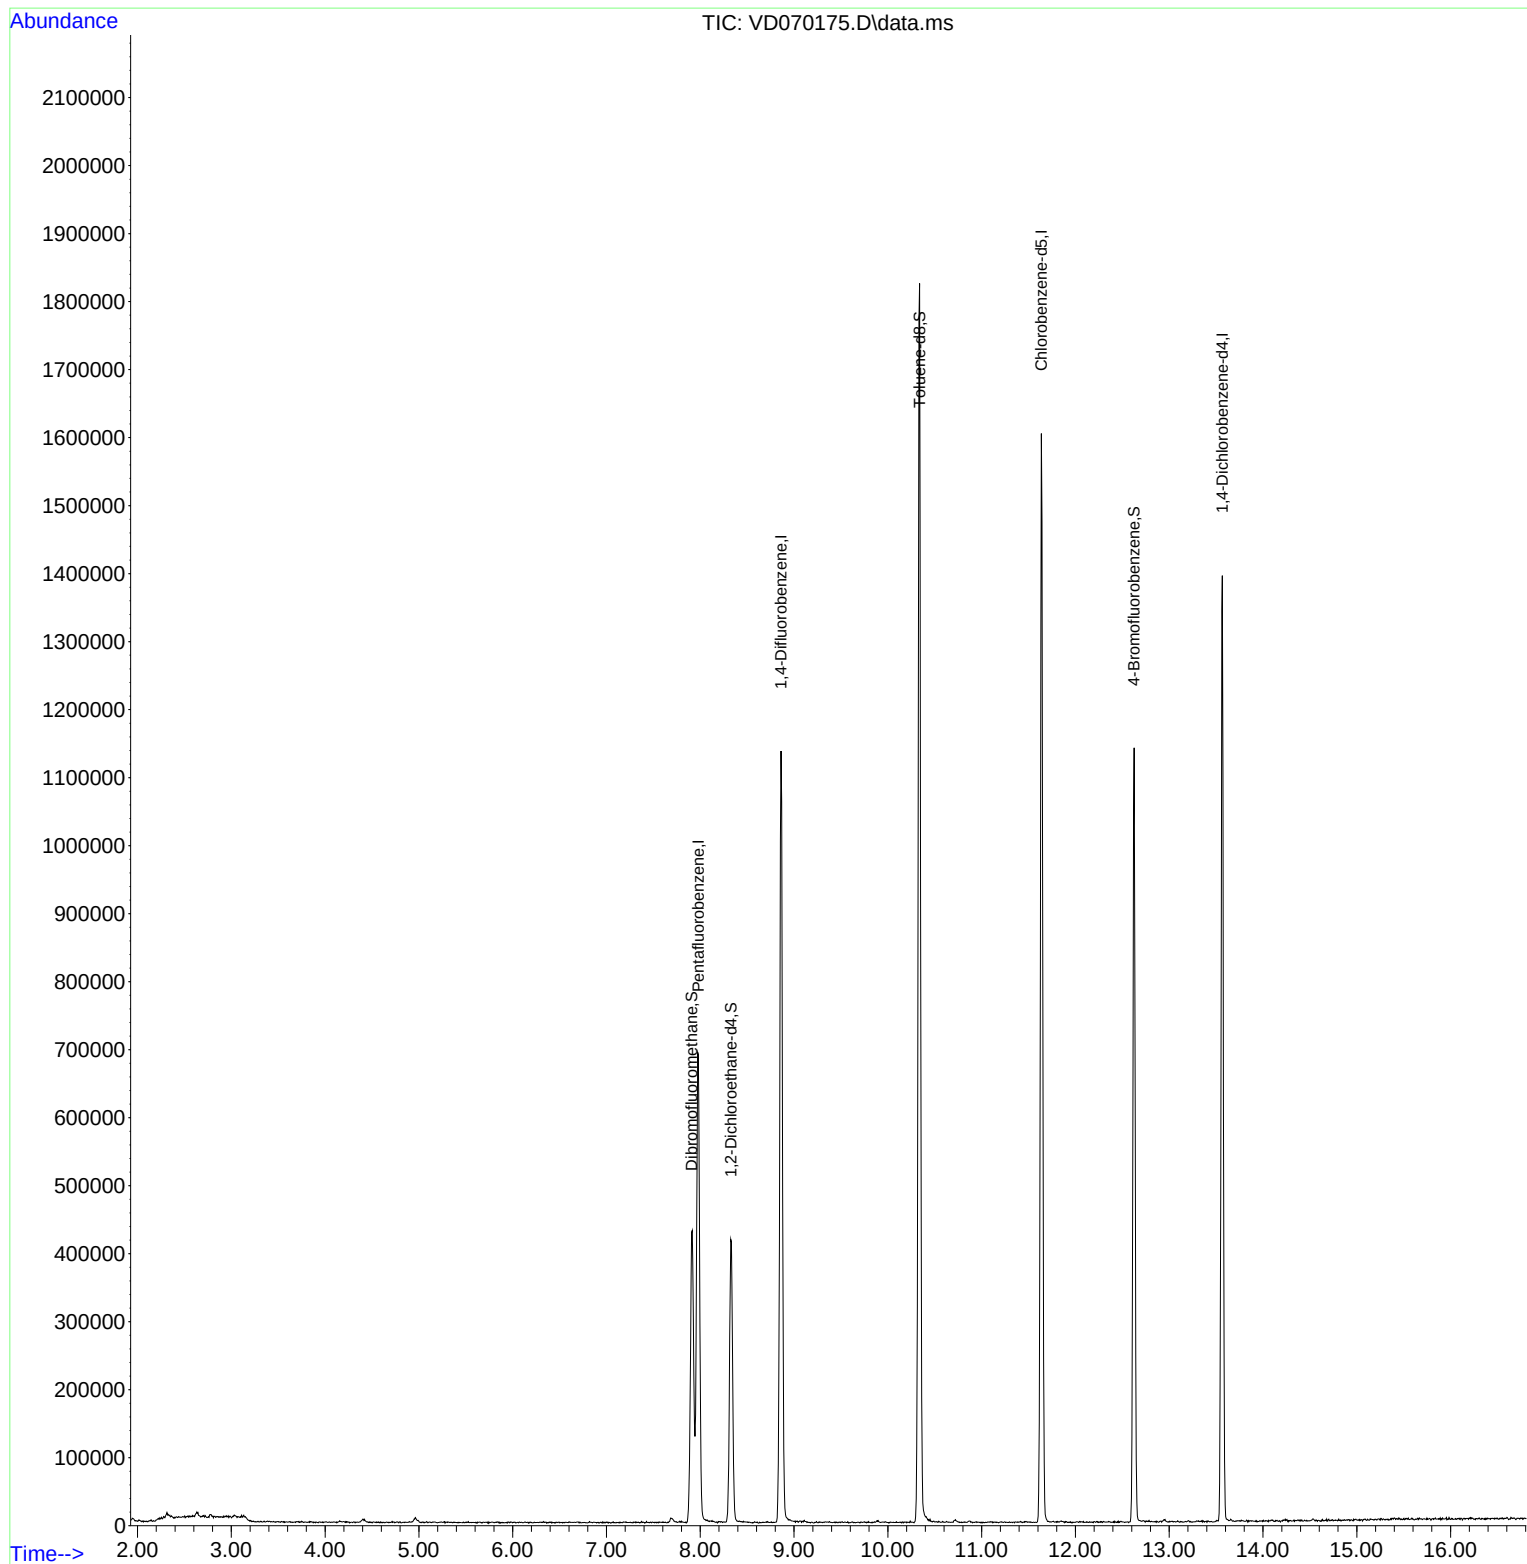


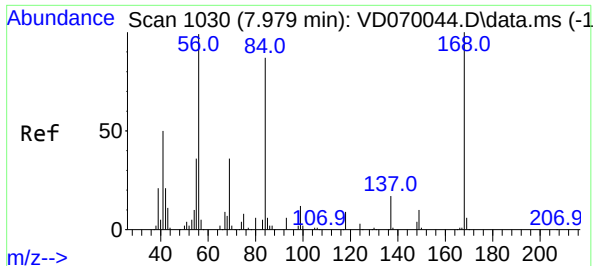

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.000 min
Lab File: VD070175.D
Acq: 19 Aug 2021 18:41




Instrument :
MSVOA_D
ClientSampleId :
SWCS-11-0002


Tgt Ion:168 Resp: 499916
Ion Ratio Lower Upper
168 100
99 60.4 50.3 75.5

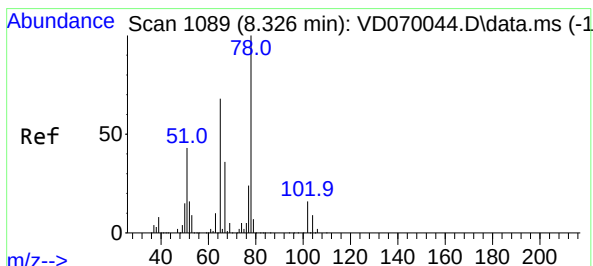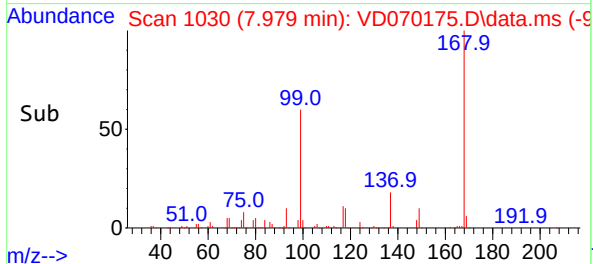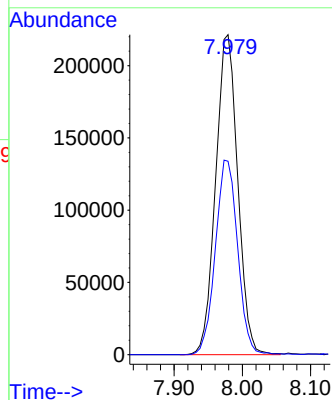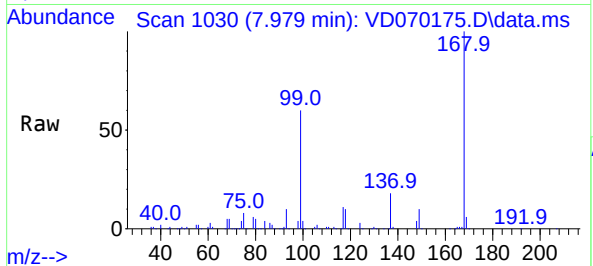

#33
1,2-Dichloroethane-d4
Concen: 56.730 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. -0.000 min
Lab File: VD070175.D
Acq: 19 Aug 2021 18:41

Tgt Ion: 65 Resp: 333562
Ion Ratio Lower Upper
65 100
67 54.8 0.0 107.8


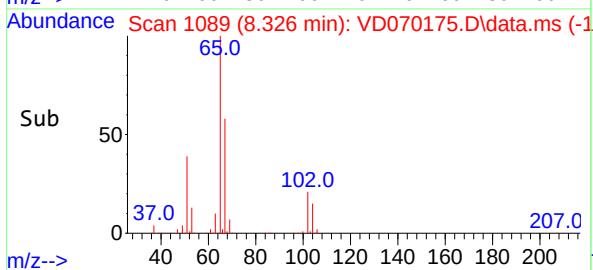
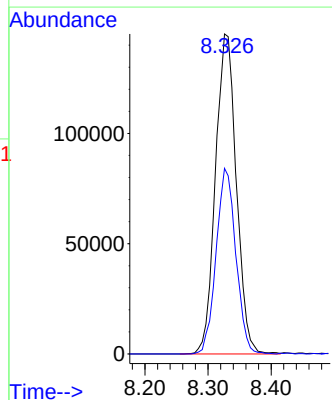
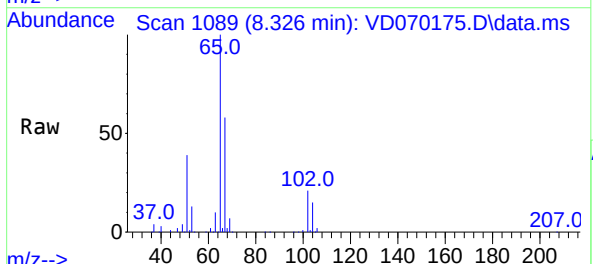


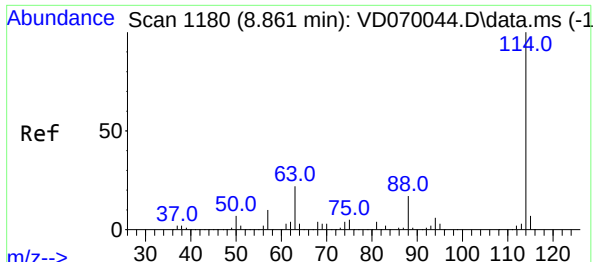

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. -0.000 min
Lab File: VD070175.D
Acq: 19 Aug 2021 18:41




Instrument :
MSVOA_D
ClientSampleId :
SWCS-11-0002


Tgt Ion:114 Resp: 970334
Ion Ratio Lower Upper
114 100
63 20.9 0.0 43.6
88 15.7 0.0 33.4

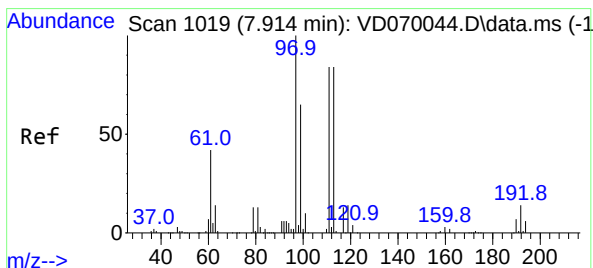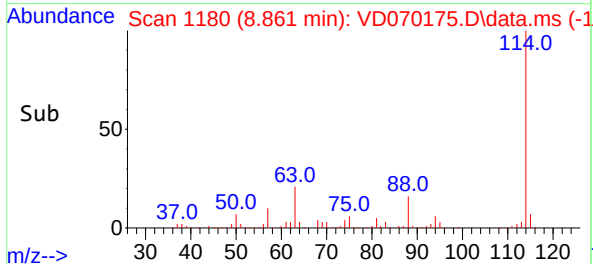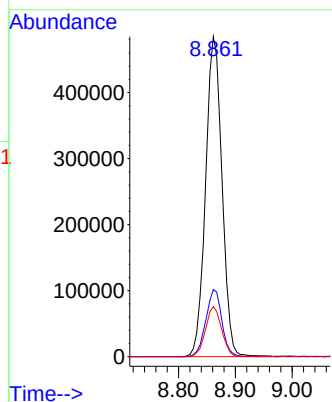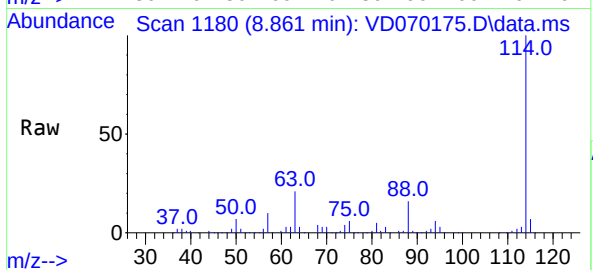

#35
Dibromofluoromethane
Concen: 51.792 ug/l
RT: 7.908 min Scan# 1018
Delta R.T. -0.006 min
Lab File: VD070175.D
Acq: 19 Aug 2021 18:41

Tgt Ion:113 Resp: 324686
Ion Ratio Lower Upper
113 100
111 103.1 81.8 122.6
192 16.4 13.2 19.8


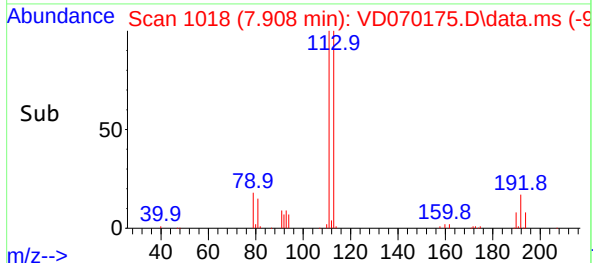
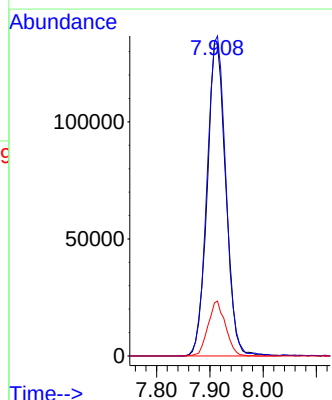
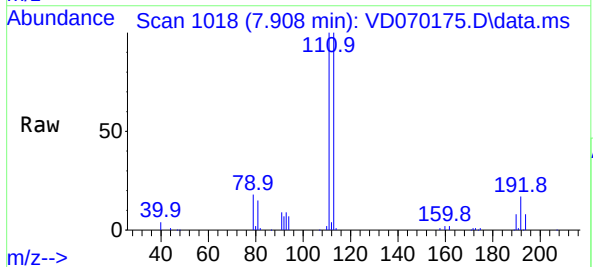


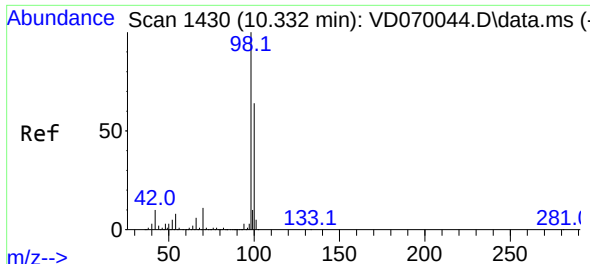

#50
Toluene-d8
Concen: 51.616 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. 0.006 min
Lab File: VD070175.D
Acq: 19 Aug 2021 18:41




Instrument :
MSVOA_D
ClientSampleId :
SWCS-11-0002


Tgt Ion: 98 Resp: 1258550
Ion Ratio Lower Upper
98 100
100 64.1 52.6 78.8

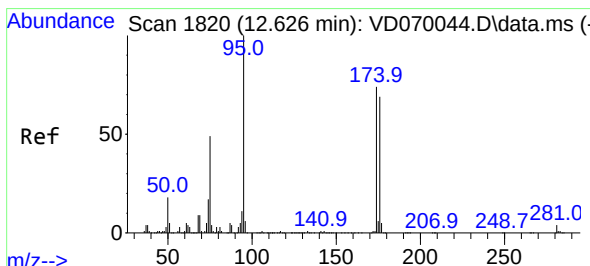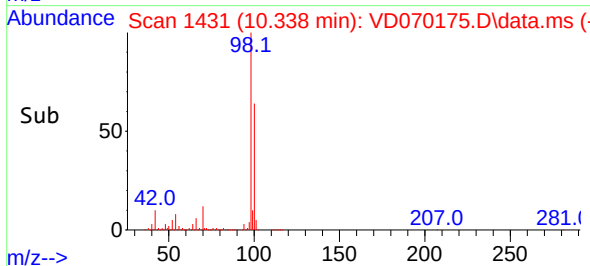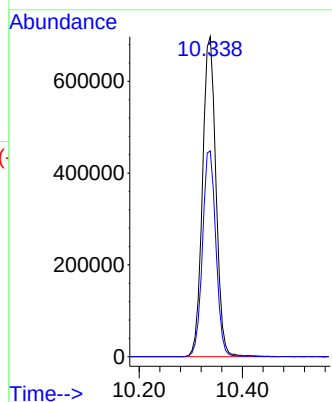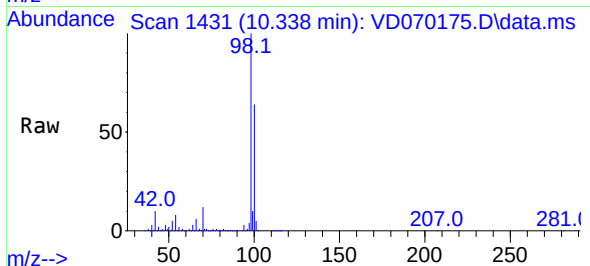

#62
4-Bromofluorobenzene
Concen: 47.625 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. -0.000 min
Lab File: VD070175.D
Acq: 19 Aug 2021 18:41

Tgt Ion: 95 Resp: 382484
Ion Ratio Lower Upper
95 100
174 75.1 0.0 141.6
176 72.4 0.0 138.2


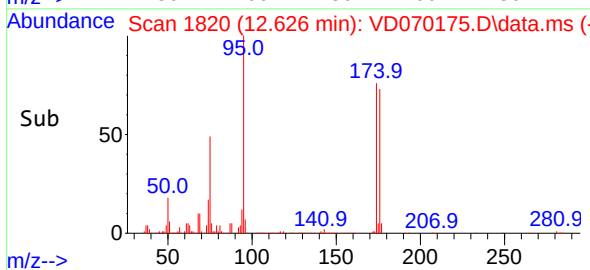
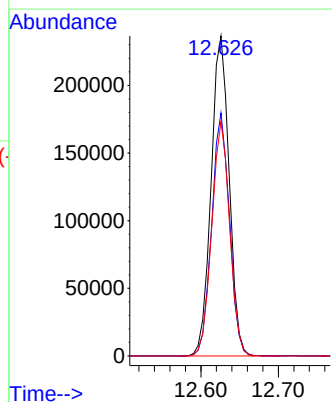
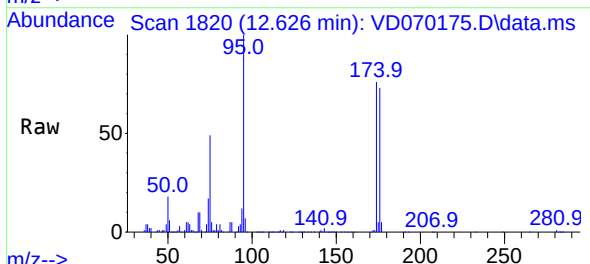


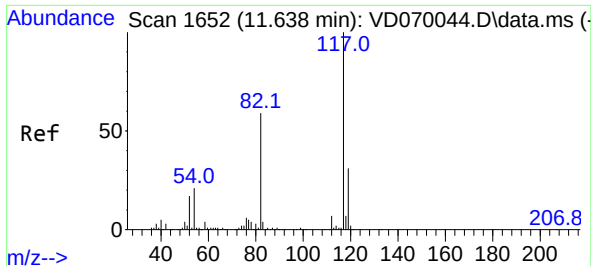

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1652
Delta R.T. -0.000 min
Lab File: VD070175.D
Acq: 19 Aug 2021 18:41

Instrument :
MSVOA_D
ClientSampleId :
SWCS-11-0002

Tgt Ion:	117	Resp:	943557
Ion	Ratio	Lower	Upper
117	100		
82	56.6	47.5	71.3
119	31.2	25.1	37.7

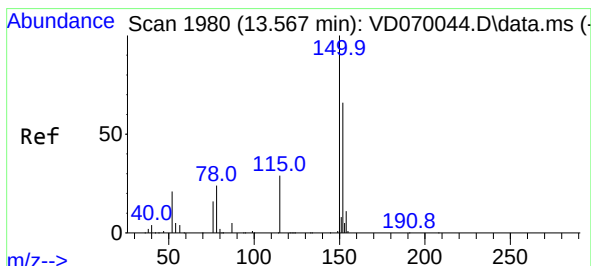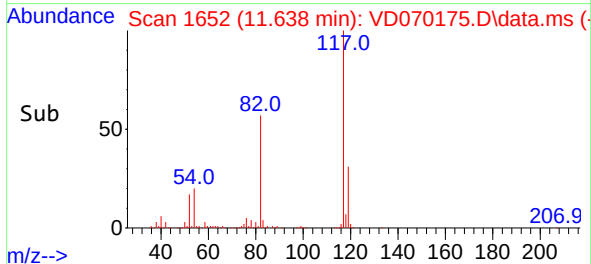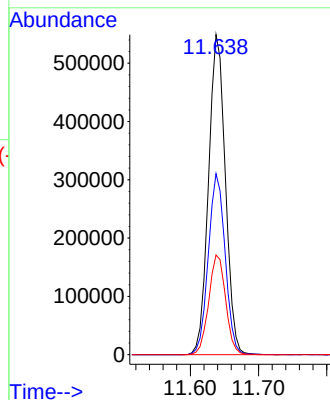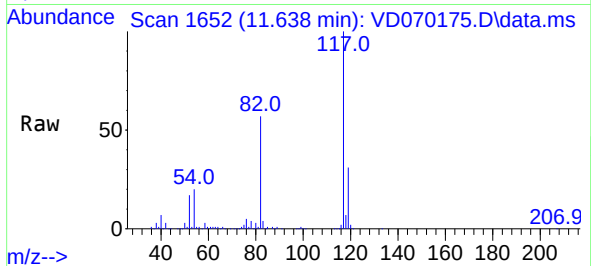

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.567 min Scan# 1980
Delta R.T. -0.000 min
Lab File: VD070175.D
Acq: 19 Aug 2021 18:41

Tgt Ion:	152	Resp:	372000
Ion	Ratio	Lower	Upper
152	100		
115	61.5	31.2	93.6
150	157.7	0.0	352.0

