




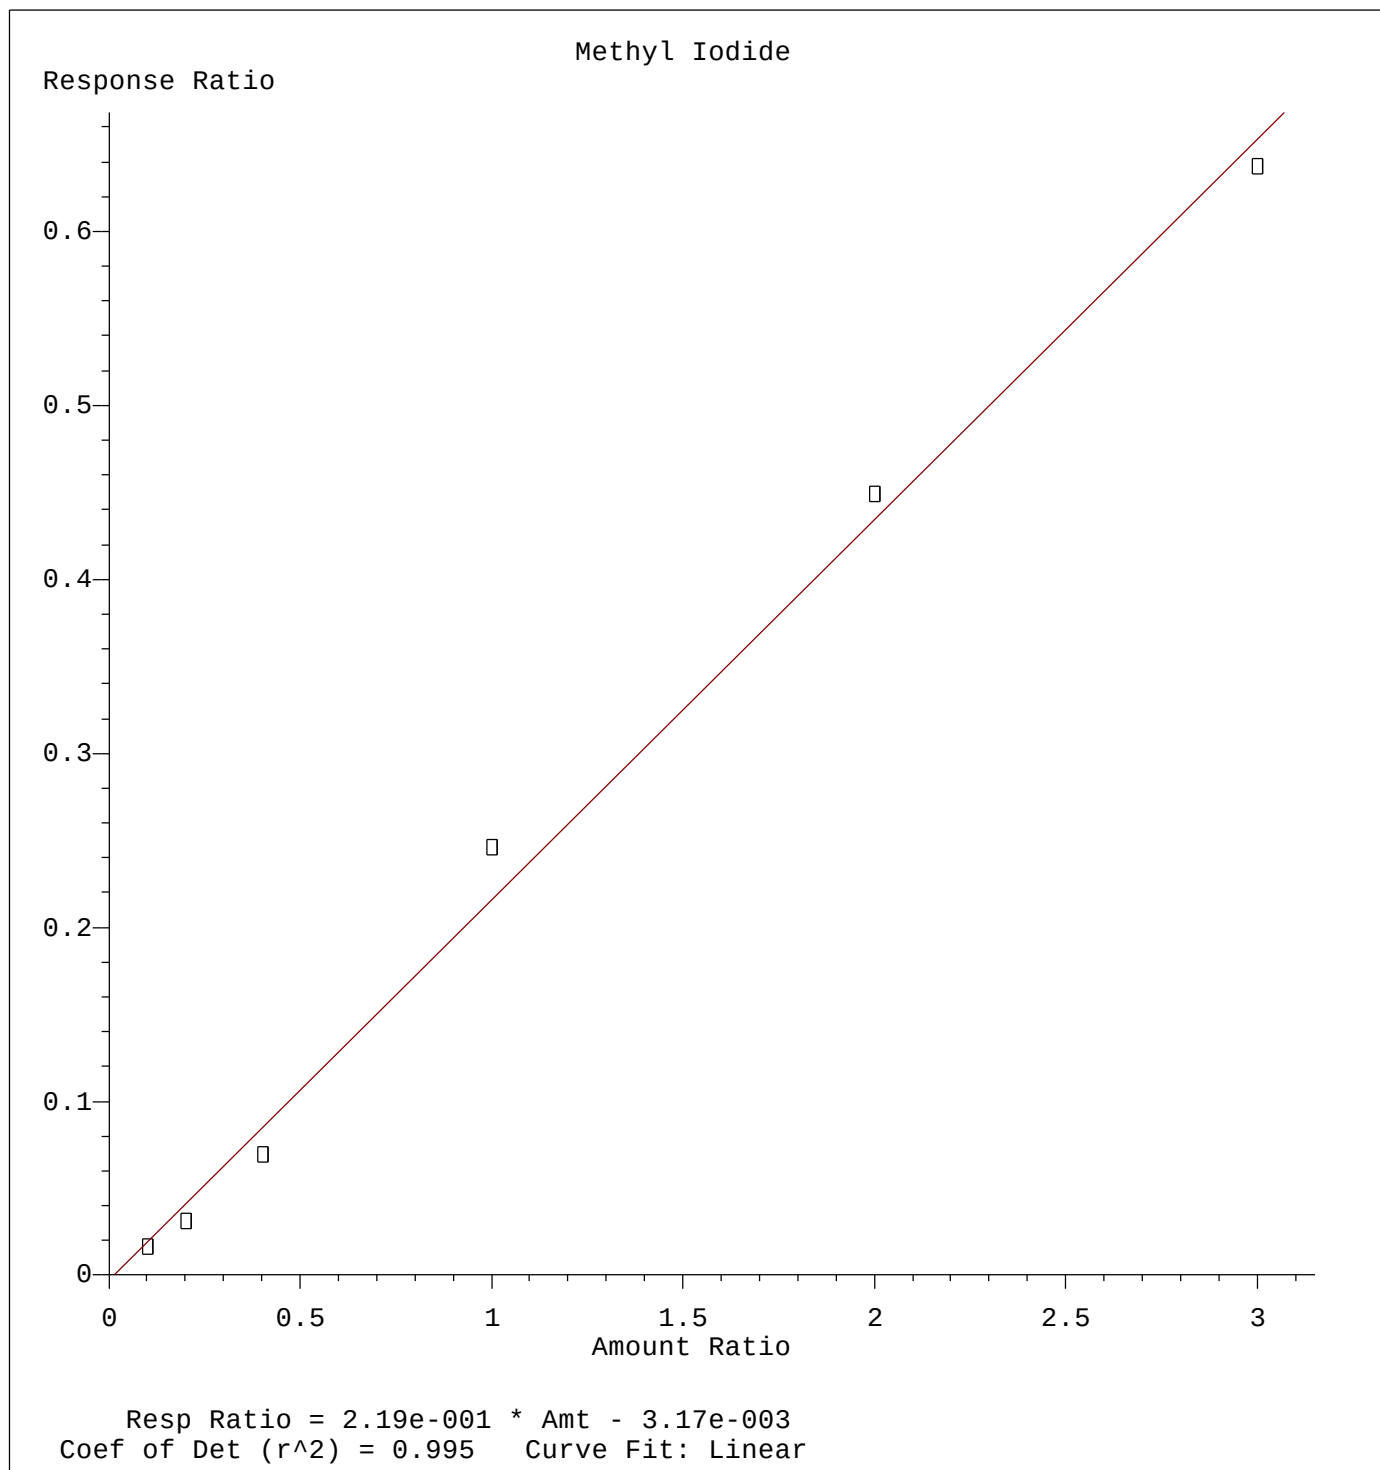


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082018S.M
Calibration Table Last Updated: Tue Aug 21 11:41:02 2018

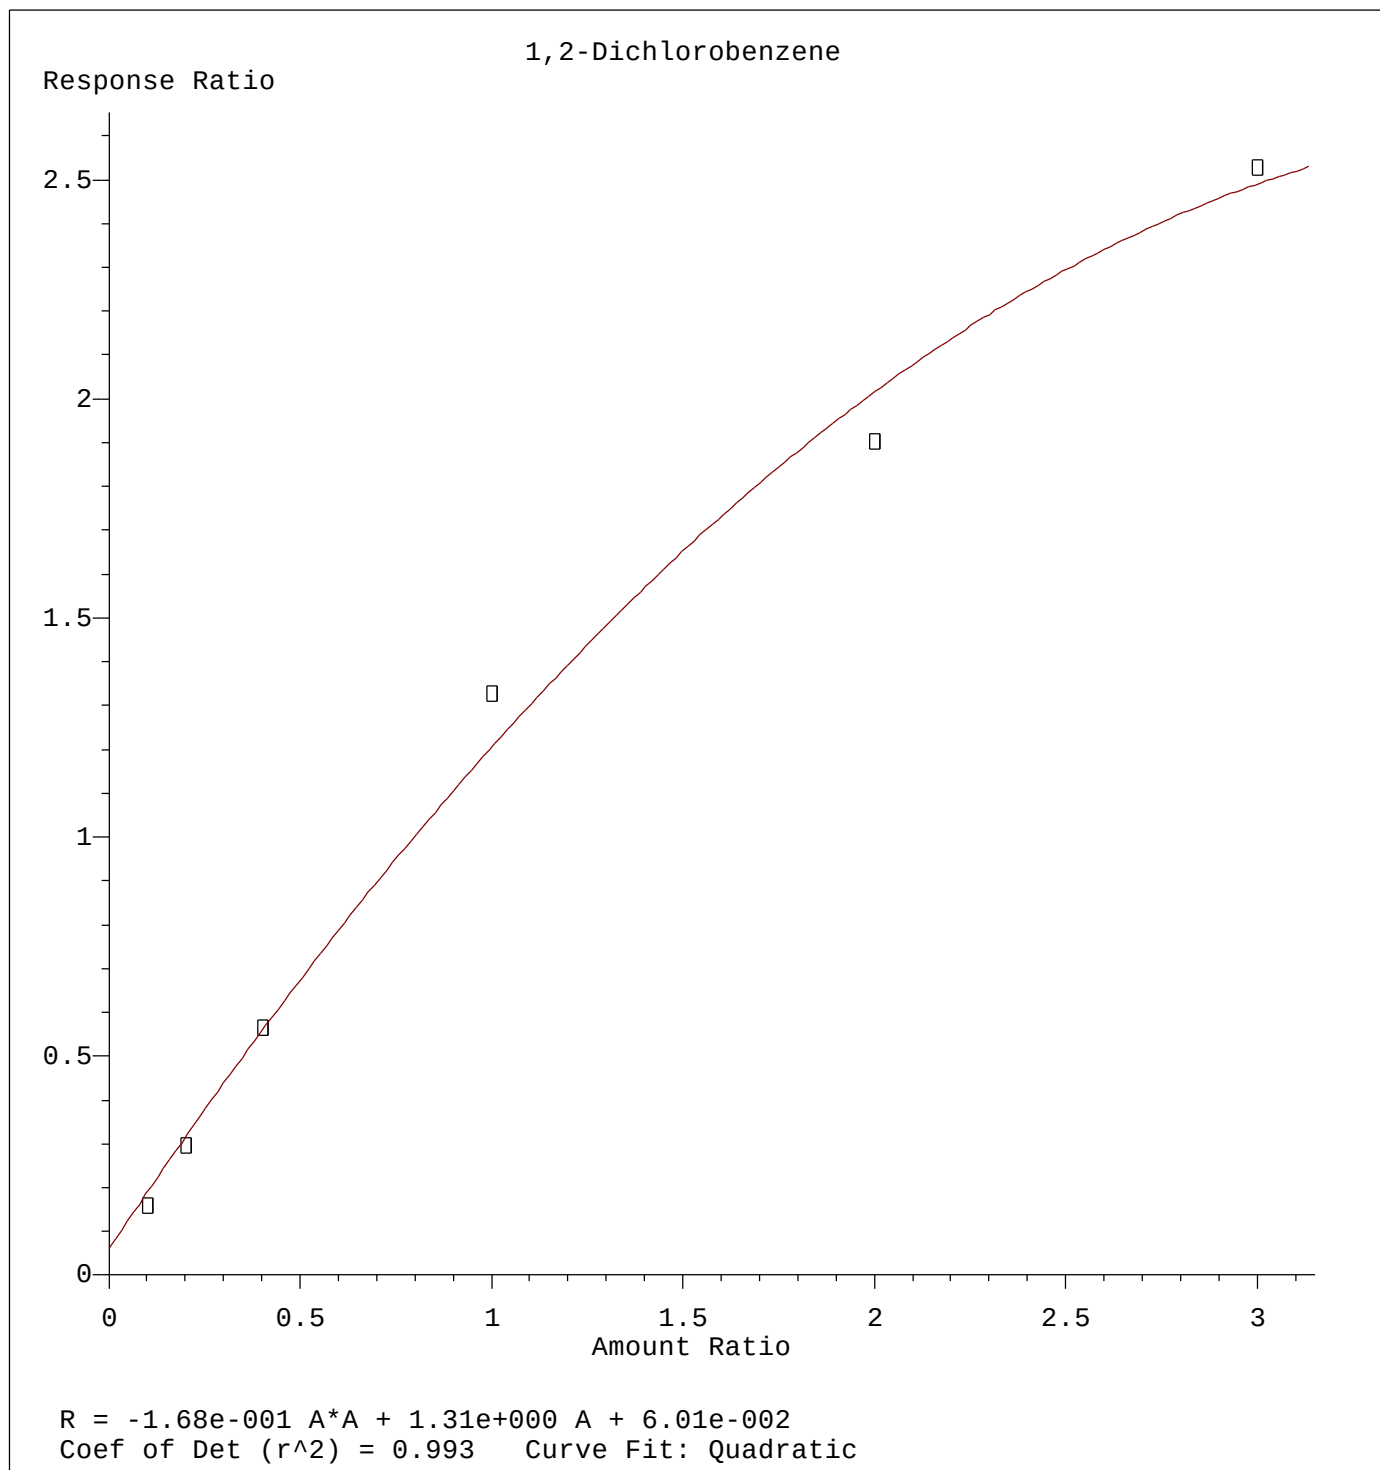

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082018S.M
Calibration Table Last Updated: Tue Aug 21 11:41:02 2018

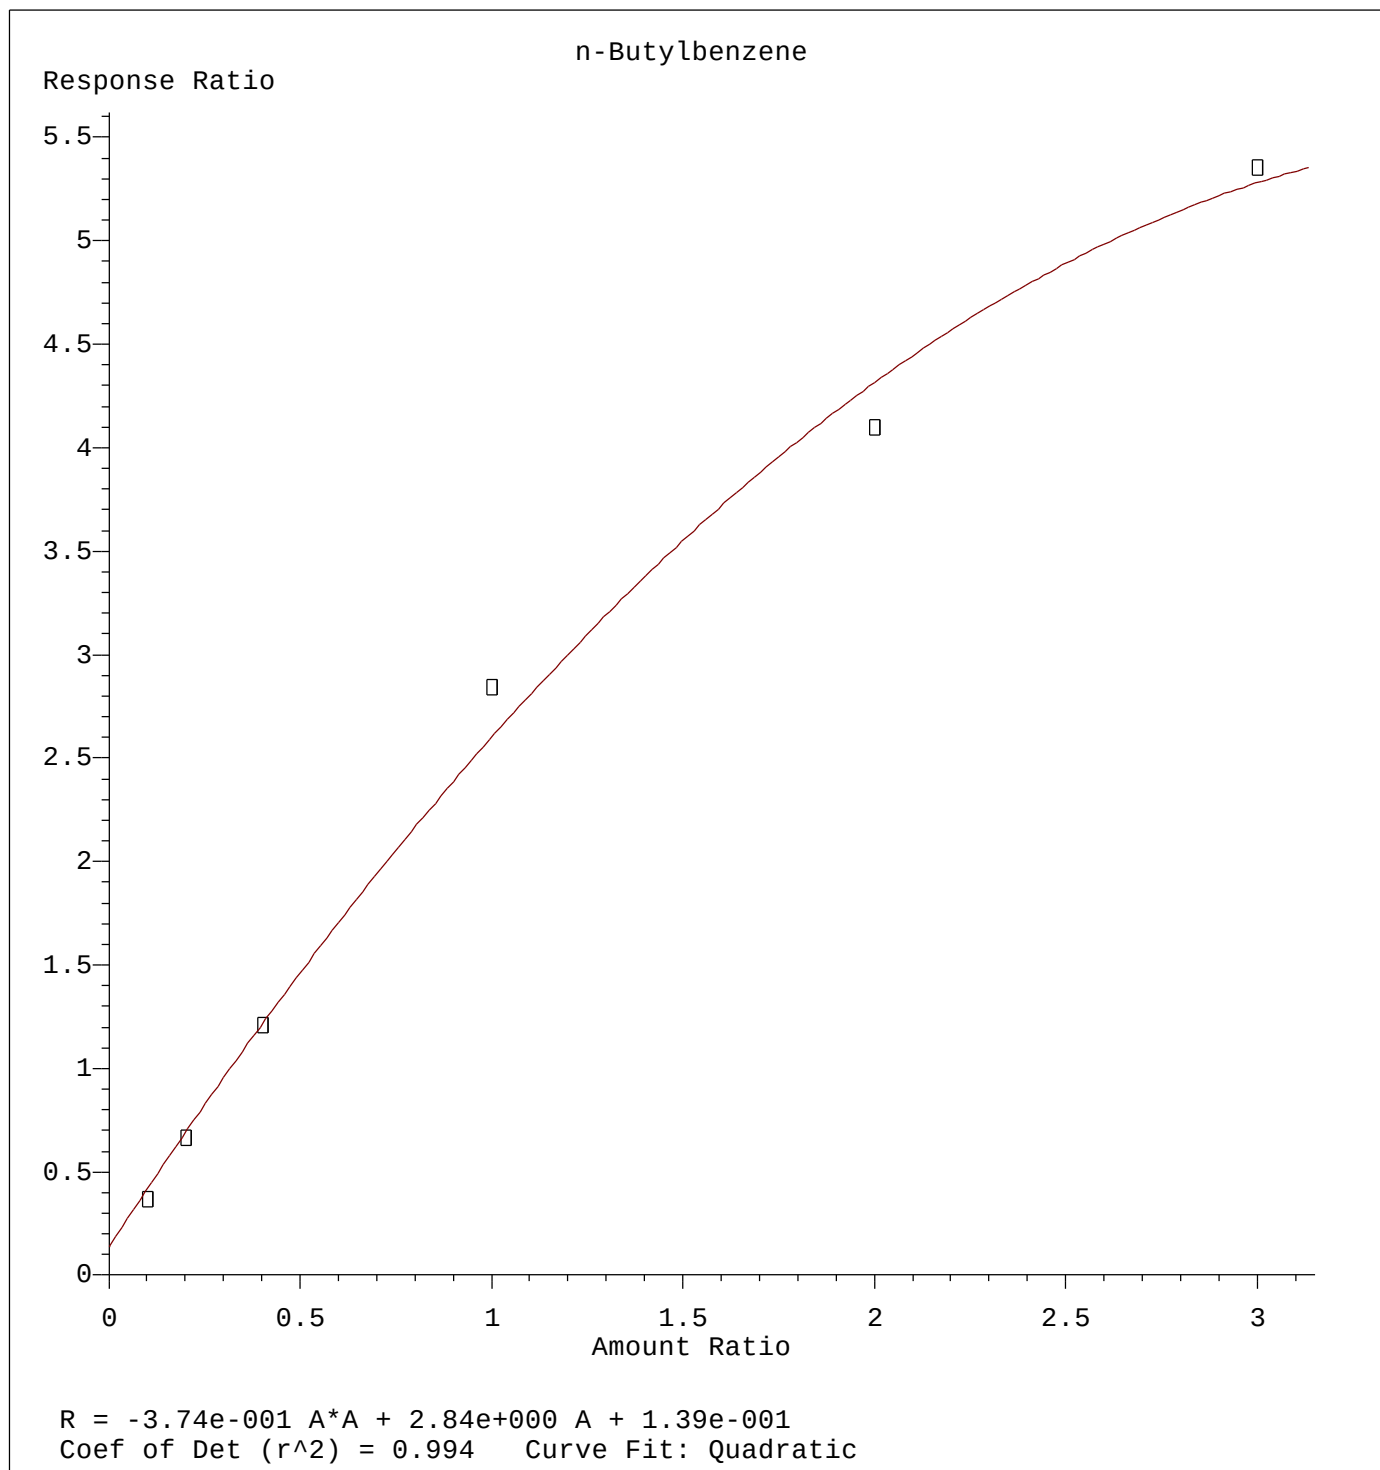


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082018S.M
Calibration Table Last Updated: Tue Aug 21 11:41:02 2018

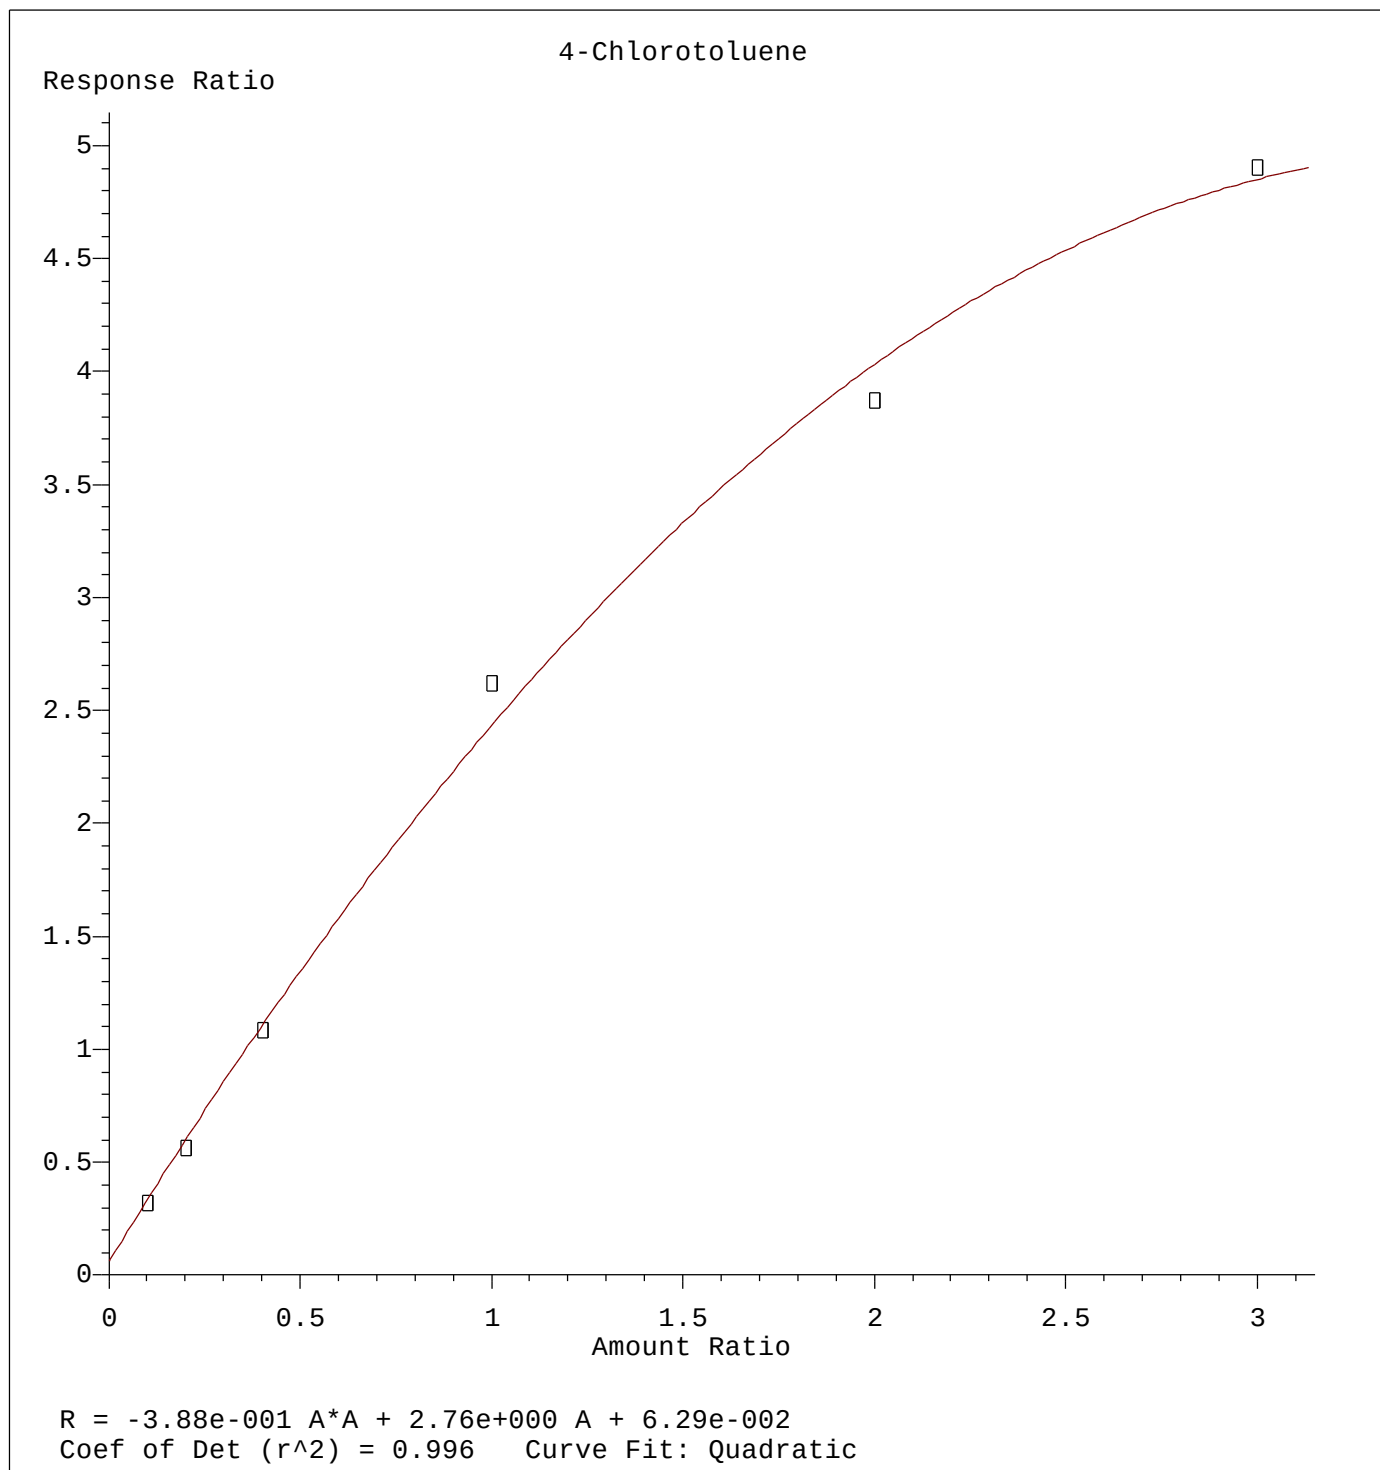

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082018S.M
Calibration Table Last Updated: Tue Aug 21 11:41:02 2018


1,3,5-Trimethylbenzene

Response Ratio

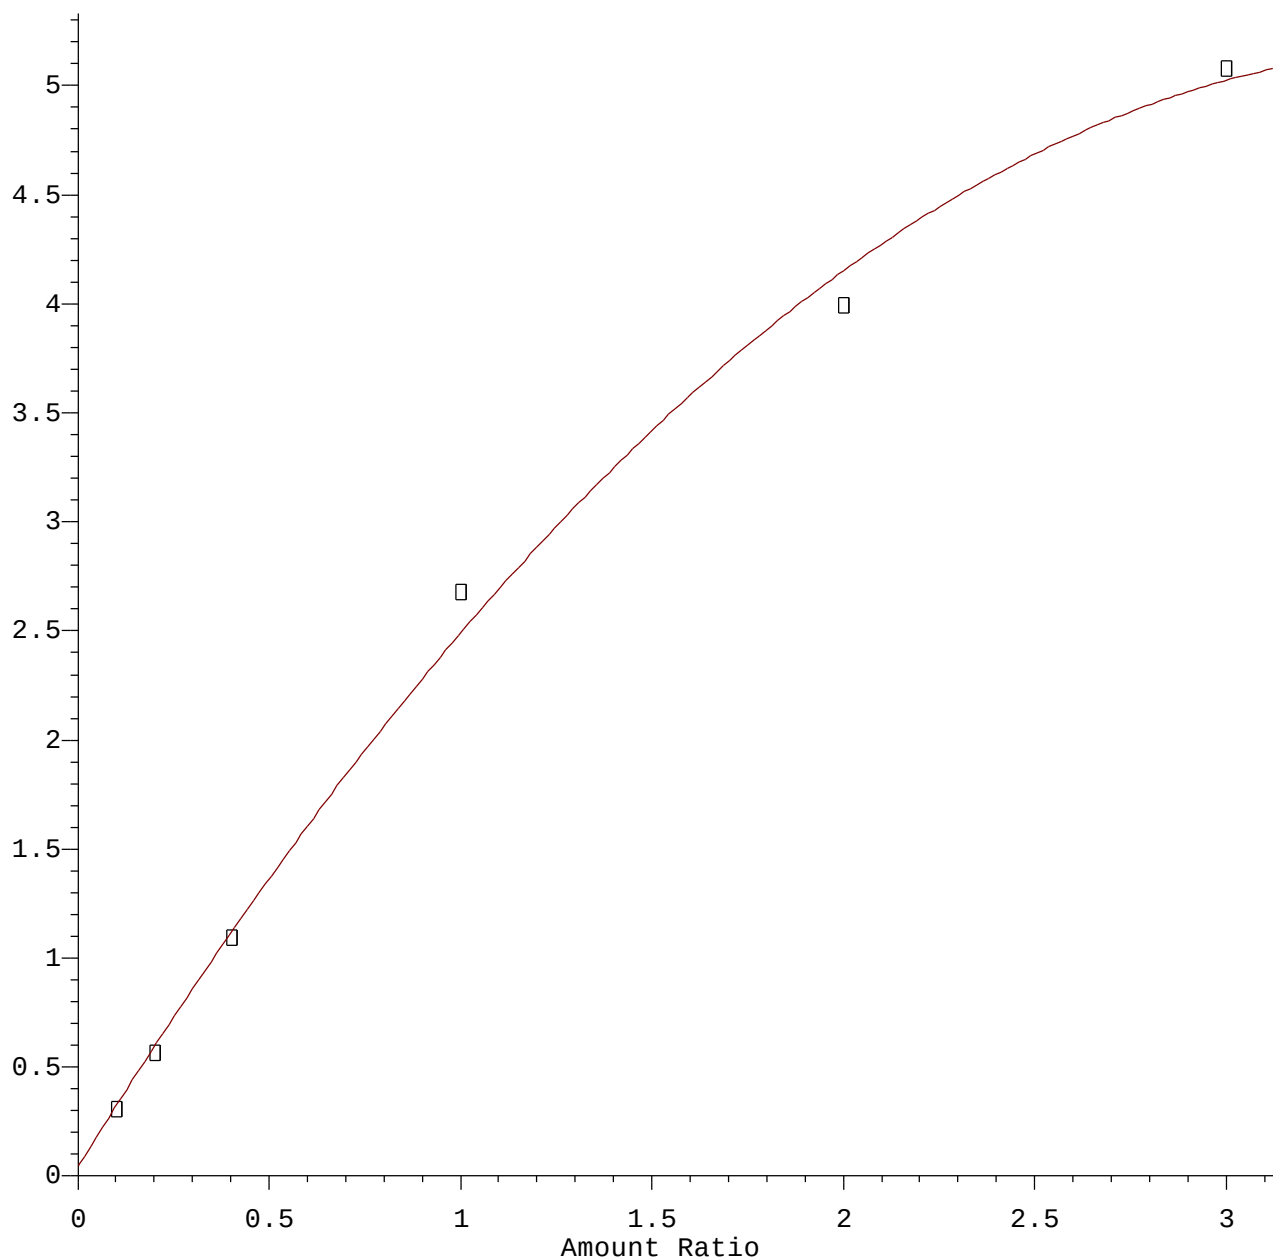


$R = -3.93e-001 A^2 + 2.84e+000 A + 4.48e-002$
Coef of Det (r^2) = 0.997 Curve Fit: Quadratic

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082018S.M
Calibration Table Last Updated: Tue Aug 21 11:41:02 2018

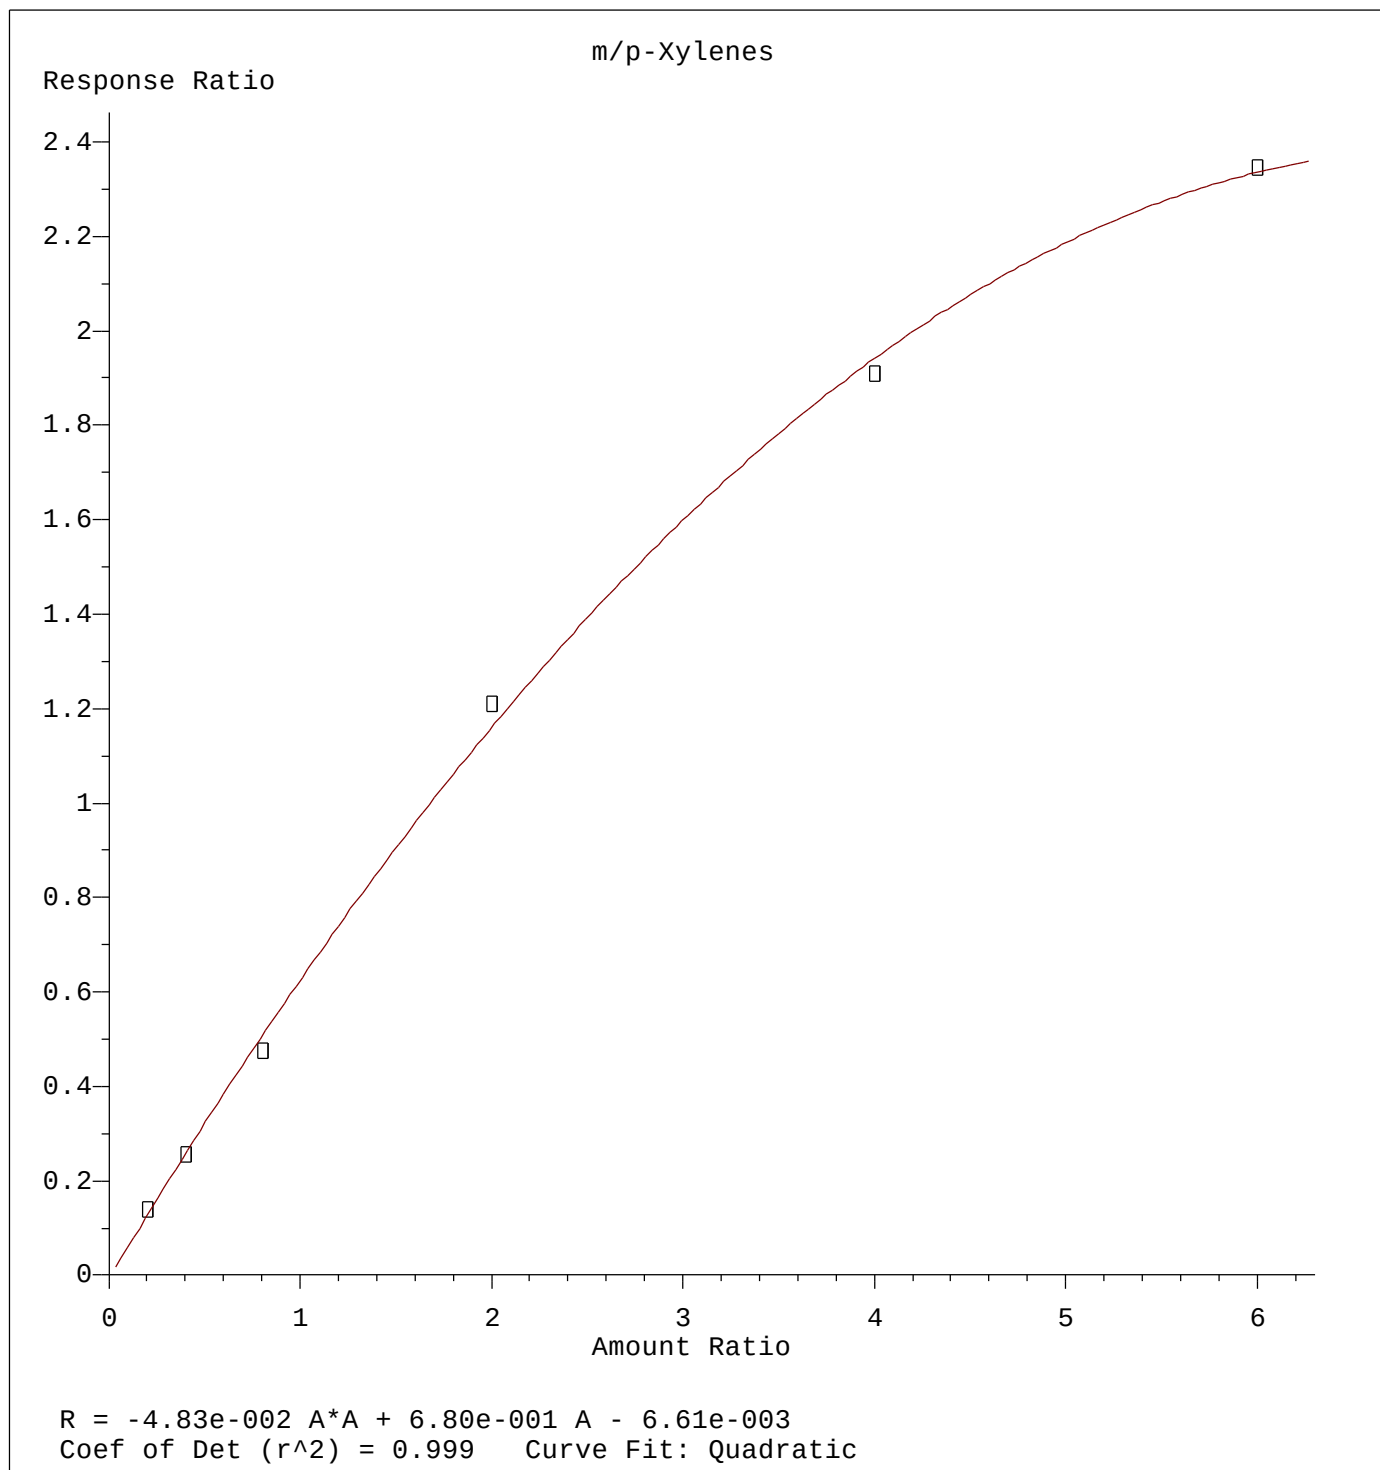


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082018S.M
Calibration Table Last Updated: Tue Aug 21 11:41:02 2018

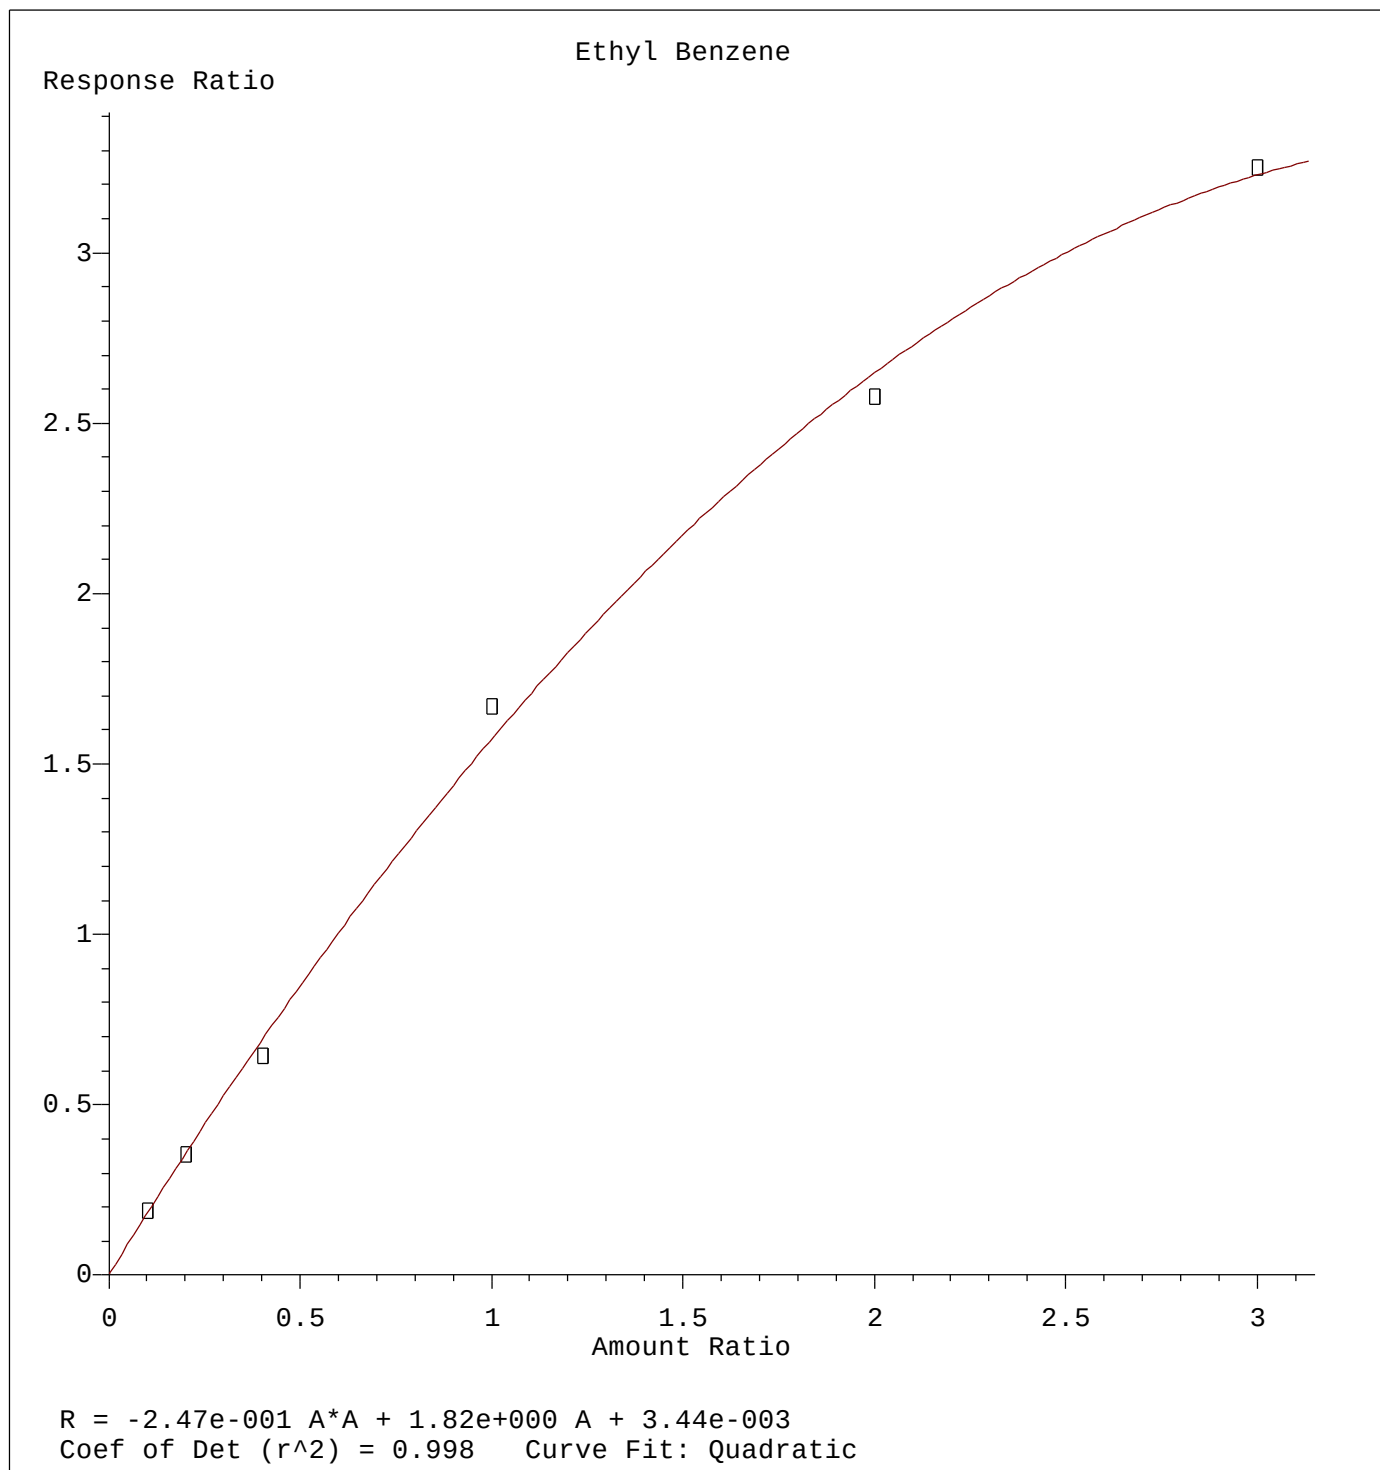

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082018S.M
Calibration Table Last Updated: Tue Aug 21 11:41:02 2018


2-Chloroethyl Vinyl ether

Response Ratio

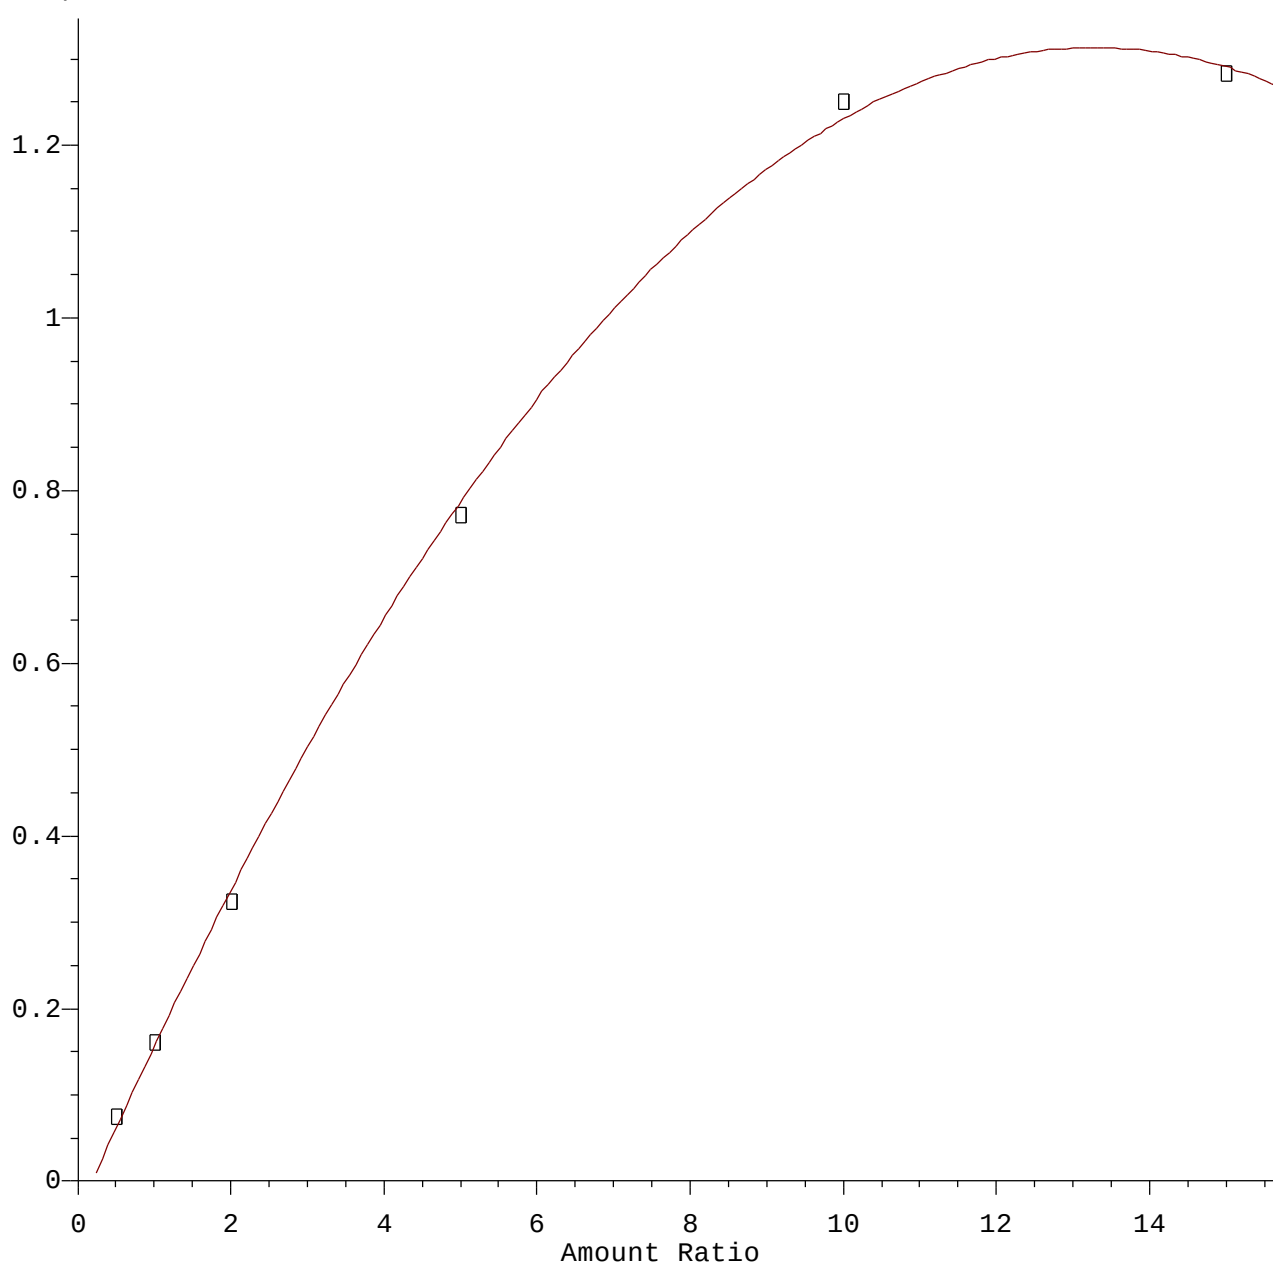

$R = -7.66e-003 A^2 + 2.03e-001 A - 3.84e-002$
Coef of Det (r^2) = 0.999 Curve Fit: Quadratic


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082018S.M
Calibration Table Last Updated: Tue Aug 21 11:41:02 2018

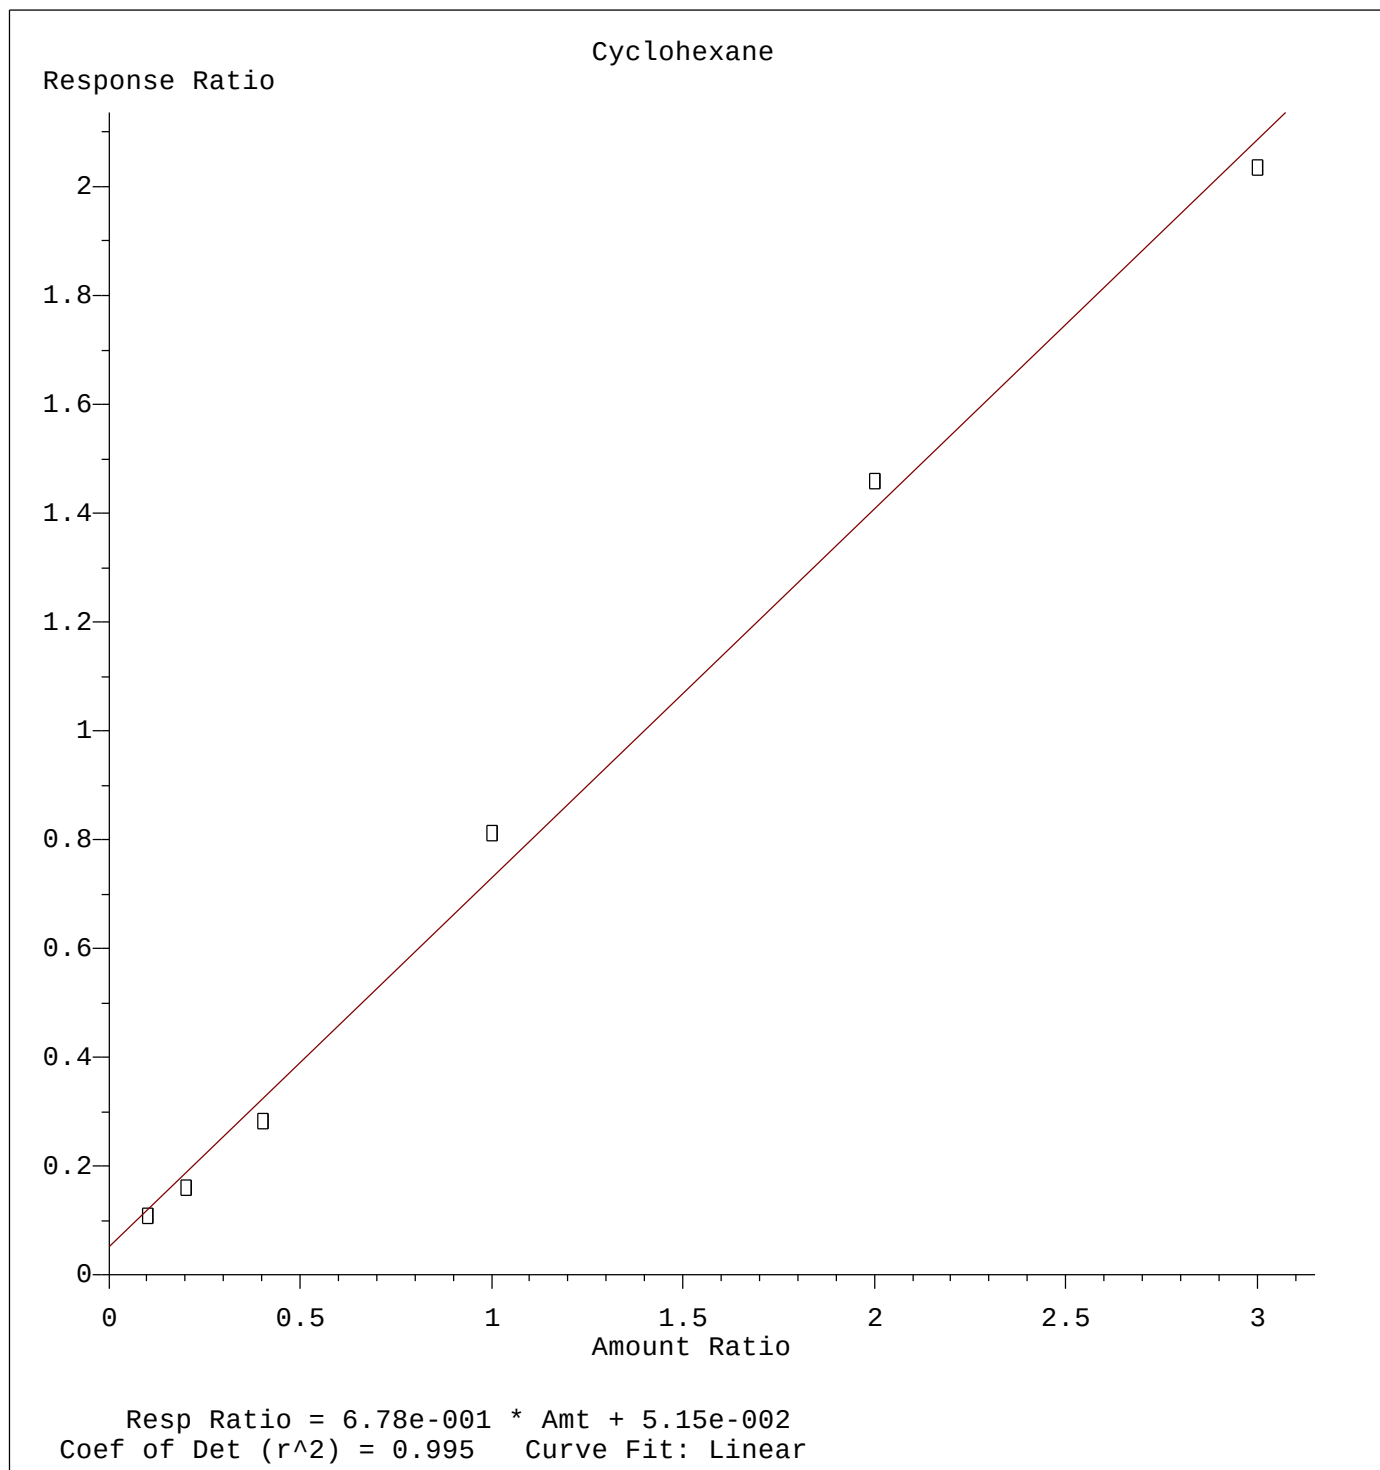

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082018S.M
Calibration Table Last Updated: Tue Aug 21 11:41:02 2018


trans-1,2-Dichloroethene

Response Ratio

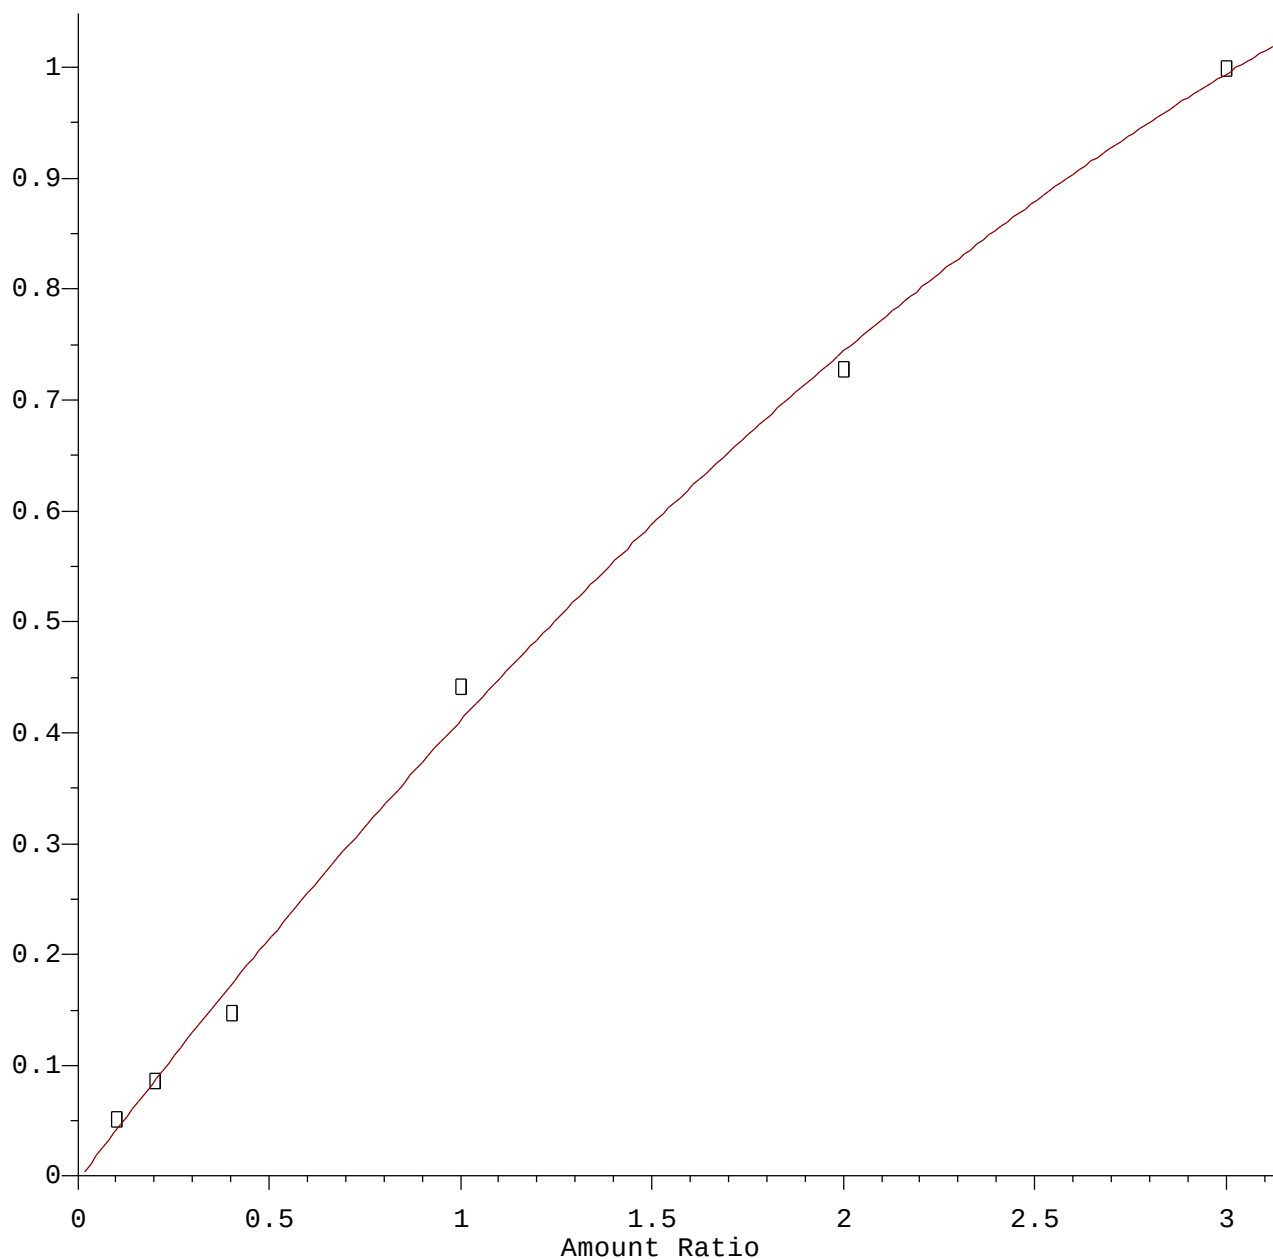


$R = -4.11e-002 A^2 + 4.56e-001 A - 3.30e-003$
Coef of Det (r^2) = 0.997 Curve Fit: Quadratic


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082018S.M
Calibration Table Last Updated: Tue Aug 21 11:41:02 2018

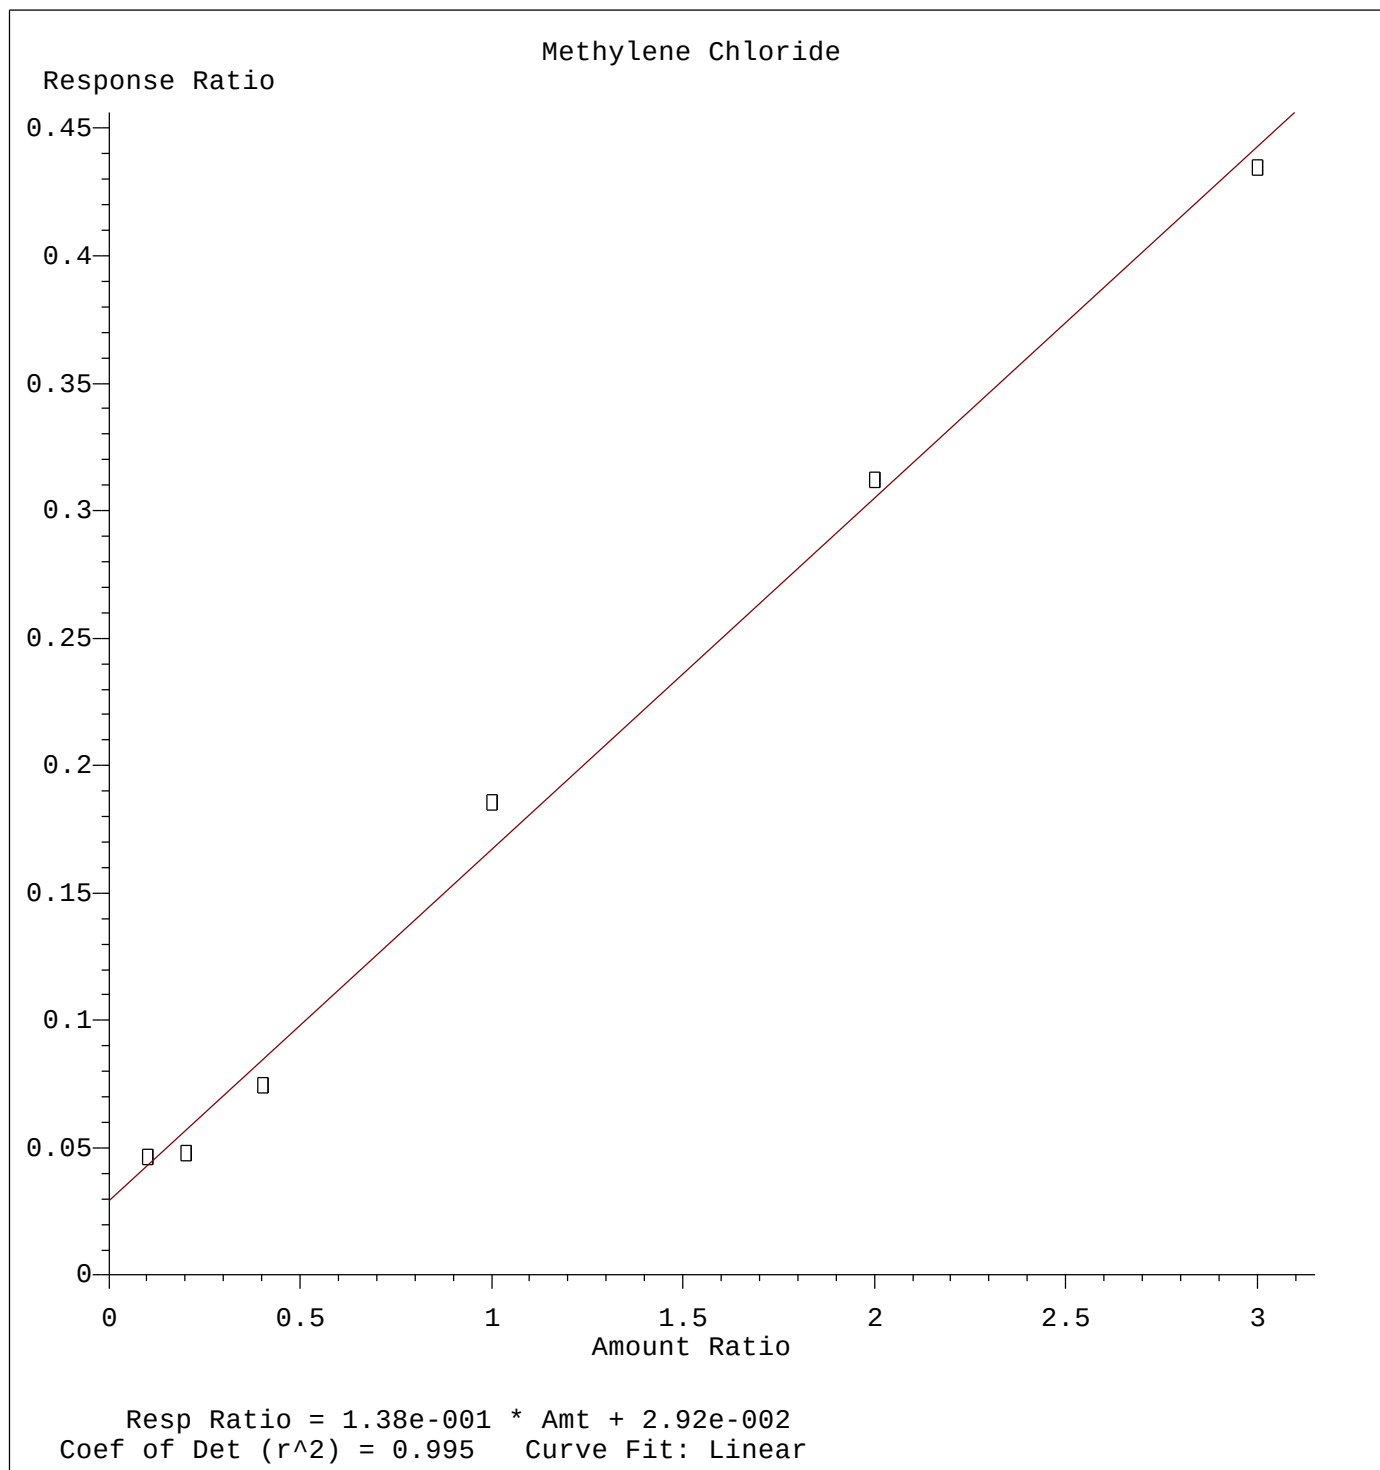


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082018S.M
Calibration Table Last Updated: Tue Aug 21 11:41:02 2018

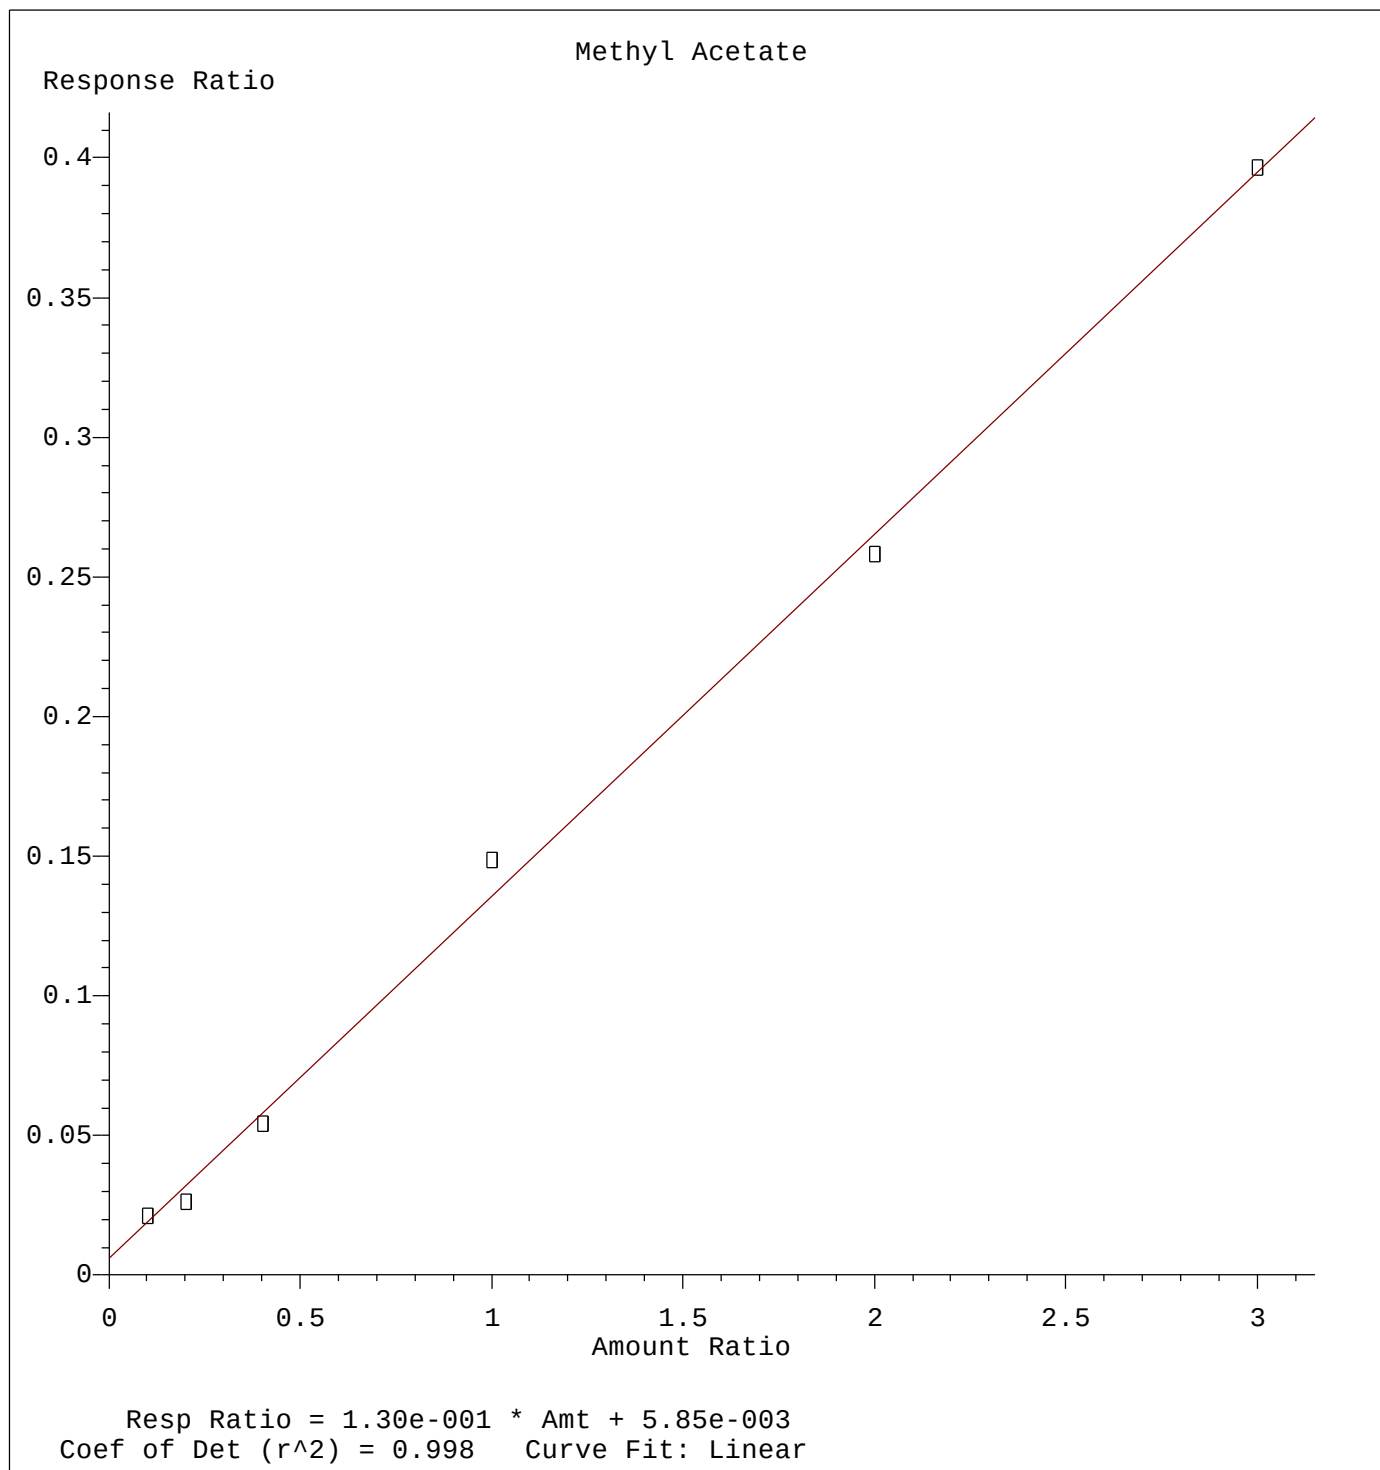


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082018S.M
Calibration Table Last Updated: Tue Aug 21 11:41:02 2018

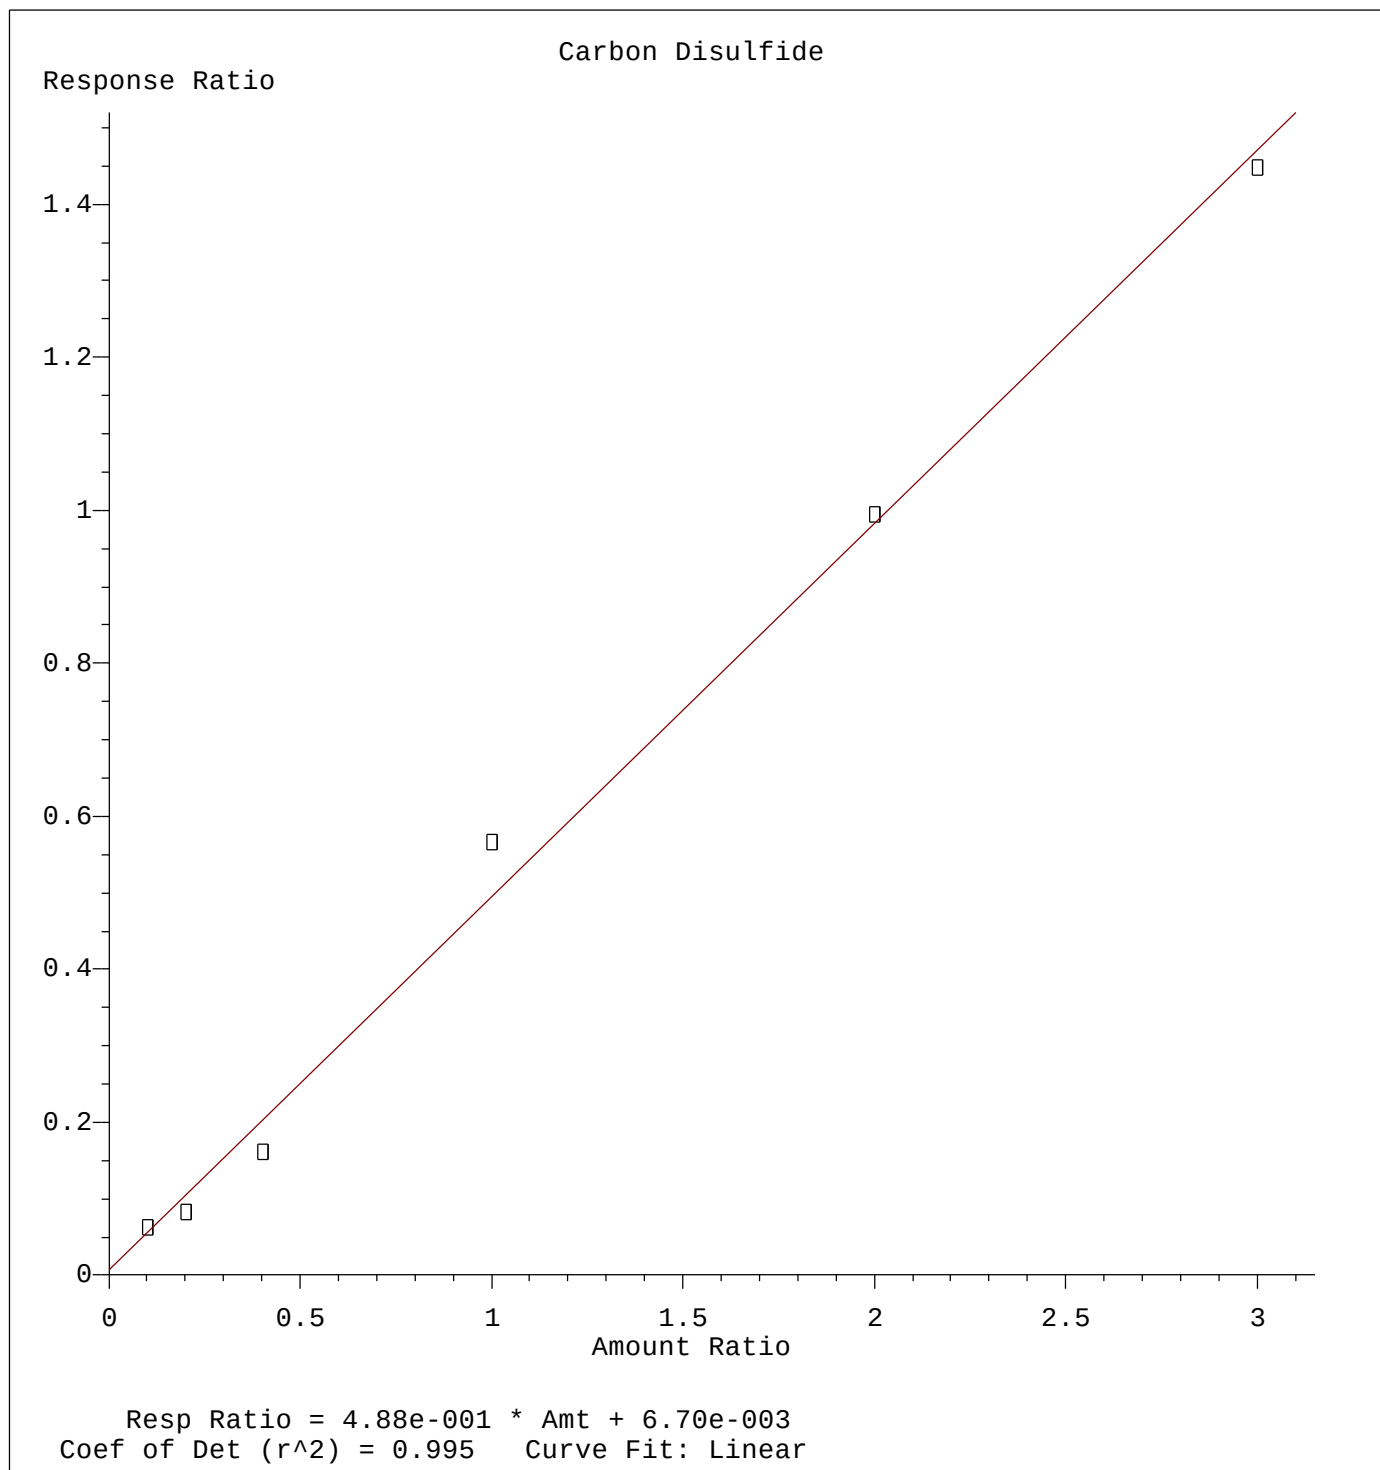

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082018S.M
Calibration Table Last Updated: Tue Aug 21 11:41:02 2018

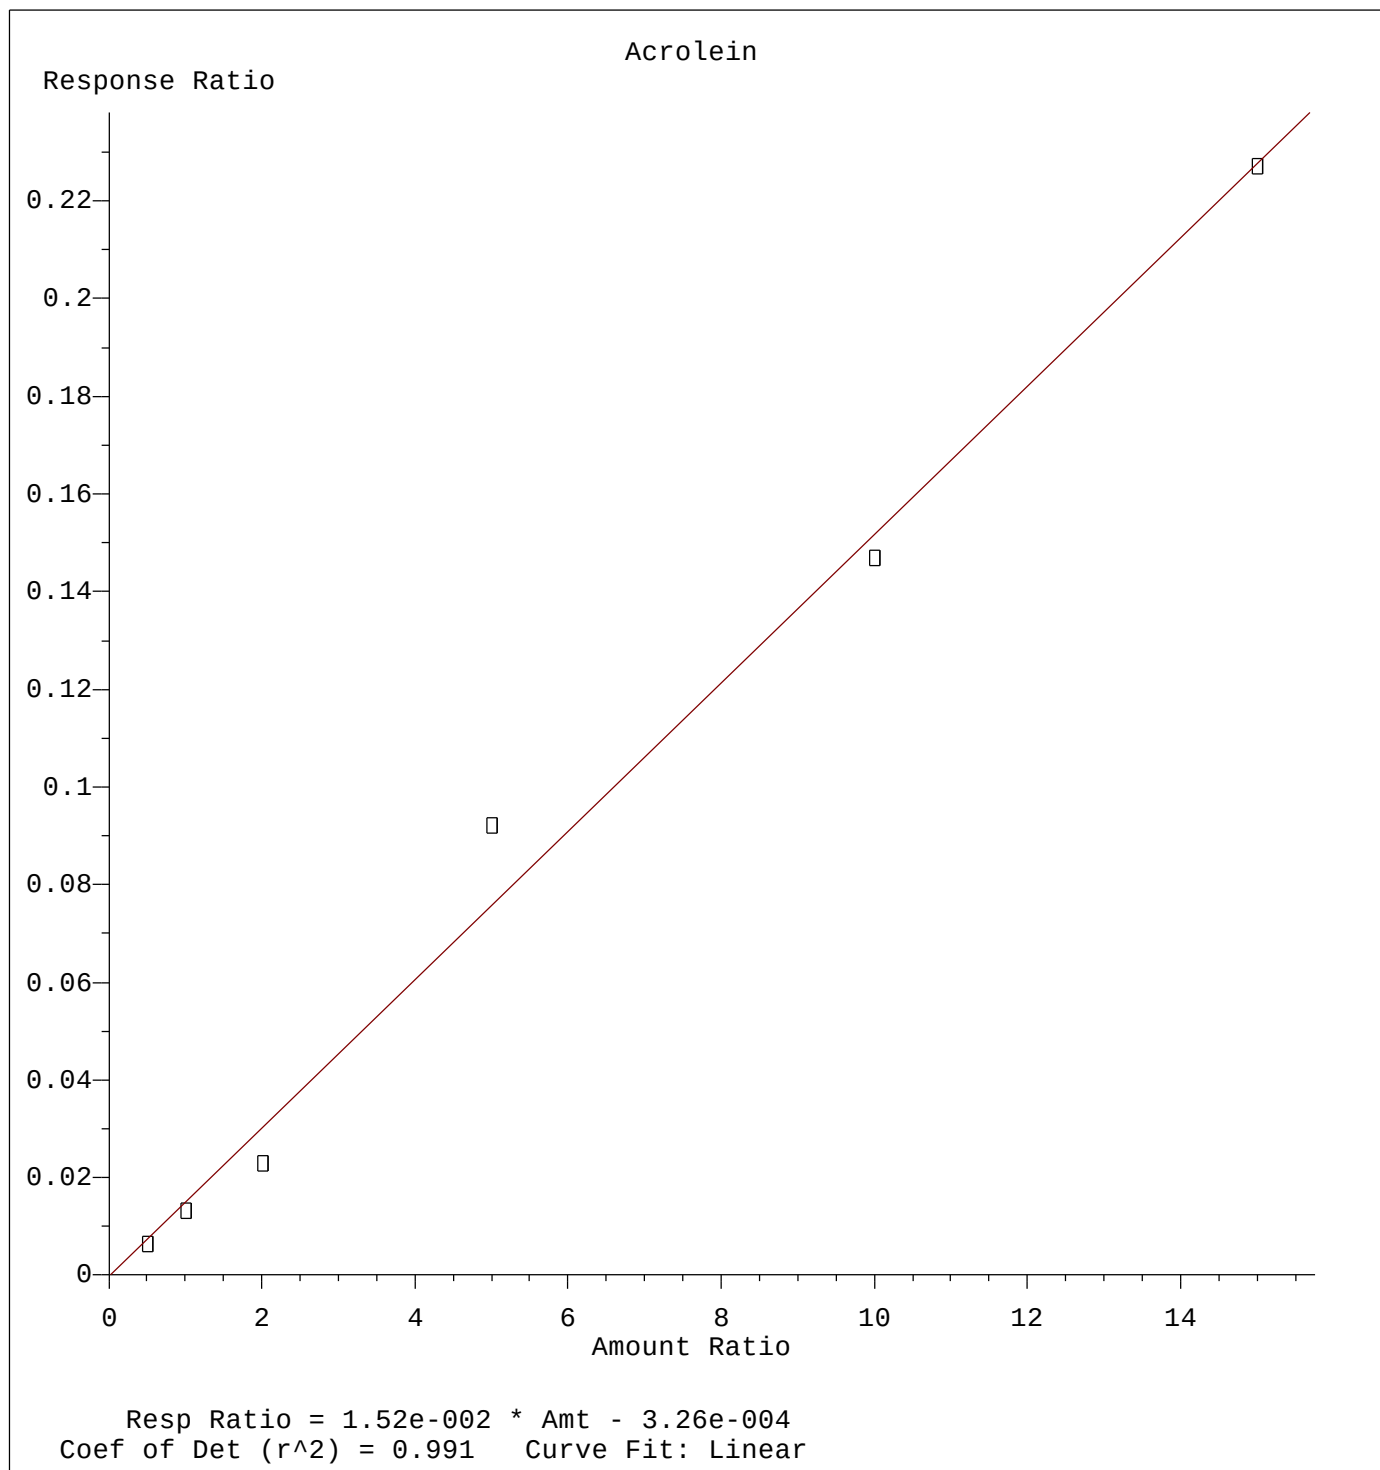

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082018S.M
Calibration Table Last Updated: Tue Aug 21 11:41:02 2018

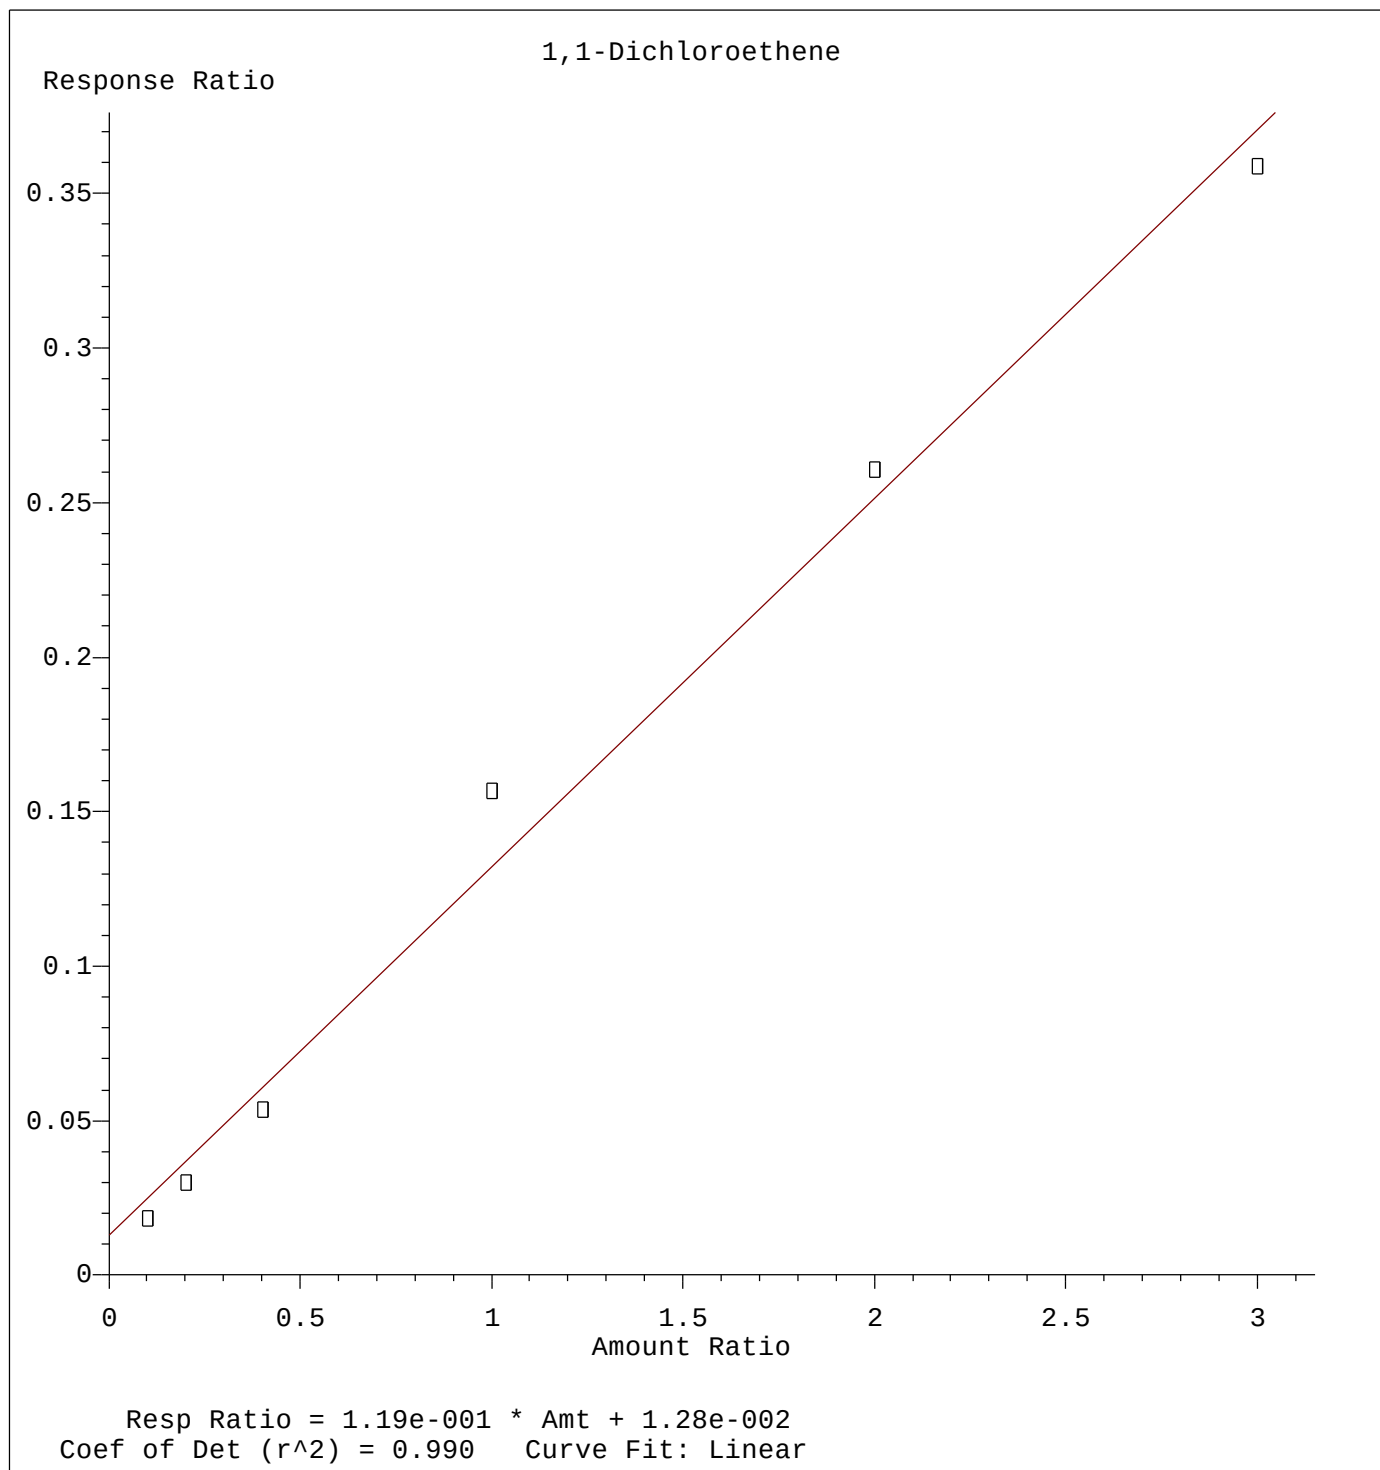

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082018S.M
Calibration Table Last Updated: Tue Aug 21 11:41:02 2018