


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD082018\
 Data File : VD059824.D
 Acq On : 20 Aug 2018 10:33
 Operator : JC/SY
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082018S.M
 Title : SW846 8260
 Last Update : Tue Aug 21 04:40:12 2018

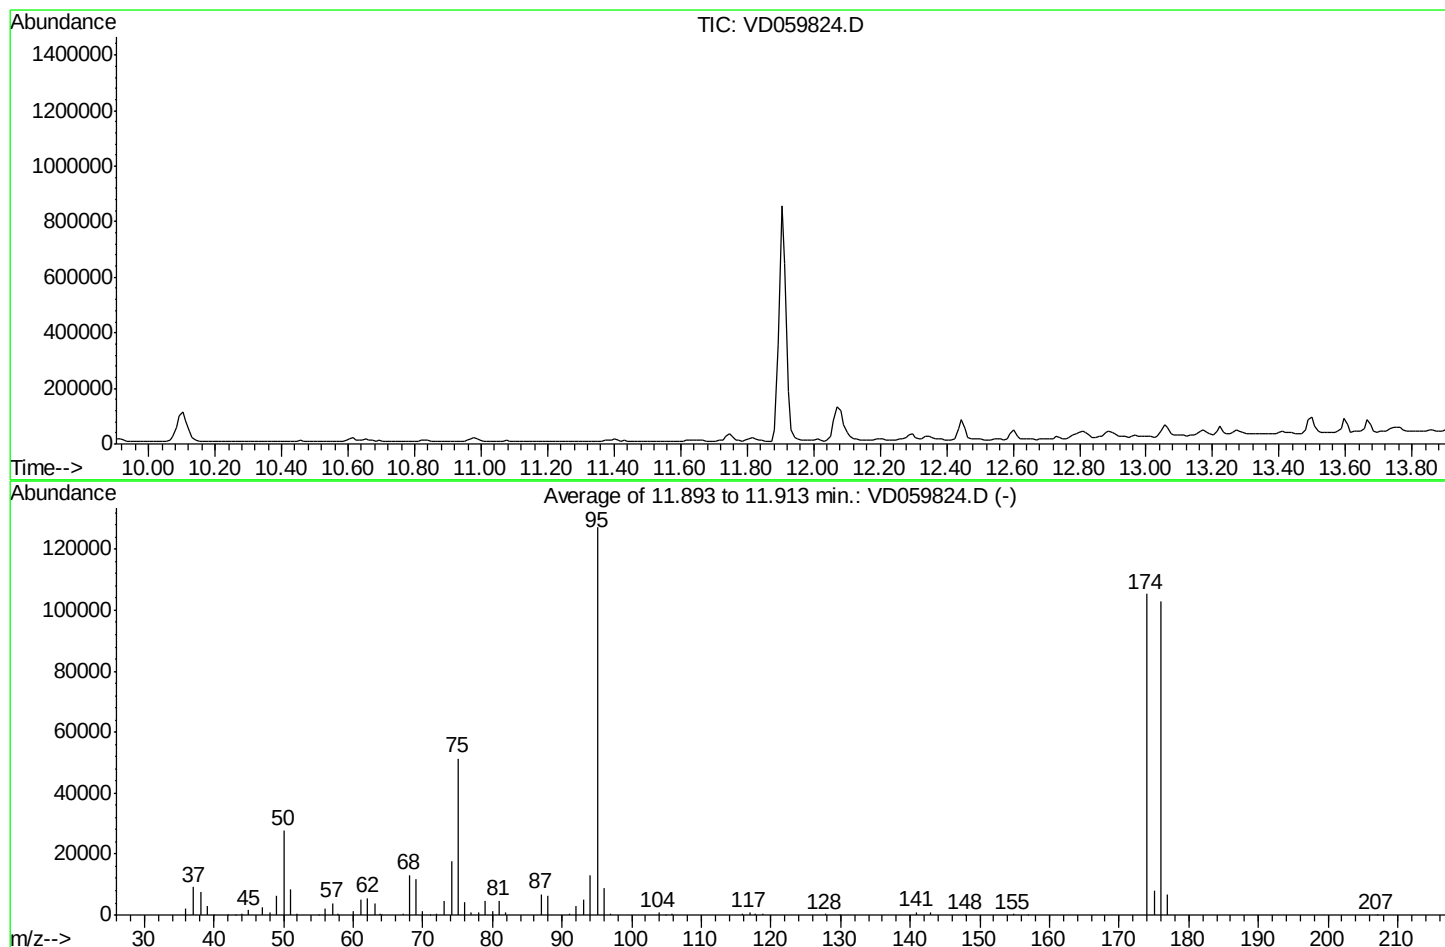

AutoFind: Scans 1186, 1187, 1188; Background Corrected with Scan 1181

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	27533	PASS
75	95	30	60	40.4	51352	PASS
95	95	100	100	100.0	127208	PASS
96	95	5	9	6.9	8781	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	82.8	105338	PASS
175	174	5	9	7.5	7867	PASS
176	174	95	101	97.7	102960	PASS
177	176	5	9	6.6	6794	PASS