


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD082118\
Data File : VD059847.D
Acq On : 21 Aug 2018 9:53
Operator : JC/SY
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082018S.M
Title : SW846 8260
Last Update : Wed Aug 22 03:46:30 2018

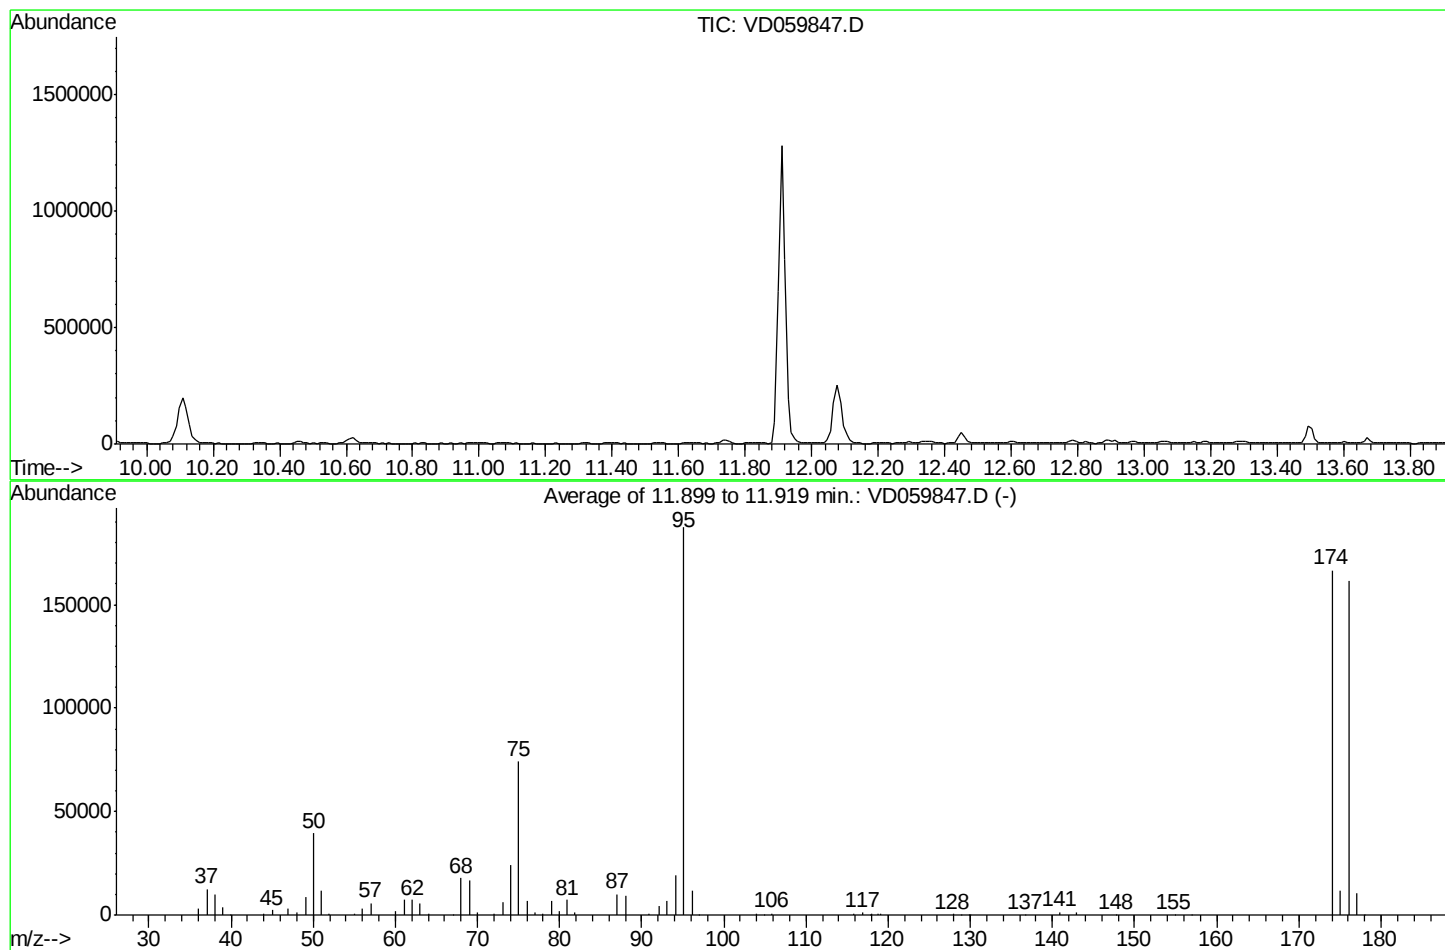

AutoFind: Scans 1186, 1187, 1188; Background Corrected with Scan 1181

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	39472	PASS
75	95	30	60	39.5	74058	PASS
95	95	100	100	100.0	187434	PASS
96	95	5	9	6.4	12044	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	88.8	166512	PASS
175	174	5	9	7.3	12083	PASS
176	174	95	101	97.2	161792	PASS
177	176	5	9	6.4	10385	PASS