


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082120S.M
Calibration Table Last Updated: Fri Aug 21 13:36:12 2020

Methylene Chloride

Response Ratio

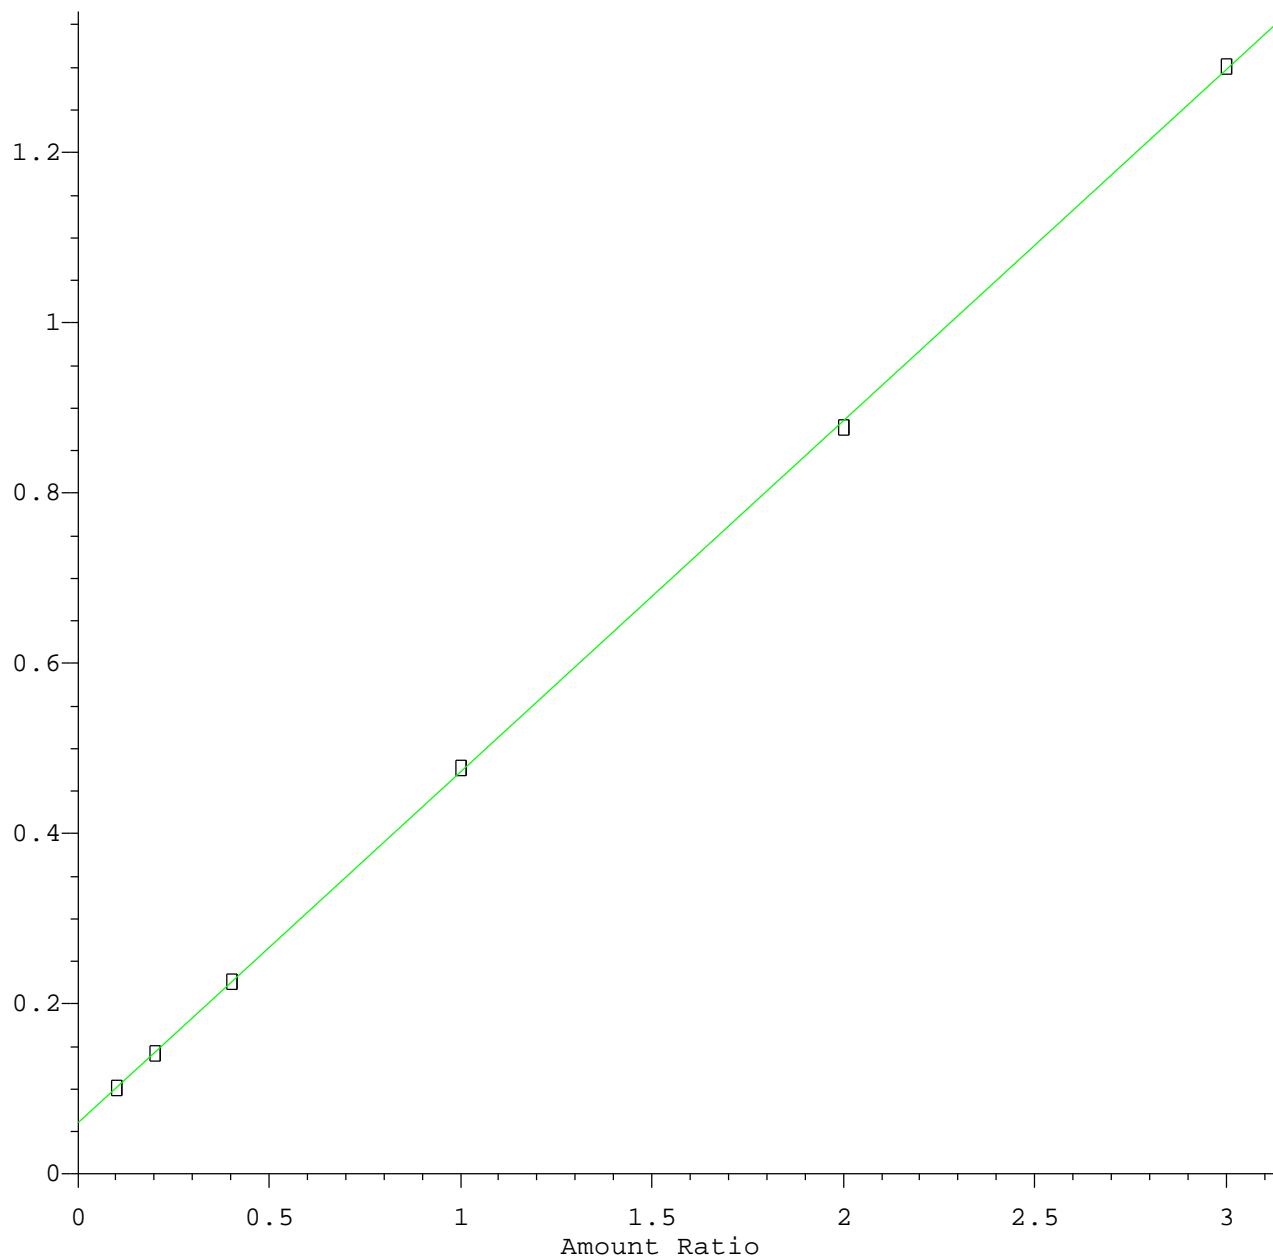

Resp Ratio = $4.12 \times 10^{-1} \times \text{Amt} + 5.98 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082120S.M
Calibration Table Last Updated: Fri Aug 21 13:36:12 2020