



Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082218S.M
Calibration Table Last Updated: Thu Aug 23 11:31:20 2018

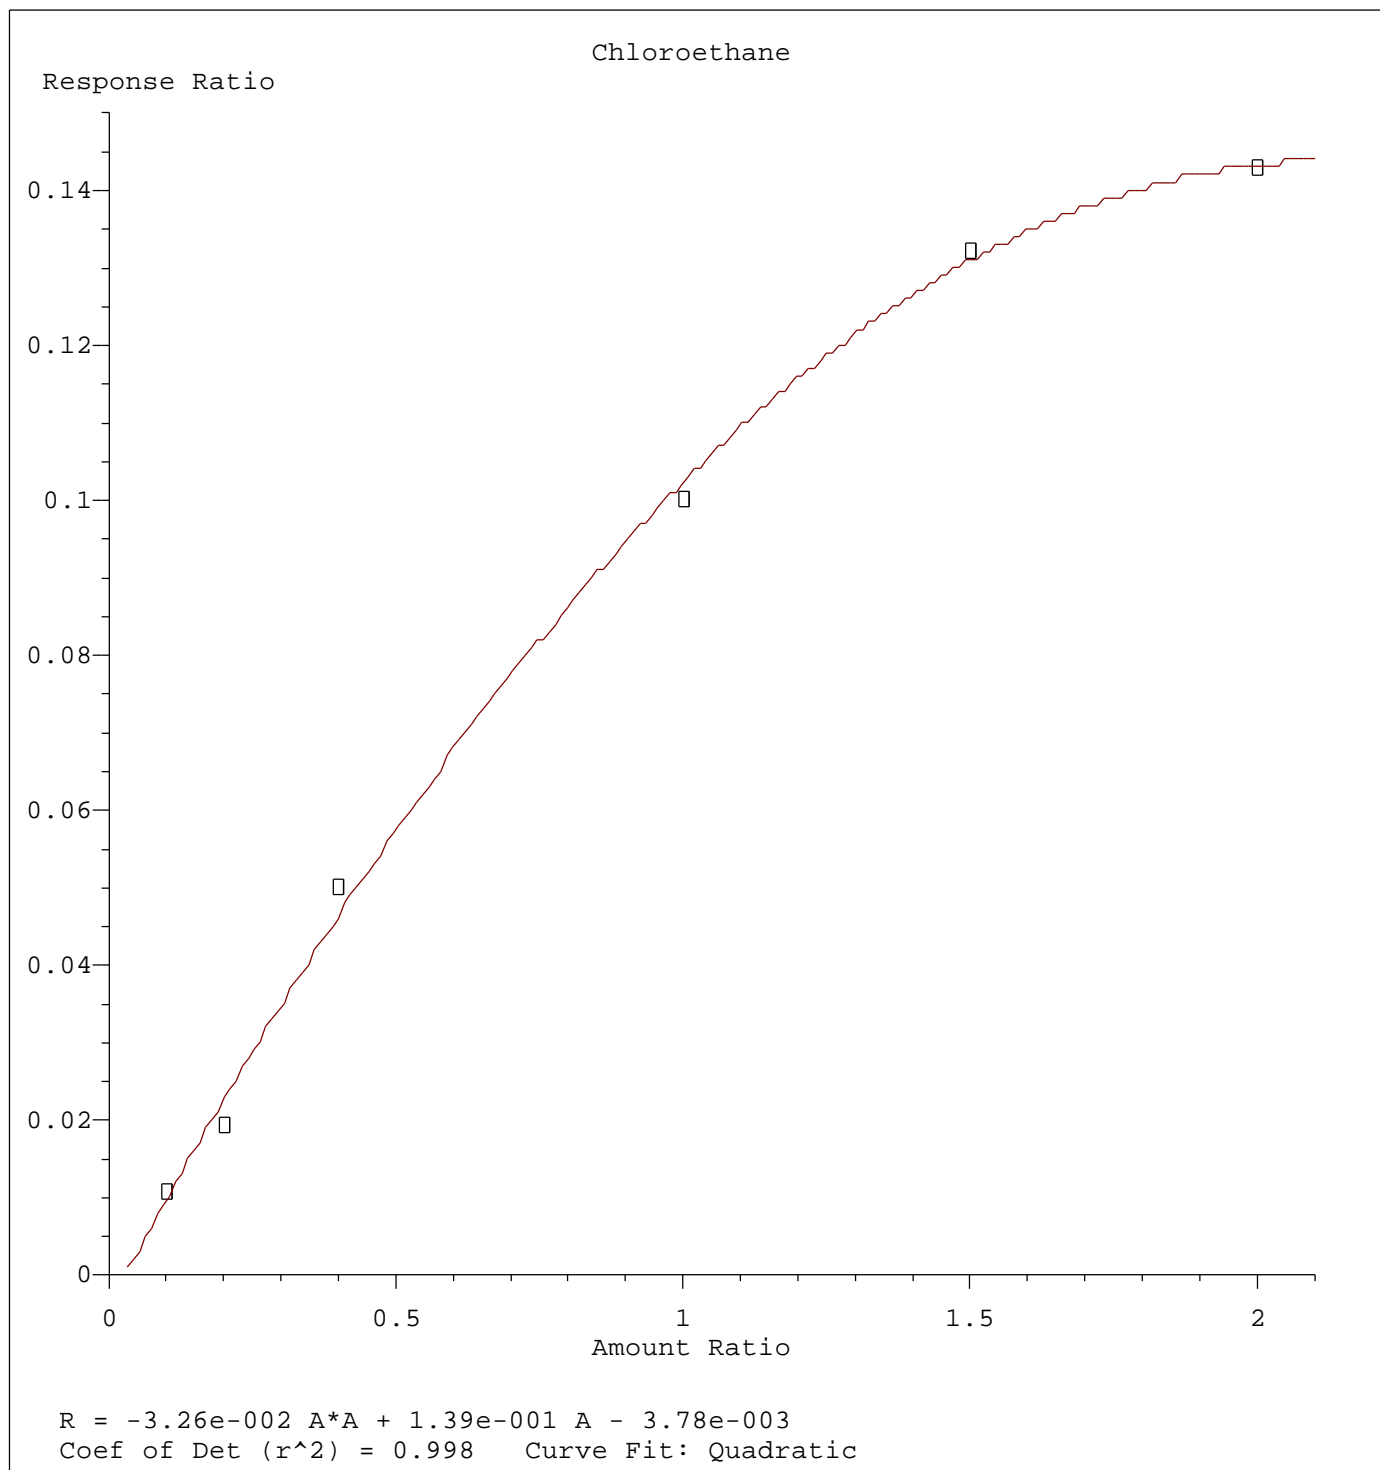

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082218S.M
Calibration Table Last Updated: Thu Aug 23 11:31:20 2018

n-Butylbenzene

Response Ratio

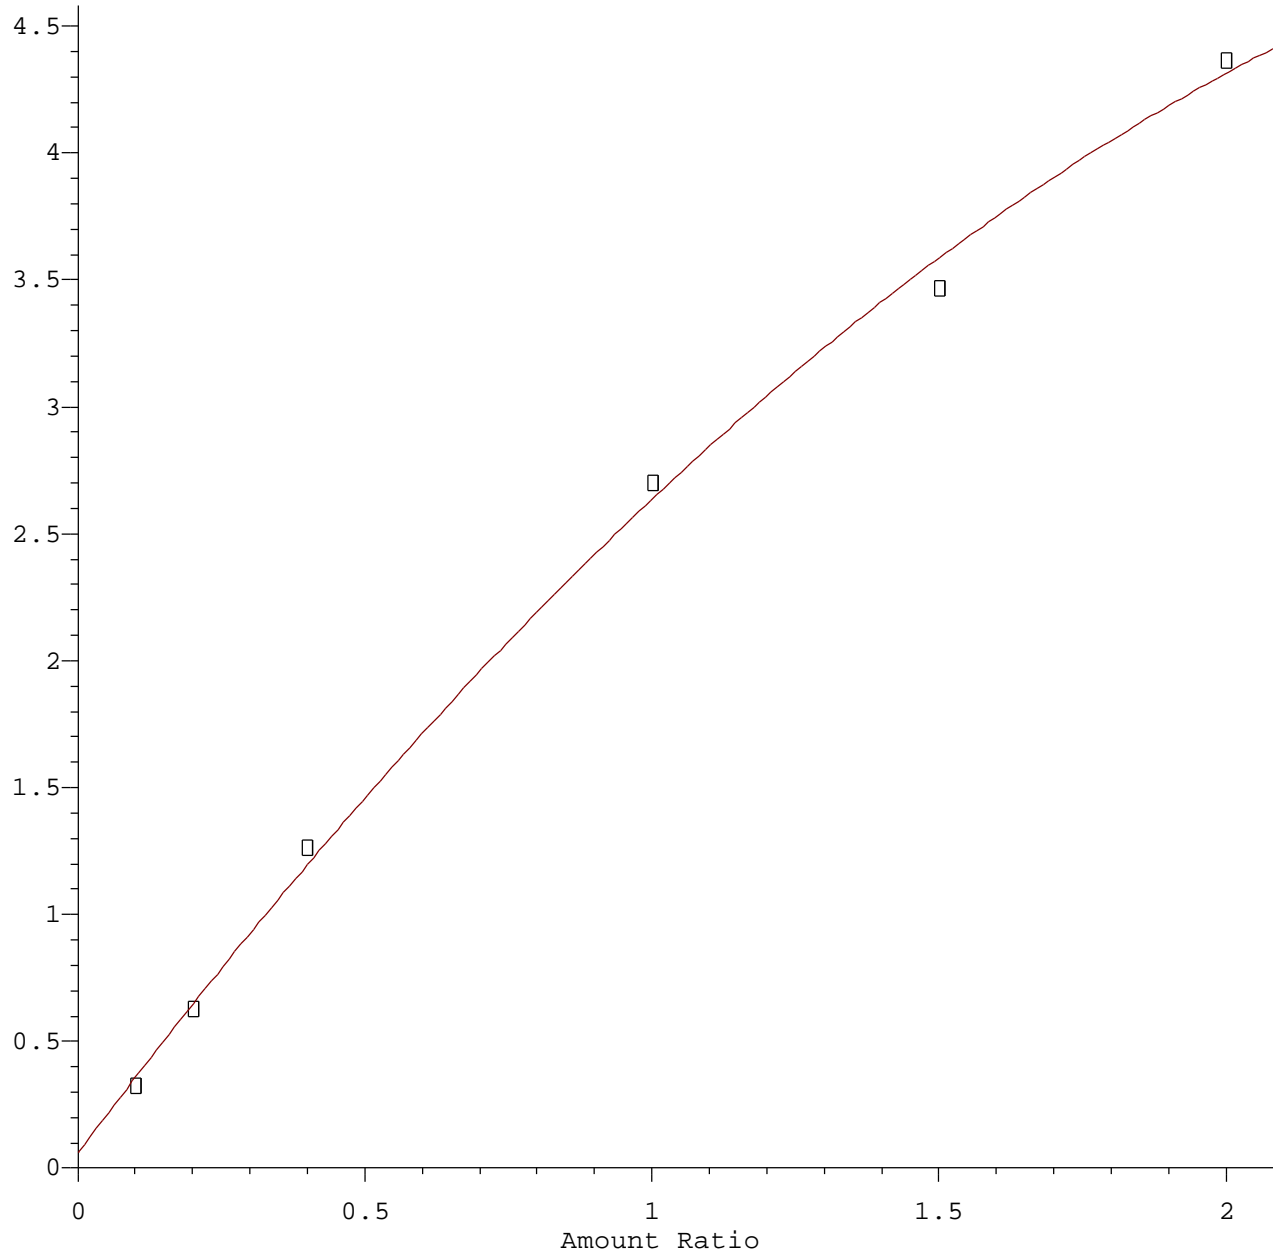


$R = -4.49e-001 A^2 + 3.02e+000 A + 5.94e-002$
Coef of Det (r^2) = 0.998 Curve Fit: Quadratic

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082218S.M
Calibration Table Last Updated: Thu Aug 23 11:31:20 2018

Methylene Chloride

Response Ratio

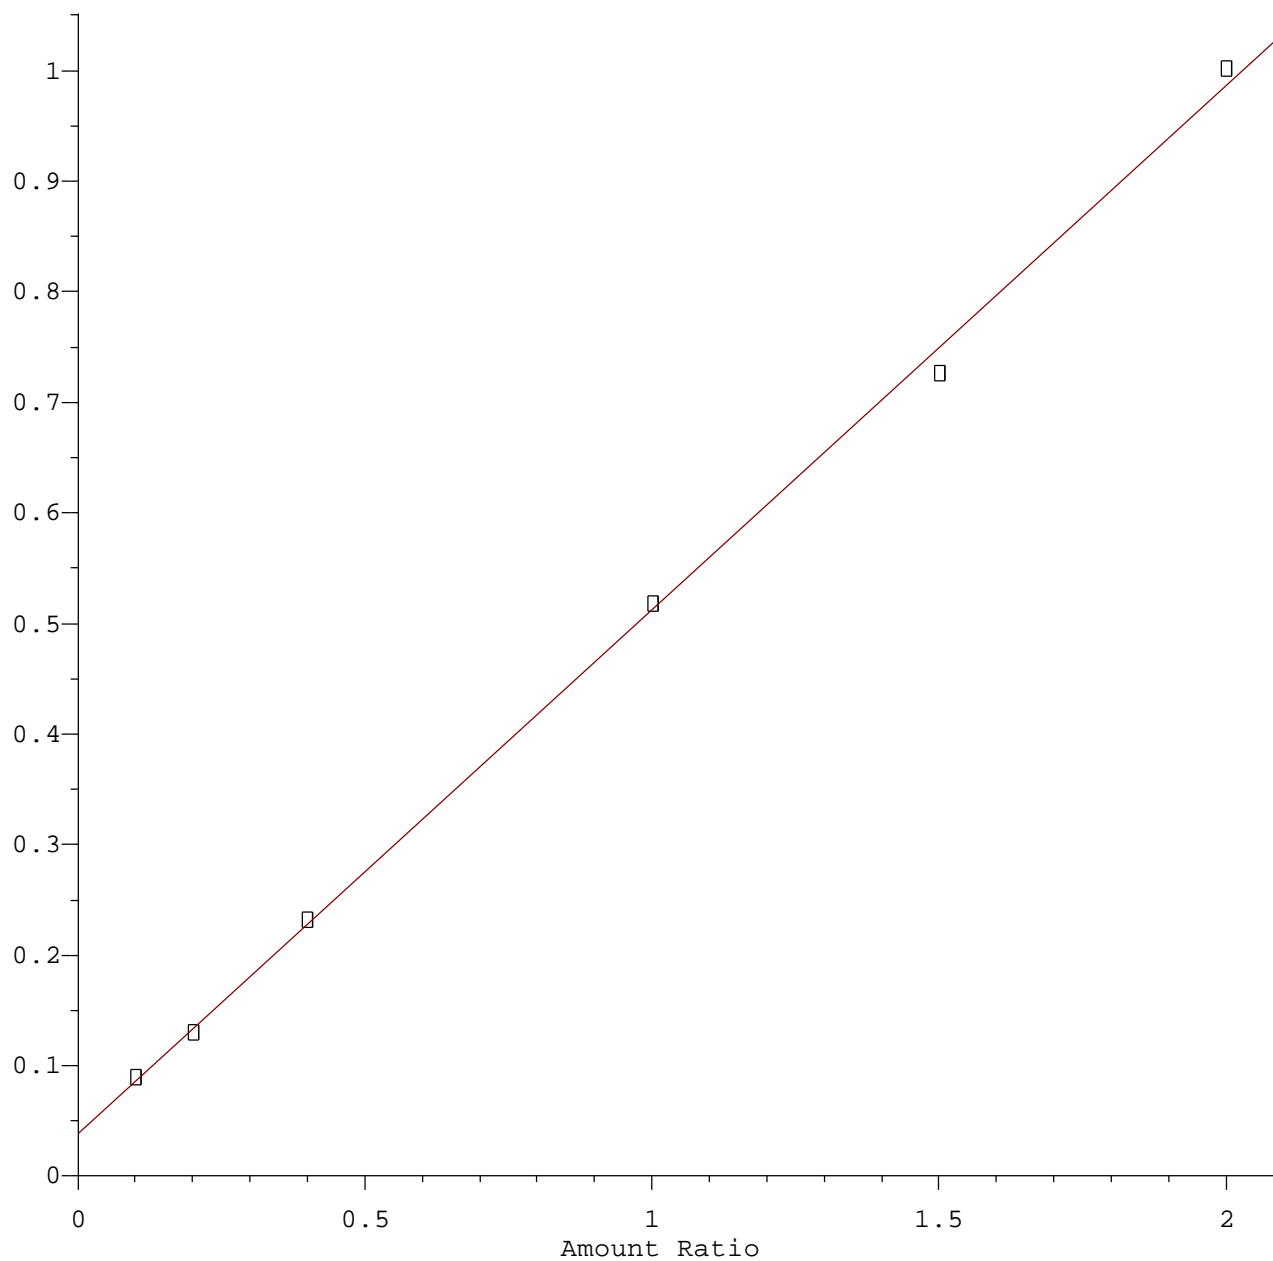

Resp Ratio = $4.74 \times 10^{-1} \times \text{Amt} + 3.81 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082218S.M
Calibration Table Last Updated: Thu Aug 23 11:31:20 2018