


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD082318\
 Data File : VD059880.D
 Acq On : 23 Aug 2018 9:42
 Operator : JC/SY
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082218S.M
 Title : SW846 8260
 Last Update : Thu Aug 23 03:03:08 2018

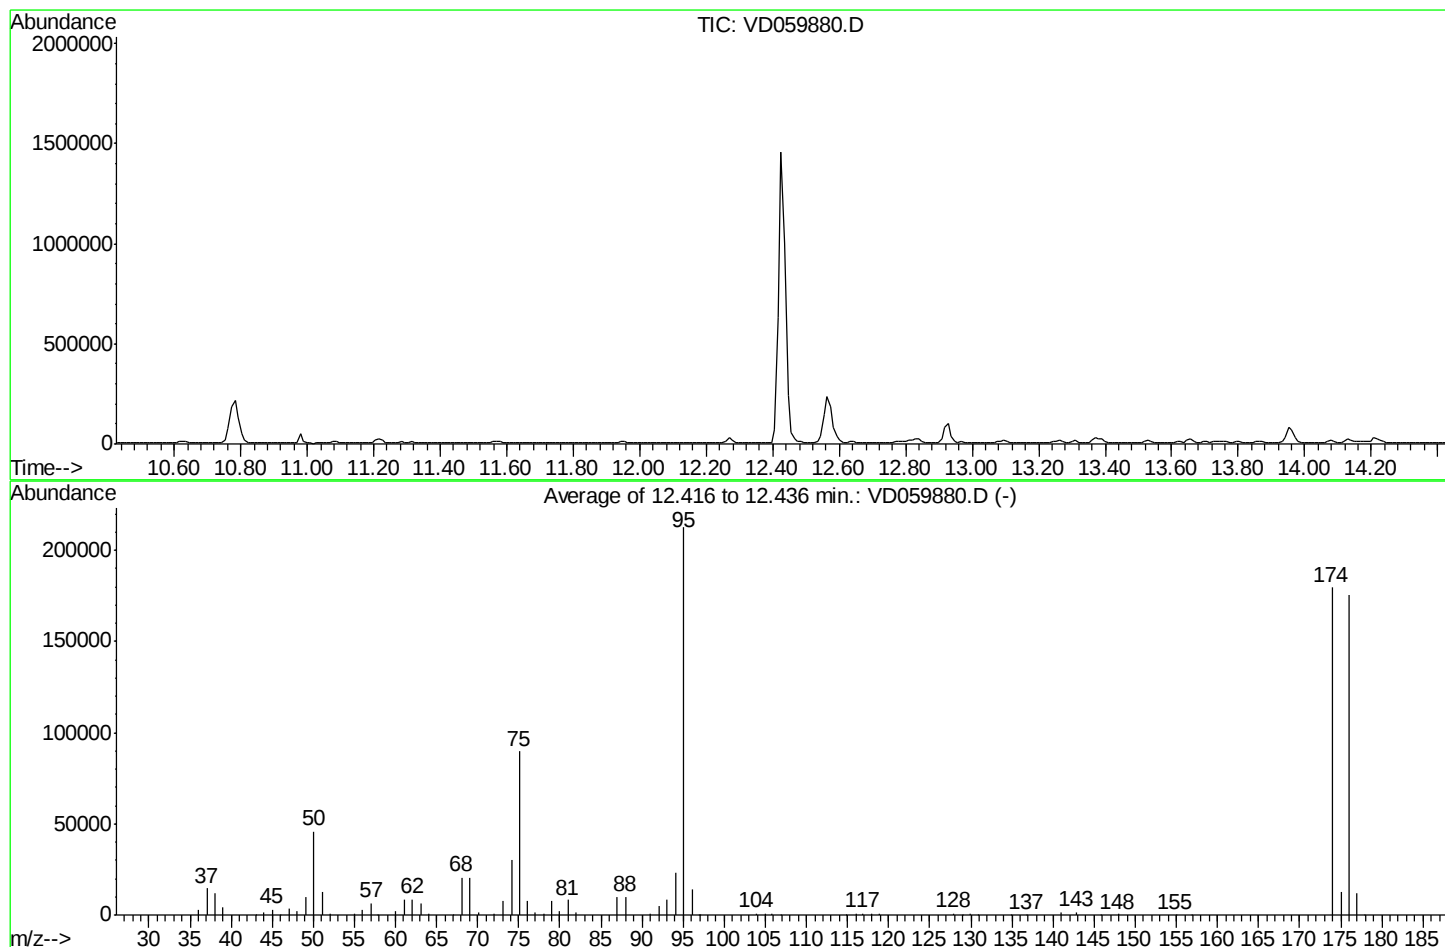

AutoFind: Scans 1239, 1240, 1241; Background Corrected with Scan 1234

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	45994	PASS
75	95	30	60	42.2	89656	PASS
95	95	100	100	100.0	212586	PASS
96	95	5	9	6.6	14067	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.5	179565	PASS
175	174	5	9	7.0	12588	PASS
176	174	95	101	97.8	175608	PASS
177	176	5	9	6.8	11900	PASS