

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD082321\
 Data File : VD070218.D
 Acq On : 23 Aug 2021 13:29
 Operator : VA/SY
 Sample : M3451-01
 Misc : 4.61G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 TP-0-5-COMP

Quant Time: Aug 24 01:30:42 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D081321S.M
 Quant Title : SW846 8260
 QLast Update : Sat Aug 14 02:33:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	525811	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	1033979	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	986155	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.567	152	393946	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	342281	55.346	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	110.700%
35) Dibromofluoromethane	7.914	113	335767	50.263	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.520%
50) Toluene-d8	10.338	98	1328119	51.116	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	102.240%
62) 4-Bromofluorobenzene	12.626	95	415329	48.532	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	97.060%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD082321\
Data File : VD070218.D
Acq On : 23 Aug 2021 13:29
Operator : VA/SY
Sample : M3451-01
Misc : 4.61G/5.00ml/MSVOA_D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
TP-0-5-COMP

Quant Time: Aug 24 01:30:42 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D081321S.M
Quant Title : SW846 8260
QLast Update : Sat Aug 14 02:33:51 2021
Response via : Initial Calibration




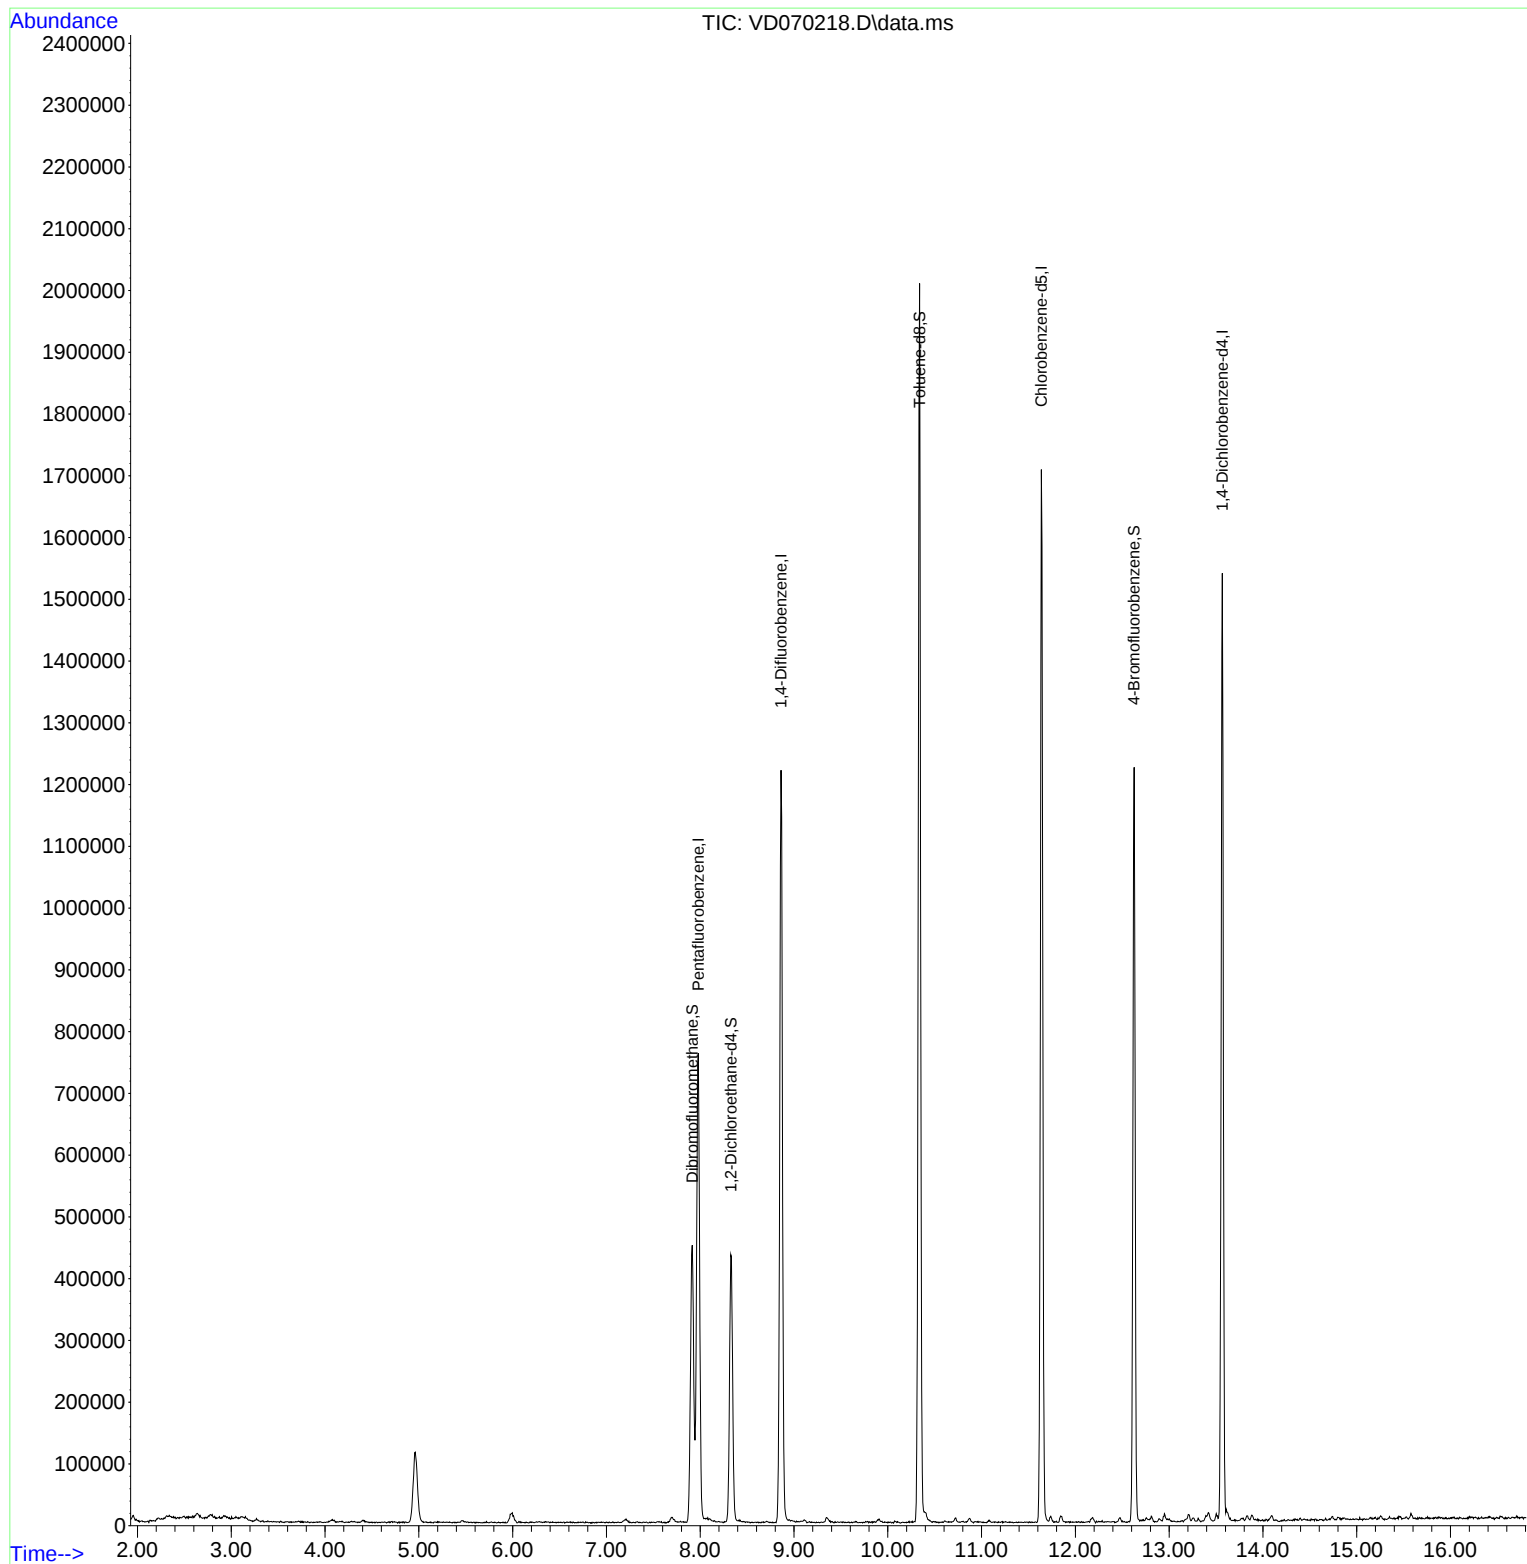


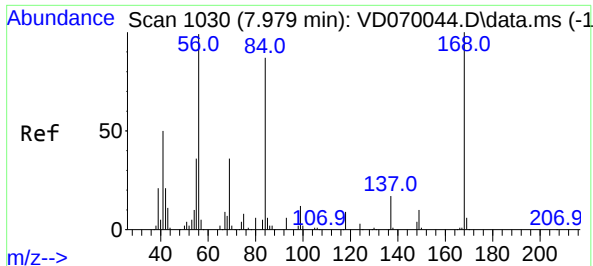

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. 0.000 min
Lab File: VD070218.D
Acq: 23 Aug 2021 13:29




Instrument :
MSVOA_D
ClientSampleId :
TP-0-5-COMP


Tgt Ion:168 Resp: 525811
Ion Ratio Lower Upper
168 100
99 63.8 50.3 75.5

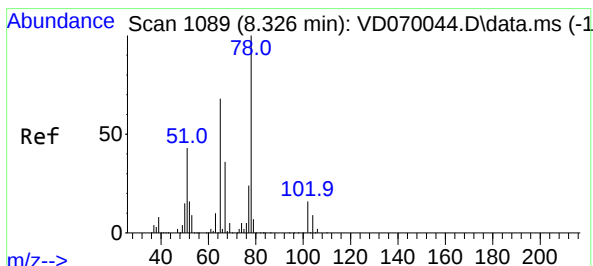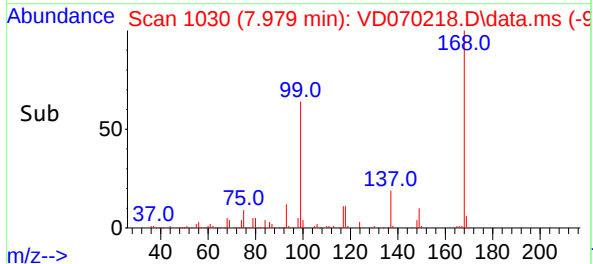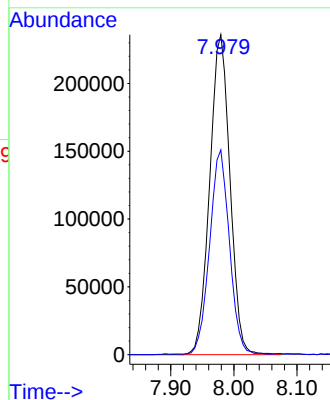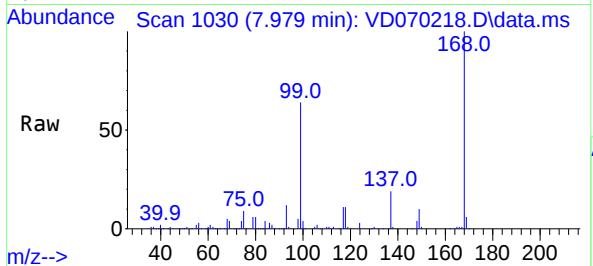

#33
1,2-Dichloroethane-d4
Concen: 55.346 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. 0.000 min
Lab File: VD070218.D
Acq: 23 Aug 2021 13:29

Tgt Ion: 65 Resp: 342281
Ion Ratio Lower Upper
65 100
67 54.5 0.0 107.8

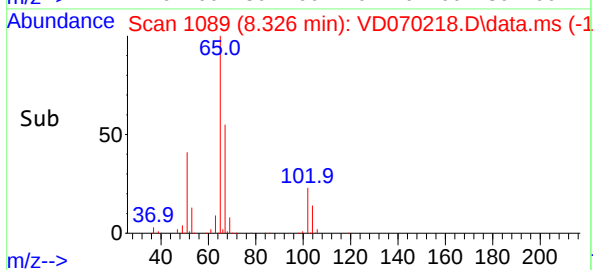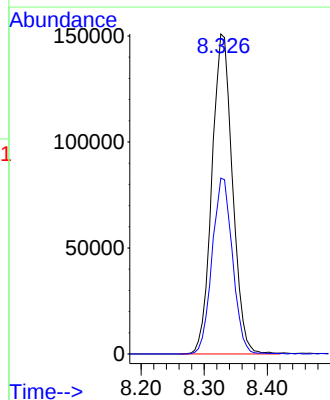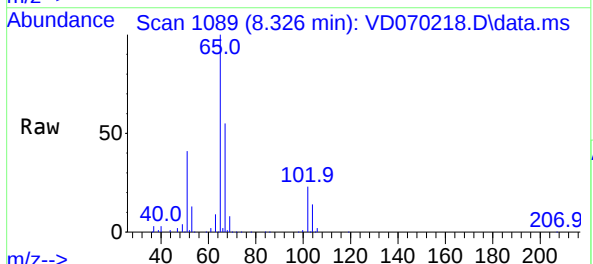




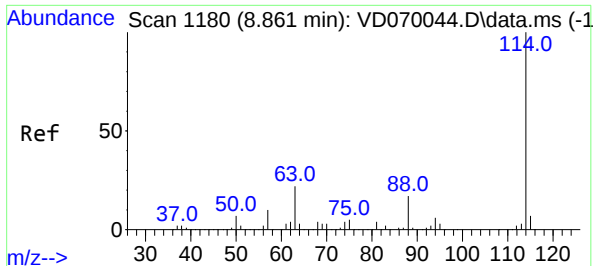


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. 0.000 min
Lab File: VD070218.D
Acq: 23 Aug 2021 13:29

Instrument :
MSVOA_D
ClientSampleId :
TP-0-5-COMP




Tgt Ion:114 Resp: 1033979
Ion Ratio Lower Upper
114 100
63 22.2 0.0 43.6
88 16.5 0.0 33.4

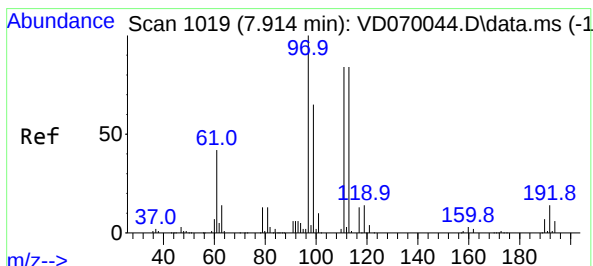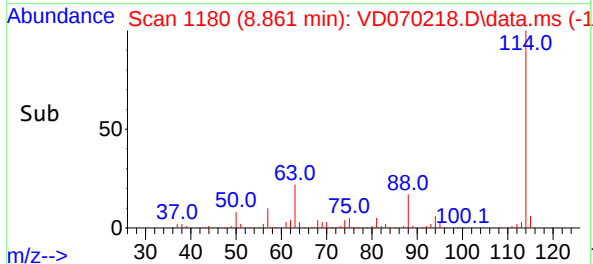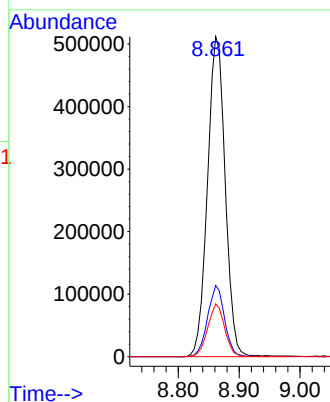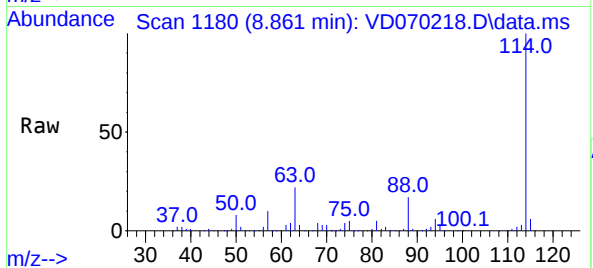


#35

Dibromofluoromethane
Concen: 50.263 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. 0.000 min
Lab File: VD070218.D
Acq: 23 Aug 2021 13:29

Tgt Ion:113 Resp: 335767
Ion Ratio Lower Upper
113 100
111 103.6 81.8 122.6
192 16.4 13.2 19.8


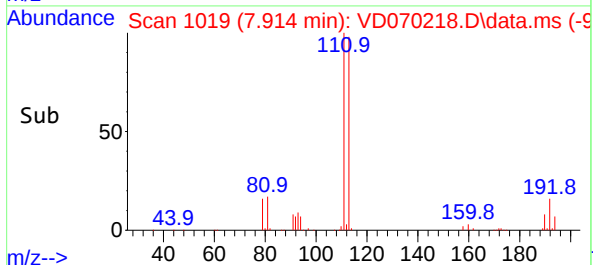
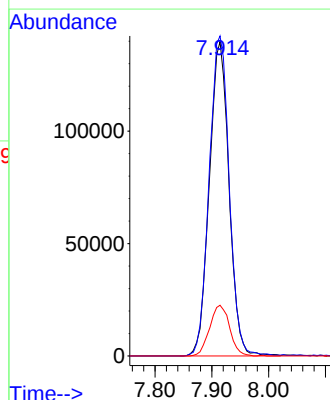
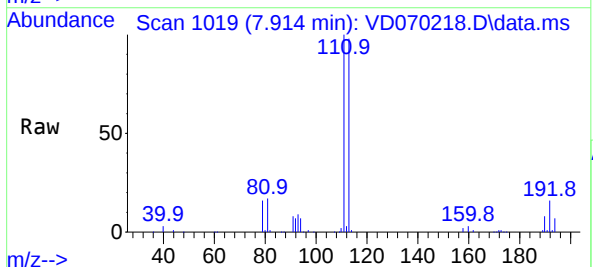


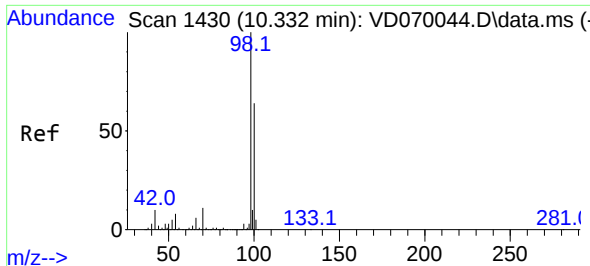

#50
Toluene-d8
Concen: 51.116 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. 0.006 min
Lab File: VD070218.D
Acq: 23 Aug 2021 13:29




Instrument :
MSVOA_D
ClientSampleId :
TP-0-5-COMP


Tgt Ion: 98 Resp: 1328119
Ion Ratio Lower Upper
98 100
100 63.8 52.6 78.8

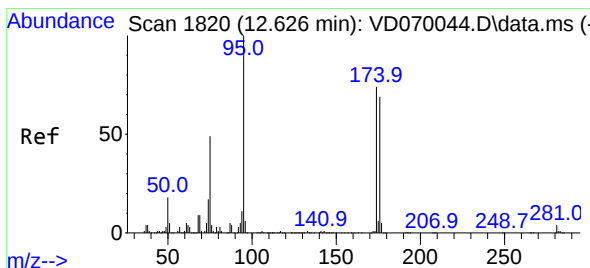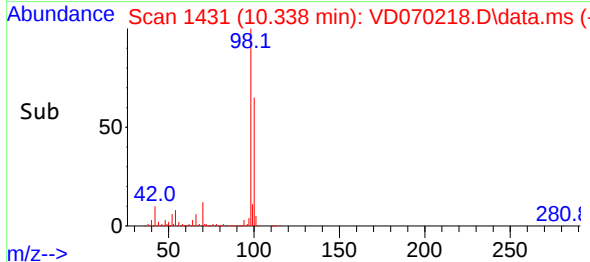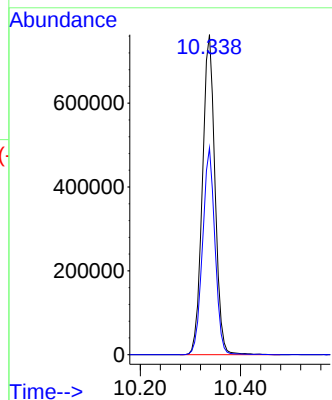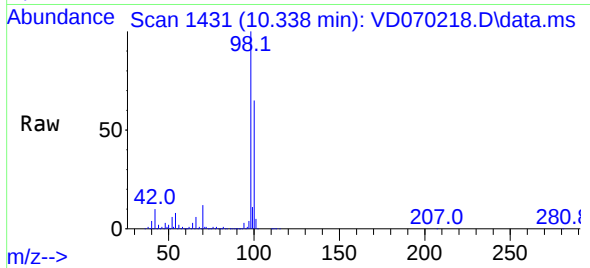

#62
4-Bromofluorobenzene
Concen: 48.532 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. 0.000 min
Lab File: VD070218.D
Acq: 23 Aug 2021 13:29

Tgt Ion: 95 Resp: 415329
Ion Ratio Lower Upper
95 100
174 72.6 0.0 141.6
176 69.2 0.0 138.2


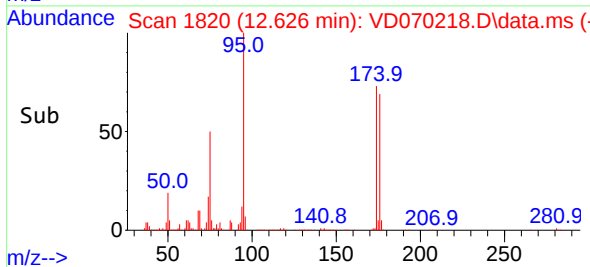
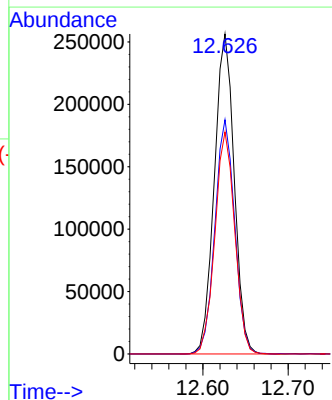
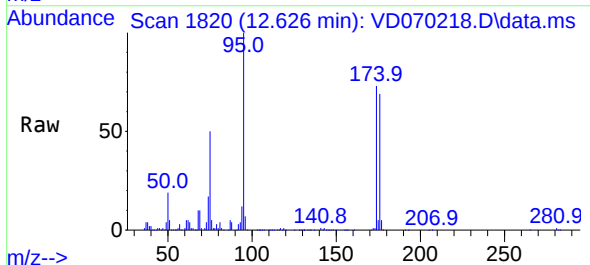


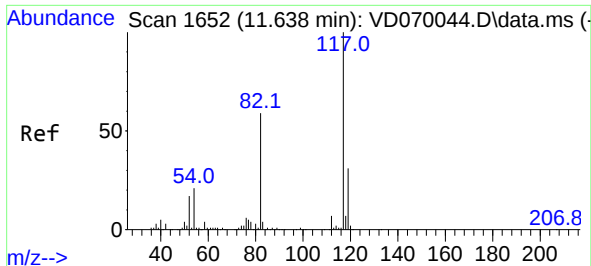

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1652
Delta R.T. 0.000 min
Lab File: VD070218.D
Acq: 23 Aug 2021 13:29

Instrument :
MSVOA_D
ClientSampleId :
TP-0-5-COMP

Tgt Ion:	117	Resp:	986155
Ion	Ratio	Lower	Upper
117	100		
82	58.3	47.5	71.3
119	31.7	25.1	37.7

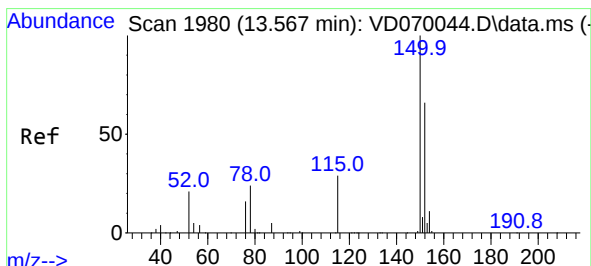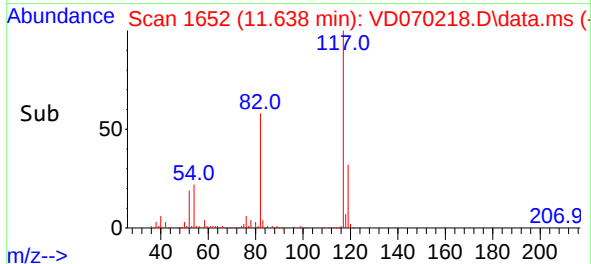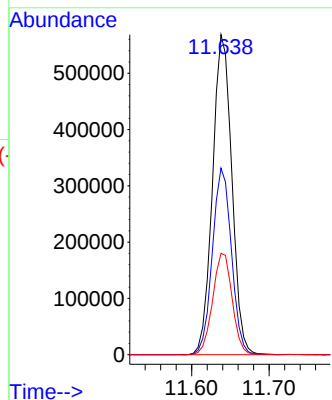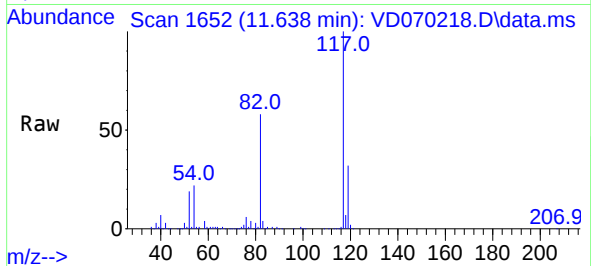

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.567 min Scan# 1980
Delta R.T. 0.000 min
Lab File: VD070218.D
Acq: 23 Aug 2021 13:29

Tgt Ion:	152	Resp:	393946
Ion	Ratio	Lower	Upper
152	100		
115	62.9	31.2	93.6
150	158.8	0.0	352.0

