


Methyl Iodide

Response Ratio

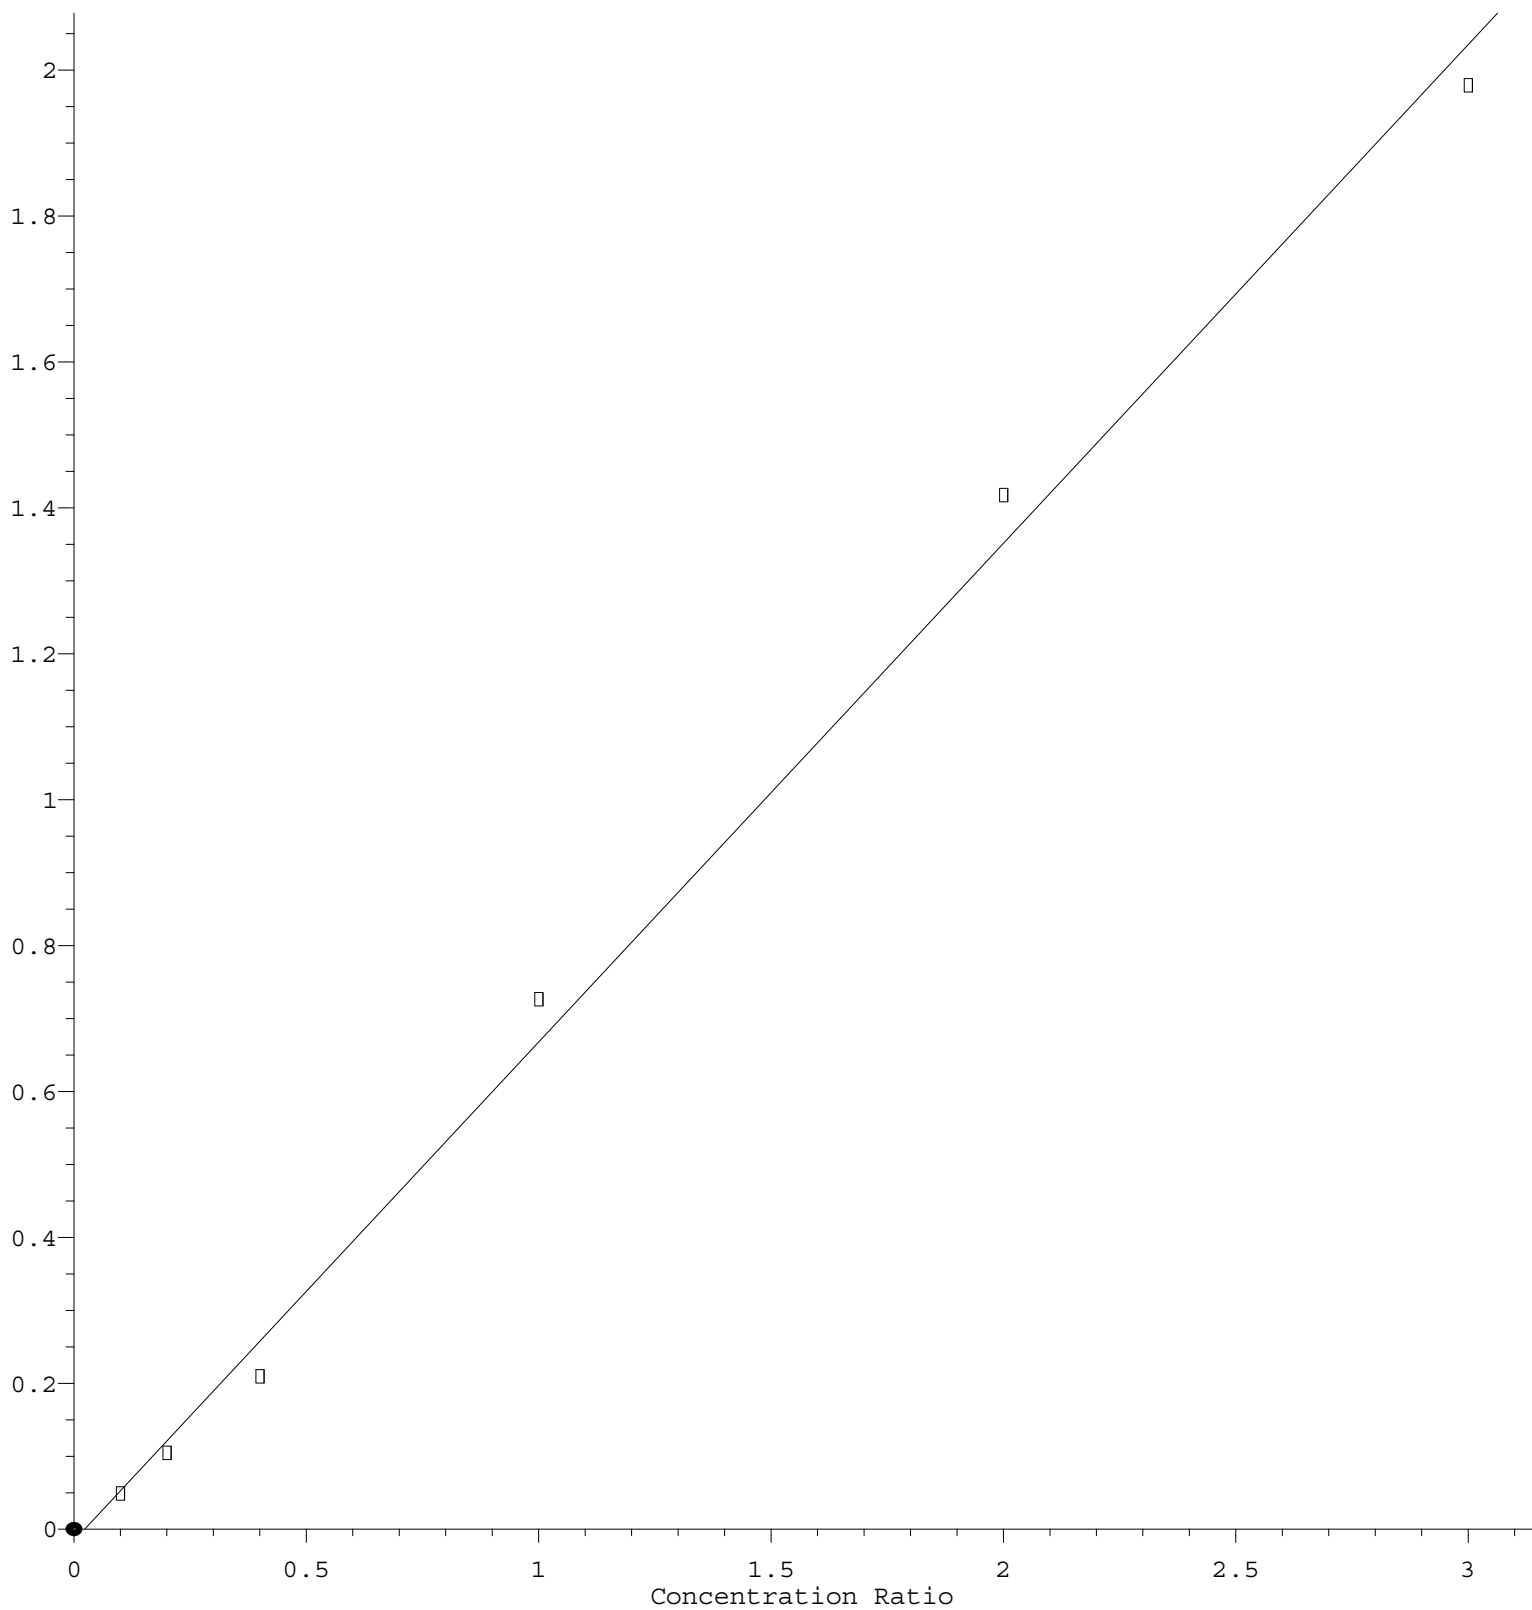


$$\text{Response} = 6.835\text{e-}001 * \text{Amt} - 1.561\text{e-}002$$

Coef of Det (r^2) = 0.995720 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D082322S.M

Calibration Table Last Updated: Tue Aug 23 13:12:17 2022


Acrolein

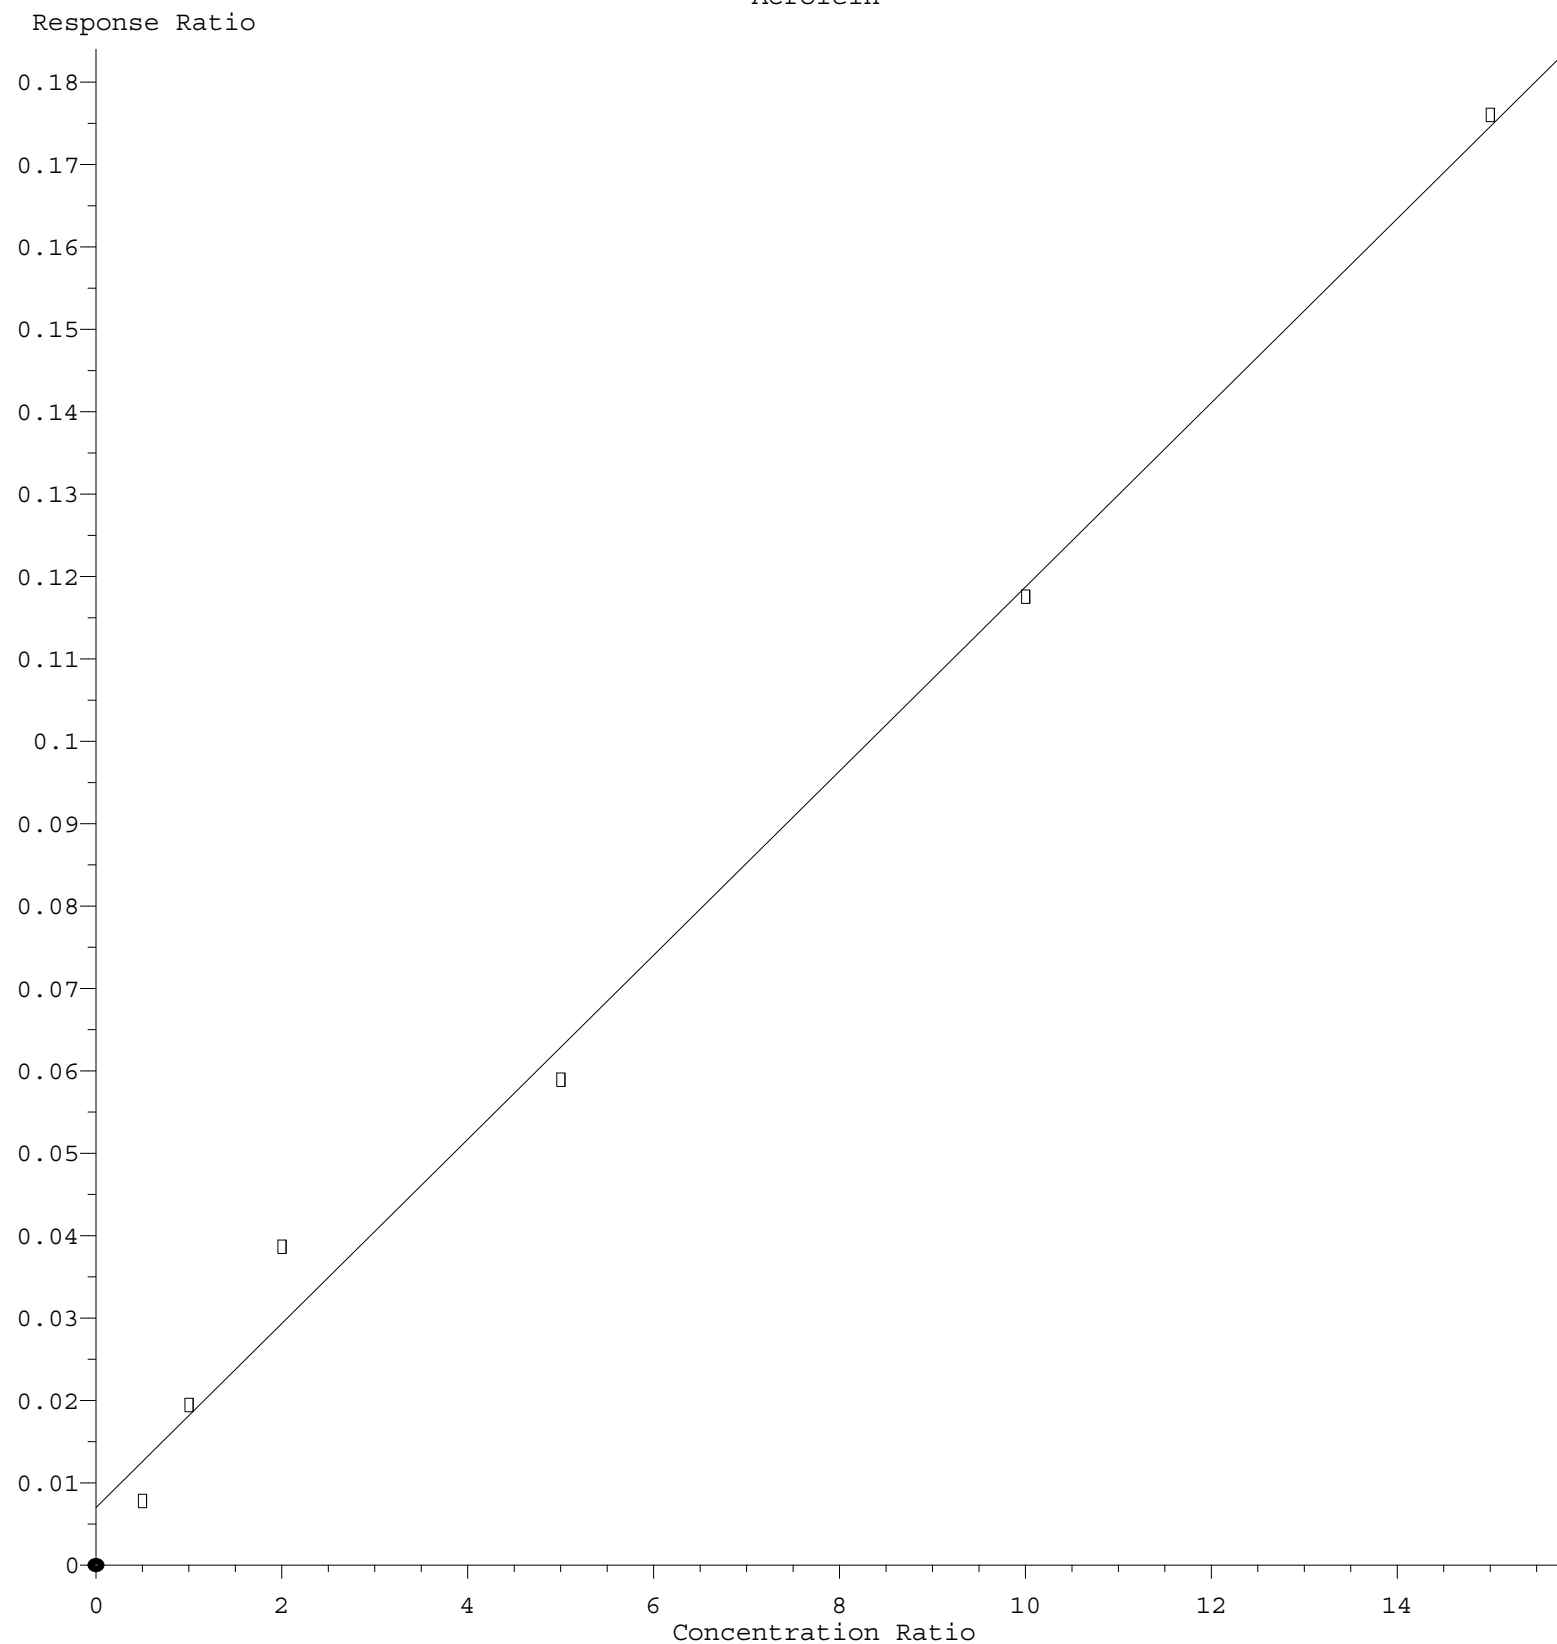

Response = $1.115 \times 10^{-2} \times \text{Amt} + 7.486 \times 10^{-3}$
 Coef of Det (r^2) = 0.993850 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D082322S.M
 Calibration Table Last Updated: Tue Aug 23 13:12:17 2022

Carbon Disulfide

Response Ratio

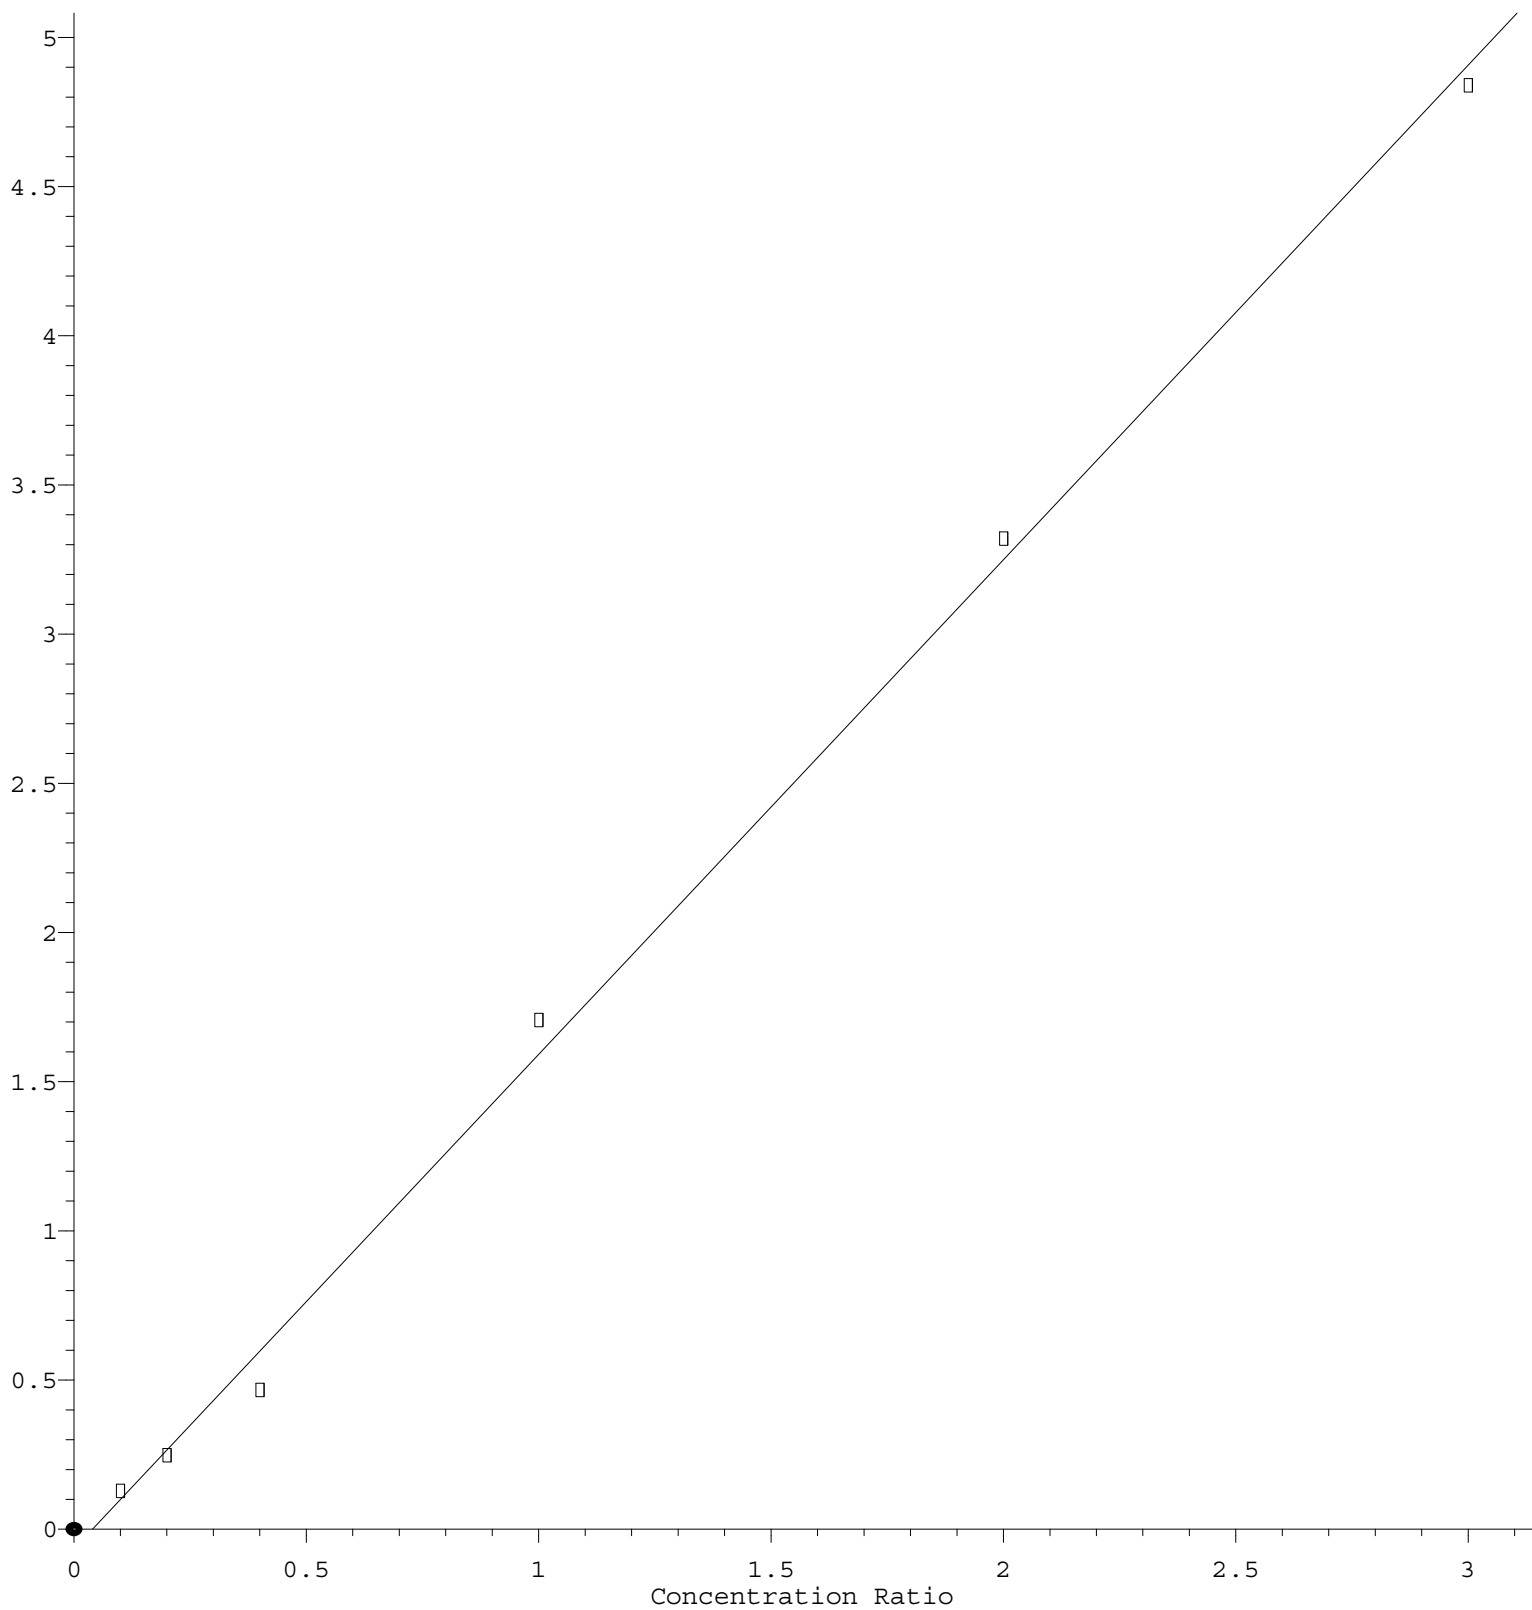


$$\text{Response} = 1.658\text{e}+000 * \text{Amt} - 6.674\text{e}-002$$

Coef of Det (r^2) = 0.997799 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D082322S.M

Calibration Table Last Updated: Tue Aug 23 13:12:17 2022

Methyl Acetate

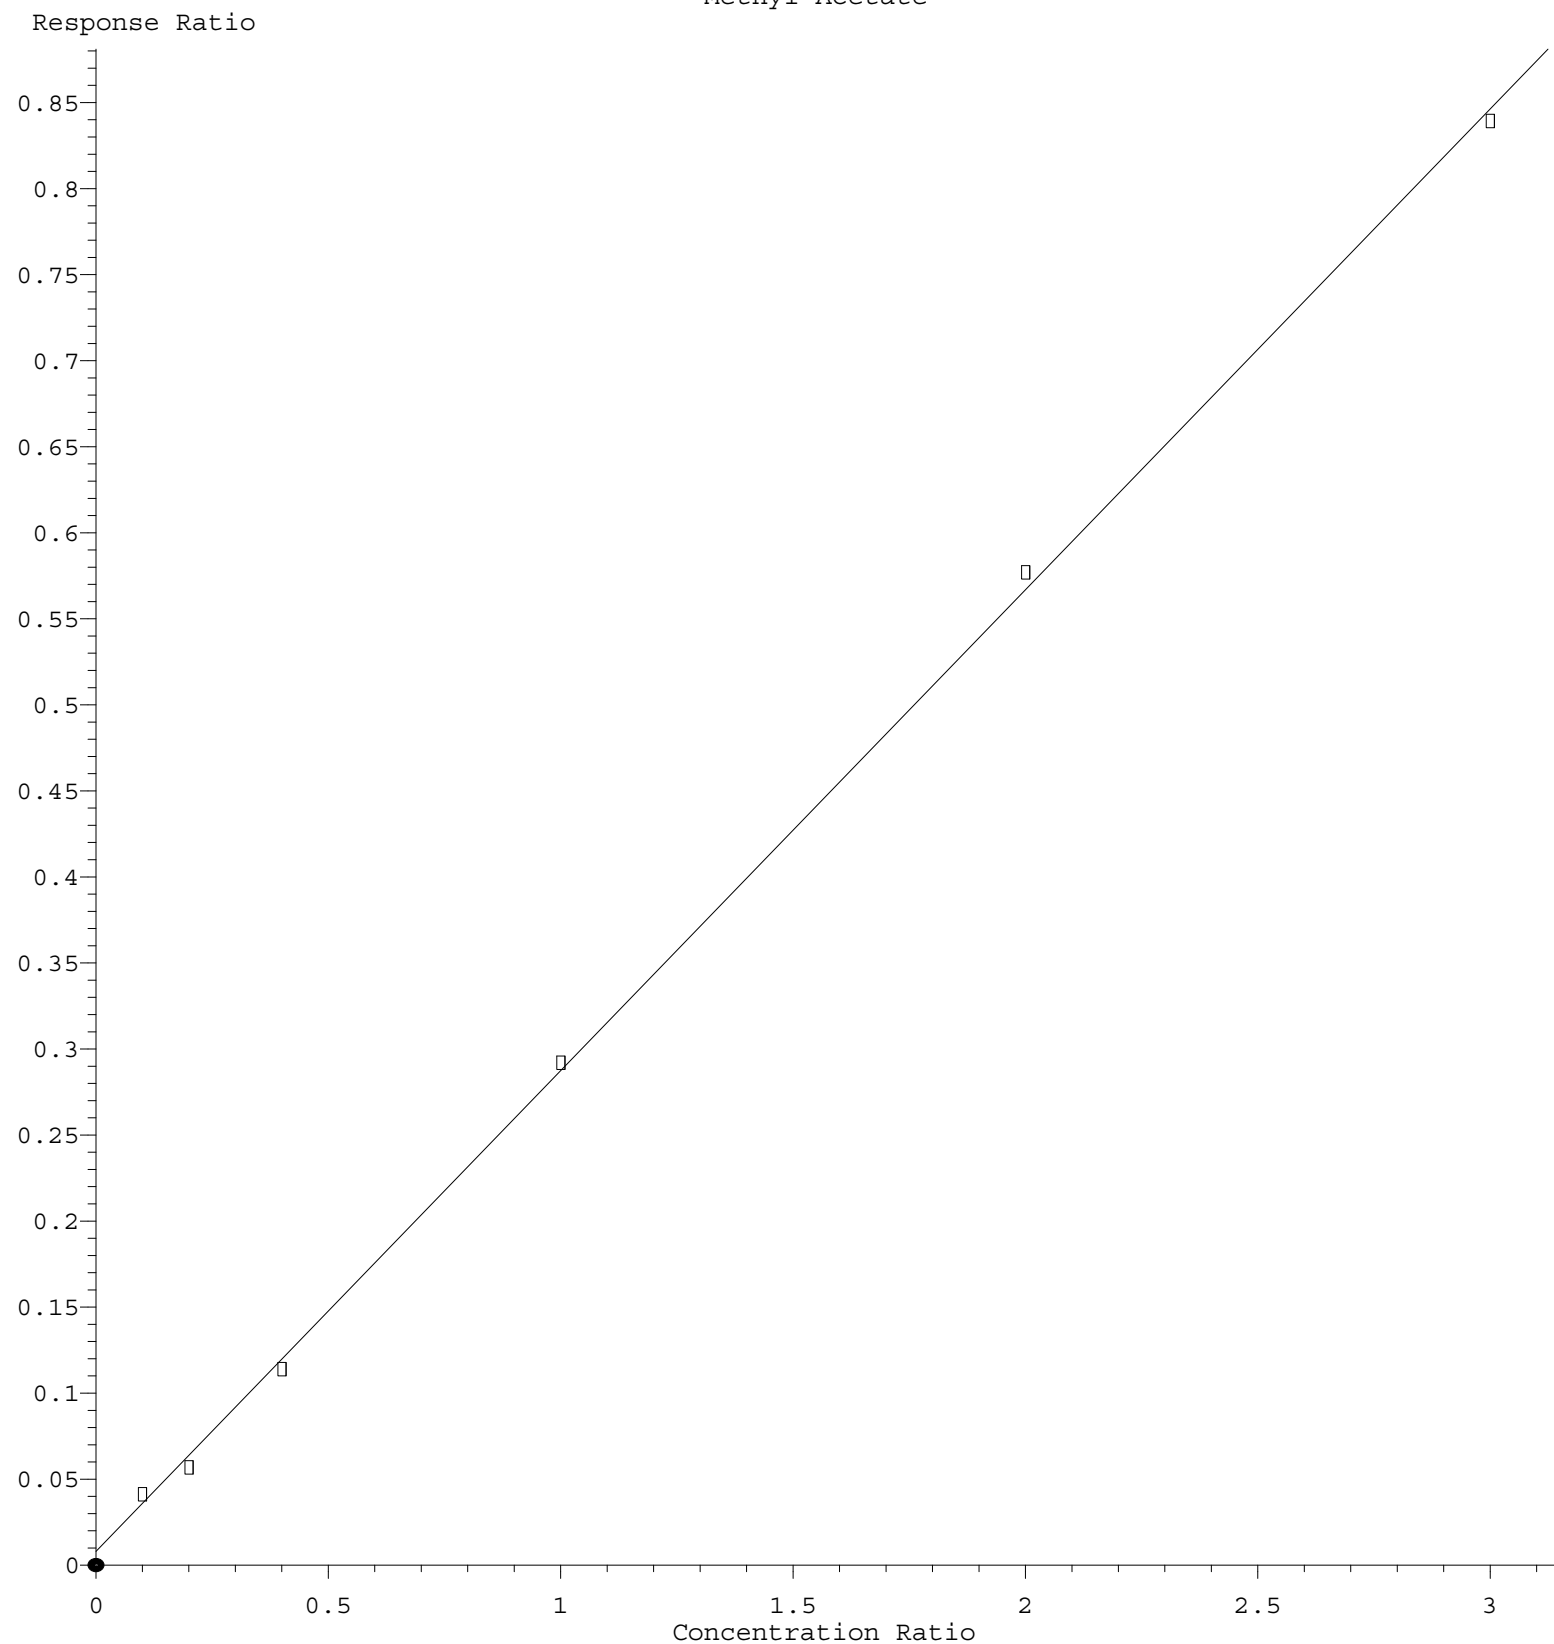

$$\text{Response} = 2.795\text{e-}001 * \text{Amt} + 7.888\text{e-}003$$


Coef of Det (r^2) = 0.999457 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D082322S.M

Calibration Table Last Updated: Tue Aug 23 13:12:17 2022

Methylene Chloride

Response Ratio

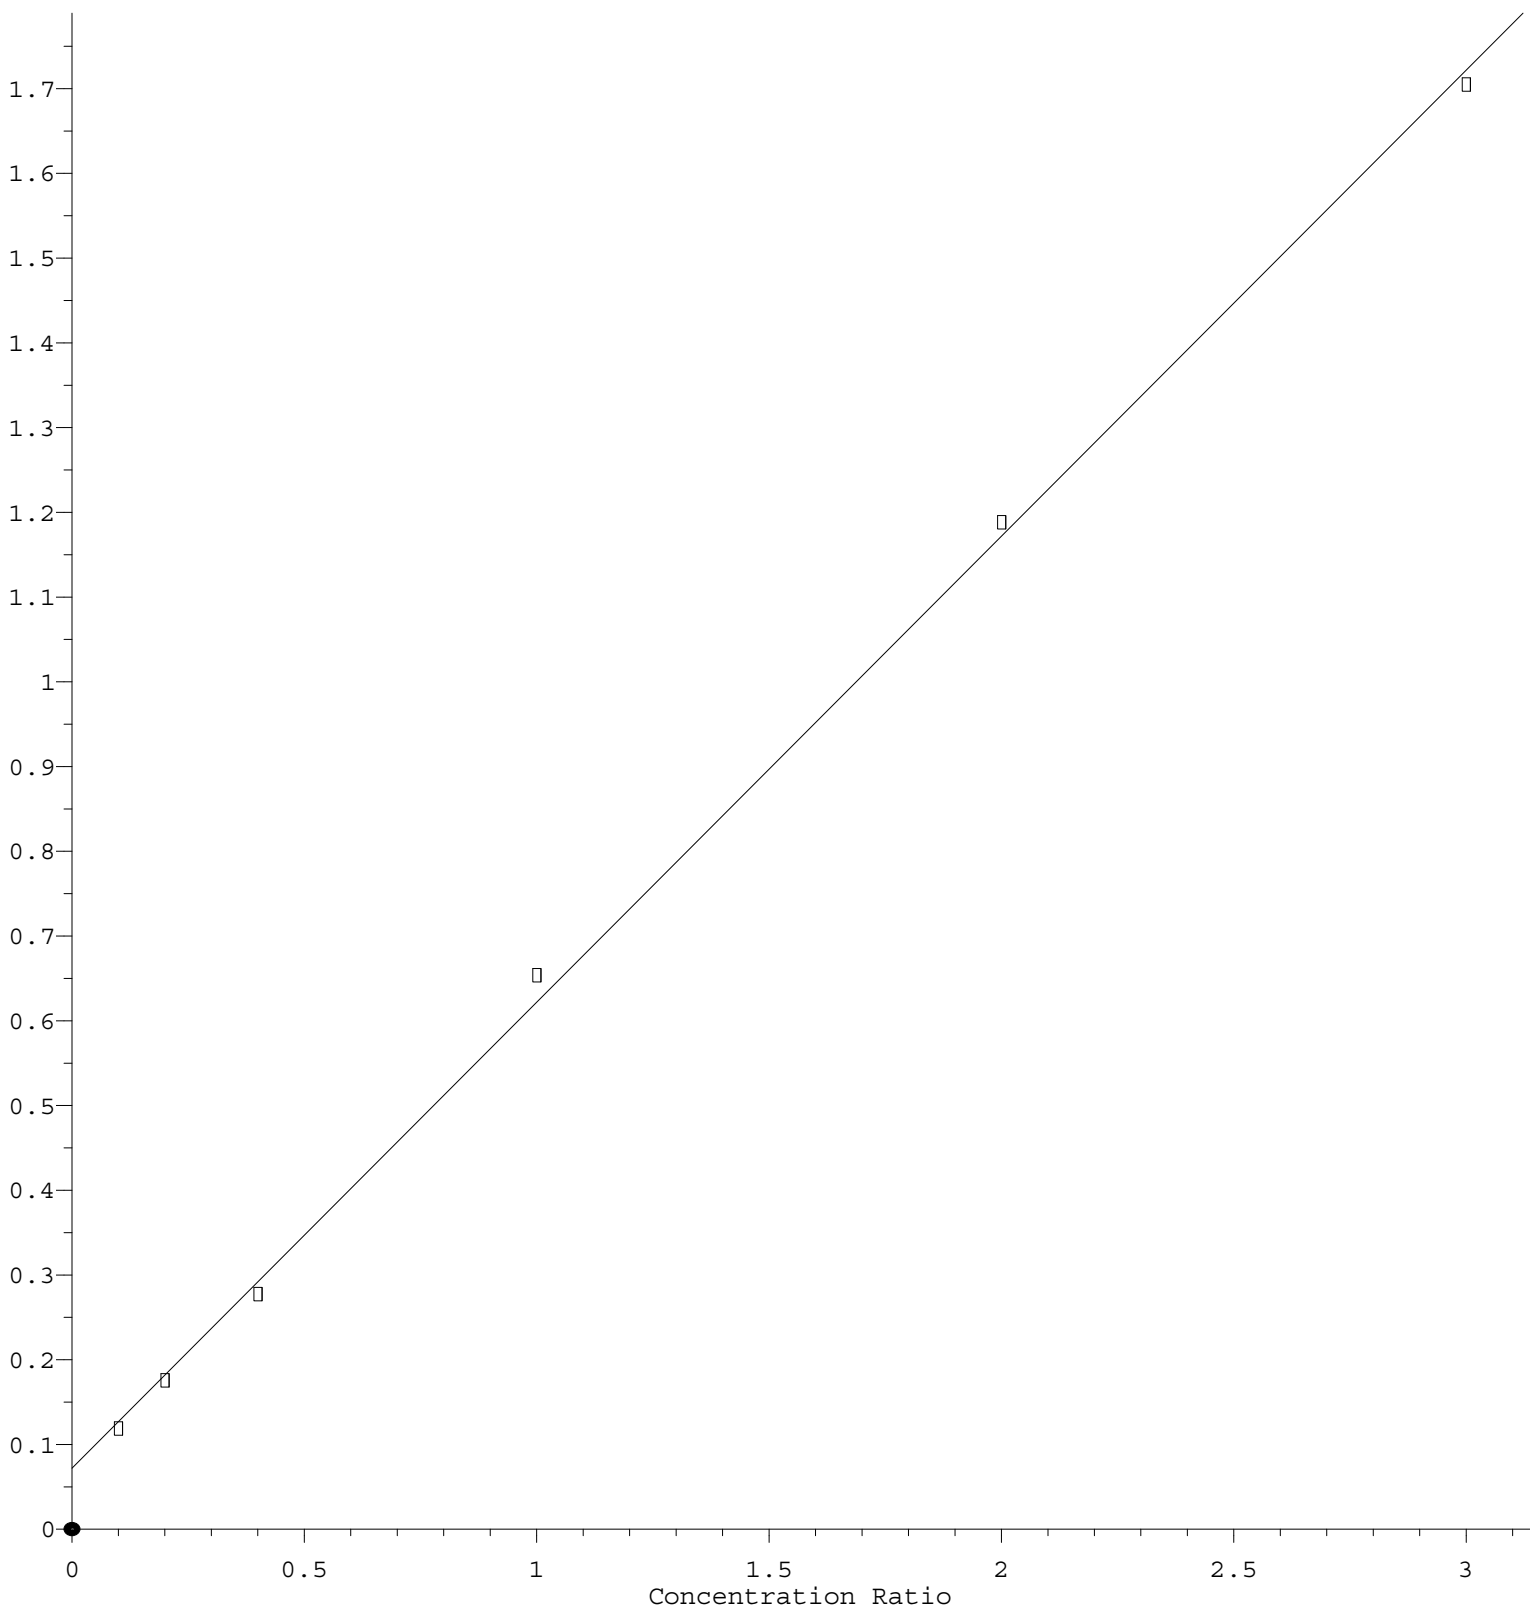

$$\text{Response} = 5.504\text{e-}001 * \text{Amt} + 7.174\text{e-}002$$


Coef of Det (r^2) = 0.999081 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D082322S.M

Calibration Table Last Updated: Tue Aug 23 13:12:17 2022

Vinyl Acetate

Response Ratio

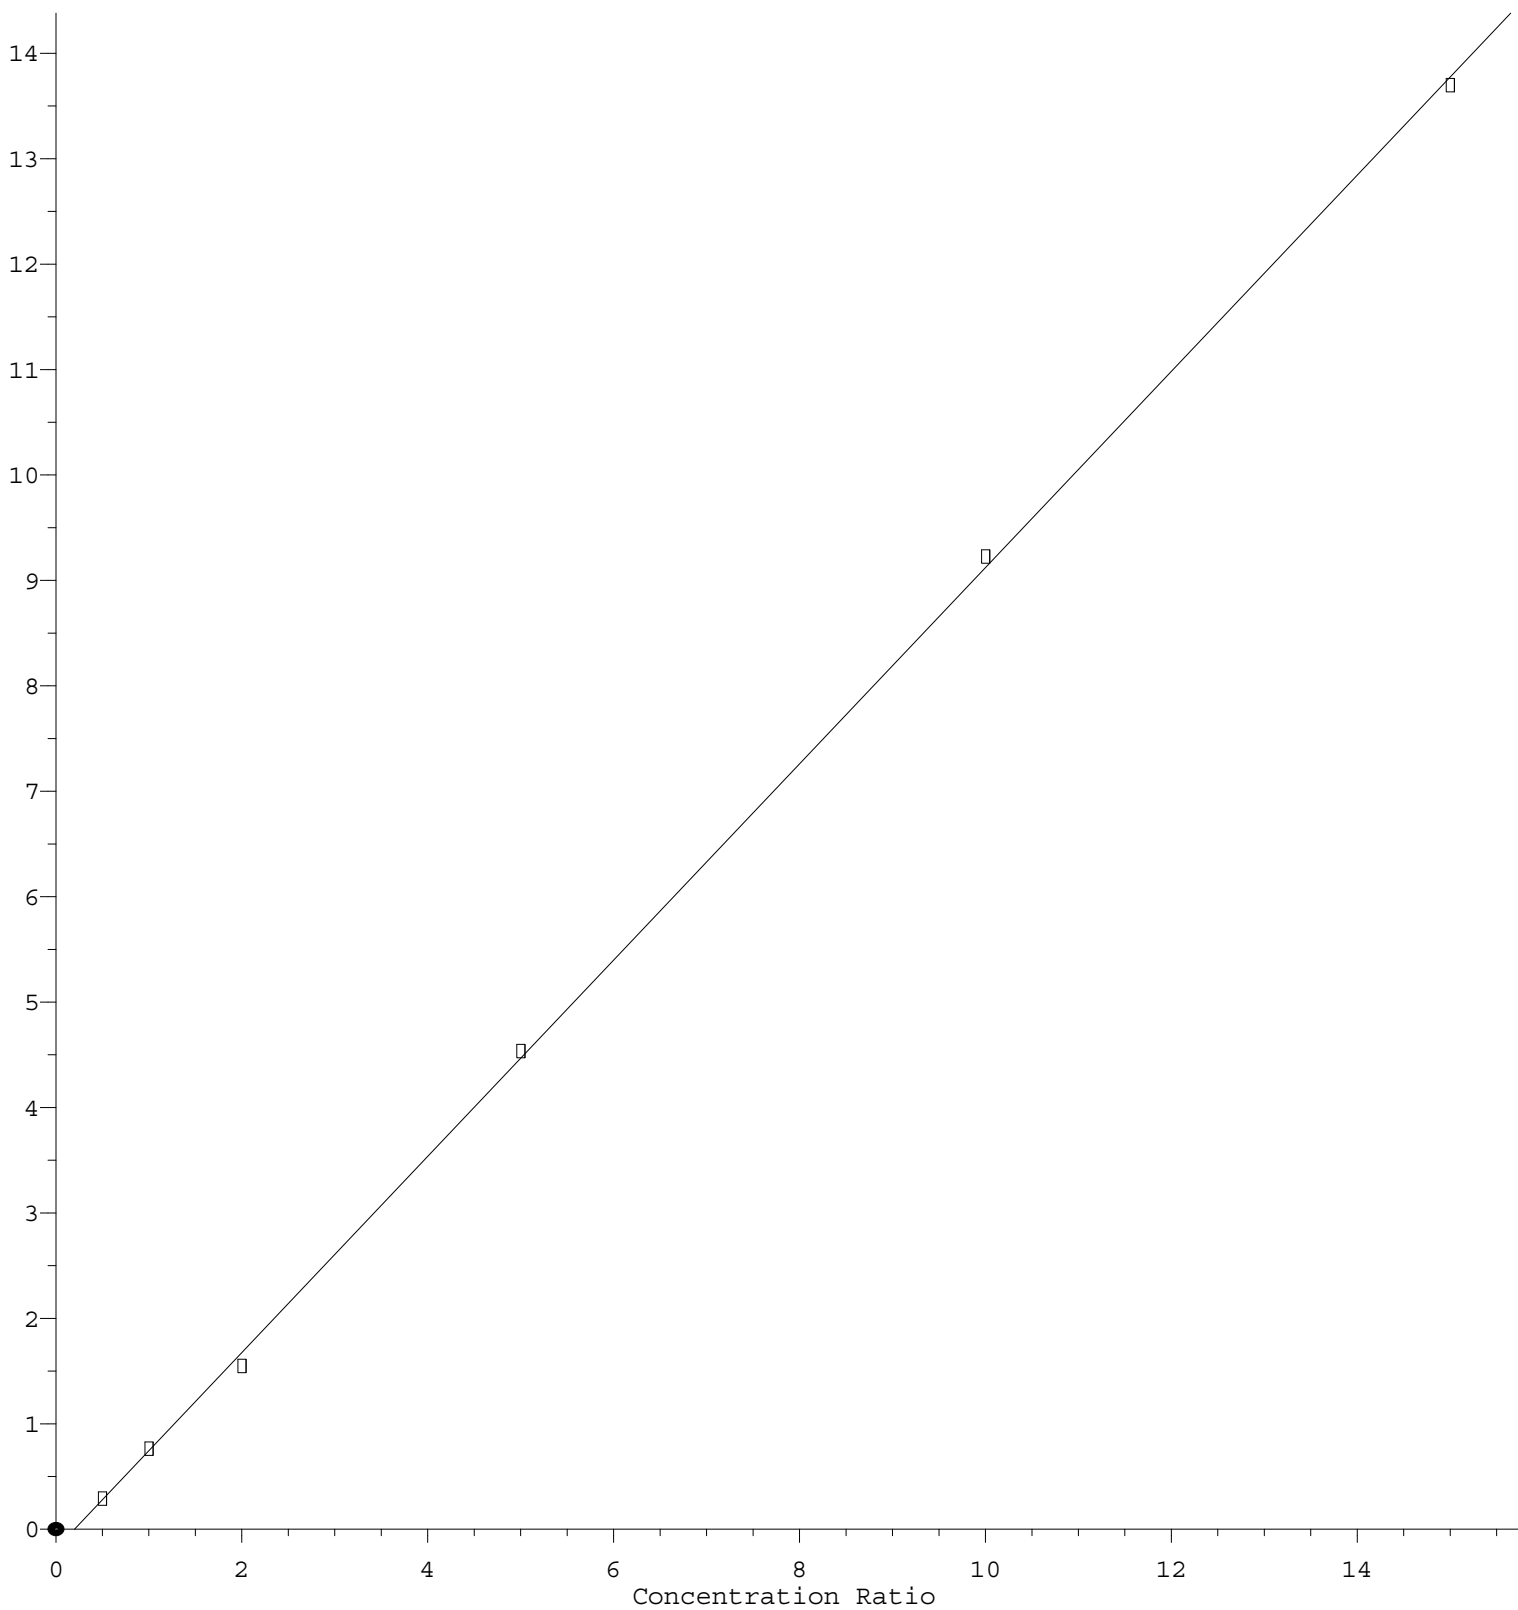

$$\text{Response} = 9.308\text{e-}001 * \text{Amt} - 1.875\text{e-}001$$


Coef of Det (r^2) = 0.999738 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D082322S.M

Calibration Table Last Updated: Tue Aug 23 13:12:17 2022

Methylcyclohexane

Response Ratio

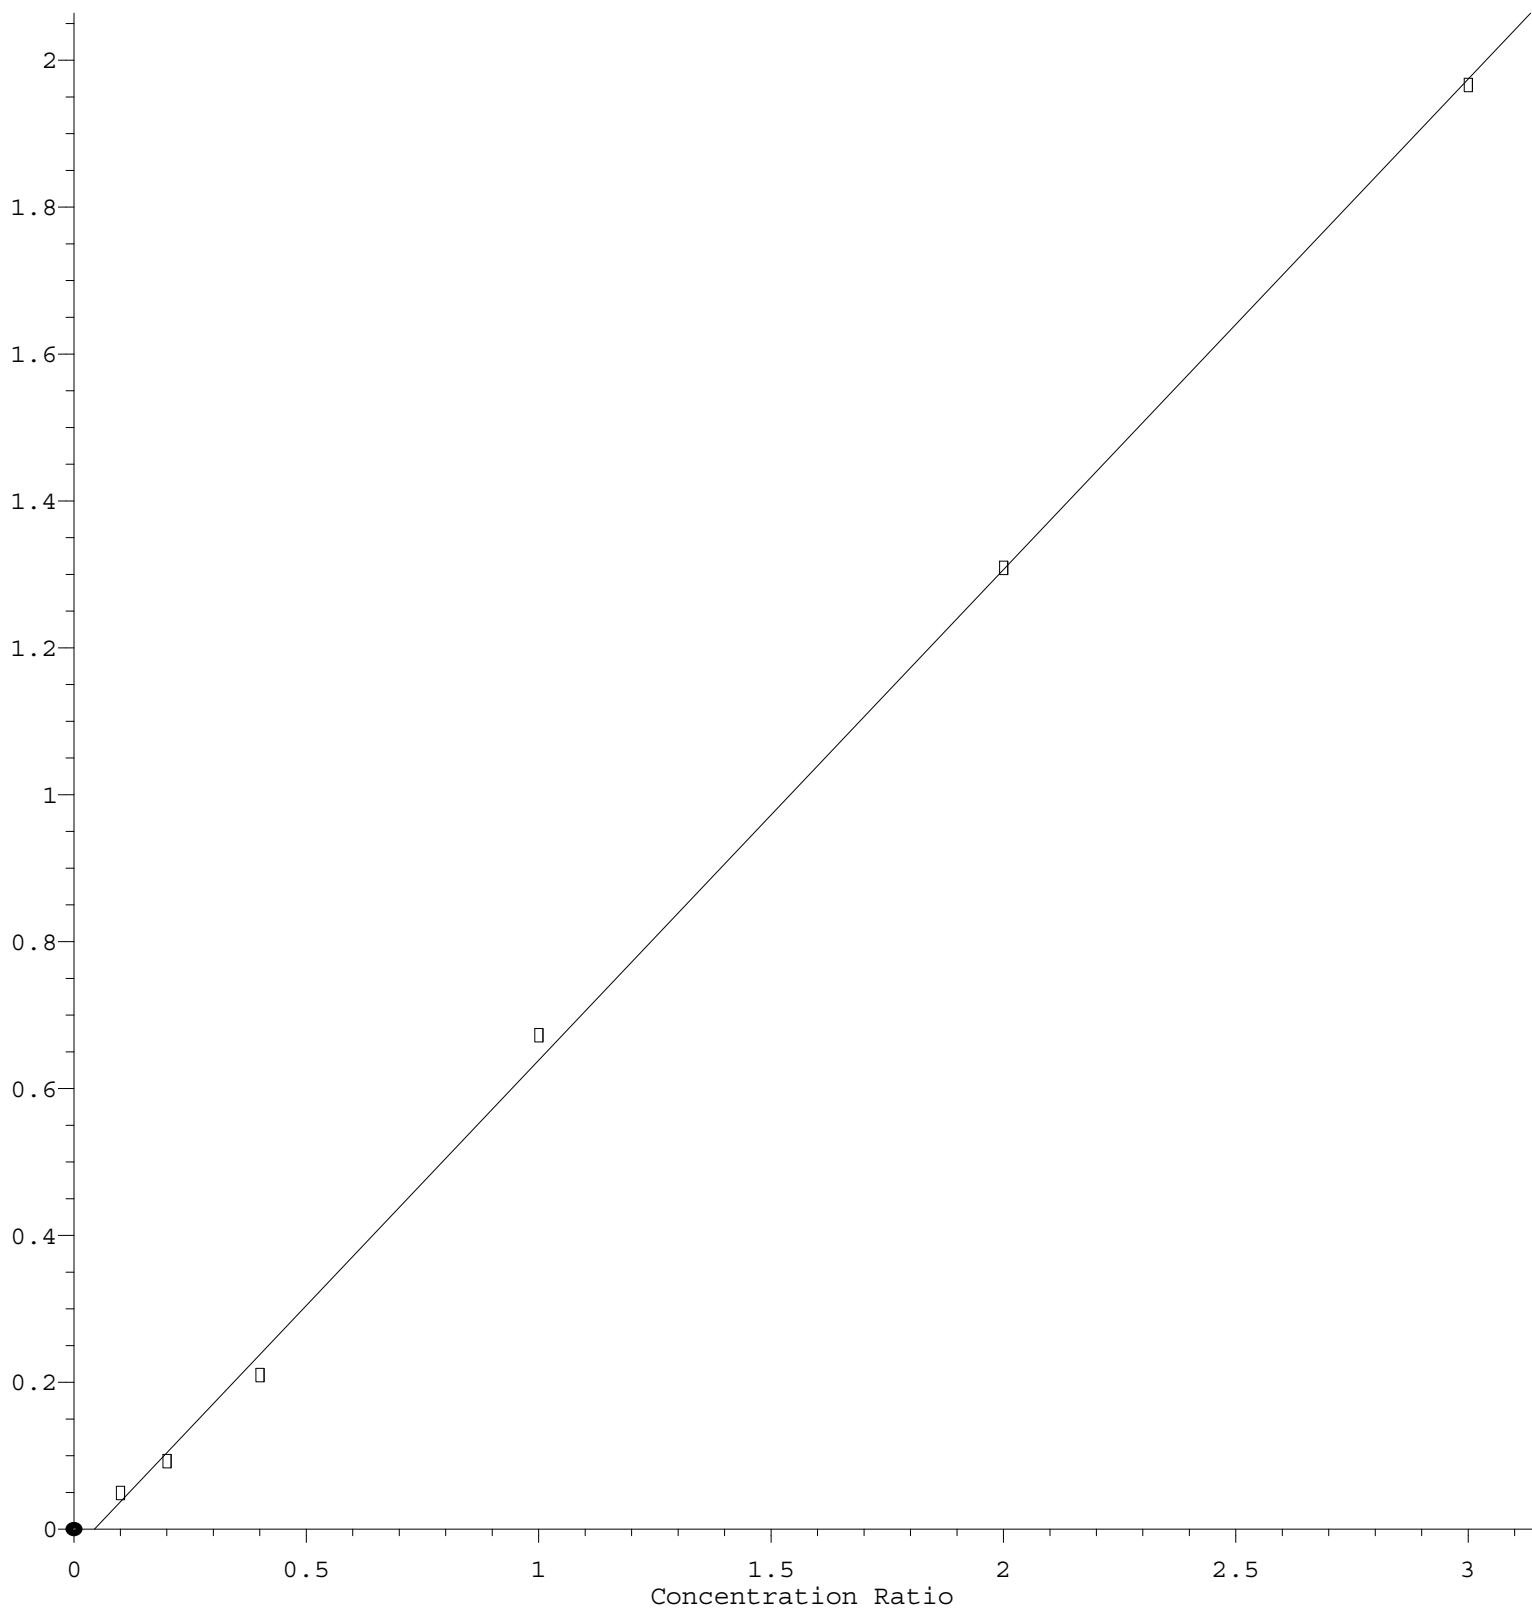

$$\text{Response} = 6.681\text{e-}001 * \text{Amt} - 2.960\text{e-}002$$


Coef of Det (r^2) = 0.999241 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D082322S.M

Calibration Table Last Updated: Tue Aug 23 13:12:17 2022

Naphthalene

Response Ratio

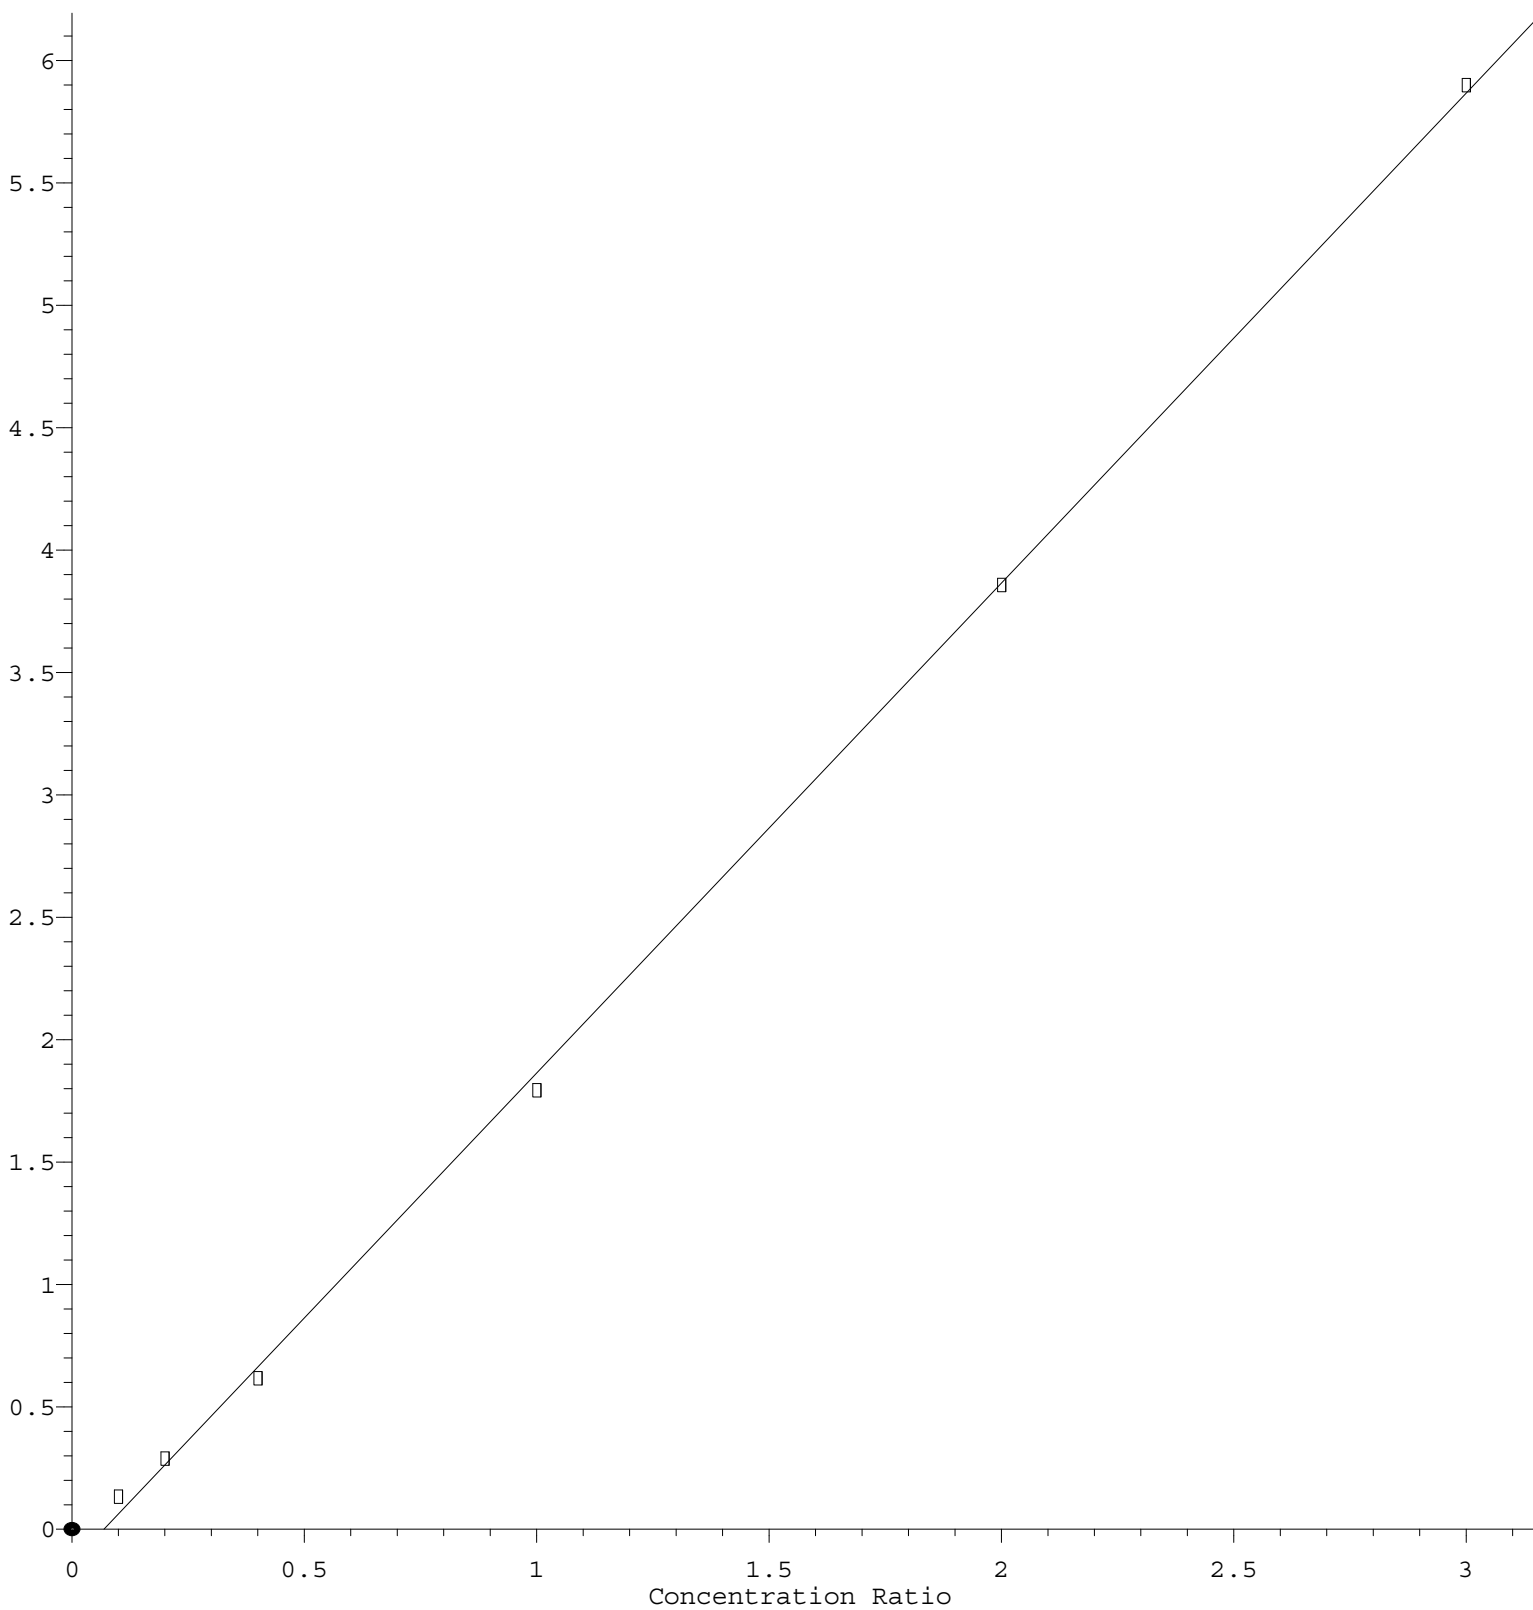

$$\text{Response} = 2.001\text{e}+000 * \text{Amt} - 1.372\text{e}-001$$

Coef of Det (r^2) = 0.999488 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D082322S.M

Calibration Table Last Updated: Tue Aug 23 13:12:17 2022