

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD082322\
 Data File : VD074186.D
 Acq On : 23 Aug 2022 13:07
 Operator : VA/SY
 Sample : VIBLK
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VIBLK

Quant Time: Aug 23 13:31:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D082322S.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 23 13:12:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.973	168	121461	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.855	114	265528	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.632	117	270353	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	132223	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.320	65	78841	63.523	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 127.040%			
35) Dibromofluoromethane	7.908	113	93215	52.484	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 104.960%			
50) Toluene-d8	10.332	98	323543	56.602	ug/l	0.00
Spiked Amount 50.000	Range 49 - 140		Recovery = 113.200%			
62) 4-Bromofluorobenzene	12.620	95	126745	56.127	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery = 112.260%			
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.997	85	1697	1.665	ug/l	91
3) Chloromethane	2.209	50	1637	2.254	ug/l #	80
4) Vinyl Chloride	2.344	62	1106	1.451	ug/l	100
5) Bromomethane	2.773	94	895	1.818	ug/l #	59
6) Chloroethane	2.915	64	905	1.829	ug/l #	42
7) Trichlorofluoromethane	3.267	101	3134	1.415	ug/l #	81
9) 1,1,2-Trichlorotrifluo...	4.091	101	1987	1.483	ug/l #	81
10) Methyl Iodide	4.297	142	1514	2.053	ug/l #	86
11) Tert butyl alcohol	5.226	59	419	5.421	ug/l #	74
12) 1,1-Dichloroethene	4.067	96	2167	1.808	ug/l #	47
14) Allyl chloride	4.709	41	1947	1.038	ug/l	94
16) Acetone	4.173	43	1242	5.252	ug/l #	47
17) Carbon Disulfide	4.409	76	8844	4.208	ug/l	100
18) Methyl Acetate	4.720	43	70	Below Cal	#	55
20) Methylene Chloride	4.962	84	11914	2.393	ug/l #	83
21) trans-1,2-Dichloroethene	5.467	96	1761	1.257	ug/l	85
23) Vinyl Acetate	6.291	43	1628	10.793	ug/l #	75
25) 2-Butanone	7.197	43	1849	5.051	ug/l #	52
26) 2,2-Dichloropropane	7.197	77	4301	1.882	ug/l #	73
29) Tetrahydrofuran	7.556	42	391	1.770	ug/l #	53
31) Cyclohexane	7.973	56	5410	2.449	ug/l #	22
32) 1,1,1-Trichloroethane	7.897	97	3134	1.264	ug/l #	44
39) Methylcyclohexane	9.355	83	3835	3.296	ug/l #	78
48) Methyl methacrylate	9.350	41	2094	2.128	ug/l #	70
51) 4-Methyl-2-Pentanone	10.214	43	4630	4.353	ug/l	97
59) 2-Hexanone	10.979	43	2110	2.942	ug/l	93
64) Tetrachloroethene	10.873	164	2164	1.097	ug/l #	67
68) m/p-Xylenes	11.844	106	4911	1.223	ug/l	88
76) 1,2,3-Trichloropropane	12.620	75	63988	49.562	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.620	75	63988	127.457	ug/l #	7
95) Naphthalene	15.373	128	3819	4.149	ug/l #	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD082322\
Data File : VD074186.D
Acq On : 23 Aug 2022 13:07
Operator : VA/SY
Sample : VIBLK
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VIBLK

Quant Time: Aug 23 13:31:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D082322S.M
Quant Title : SW846 8260
QLast Update : Tue Aug 23 13:12:17 2022
Response via : Initial Calibration




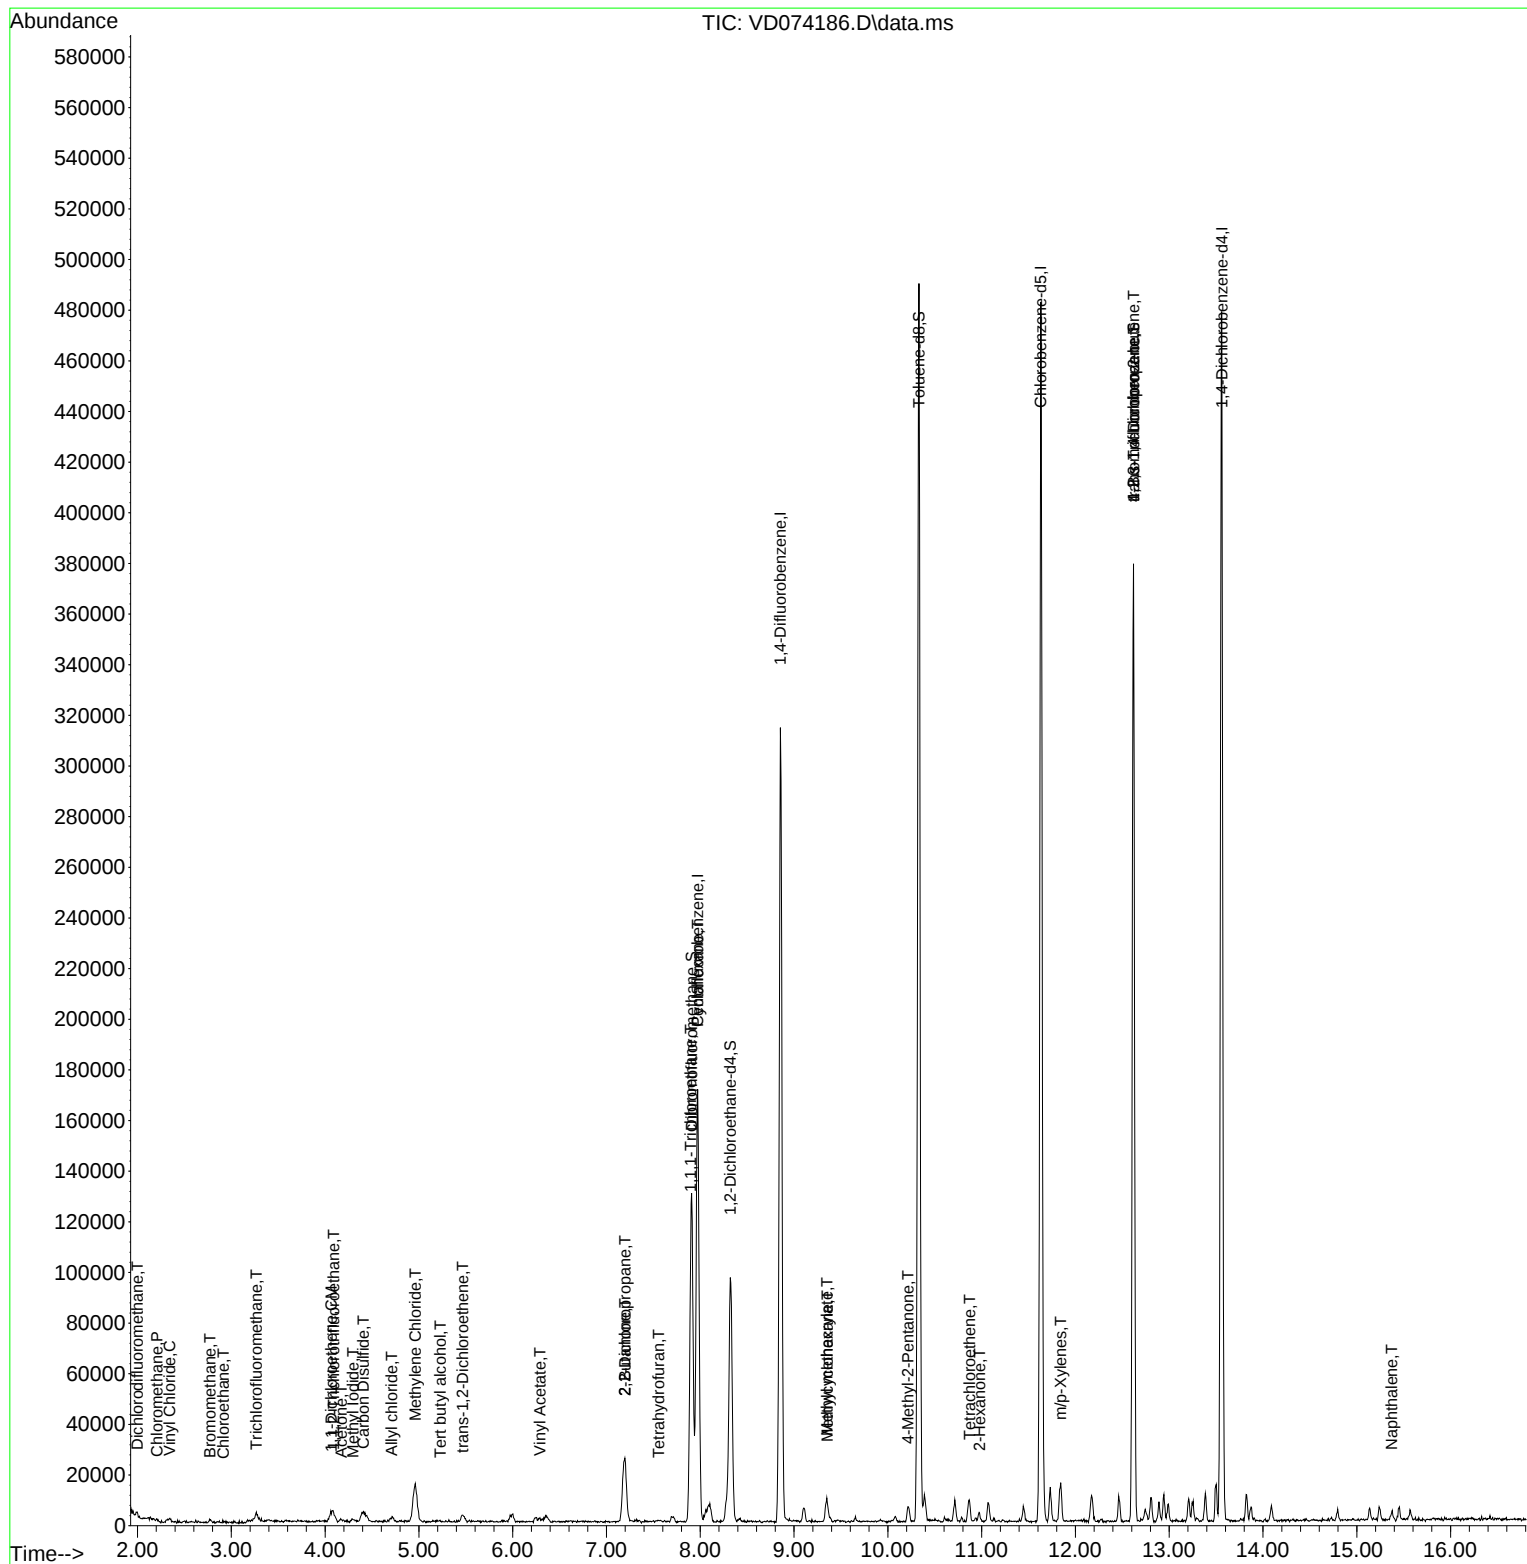




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.973 min Scan# 10
Delta R.T. 0.000 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07




Instrument :
MSVOA_D
ClientSampleId :
VIBLK


Tgt Ion:168 Resp: 121461
Ion Ratio Lower Upper
168 100
99 58.2 49.8 74.6

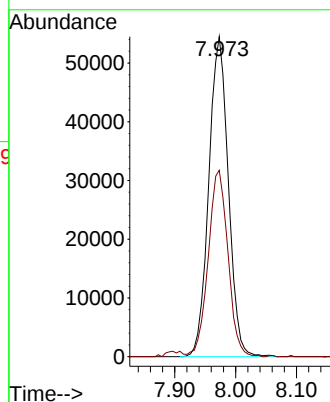

#2
Dichlorodifluoromethane
Concen: 1.665 ug/l
RT: 1.997 min Scan# 13
Delta R.T. 0.006 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07

Tgt Ion: 85 Resp: 1697
Ion Ratio Lower Upper
85 100
87 26.4 15.7 47.0


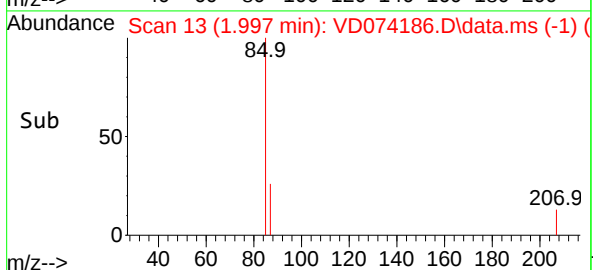
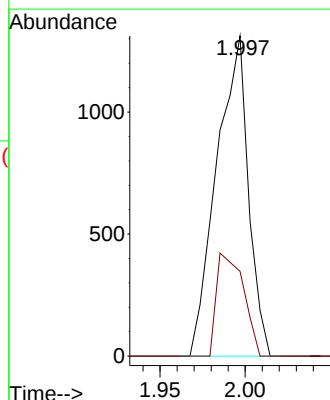
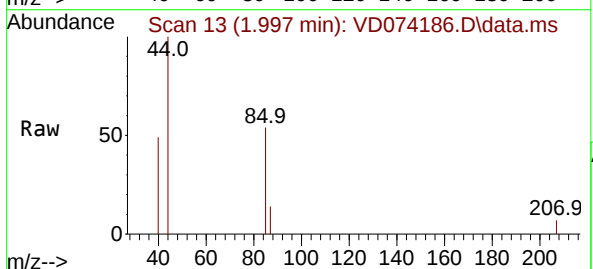


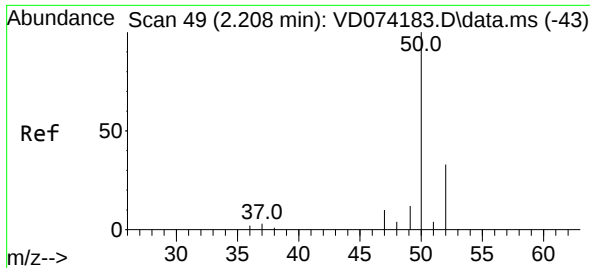

#3
Chloromethane
Concen: 2.254 ug/l
RT: 2.209 min Scan# 49
Delta R.T. 0.001 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07




Instrument :
MSVOA_D
ClientSampleId :
VIBLK


Tgt Ion: 50 Resp: 1637
Ion Ratio Lower Upper
50 100
52 45.5 27.4 41.0#

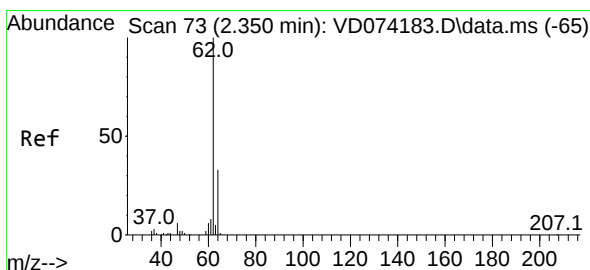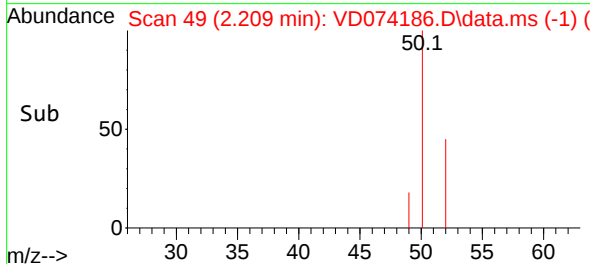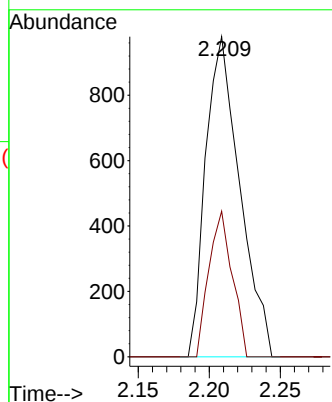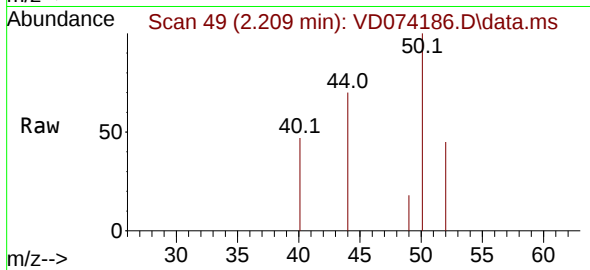

#4
Vinyl Chloride
Concen: 1.451 ug/l
RT: 2.344 min Scan# 72
Delta R.T. -0.006 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07

Tgt Ion: 62 Resp: 1106
Ion Ratio Lower Upper
62 100
64 31.8 25.4 38.0


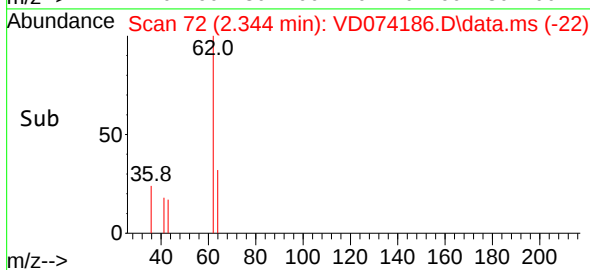
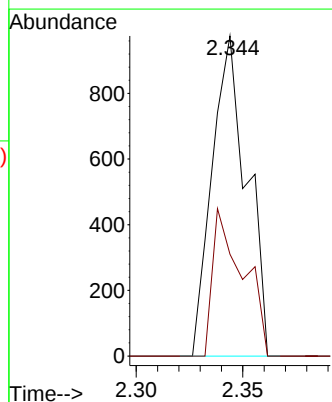
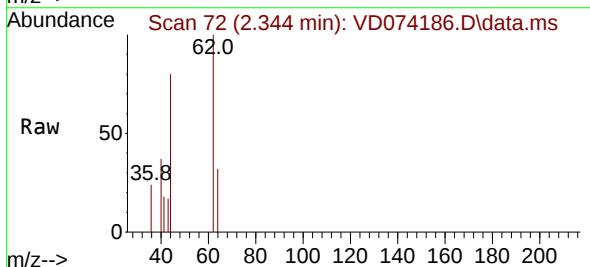




#5
Bromomethane
Concen: 1.818 ug/l
RT: 2.773 min Scan# 144
Delta R.T. 0.006 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07




Instrument :
MSVOA_D
ClientSampleId :
VIBLK


Tgt Ion: 94 Resp: 895
Ion Ratio Lower Upper
94 100
96 56.9 77.6 116.4#

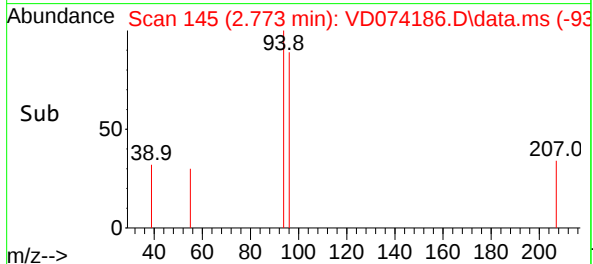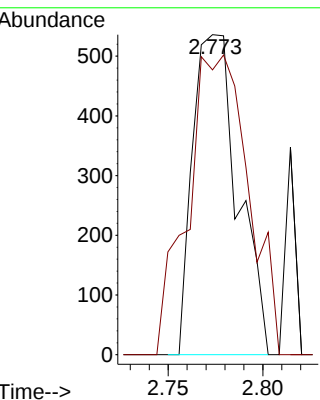

#6
Chloroethane
Concen: 1.829 ug/l
RT: 2.915 min Scan# 169
Delta R.T. 0.001 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07

Tgt Ion: 64 Resp: 905
Ion Ratio Lower Upper
64 100
66 0.0 25.9 38.9#


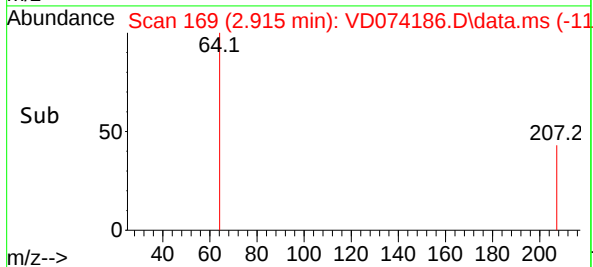
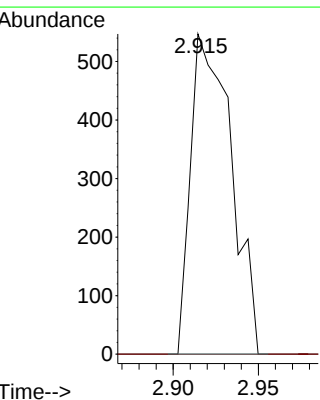
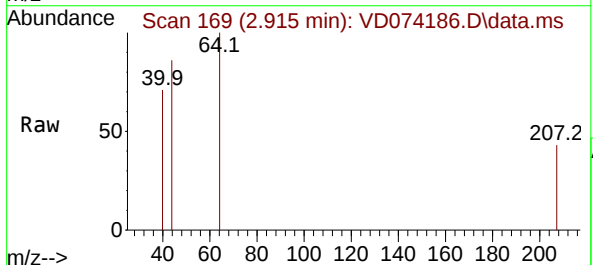




#7
 Trichlorofluoromethane
 Concen: 1.415 ug/l
 RT: 3.267 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VD074186.D
 Acq: 23 Aug 2022 13:07




Instrument :
 MSVOA_D
 ClientSampleId :
 VIBLK


Tgt Ion:101 Resp: 3134
 Ion Ratio Lower Upper
 101 100
 103 77.6 50.1 75.1#

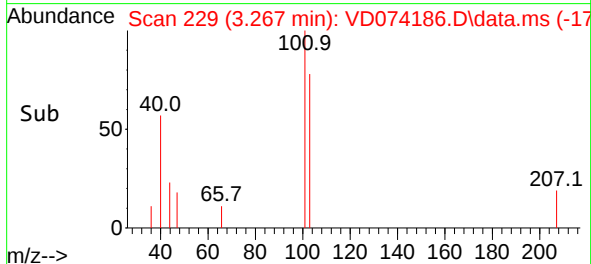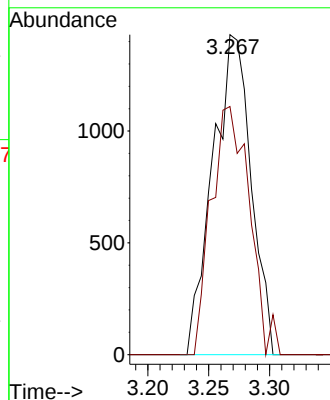

#9
 1,1,2-Trichlorotrifluoroethane
 Concen: 1.483 ug/l
 RT: 4.091 min Scan# 369
 Delta R.T. -0.000 min
 Lab File: VD074186.D
 Acq: 23 Aug 2022 13:07

Tgt Ion:101 Resp: 1987
 Ion Ratio Lower Upper
 101 100
 85 14.4 36.4 54.6#
 151 72.6 57.3 85.9


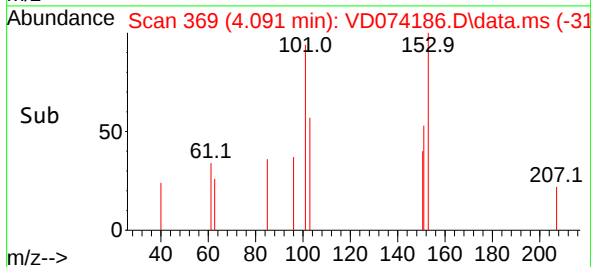
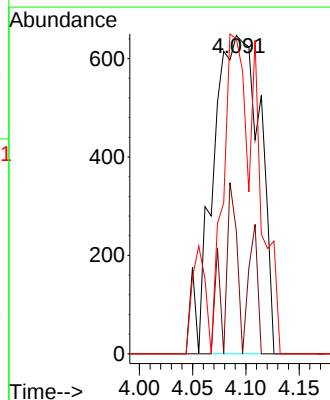
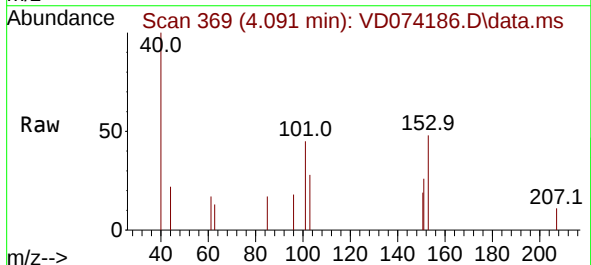




#10
Methyl Iodide
Concen: 2.053 ug/l
RT: 4.297 min Scan# 403
Delta R.T. 0.006 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07




Instrument :
MSVOA_D
ClientSampleId :
VIBLK


Tgt Ion:142 Resp: 1514
Ion Ratio Lower Upper
142 100
127 40.0 37.3 55.9
141 3.9 11.7 17.5#

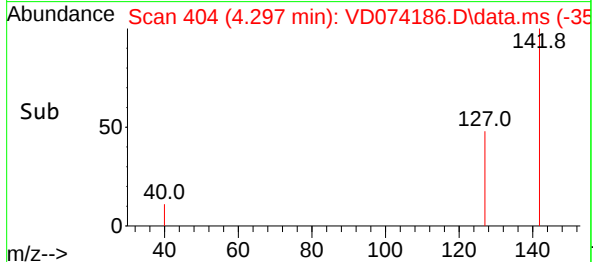

#11
Tert butyl alcohol
Concen: 5.421 ug/l
RT: 5.226 min Scan# 562
Delta R.T. -0.006 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07

Tgt Ion: 59 Resp: 419
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.6#


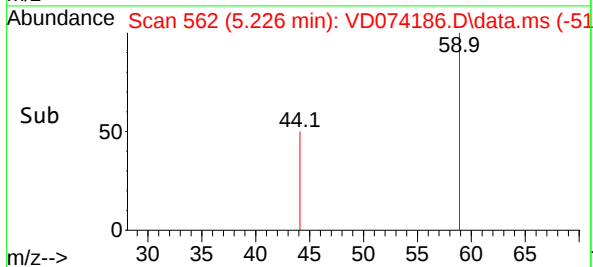

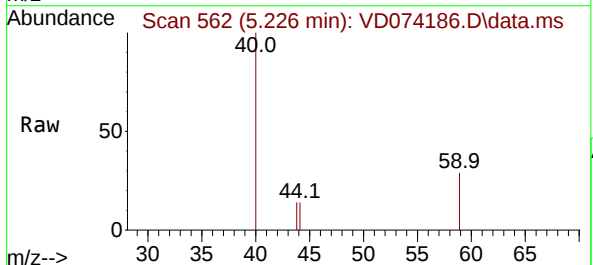




#12
1,1-Dichloroethene
Concen: 1.808 ug/l
RT: 4.067 min Scan# 30
Delta R.T. 0.006 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07




Instrument :
MSVOA_D
ClientSampleId :
VIBLK


Tgt Ion: 96 Resp: 2167
Ion Ratio Lower Upper
96 100
61 93.3 138.5 207.7#
98 29.5 48.6 73.0#

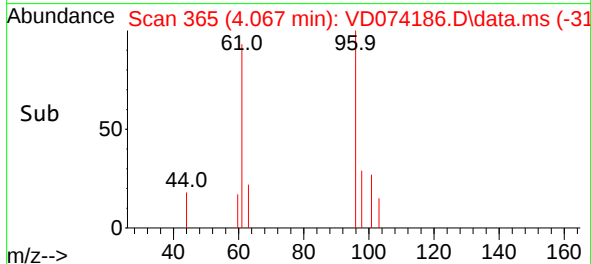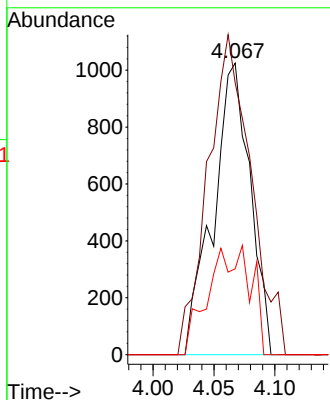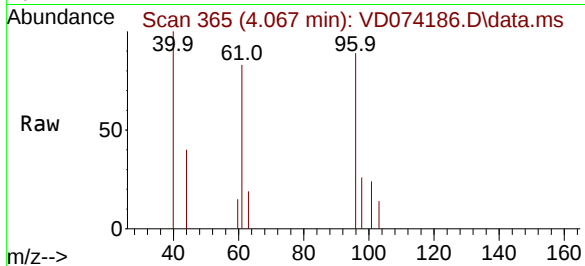

#14
Allyl chloride
Concen: 1.038 ug/l
RT: 4.709 min Scan# 474
Delta R.T. 0.001 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07

Tgt Ion: 41 Resp: 1947
Ion Ratio Lower Upper
41 100
39 77.8 59.3 88.9
76 36.9 25.7 38.5

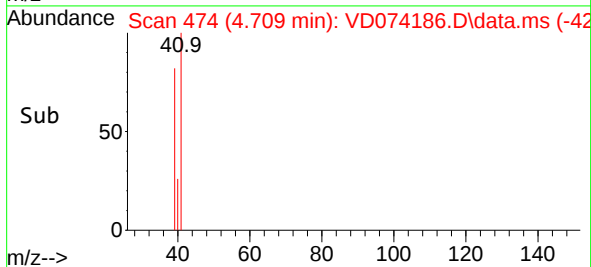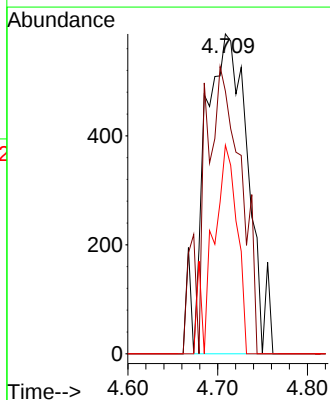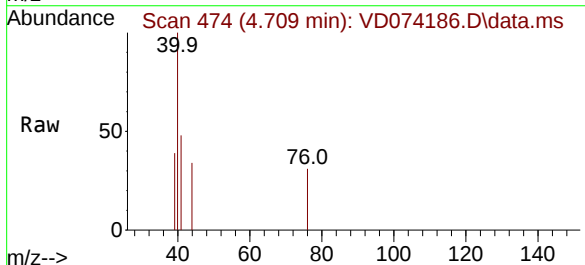



#16

Acetone

Concen: 5.252 ug/l

RT: 4.173 min Scan# 380

Delta R.T. 0.018 min

Lab File: VD074186.D

Acq: 23 Aug 2022 13:07

Instrument :

MSVOA_D

ClientSampleId :





VIBLK

Tgt Ion: 43 Resp: 1242

Ion Ratio Lower Upper

43 100

58 0.0 22.1 33.1#

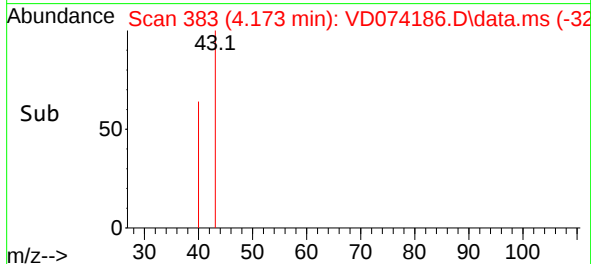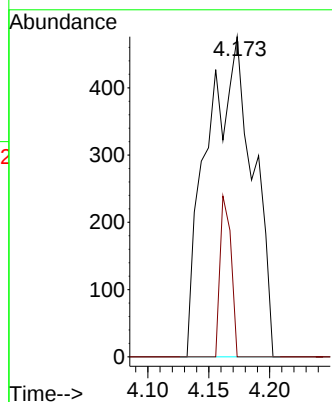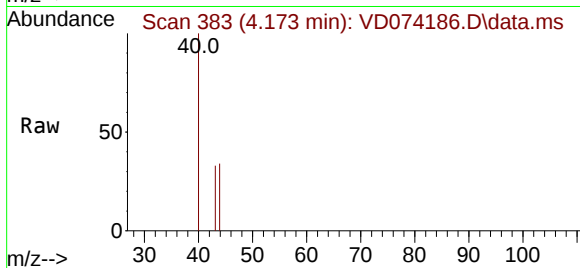

#17

Carbon Disulfide

Concen: 4.208 ug/l

RT: 4.409 min Scan# 423

Delta R.T. 0.007 min

Lab File: VD074186.D




Acq: 23 Aug 2022 13:07


Tgt Ion: 76 Resp: 8844

Ion Ratio Lower Upper

76 100

78 9.4 7.5 11.3




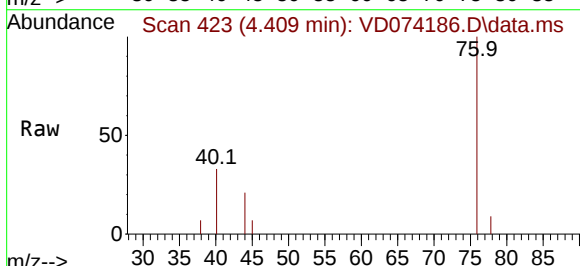




#18
Methyl Acetate
Concen: Below Cal
RT: 4.720 min Scan# 41
Delta R.T. 0.000 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07




Instrument :
MSVOA_D
ClientSampleId :
VIBLK


Tgt Ion: 43 Resp: 70
Ion Ratio Lower Upper
43 100
74 0.0 16.7 25.1#

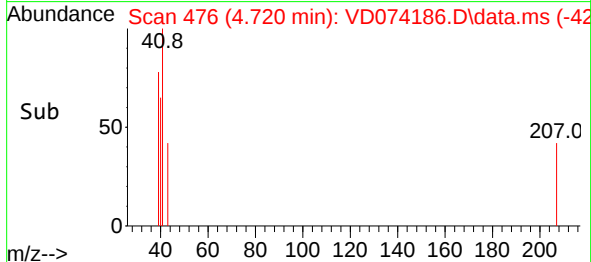

#20
Methylene Chloride
Concen: 2.393 ug/l
RT: 4.962 min Scan# 517
Delta R.T. 0.007 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07

Tgt Ion: 84 Resp: 11914
Ion Ratio Lower Upper
84 100
49 112.3 112.8 169.2#
51 35.7 32.6 48.8
86 65.0 47.9 71.9


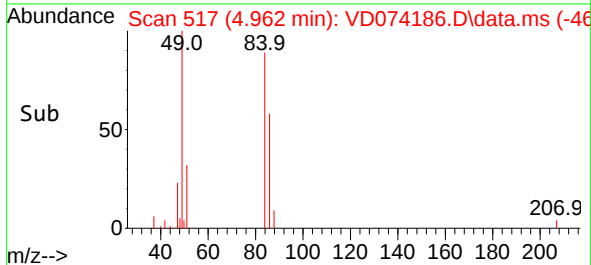

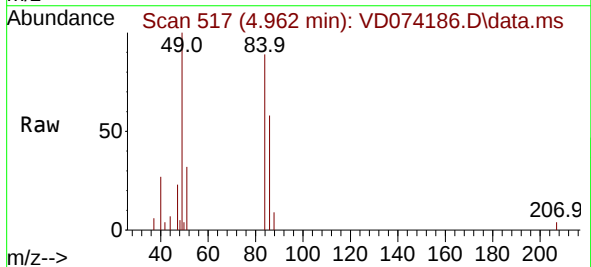




#21
trans-1,2-Dichloroethene
Concen: 1.257 ug/l
RT: 5.467 min Scan# 603
Delta R.T. 0.000 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07




Instrument :
MSVOA_D
ClientSampleId :
VIBLK


Tgt Ion: 96 Resp: 1761
Ion Ratio Lower Upper
96 100
61 121.7 117.9 176.9
98 63.6 49.4 74.2

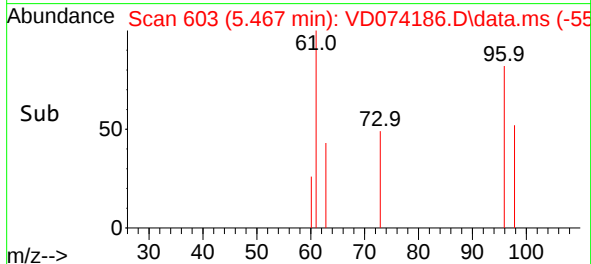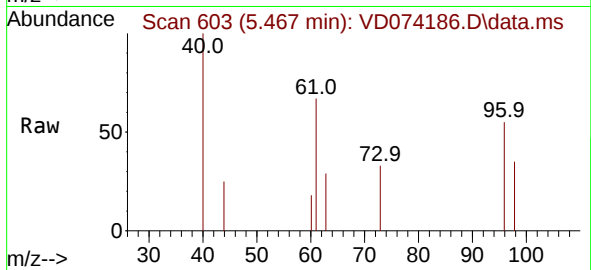

#23
Vinyl Acetate
Concen: 10.793 ug/l
RT: 6.291 min Scan# 743
Delta R.T. -0.011 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07

Tgt Ion: 43 Resp: 1628
Ion Ratio Lower Upper
43 100
86 0.0 7.1 10.7#




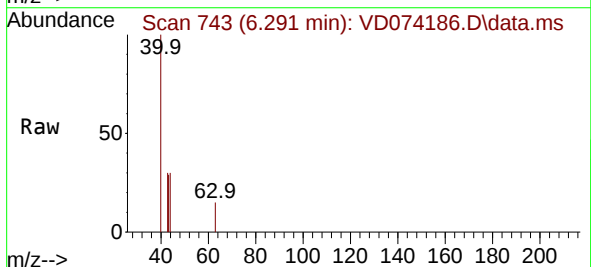




#25
2-Butanone
Concen: 5.051 ug/l
RT: 7.197 min Scan# 897
Delta R.T. -0.011 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07




Instrument :
MSVOA_D
ClientSampleId :
VIBLK


Tgt Ion: 43 Resp: 1849
Ion Ratio Lower Upper
43 100
72 0.0 18.6 27.8#

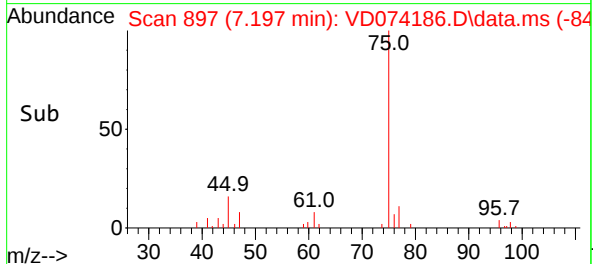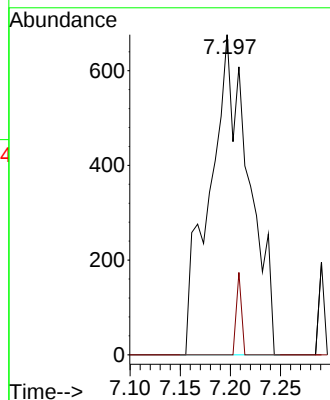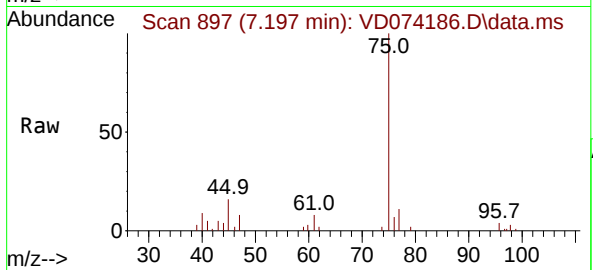

#26
2,2-Dichloropropane
Concen: 1.882 ug/l
RT: 7.197 min Scan# 897
Delta R.T. -0.005 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07

Tgt Ion: 77 Resp: 4301
Ion Ratio Lower Upper
77 100
97 8.9 10.8 32.4#

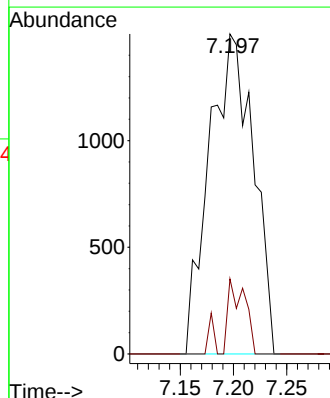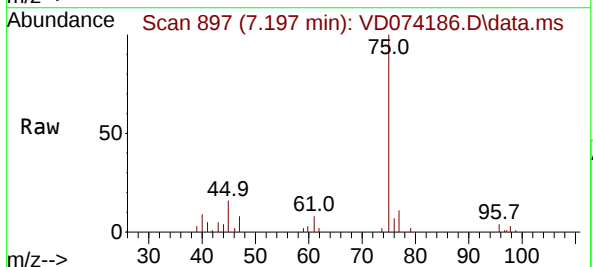



#29

Tetrahydrofuran

Concen: 1.770 ug/l

RT: 7.556 min Scan# 91

Delta R.T. -0.005 min

Lab File: VD074186.D

Acq: 23 Aug 2022 13:07

Instrument :

MSVOA_D

ClientSampleId :

VIBLK





Tgt Ion: 42 Resp: 391

Ion Ratio Lower Upper

42 100

72 18.2 30.7 46.1#

71 0.0 28.6 43.0#

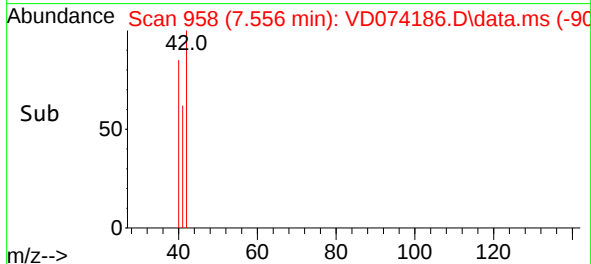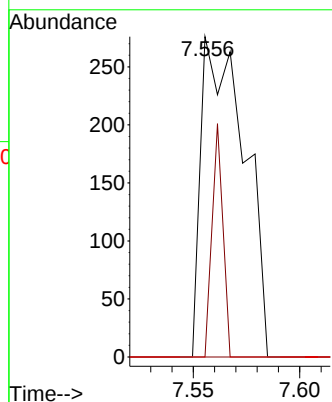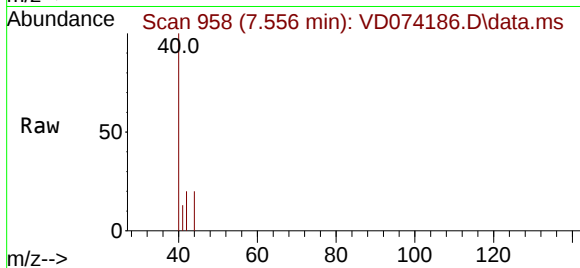

#31

Cyclohexane

Concen: 2.449 ug/l

RT: 7.973 min Scan# 1029

Delta R.T. -0.006 min

Lab File: VD074186.D

Acq: 23 Aug 2022 13:07




Tgt Ion: 56 Resp: 5410


Ion Ratio Lower Upper

56 100

69 107.1 25.4 38.2#

84 126.9 63.0 94.4#

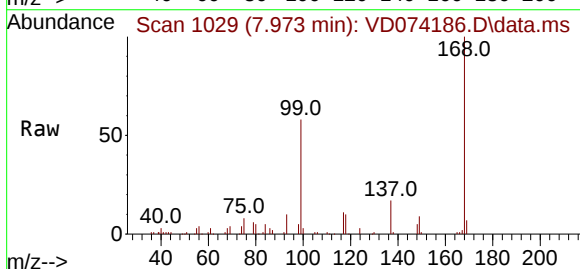



#32

1,1,1-Trichloroethane

Concen: 1.264 ug/l

RT: 7.897 min Scan# 1016

Delta R.T. 0.001 min

Lab File: VD074186.D

Acq: 23 Aug 2022 13:07

Instrument :

MSVOA_D

ClientSampleId :

VIBLK





Tgt Ion: 97 Resp: 3134

Ion Ratio Lower Upper

97 100

99 0.0 52.4 78.6#

61 35.1 38.0 57.0#

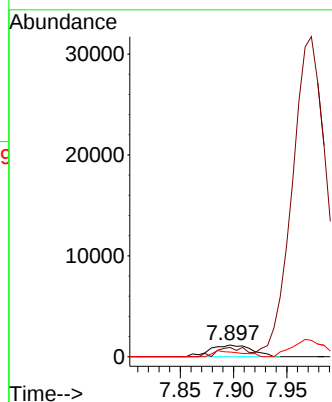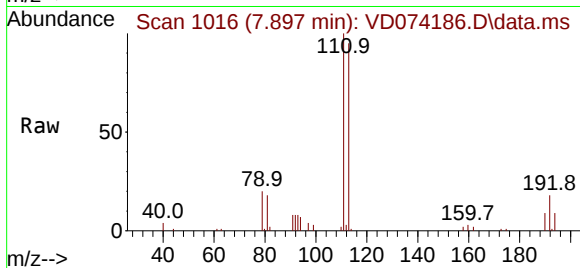

#33

1,2-Dichloroethane-d4

Concen: 63.523 ug/l

RT: 8.320 min Scan# 1088

Delta R.T. -0.006 min

Lab File: VD074186.D




Acq: 23 Aug 2022 13:07


Tgt Ion: 65 Resp: 78841

Ion Ratio Lower Upper

65 100

67 51.1 0.0 101.4

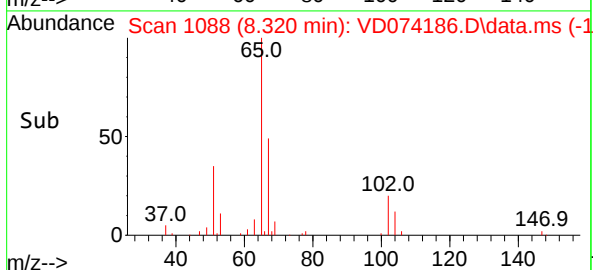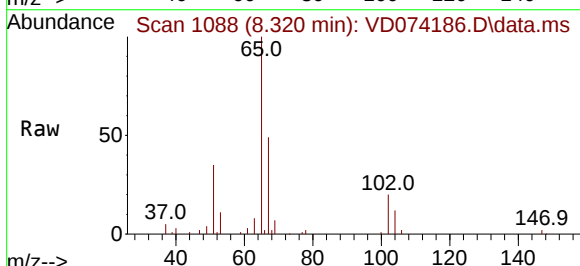



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.855 min Scan# 1179

Delta R.T. -0.006 min

Lab File: VD074186.D

Acq: 23 Aug 2022 13:07

Instrument :

MSVOA_D

ClientSampleId :

VIBLK





Tgt Ion:114 Resp: 265528

Ion Ratio Lower Upper

114 100

63 19.4 0.0 46.6

88 16.4 0.0 33.2

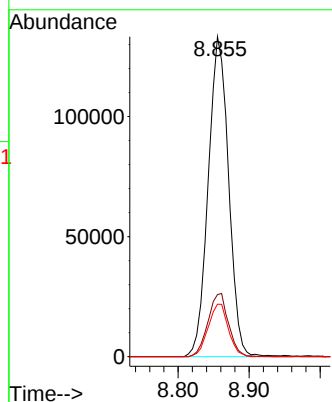

#35

Dibromofluoromethane

Concen: 52.484 ug/l

RT: 7.908 min Scan# 1018

Delta R.T. 0.000 min

Lab File: VD074186.D

Acq: 23 Aug 2022 13:07




Tgt Ion:113 Resp: 93215


Ion Ratio Lower Upper

113 100

111 103.2 83.8 125.6

192 18.9 14.6 21.8

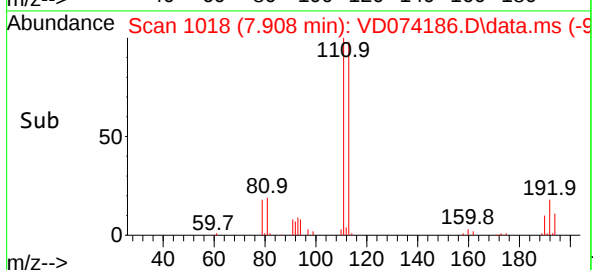



#39

Methylcyclohexane

Concen: 3.296 ug/l

RT: 9.355 min Scan# 1

Delta R.T. 0.006 min

Lab File: VD074186.D

Acq: 23 Aug 2022 13:07

Instrument :

MSVOA_D

ClientSampleId :

VIBLK





Tgt Ion: 83 Resp: 3835

Ion Ratio Lower Upper

83 100

55 54.4 63.2 94.8#

98 40.4 38.2 57.4

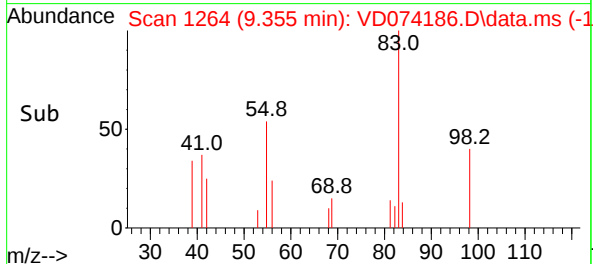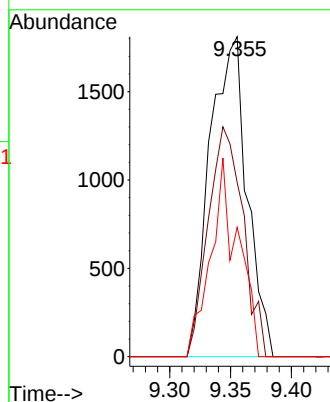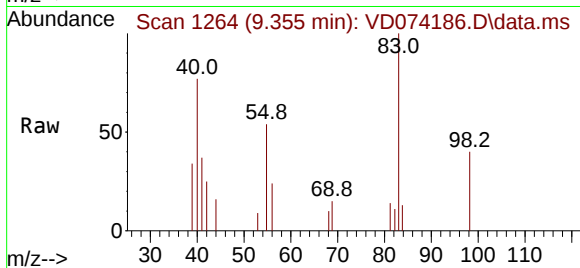

#48

Methyl methacrylate

Concen: 2.128 ug/l

RT: 9.350 min Scan# 1263

Delta R.T. -0.099 min

Lab File: VD074186.D

Acq: 23 Aug 2022 13:07




Tgt Ion: 41 Resp: 2094


Ion Ratio Lower Upper

41 100

69 32.3 56.7 85.1#

39 59.2 42.7 64.1


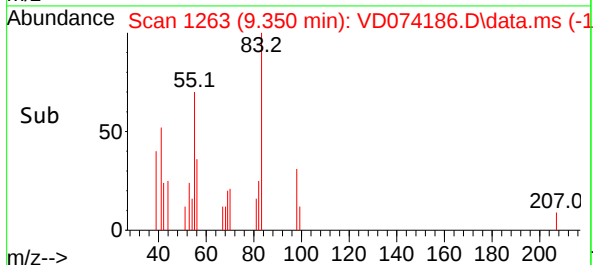
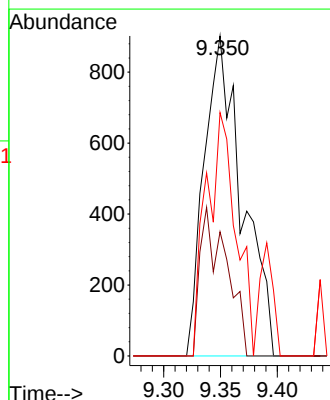
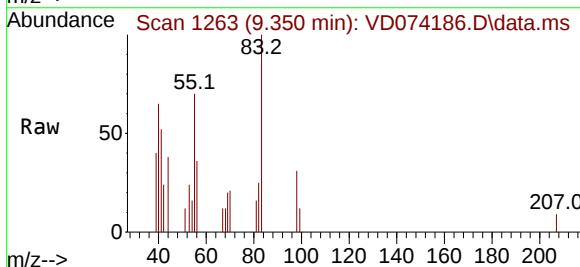




#50
Toluene-d8
Concen: 56.602 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. -0.000 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07




Instrument :
MSVOA_D
ClientSampleId :
VIBLK


Tgt Ion: 98 Resp: 323543
Ion Ratio Lower Upper
98 100
100 67.4 52.4 78.6

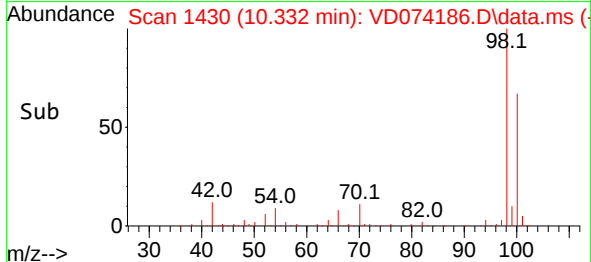

#51
4-Methyl-2-Pentanone
Concen: 4.353 ug/l
RT: 10.214 min Scan# 1410
Delta R.T. -0.006 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07

Tgt Ion: 43 Resp: 4630
Ion Ratio Lower Upper
43 100
58 34.2 28.6 43.0


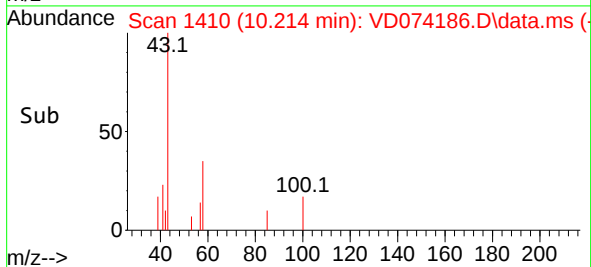

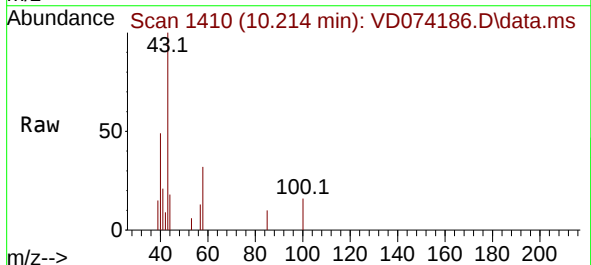




#59
2-Hexanone
Concen: 2.942 ug/l
RT: 10.979 min Scan# 1539
Delta R.T. 0.006 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07




Instrument :
MSVOA_D
ClientSampleId :
VIBLK


Tgt Ion: 43 Resp: 2110
Ion Ratio Lower Upper
43 100
58 55.6 25.3 75.9

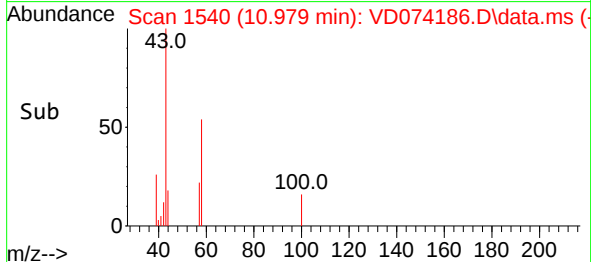

#62
4-Bromofluorobenzene
Concen: 56.127 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. -0.000 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07

Tgt Ion: 95 Resp: 126745
Ion Ratio Lower Upper
95 100
174 77.8 0.0 152.8
176 75.3 0.0 145.4


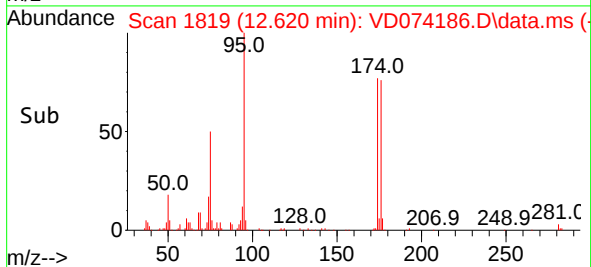

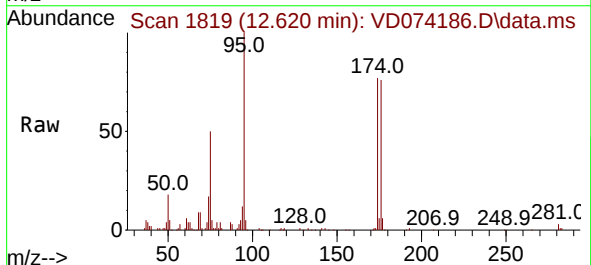




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.632 min Scan# 1
Delta R.T. 0.001 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07




Instrument :
MSVOA_D
ClientSampleId :
VIBLK


Tgt Ion:117 Resp: 270353
Ion Ratio Lower Upper
117 100
82 55.0 45.3 67.9
119 31.3 26.6 40.0

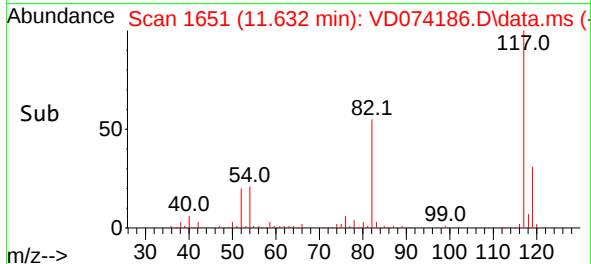

#64
Tetrachloroethene
Concen: 1.097 ug/l
RT: 10.873 min Scan# 1522
Delta R.T. 0.006 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07

Tgt Ion:164 Resp: 2164
Ion Ratio Lower Upper
164 100
166 69.6 98.5 147.7#
129 67.9 74.6 111.8#
131 70.7 72.0 108.0#


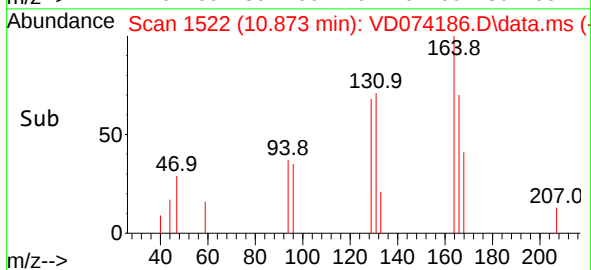

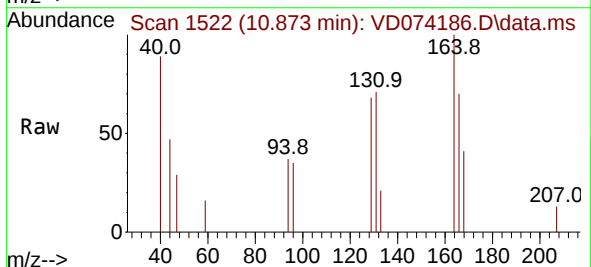




#68
m/p-Xylenes
Concen: 1.223 ug/l
RT: 11.844 min Scan# 1
Delta R.T. 0.001 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07




Instrument :
MSVOA_D
ClientSampleId :
VIBLK


Tgt Ion:106 Resp: 4911
Ion Ratio Lower Upper
106 100
91 222.3 163.7 245.5

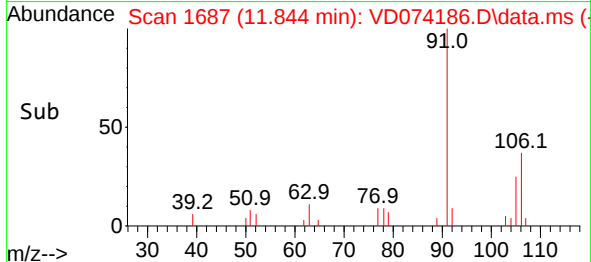

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. 0.006 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07

Tgt Ion:152 Resp: 132223
Ion Ratio Lower Upper
152 100
115 57.7 31.3 93.8
150 157.6 0.0 348.6


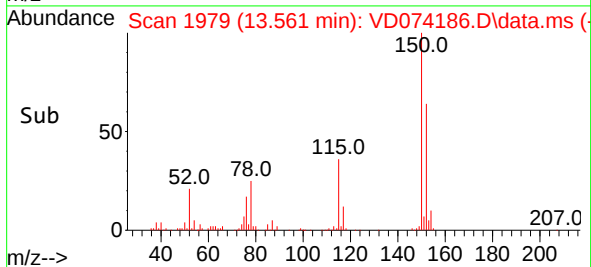

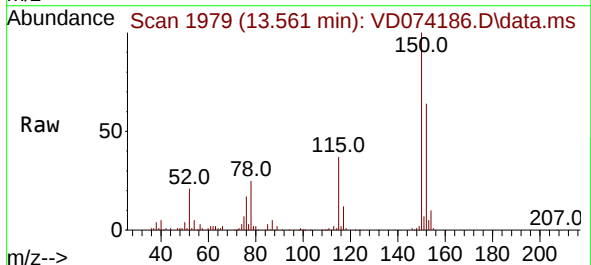




#76
1,2,3-Trichloropropane
Concen: 49.562 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. -0.147 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07




Instrument :
MSVOA_D
ClientSampleId :
VIBLK


Tgt Ion: 75 Resp: 63988
Ion Ratio Lower Upper
75 100
77 2.0 0.0 0.0#

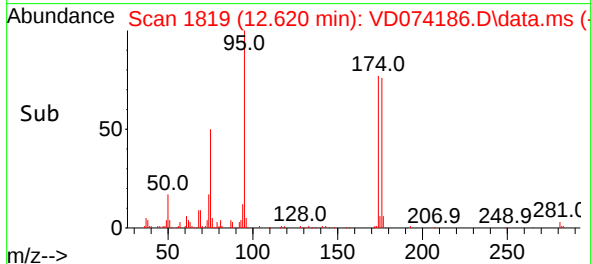

#81
trans-1,4-Dichloro-2-butene
Concen: 127.457 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. 0.106 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07


Tgt Ion: 75 Resp: 63988
Ion Ratio Lower Upper
75 100
53 0.0 86.5 129.7#
89 0.0 33.9 50.9#

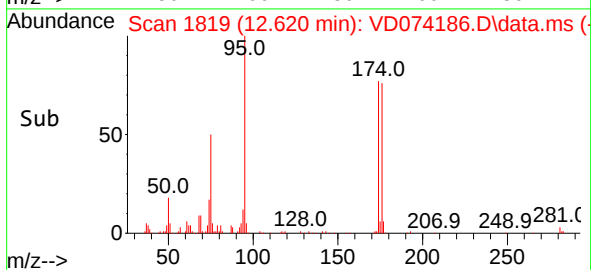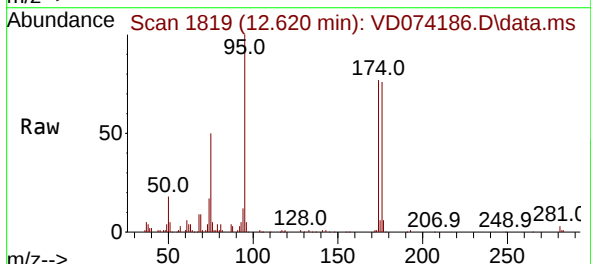



#95
Naphthalene
Concen: 4.149 ug/l
RT: 15.373 min Scan# 21
Delta R.T. -0.005 min
Lab File: VD074186.D
Acq: 23 Aug 2022 13:07

Instrument :
MSVOA_D
ClientSampleId :
VIBLK



Tgt Ion	Ratio	Lower	Upper
128	100		
127	7.7	10.3	15.5#
129	2.5	8.4	12.6#

