
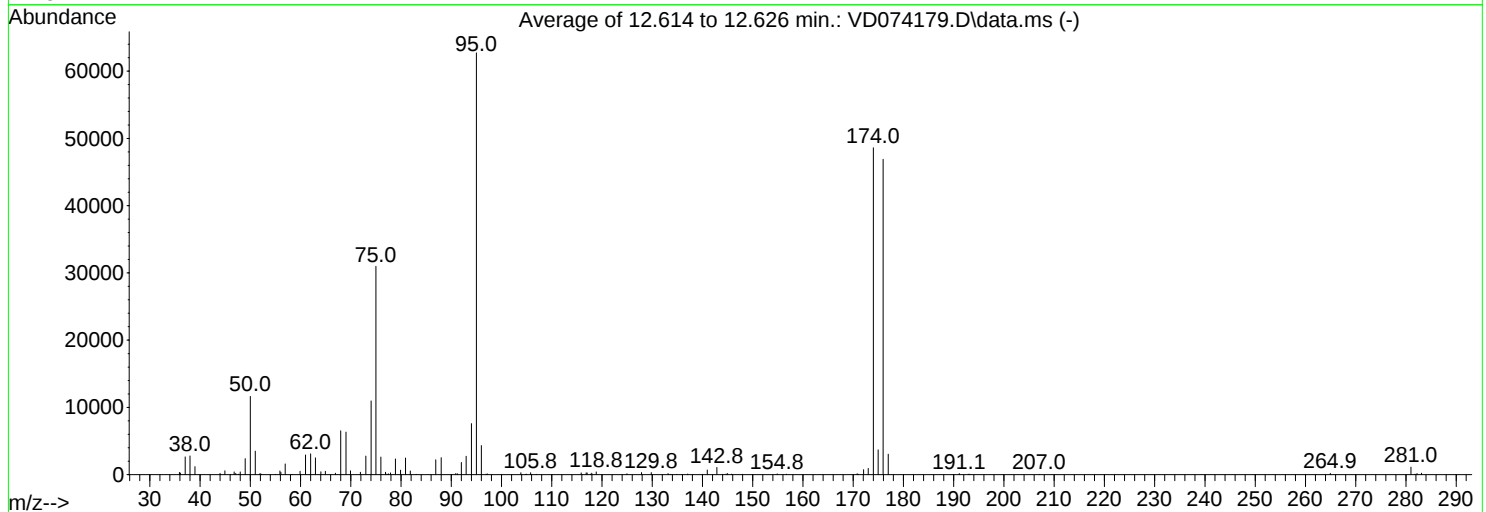


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD082322\
Data File : VD074179.D
Acq On : 23 Aug 2022 09:02
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D082322S.M
Title : SW846 8260
Last Update : Tue Aug 23 13:12:17 2022

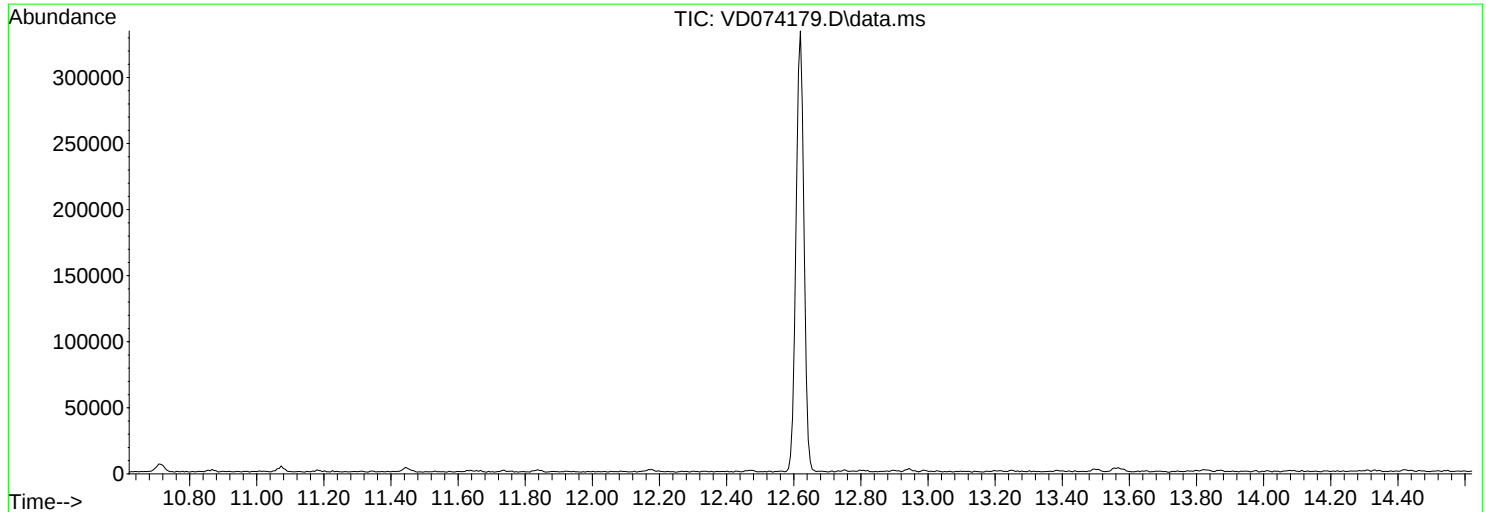

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1809

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	11646	PASS
75	95	30	60	49.4	30971	PASS
95	95	100	100	100.0	62725	PASS
96	95	5	9	6.9	4325	PASS
173	174	0.00	2	1.9	931	PASS
174	95	50	100	77.5	48621	PASS
175	174	5	9	7.6	3702	PASS
176	174	95	101	96.4	46891	PASS
177	176	5	9	6.5	3048	PASS