


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD082521\
Data File : VD070240.D
Acq On : 25 Aug 2021 09:15
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D081321S.M
Title : SW846 8260
Last Update : Sat Aug 14 02:33:51 2021

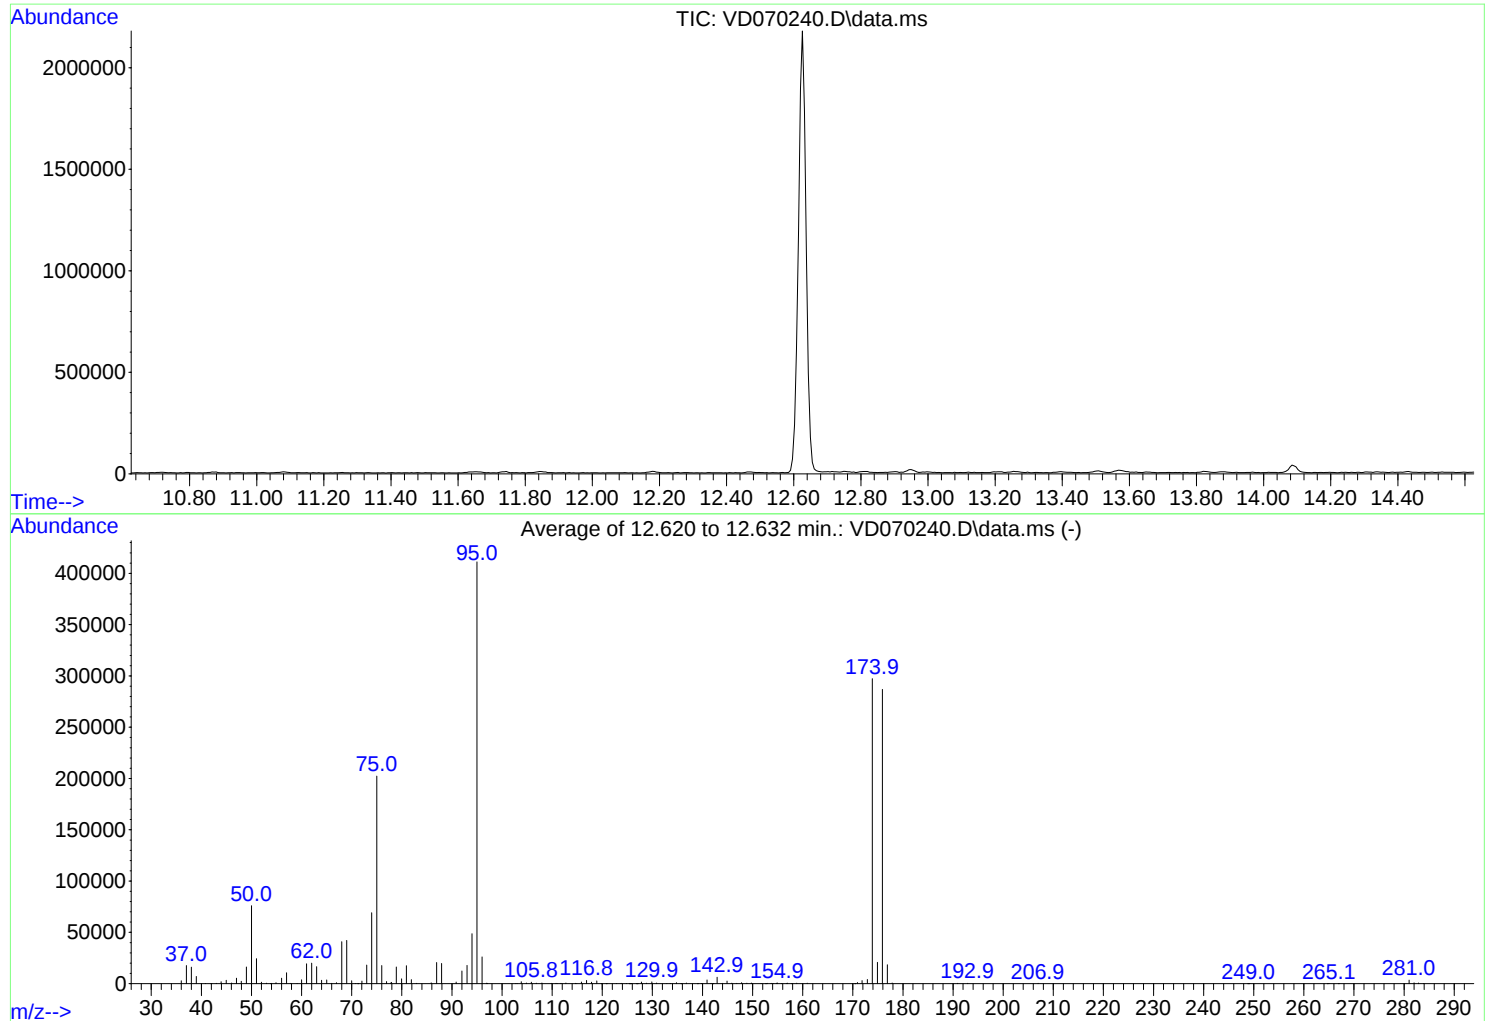

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	75947	PASS
75	95	30	60	49.2	202368	PASS
95	95	100	100	100.0	411221	PASS
96	95	5	9	6.4	26131	PASS
173	174	0.00	2	1.4	4068	PASS
174	95	50	100	72.3	297280	PASS
175	174	5	9	7.0	20781	PASS
176	174	95	101	96.5	286848	PASS
177	176	5	9	6.4	18432	PASS