

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD082523\
 Data File : VD077023.D
 Acq On : 25 Aug 2023 18:45
 Operator : JC/SY
 Sample : 04172-08
 Misc : 5.96G/10.0ml/MSVOA_D/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCHV1

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 08/28/2023
 Supervised By :Semsettin Yesilyurt 08/28/2023

Quant Time: Aug 25 23:56:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM080323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Aug 25 23:54:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	242519	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	251365	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	121340	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.264	65	99525	14.923	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	59.680%		
7) Chloroethane-d5	2.793	69	110294	17.889	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	71.560%		
11) 1,1-Dichloroethene-d2	3.911	65	24477	15.489	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	61.960%		
21) 2-Butanone-d5	6.987	46	59191	55.278	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	110.560%		
24) Chloroform-d	7.563	84	169224	21.428	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	85.720%		
26) 1,2-Dichloroethane-d4	8.228	65	95693	24.308	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	97.240%		
32) Benzene-d6	8.199	84	316170	20.006	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	80.040%		
36) 1,2-Dichloropropane-d6	9.210	67	105351	21.681	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	86.720%		
41) Toluene-d8	10.269	98	277499	19.152	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	76.600%		
43) trans-1,3-Dichloroprop...	10.522	79	45786	20.842	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	83.360%		
47) 2-Hexanone-d5	10.875	63	51536	55.524	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	111.040%		
56) 1,1,2,2-Tetrachloroeth...	12.651	84	120323	25.626	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	102.520%		
66) 1,2-Dichlorobenzene-d4	13.816	152	110917	25.003	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	100.000%		
Target Compounds						Qvalue
16) Methylene chloride	4.805	84	24547m	4.825	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD082523\
Data File : VD077023.D
Acq On : 25 Aug 2023 18:45
Operator : JC/SY
Sample : 04172-08
Misc : 5.96G/10.0ml/MSVOA_D/SOIL
ALS Vial : 10 Sample Multiplier: 1


Instrument :
MSVOA_D
ClientSampleId :
DCHV1

Quant Time: Aug 25 23:56:44 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM080323SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Aug 25 23:54:22 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 08/28/2023
Supervised By :Semsettin Yesilyurt 08/28/2023

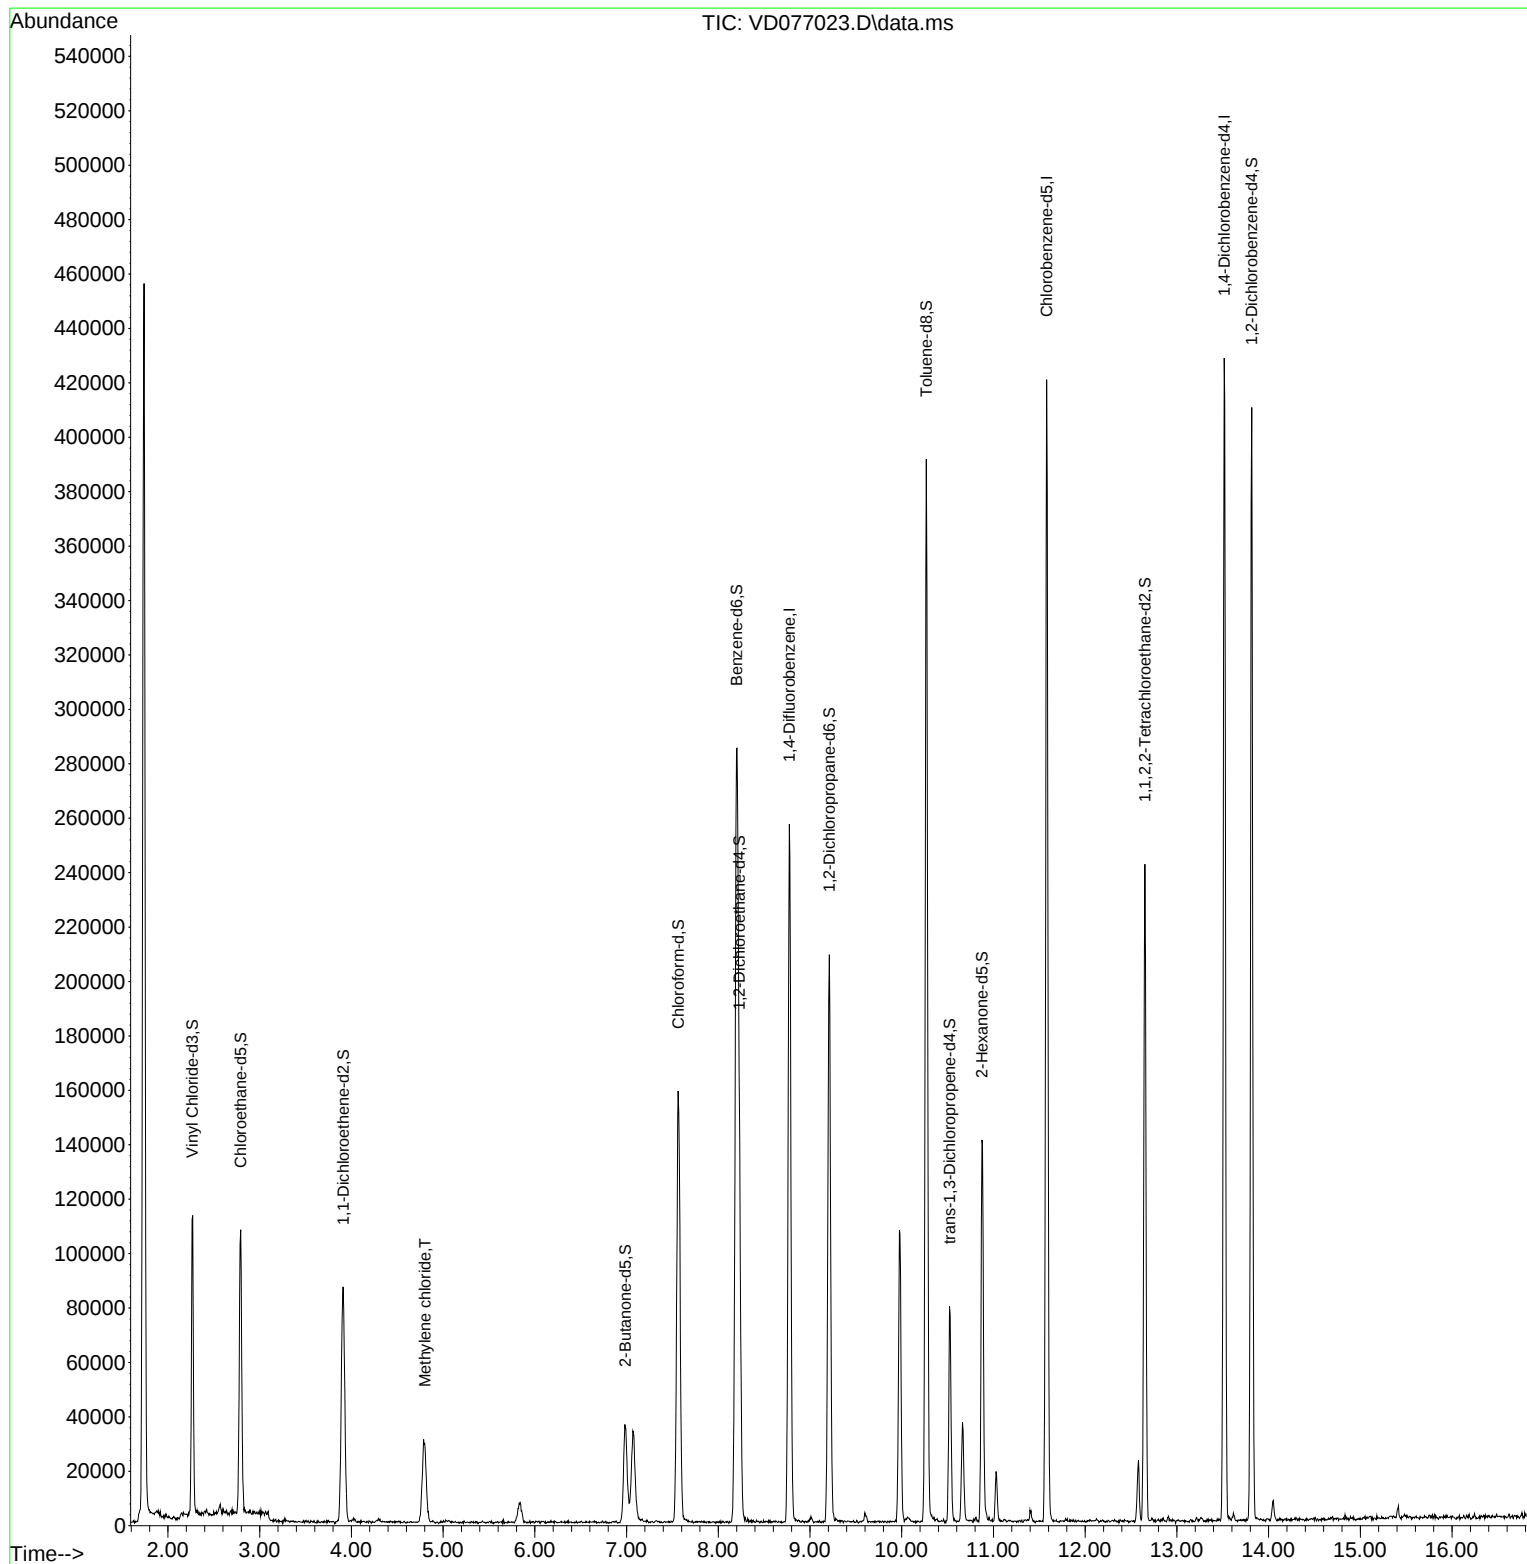

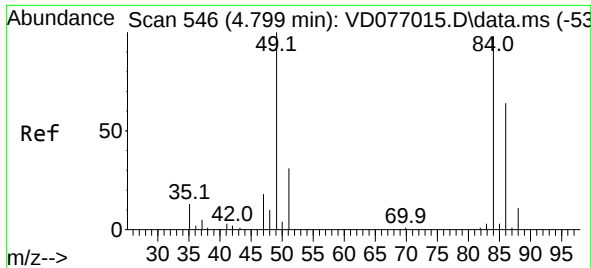

#16
Methylene chloride
Concen: 4.825 ug/L m
RT: 4.805 min Scan# 54
Delta R.T. 0.006 min
Lab File: VD077023.D
Acq: 25 Aug 2023 18:45

Instrument :
MSVOA_D
ClientSampleId :
DCHV1

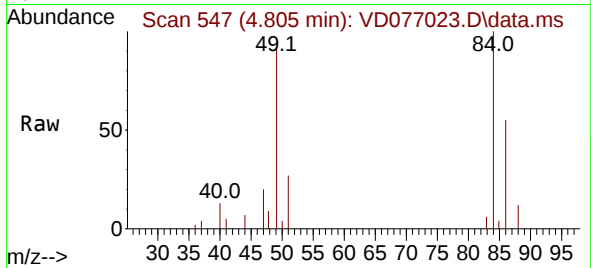

Tgt Ion: 84 Resp: 2454

Ion	Ratio	Lower	Upper
84	100		
86	54.8	45.1	83.9
49	92.5	97.2	180.6

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 08/28/2023
Supervised By :Semsettin Yesilyurt 08/28/2023

