

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD082718\
 Data File : VD059915.D
 Acq On : 27 Aug 2018 15:09
 Operator : JC/SY
 Sample : J4646-13RE
 Misc : 5.54g/5ml/MSVOA D/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EP1-Q4-D6RE

Quant Time: Aug 27 16:19:02 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082218S.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 23 03:03:08 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	6.39	168	1135739	50.00	ug/l	-0.02
34) 1,4-Difluorobenzene	7.42	114	1595609	50.00	ug/l	-0.02
63) Chlorobenzene-d5	11.28	117	1308457	50.00	ug/l	-0.02
72) 1,4-Dichlorobenzene-d4	13.37	152	644956	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.76	65	447661	46.76	ug/l	-0.03
Spiked Amount	50.000		Recovery	=	93.52%	
35) Dibromofluoromethane	6.30	113	559479	44.72	ug/l	-0.03
Spiked Amount	50.000		Recovery	=	89.44%	
50) Toluene-d8	9.45	98	1525722	43.95	ug/l	-0.02
Spiked Amount	50.000		Recovery	=	87.90%	
62) 4-Bromofluorobenzene	12.42	95	598512	42.44	ug/l	-0.02
Spiked Amount	50.000		Recovery	=	84.88%	
Target Compounds						
16) Acetone	3.13	43	35223	20.20	ug/l	93
20) Methylene Chloride	3.68	84	83209	3.70	ug/l	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD082718\
Data File : VD059915.D
Acq On : 27 Aug 2018 15:09
Operator : JC/SY
Sample : J4646-13RE
Misc : 5.54g/5ml/MSVOA D/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
EP1-Q4-D6RE

Quant Time: Aug 27 16:19:02 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D082218S.M
Quant Title : SW846 8260
QLast Update : Thu Aug 23 03:03:08 2018
Response via : Initial Calibration

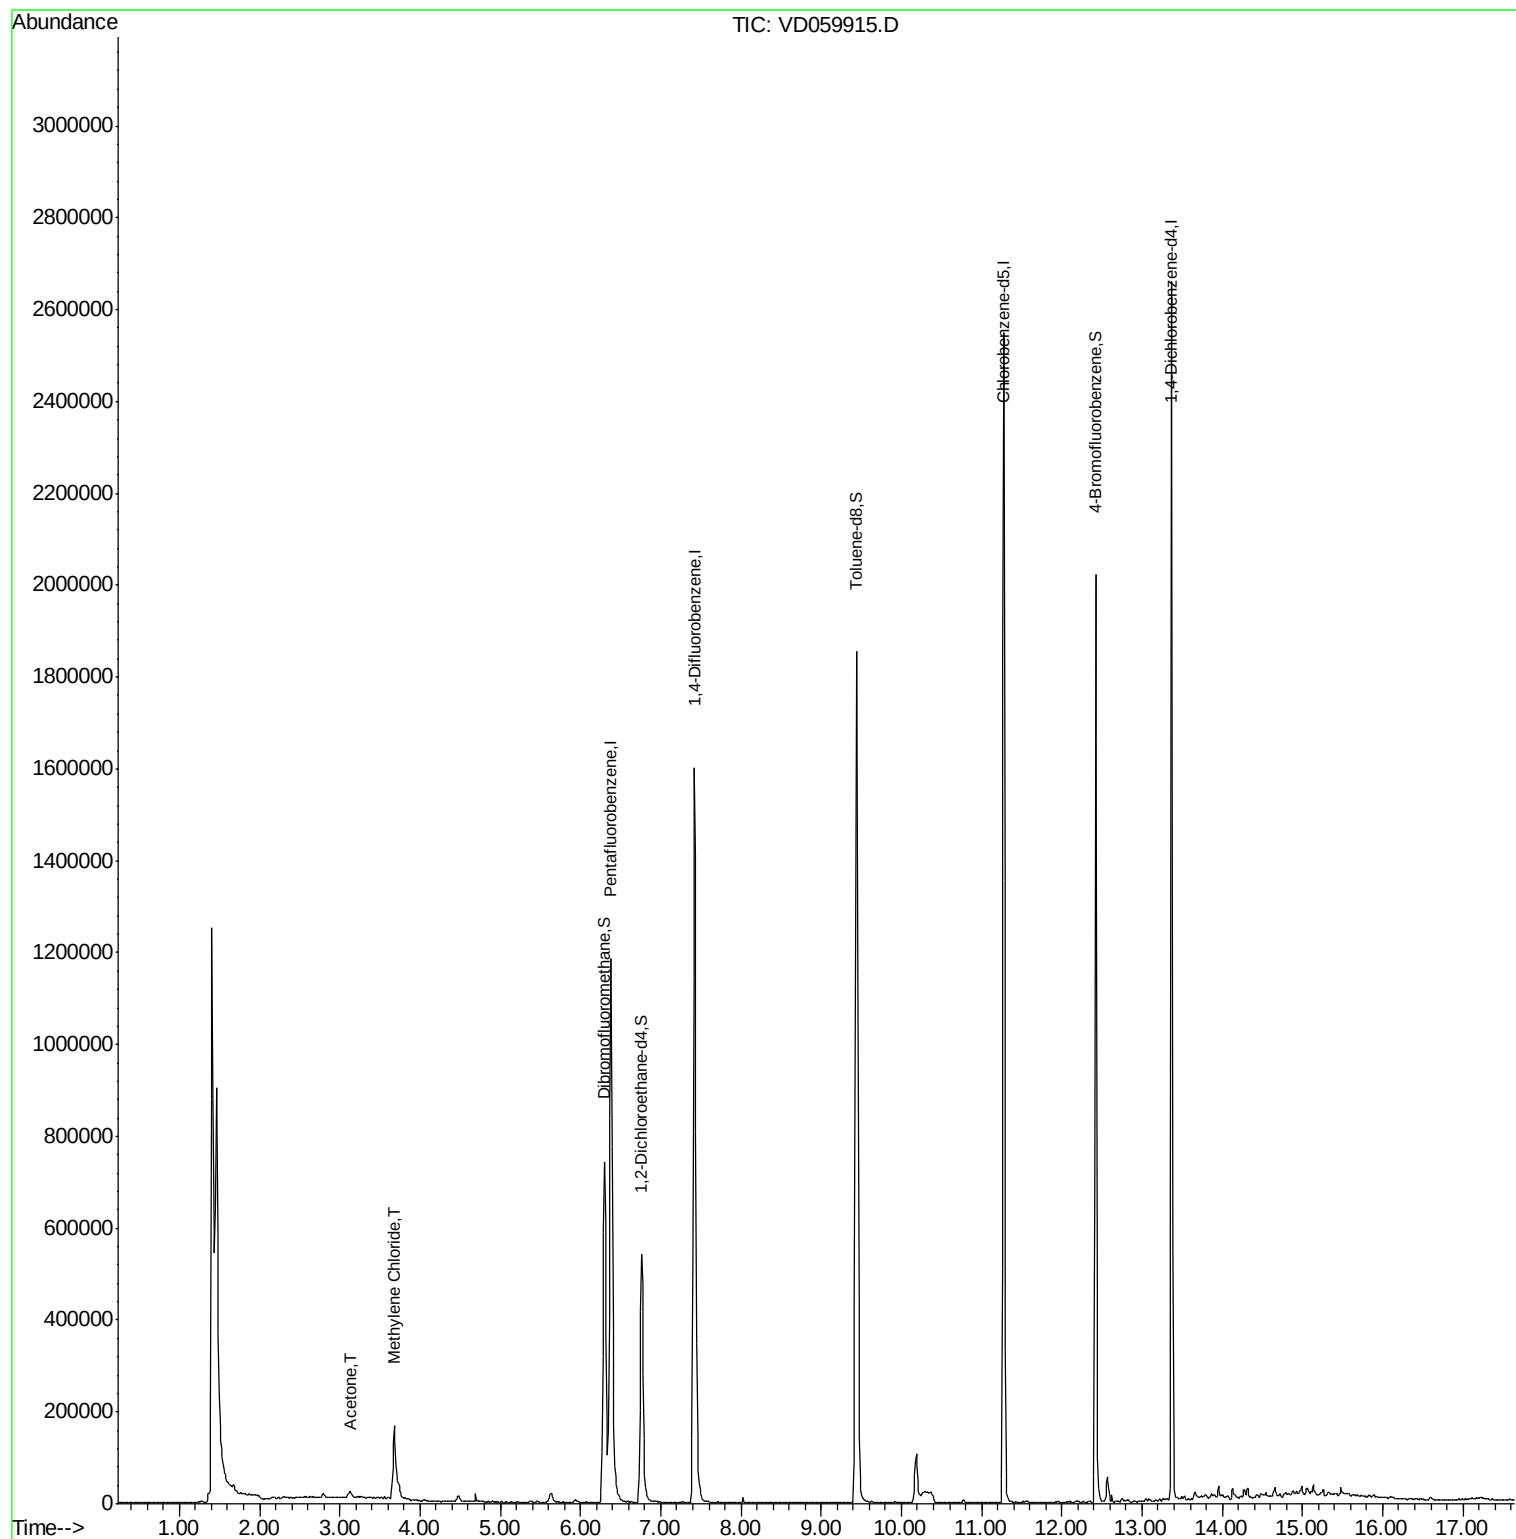

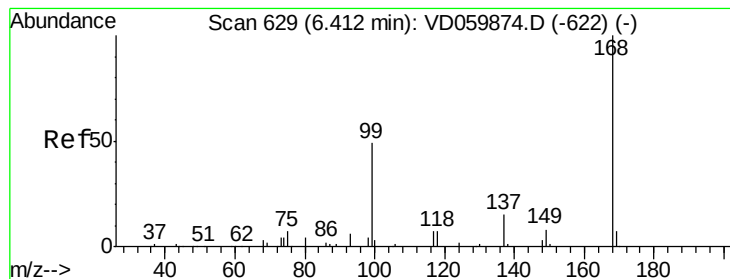

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 6.39 min Scan# 626

Delta R.T. -0.02 min

Lab File: VD059915.D

Acq: 27 Aug 2018 15:09

Instrument :

MSVOA_D

ClientSampleId :


EP1-Q4-D6RE

Tot Ion:168 Resp: 1135739

Ion Ratio Lower Upper

168 100

99 49.0 42.2 63.2

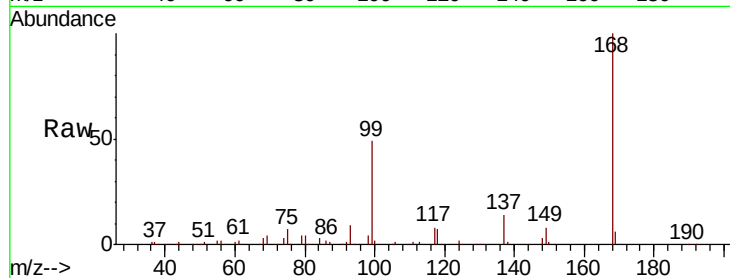

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): V

6.39

400000



300000

200000

100000

0

Time--> 6.20 6.30 6.40 6.50 6.60

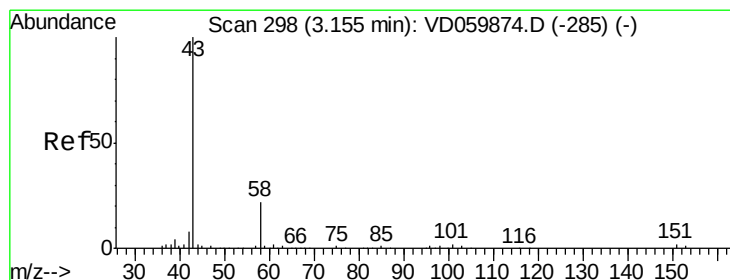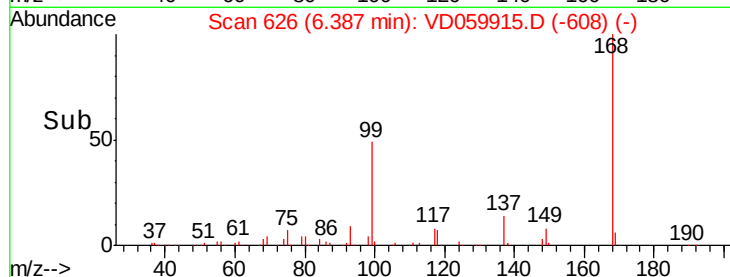

#16

Acetone

Concen: 20.20 ug/l

RT: 3.13 min Scan# 295

Delta R.T. -0.02 min

Lab File: VD059915.D


Acq: 27 Aug 2018 15:09

Tgt Ion: 43 Resp: 35223

Ion Ratio Lower Upper

43 100

58 25.5 17.6 26.4

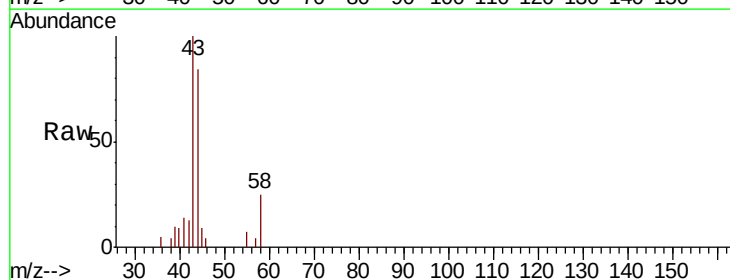

Abundance Ion 42.95 (42.65 to 43.65): V

Ion 57.95 (57.65 to 58.65): V

3.13

10000

8000


6000


4000

2000

0

Time--> 3.00 3.10 3.20

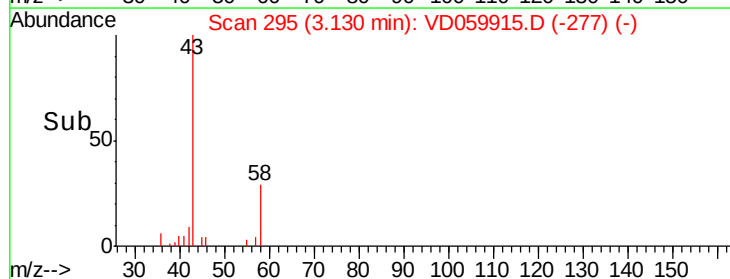


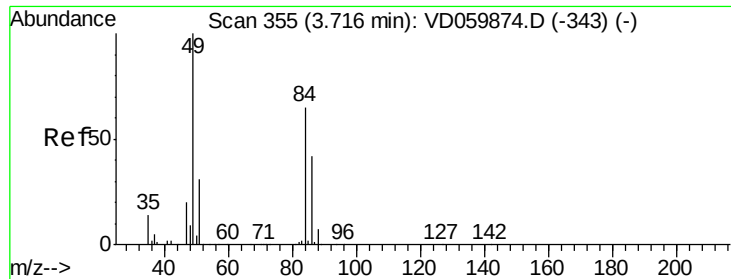




#20
Methylene Chloride
Concen: 3.70 ug/l
RT: 3.68 min Scan# 351
Delta R.T. -0.03 min
Lab File: VD059915.D
Acq: 27 Aug 2018 15:09

Instrument :
MSVOA_D
ClientSampleId :
EP1-Q4-D6RE

Tot Ion: 84 Resp: 83209
Ion Ratio Lower Upper
84 100
49 145.9 122.6 183.8
51 45.3 38.4 57.6
86 60.7 51.5 77.3

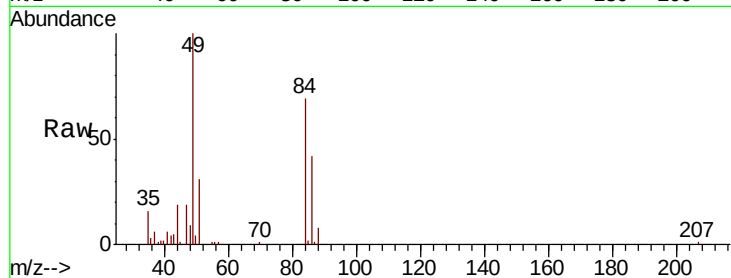


Abundance Ion 83.95 (83.65 to 84.65): VDC
Ion 48.90 (48.60 to 49.60): VDC
Ion 50.90 (50.60 to 51.60): VDC
Ion 85.90 (85.60 to 86.60): VDC

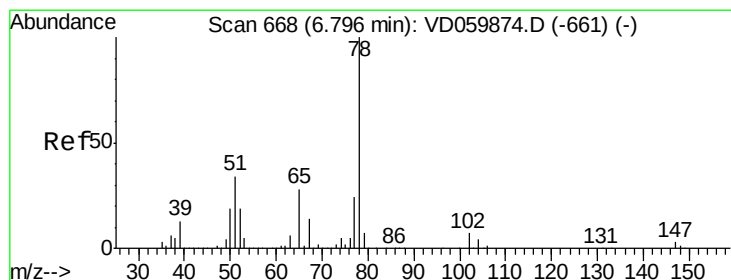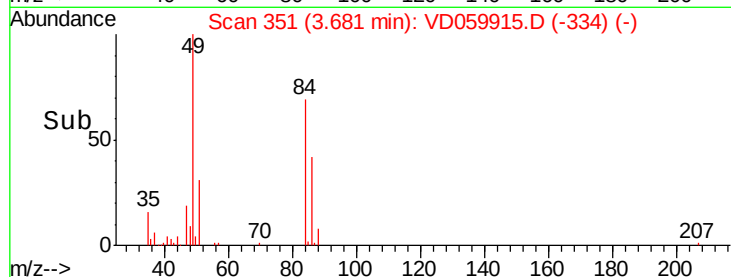
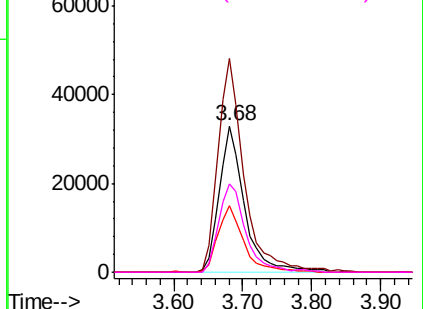



#33
1,2-Dichloroethane-d4
Concen: N.D. ug/l
RT: 6.76 min Scan# 664
Delta R.T. -0.03 min
Lab File: VD059915.D
Acq: 27 Aug 2018 15:09

Tgt Ion: 65 Resp: 447661
Ion Ratio Lower Upper
65 100
67 49.7 0.0 103.8

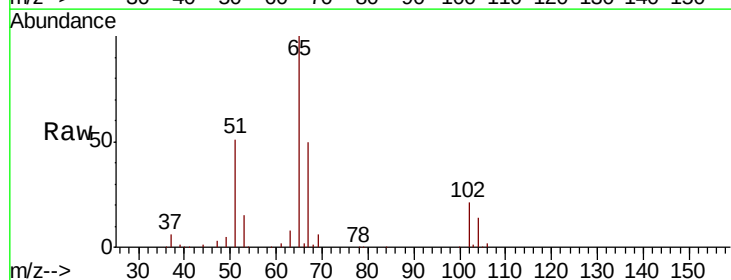

Abundance Ion 64.95 (64.65 to 65.65): VDC
Ion 66.90 (66.60 to 67.60): VDC

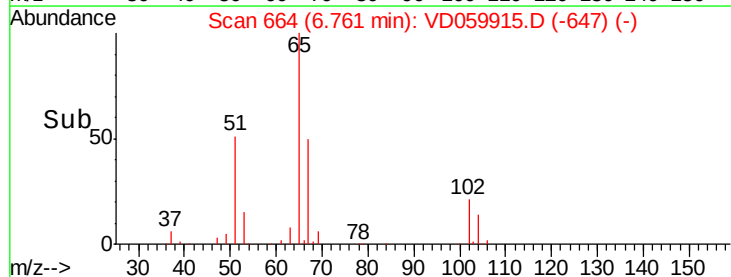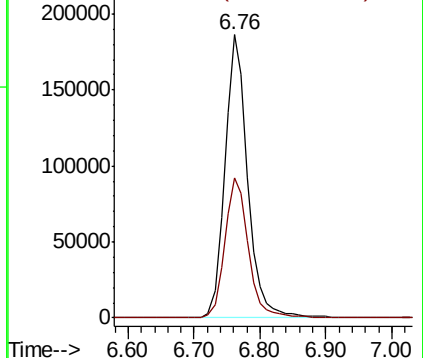

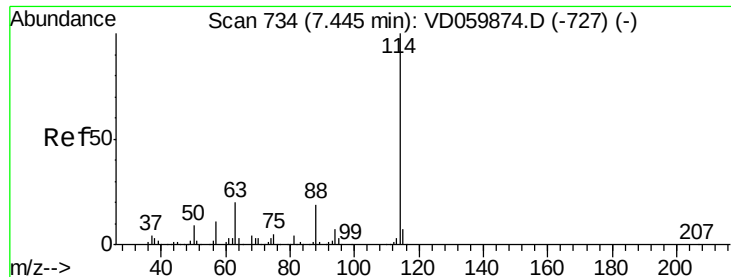

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 7.42 min Scan# 731

Delta R.T. -0.02 min

Lab File: VD059915.D

Acq: 27 Aug 2018 15:09

Instrument :

MSVOA_D

ClientSampleId :

EP1-Q4-D6RE


Tot Ion:114 Resp: 1595609

Ion Ratio Lower Upper

114 100

63 20.0 0.0 39.4




88 19.3 0.0 37.6

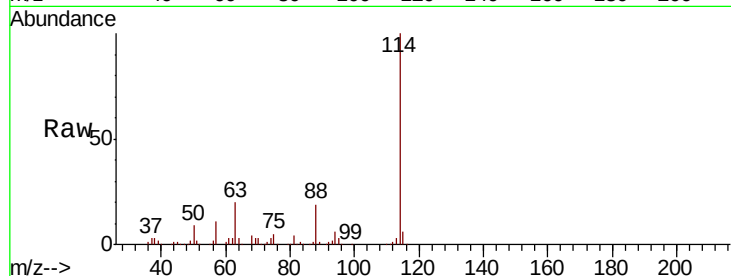

Abundance Ion 114.00 (113.70 to 114.70): V

Ion 62.95 (62.65 to 63.65): V

Ion 87.90 (87.60 to 88.60): V

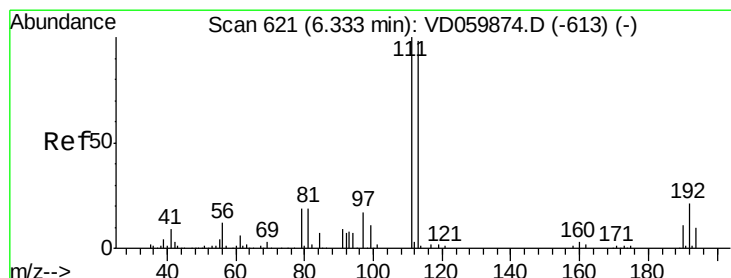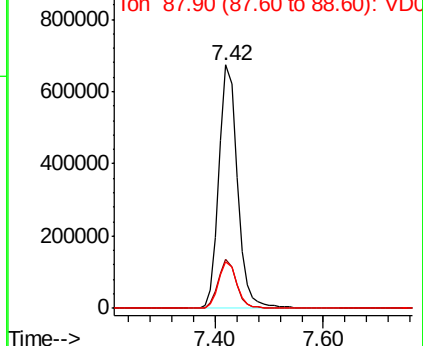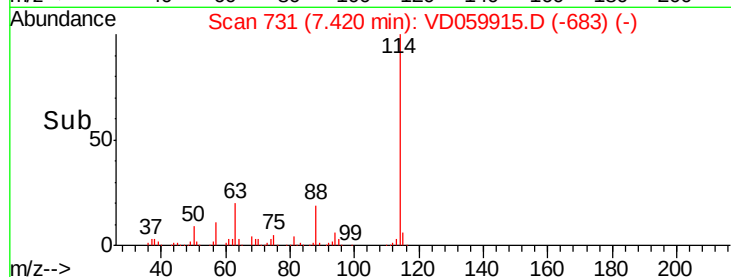

#35

Dibromofluoromethane

Concen: 50.00 ug/l

RT: 6.30 min Scan# 617

Delta R.T. -0.03 min

Lab File: VD059915.D

Acq: 27 Aug 2018 15:09


Tgt Ion:113 Resp: 559479

Ion Ratio Lower Upper

113 100

111 101.3 81.4 122.2



192 20.3 17.0 25.6

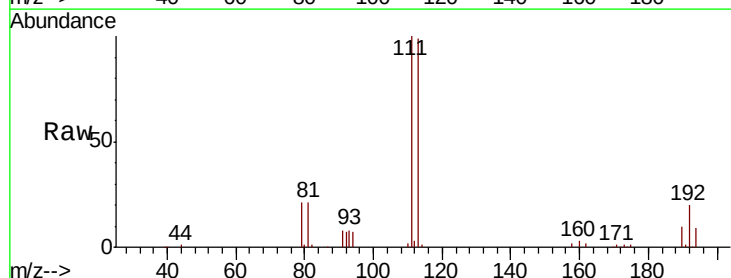


Abundance Ion 112.90 (112.60 to 113.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 191.80 (191.50 to 192.50): V

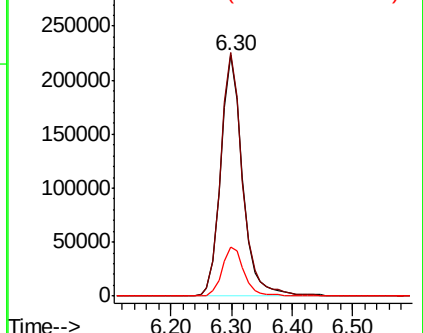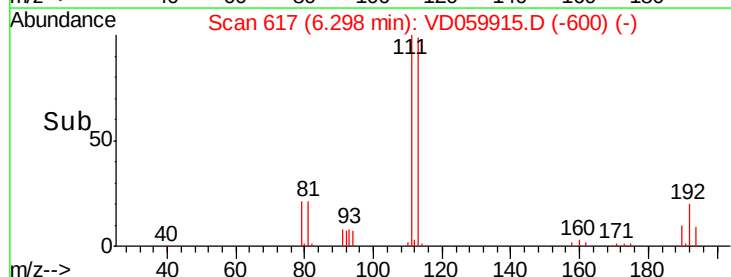


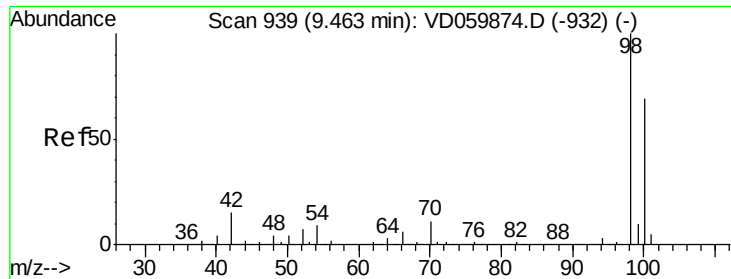




#50
Toluene-d8
Concen: N.D. ug/l
RT: 9.45 min Scan# 937
Delta R.T. -0.02 min
Lab File: VD059915.D
Acq: 27 Aug 2018 15:09

Instrument :
MSVOA_D
ClientSampleId :
EP1-Q4-D6RE

Tot Ion: 98 Resp: 1525722
Ion Ratio Lower Upper
98 100
100 68.0 55.8 83.6

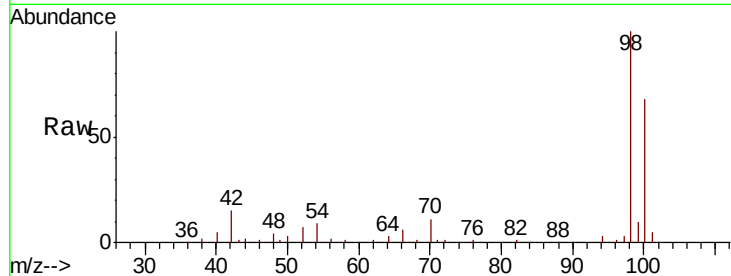


Abundance Ion 98.05 (97.75 to 98.75): VD0
Ion 100.05 (99.75 to 100.75): VD

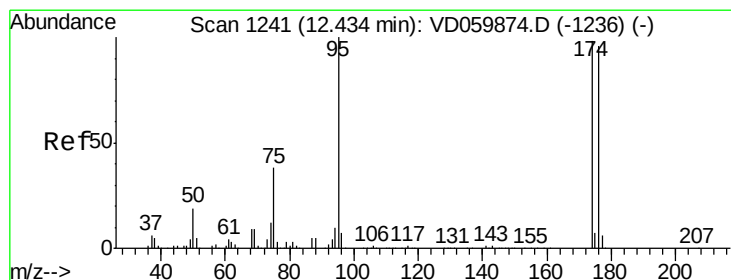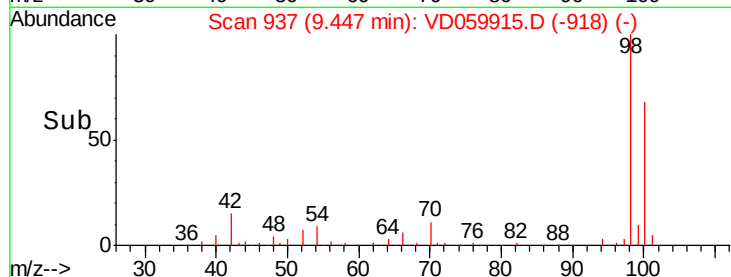
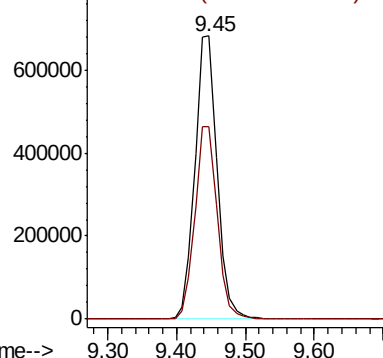



#62
4-Bromofluorobenzene
Concen: N.D. ug/l
RT: 12.42 min Scan# 1239
Delta R.T. -0.02 min
Lab File: VD059915.D
Acq: 27 Aug 2018 15:09

Tgt Ion: 95 Resp: 598512
Ion Ratio Lower Upper
95 100
174 80.7 0.0 195.6
176 78.1 0.0 191.2

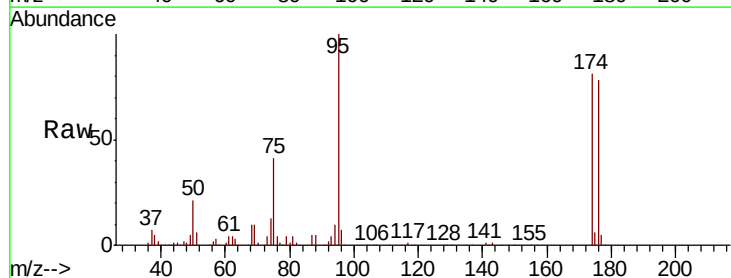

Abundance Ion 95.00 (94.70 to 95.70): VD0
Ion 173.90 (173.60 to 174.60): V
Ion 175.90 (175.60 to 176.60): V

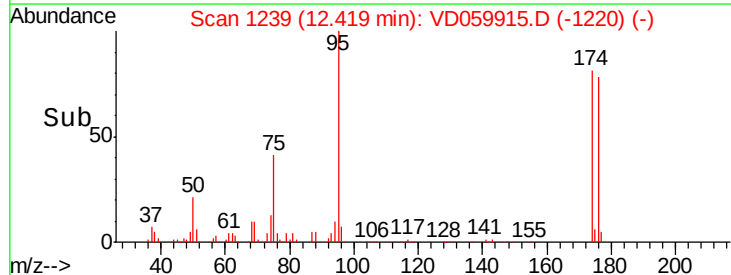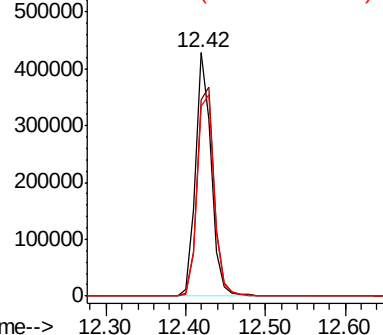


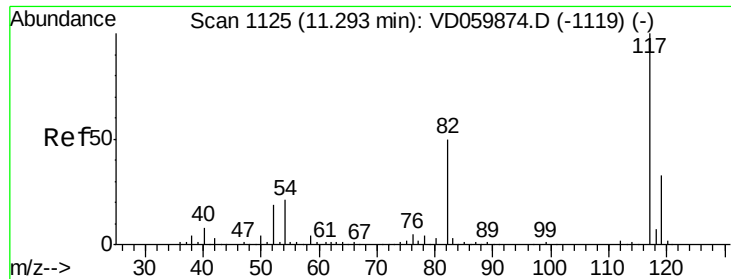




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.28 min Scan# 1123
Delta R.T. -0.02 min
Lab File: VD059915.D
Acq: 27 Aug 2018 15:09

Instrument :
MSVOA_D
ClientSampleId :
EP1-Q4-D6RE

Tot Ion:117 Resp: 1308457
Ion Ratio Lower Upper
117 100
82 53.5 40.1 60.1
119 32.5 26.7 40.1

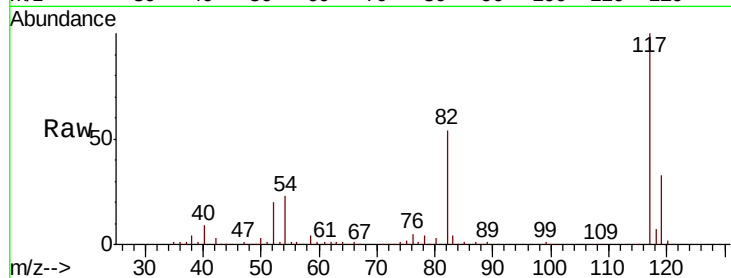


Abundance Ion 116.95 (116.65 to 117.65): V
Ion 82.05 (81.75 to 82.75): VD
Ion 118.95 (118.65 to 119.65): V

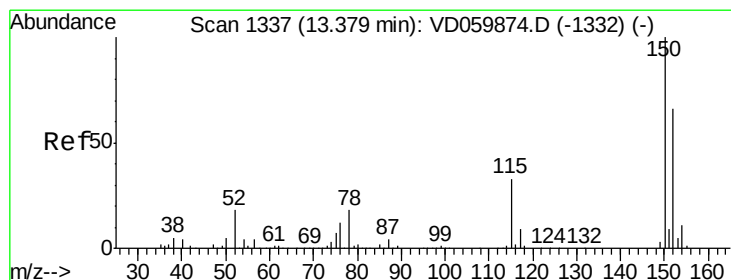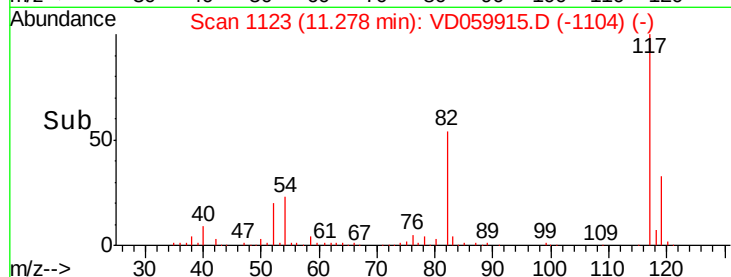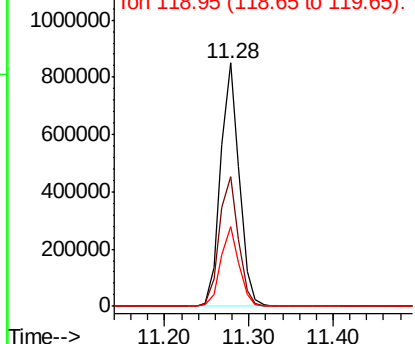

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.37 min Scan# 1336
Delta R.T. -0.01 min
Lab File: VD059915.D
Acq: 27 Aug 2018 15:09

Tgt Ion:152 Resp: 644956
Ion Ratio Lower Upper
152 100
115 47.4 25.7 77.0
150 155.3 0.0 310.2

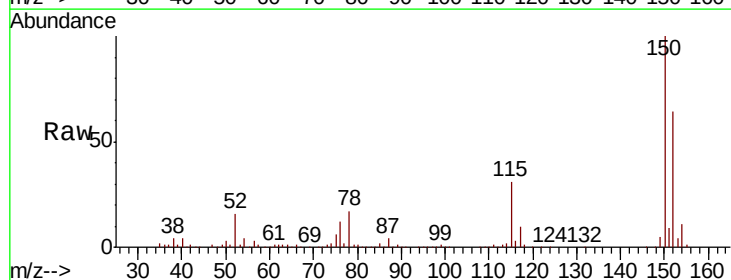

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 115.00 (114.70 to 115.70): V
Ion 149.90 (149.60 to 150.60): V

