


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD082718\  
 Data File : VD059907.D  
 Acq On : 27 Aug 2018 9:55  
 Operator : JC/SY  
 Sample : BFB  
 Misc : 5.00µl/5ml/MSVOA D/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_D  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D082218S.M  
 Title : SW846 8260  
 Last Update : Thu Aug 23 03:03:08 2018

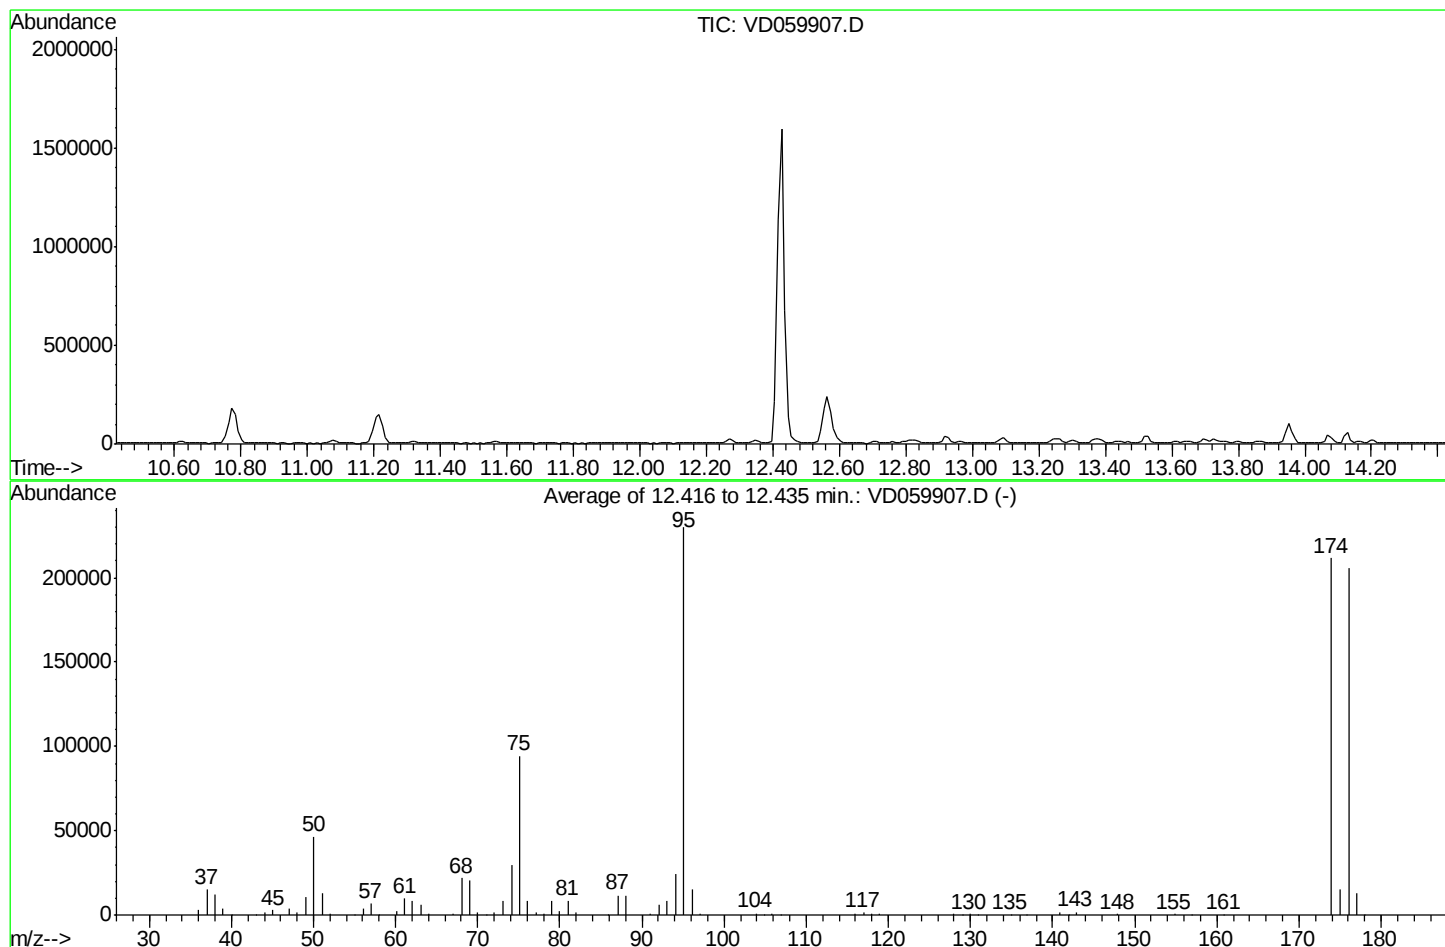

AutoFind: Scans 1239, 1240, 1241; Background Corrected with Scan 1234

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 20.1      | 46328   | PASS             |
| 75          | 95           | 30           | 60           | 41.1      | 94536   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 229976  | PASS             |
| 96          | 95           | 5            | 9            | 6.7       | 15314   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 92.0      | 211626  | PASS             |
| 175         | 174          | 5            | 9            | 7.1       | 15112   | PASS             |
| 176         | 174          | 95           | 101          | 97.2      | 205738  | PASS             |
| 177         | 176          | 5            | 9            | 6.2       | 12783   | PASS             |