


Chloromethane

Response Ratio

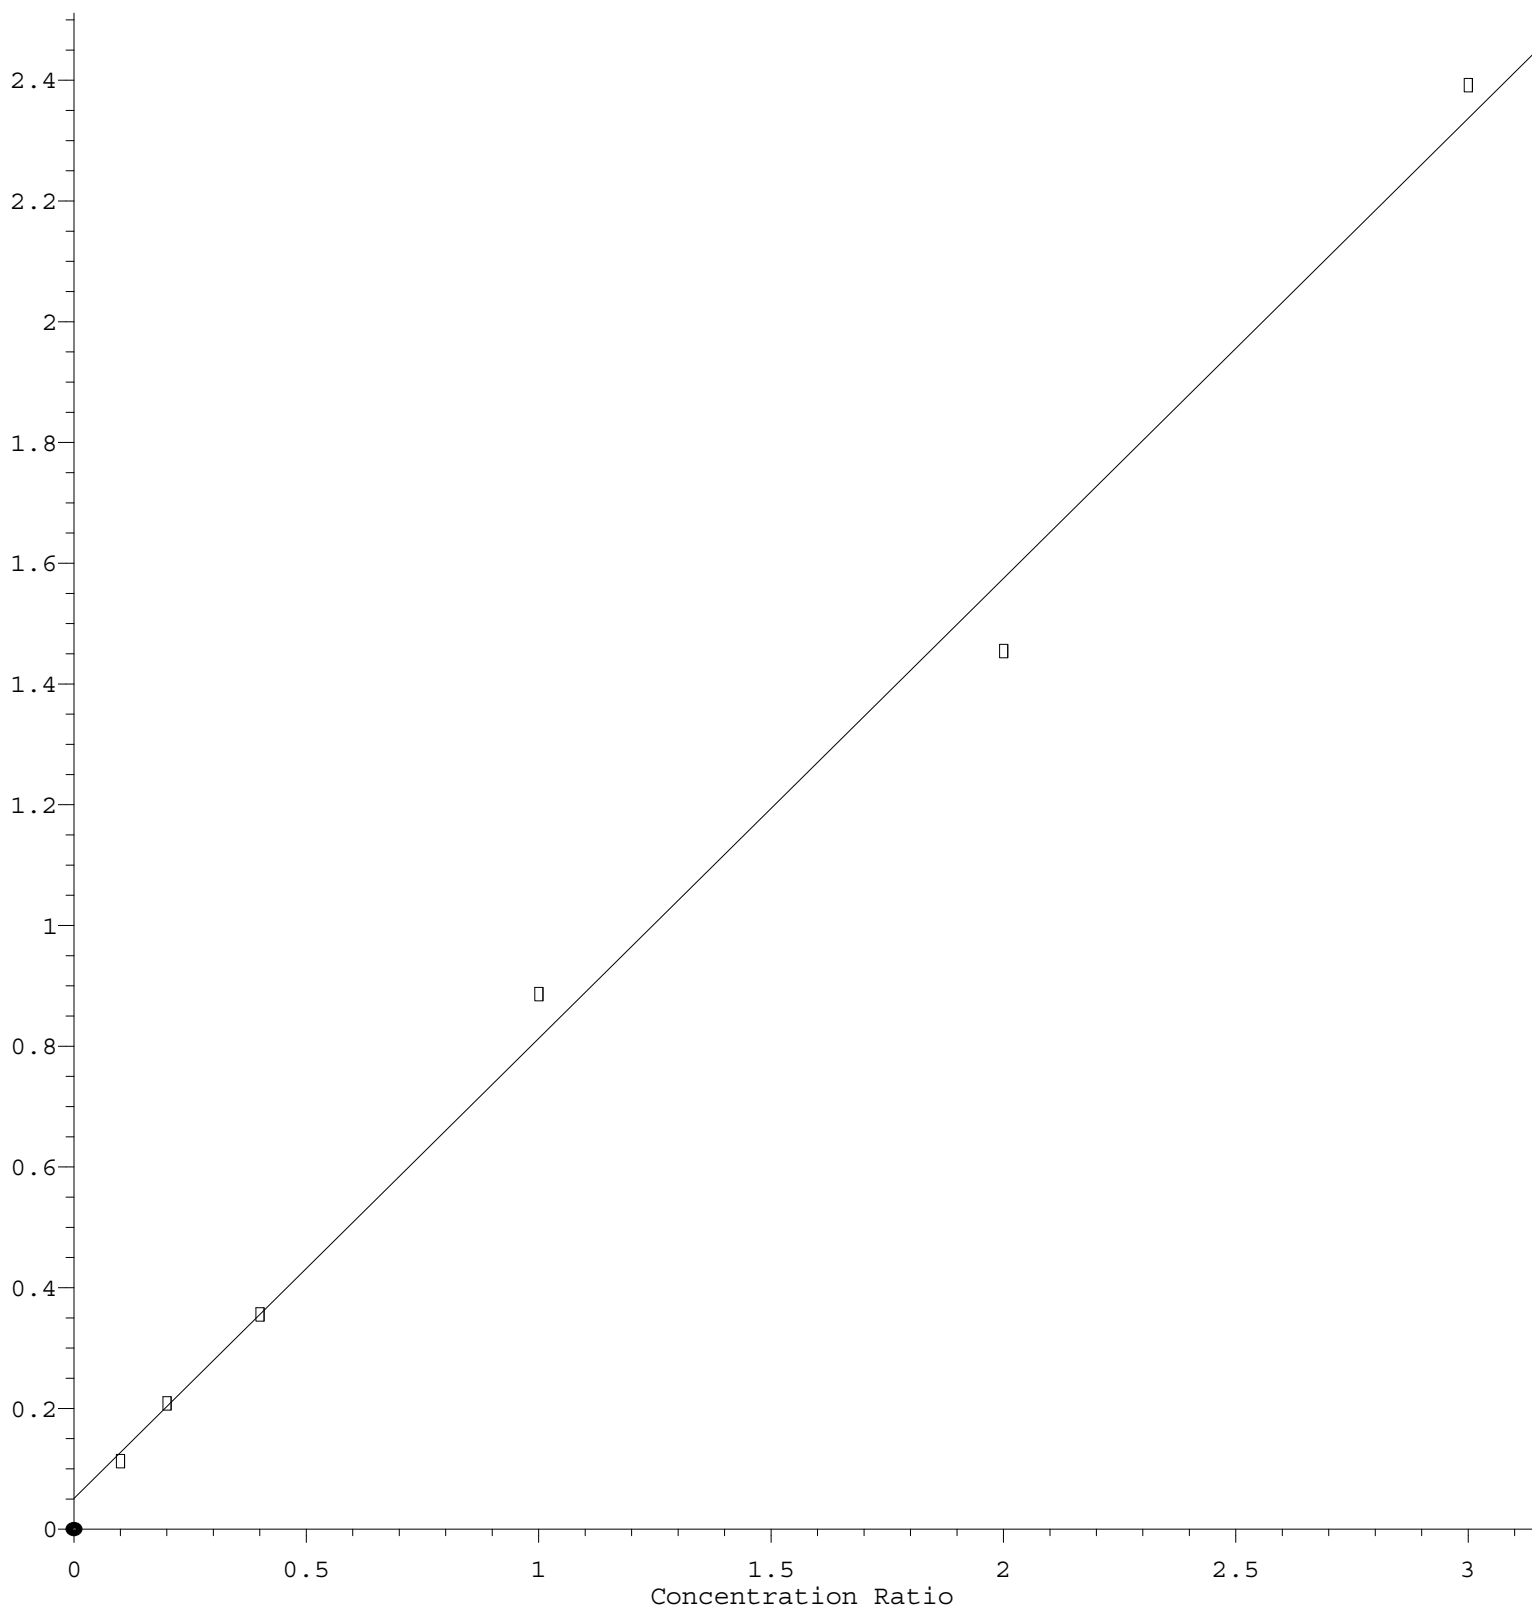

$$\text{Response} = 7.618\text{e-}001 * \text{Amt} + 5.082\text{e-}002$$


Coef of Det (r^2) = 0.994108 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D082823S.M

Calibration Table Last Updated: Tue Aug 29 02:15:23 2023

Methylene Chloride

Response Ratio

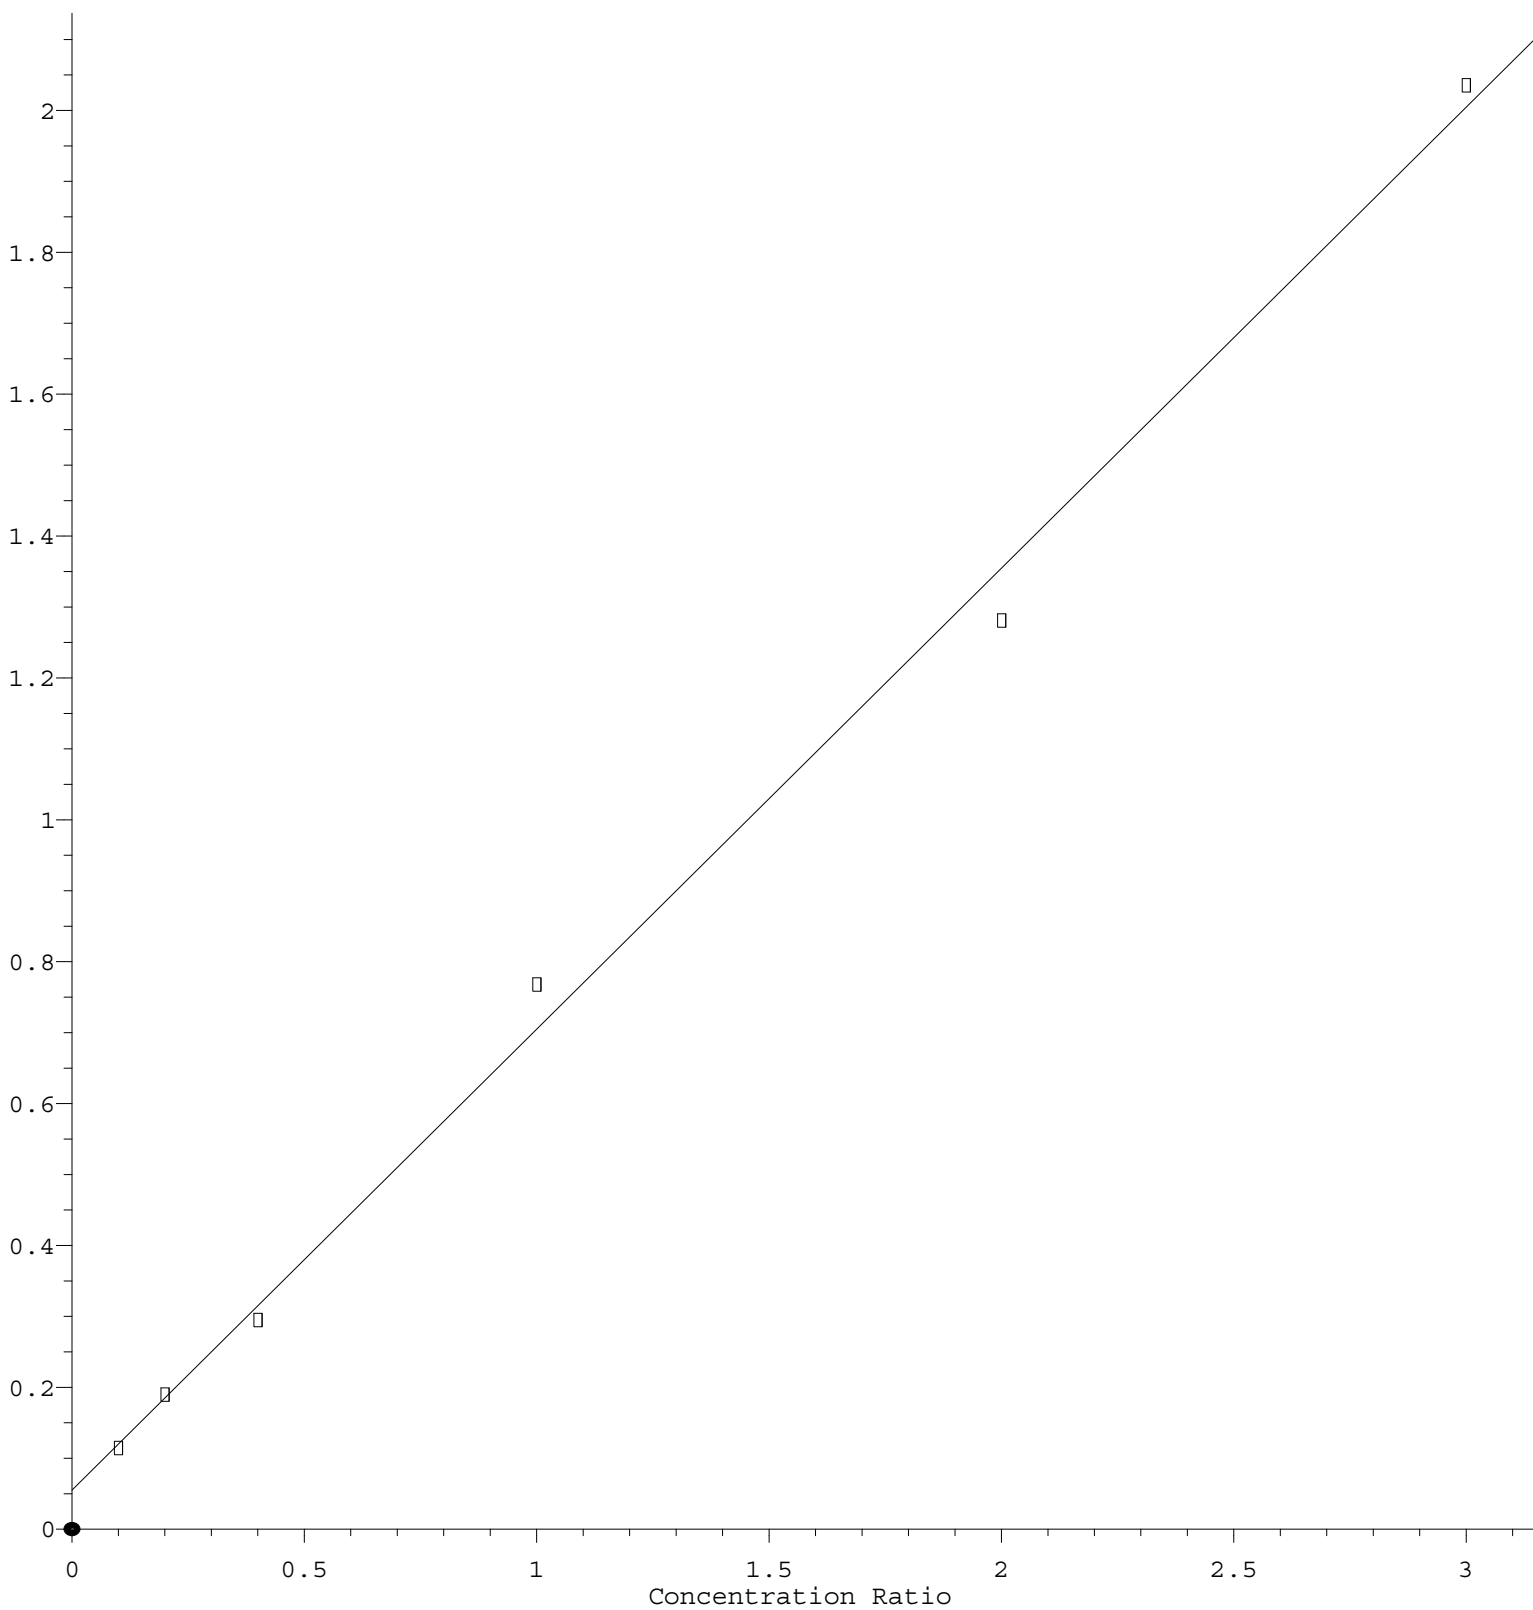

$$\text{Response} = 6.500\text{e-}001 * \text{Amt} + 5.461\text{e-}002$$


Coef of Det (r^2) = 0.996209 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D082823S.M

Calibration Table Last Updated: Tue Aug 29 02:15:23 2023

Acrolein


Response Ratio

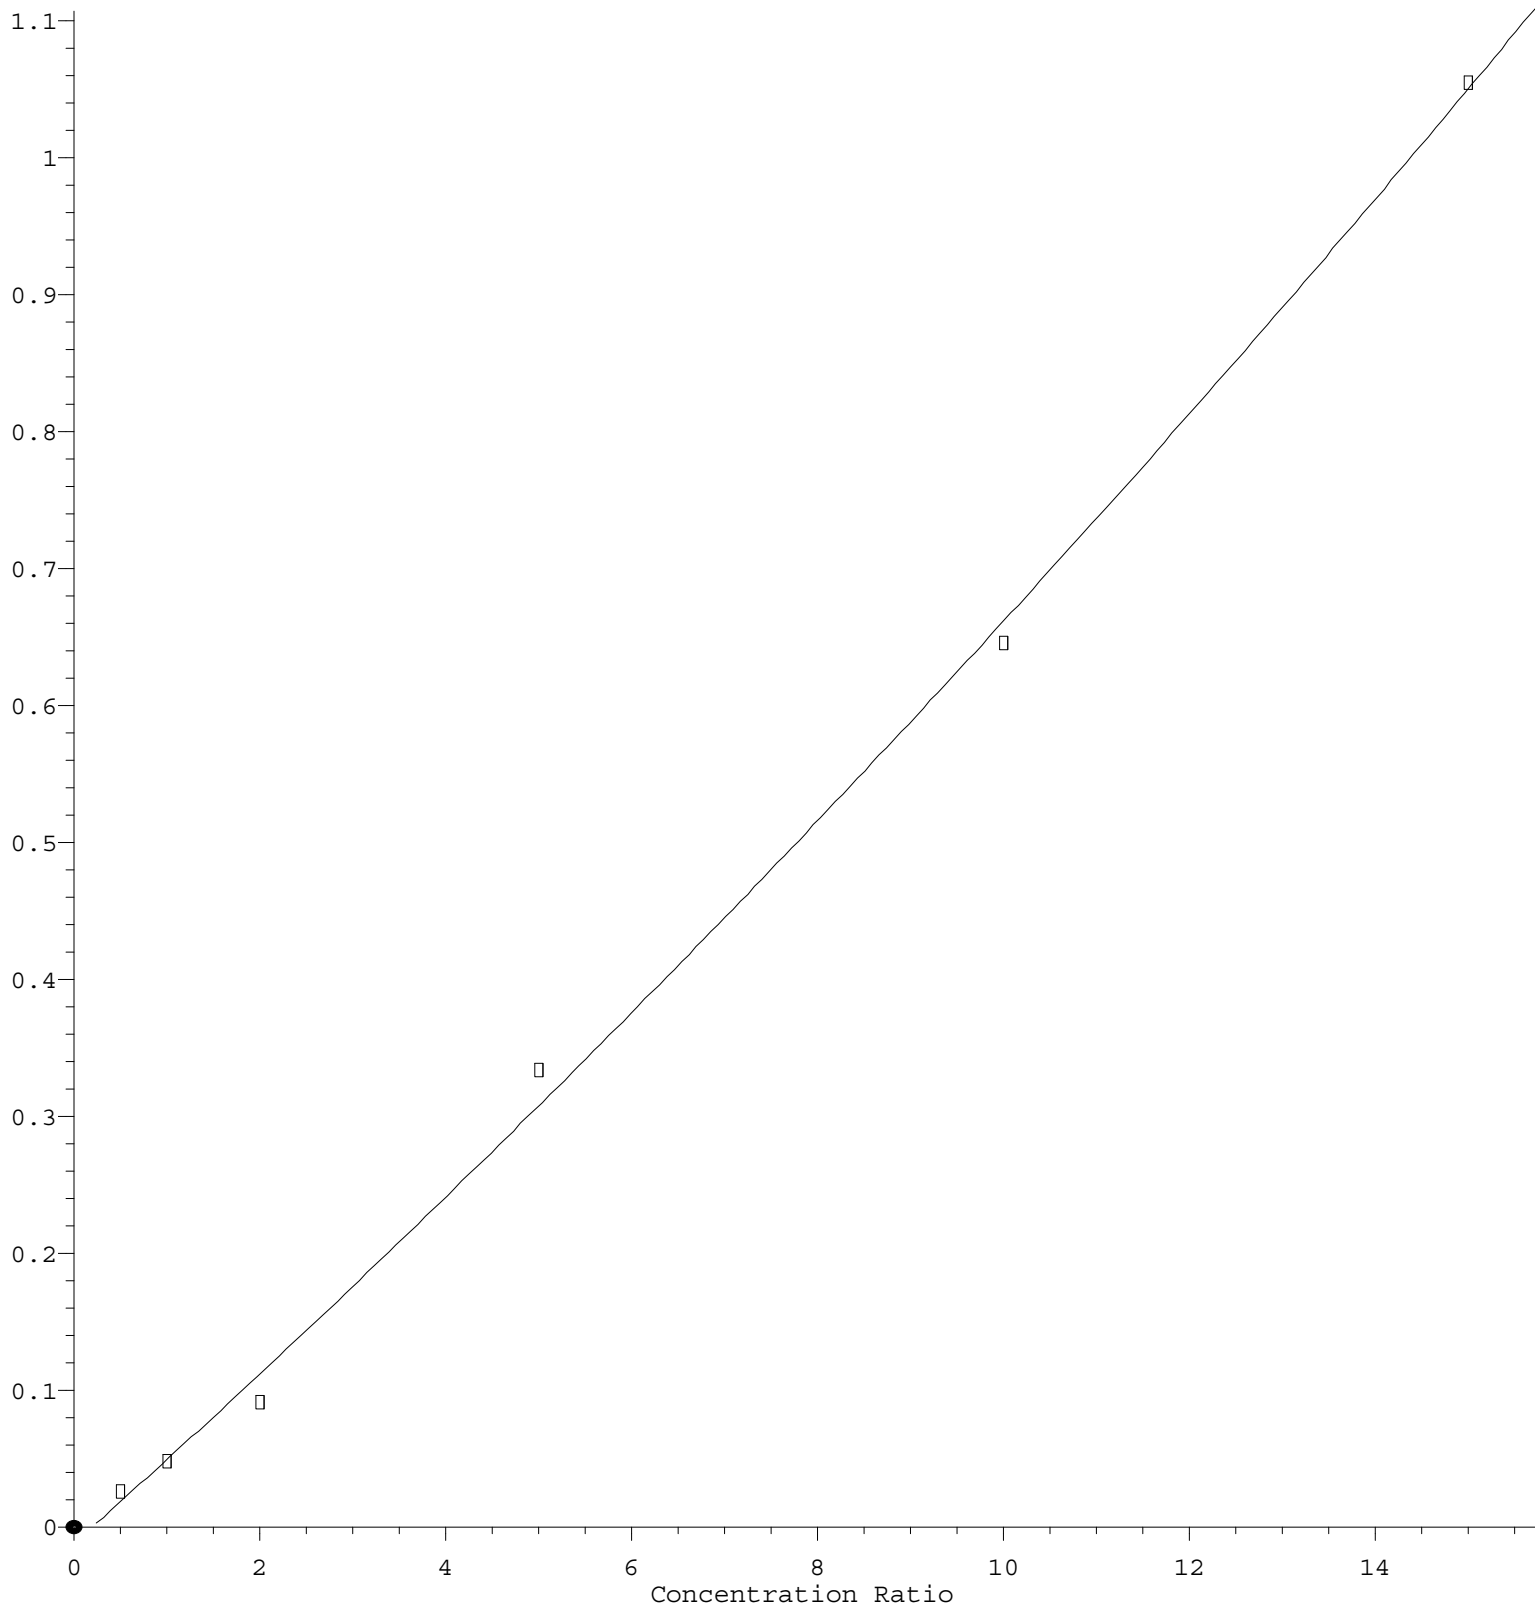

$R = 6.920e-004 A^2 + 6.041e-002 A - 1.163e-002$
 Coef of Det (r^2) = 0.998302 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D082823S.M
 Calibration Table Last Updated: Tue Aug 29 02:15:23 2023

2-Chloroethyl Vinyl ether

Response Ratio

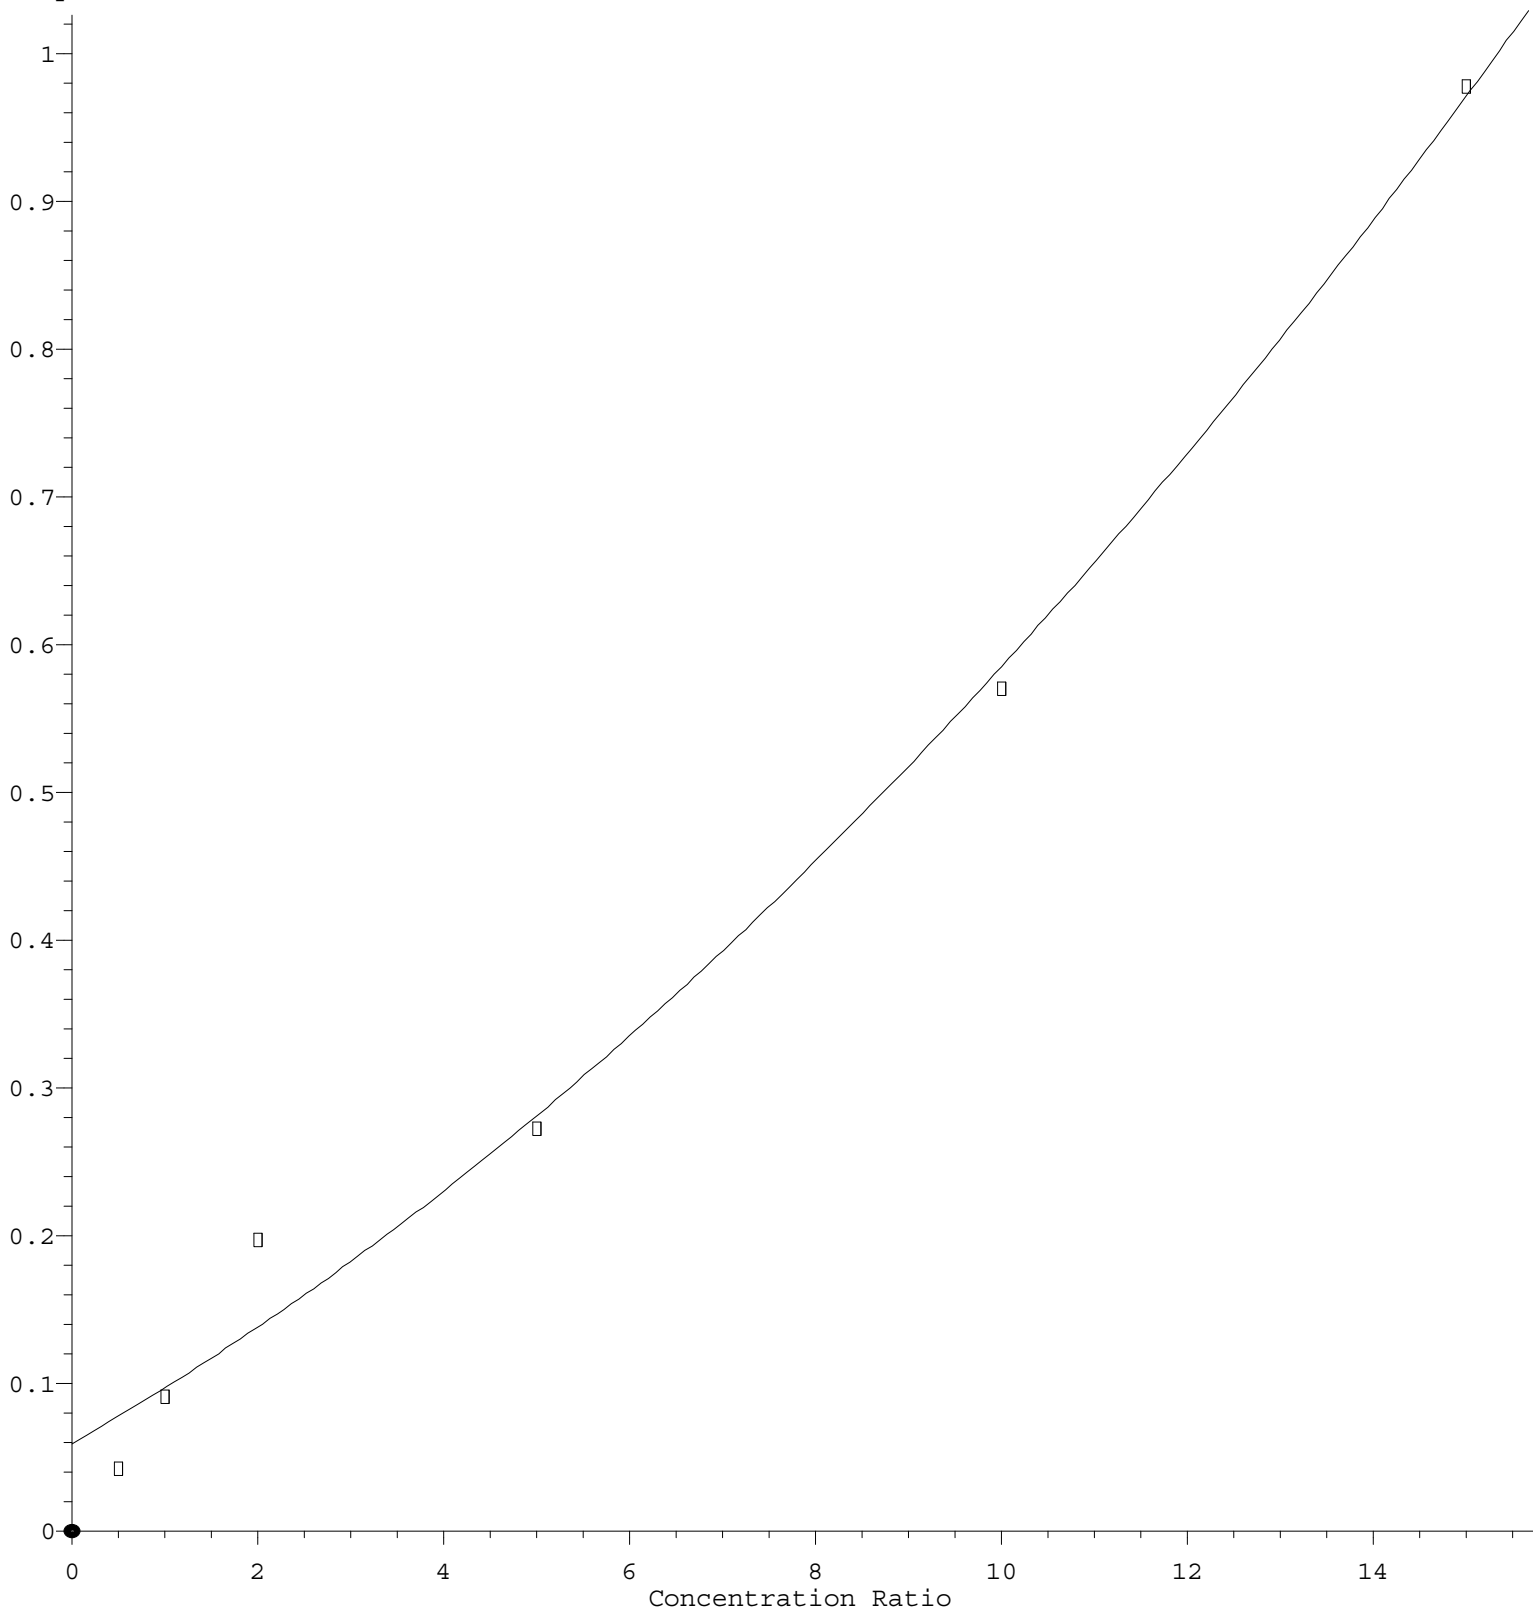

$R = 1.642e-003 A^2 + 3.615e-002 A + 5.933e-002$
 Coef of Det (r^2) = 0.991910 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D082823S.M
 Calibration Table Last Updated: Tue Aug 29 02:15:23 2023