
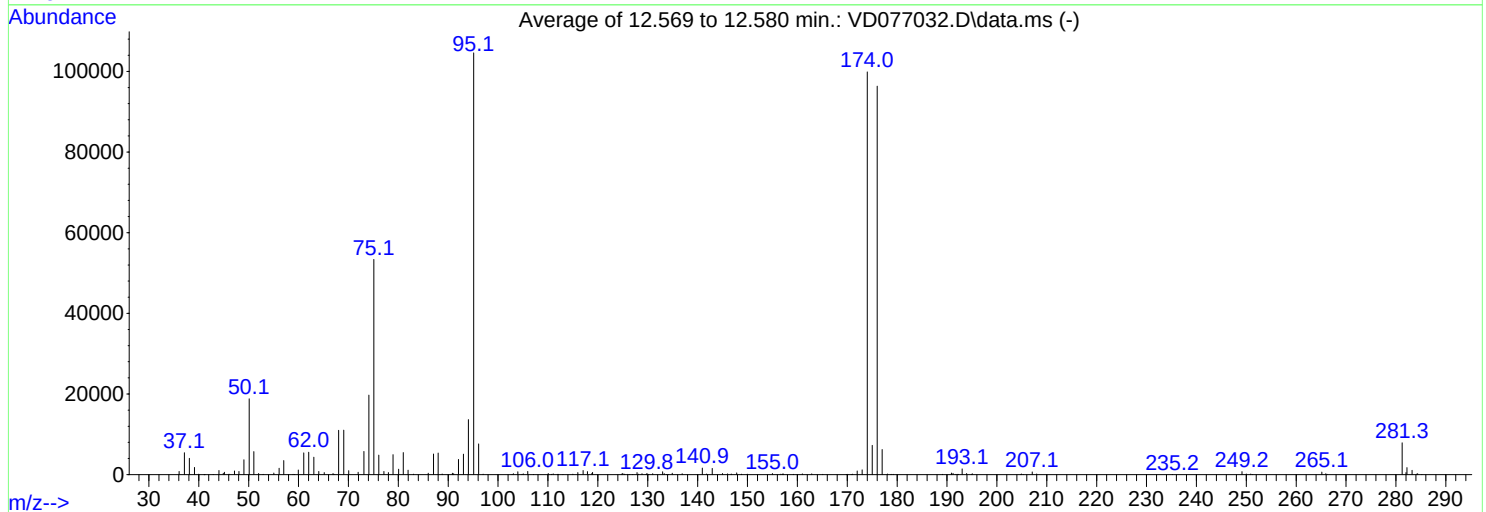


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD082823\
Data File : VD077032.D
Acq On : 28 Aug 2023 08:59
Operator : JC/SY
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D082823S.M
Title : SW846 8260
Last Update : Tue Aug 29 02:15:23 2023

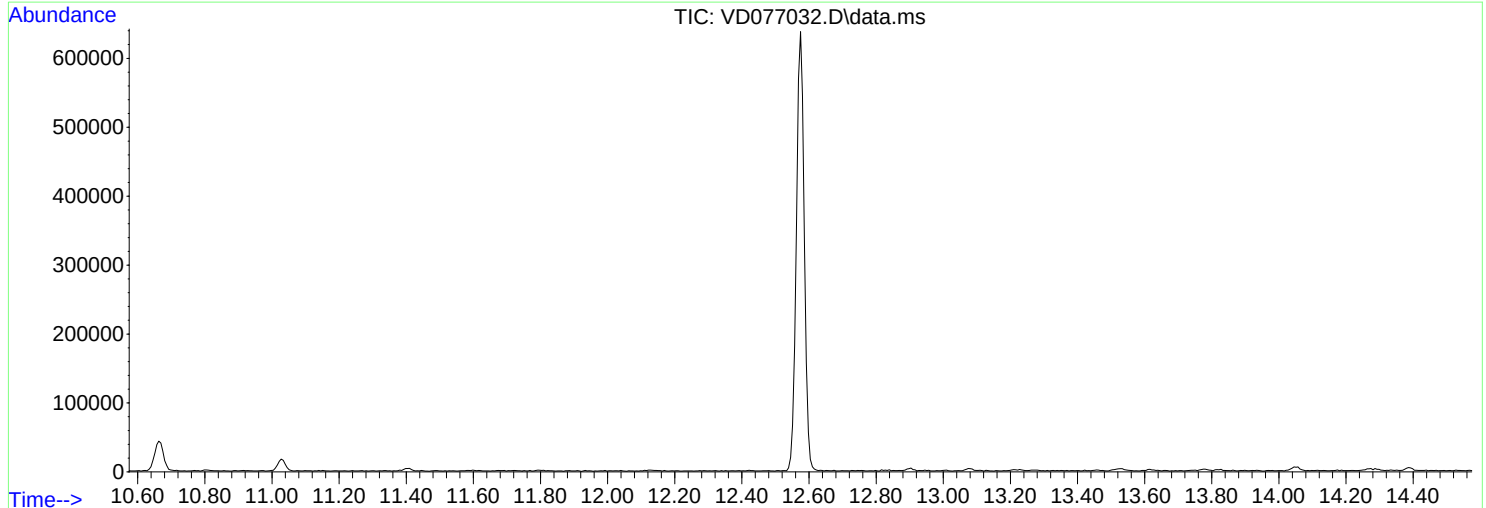

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	18822	PASS
75	95	30	60	51.0	53371	PASS
95	95	100	100	100.0	104605	PASS
96	95	5	9	7.3	7619	PASS
173	174	0.00	2	1.2	1186	PASS
174	95	50	100	95.5	99883	PASS
175	174	5	9	7.3	7282	PASS
176	174	95	101	96.5	96344	PASS
177	176	5	9	6.5	6218	PASS