
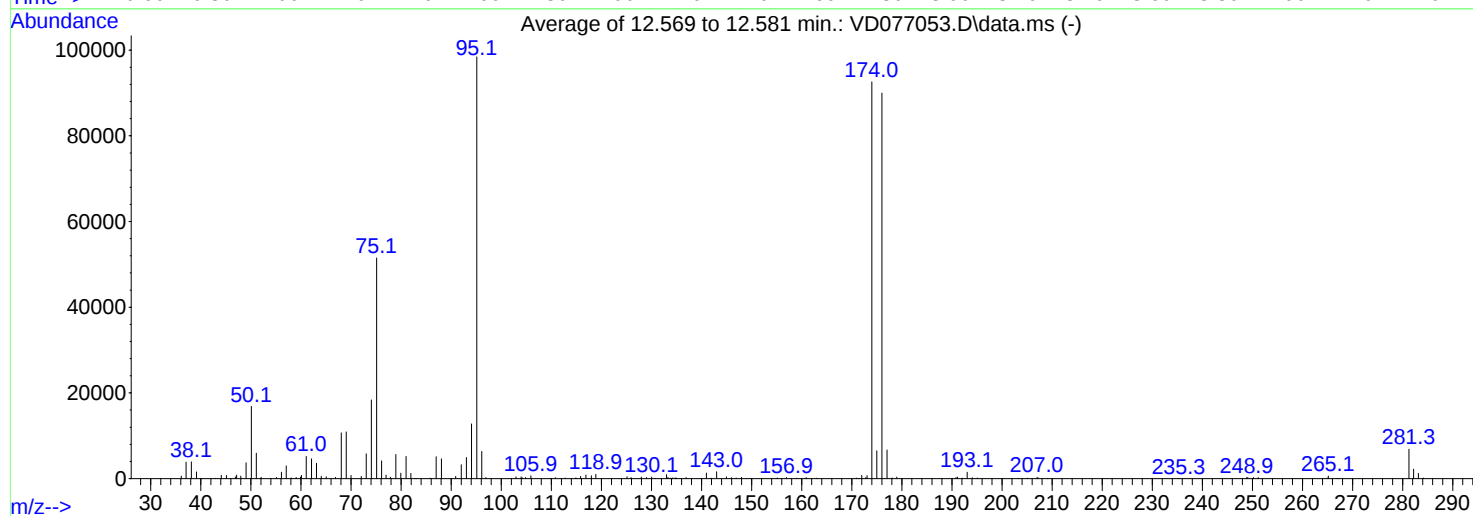


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD082923\
 Data File : VD077053.D
 Acq On : 29 Aug 2023 08:54
 Operator : JC/SY
 Sample : BFB
 Misc : 5.00G/5.0ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D082823S.M
 Title : SW846 8260
 Last Update : Tue Aug 29 02:15:23 2023

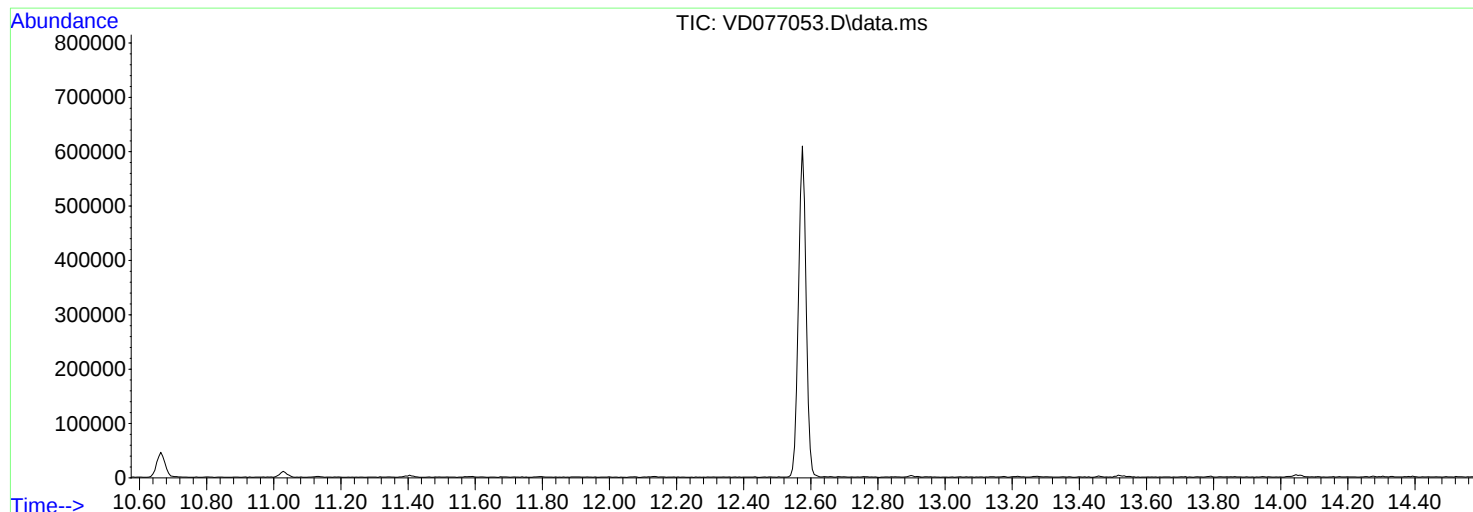

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	16877	PASS
75	95	30	60	52.3	51472	PASS
95	95	100	100	100.0	98429	PASS
96	95	5	9	6.5	6365	PASS
173	174	0.00	2	0.8	697	PASS
174	95	50	100	94.1	92584	PASS
175	174	5	9	7.0	6492	PASS
176	174	95	101	97.2	89984	PASS
177	176	5	9	7.4	6687	PASS