


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD083018\
Data File : VD059920.D
Acq On : 30 Aug 2018 10:32
Operator : JC/SY
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082218S.M
Title : SW846 8260
Last Update : Thu Aug 23 03:03:08 2018

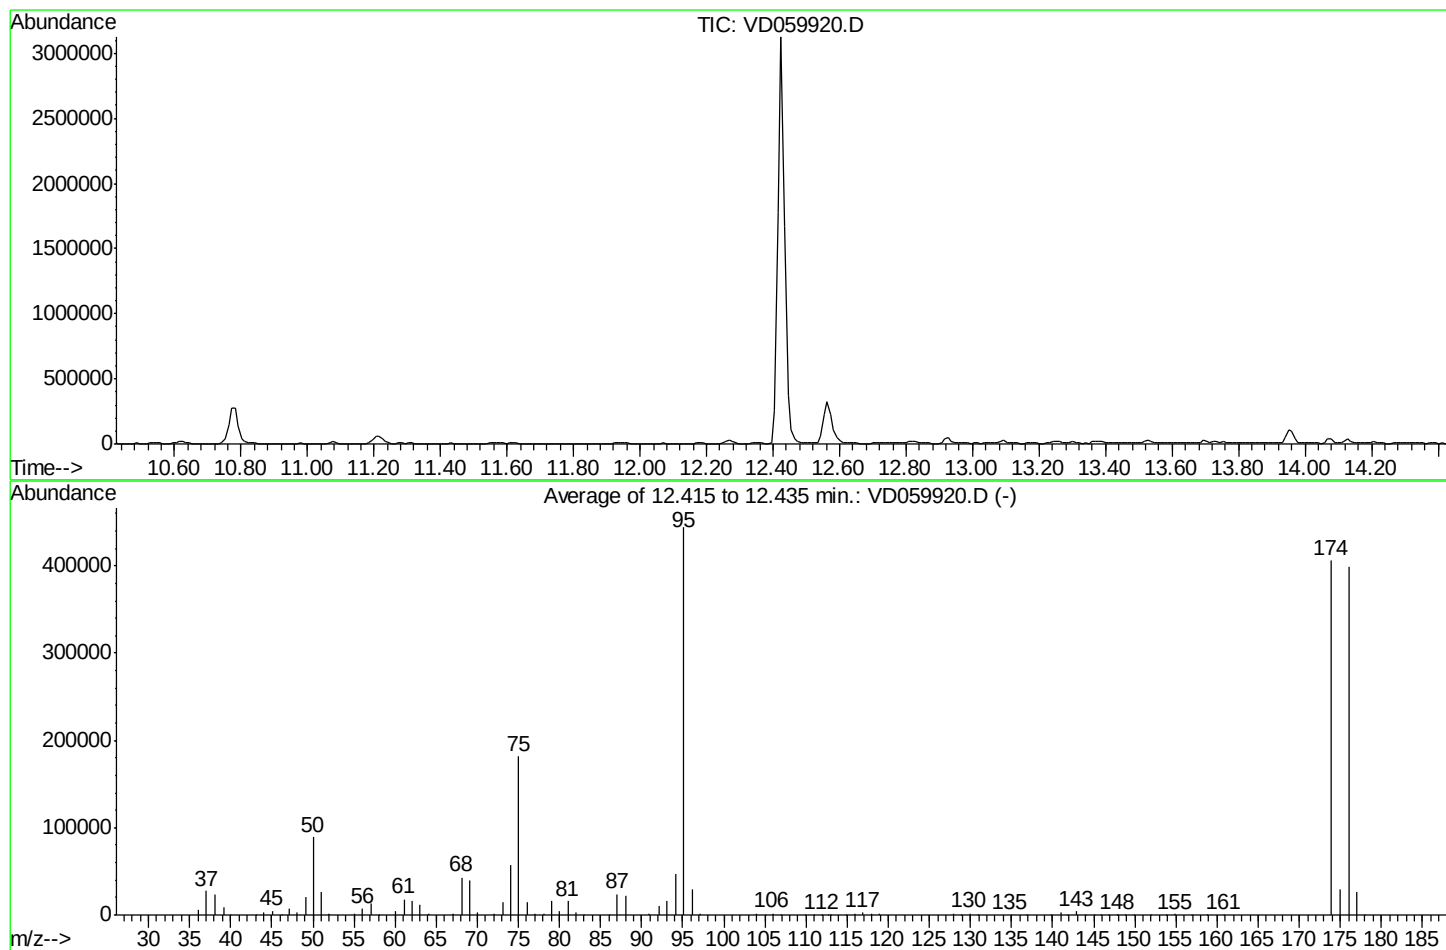

AutoFind: Scans 1239, 1240, 1241; Background Corrected with Scan 1234

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	89224	PASS
75	95	30	60	40.8	181328	PASS
95	95	100	100	100.0	444053	PASS
96	95	5	9	6.7	29624	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	91.4	405696	PASS
175	174	5	9	7.4	30077	PASS
176	174	95	101	98.1	398186	PASS
177	176	5	9	6.7	26541	PASS