


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD083120\
Data File : VD066473.D
Acq On : 31 Aug 2020 09:36
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082120S.M
Title : SW846 8260
Last Update : Fri Aug 21 13:36:12 2020

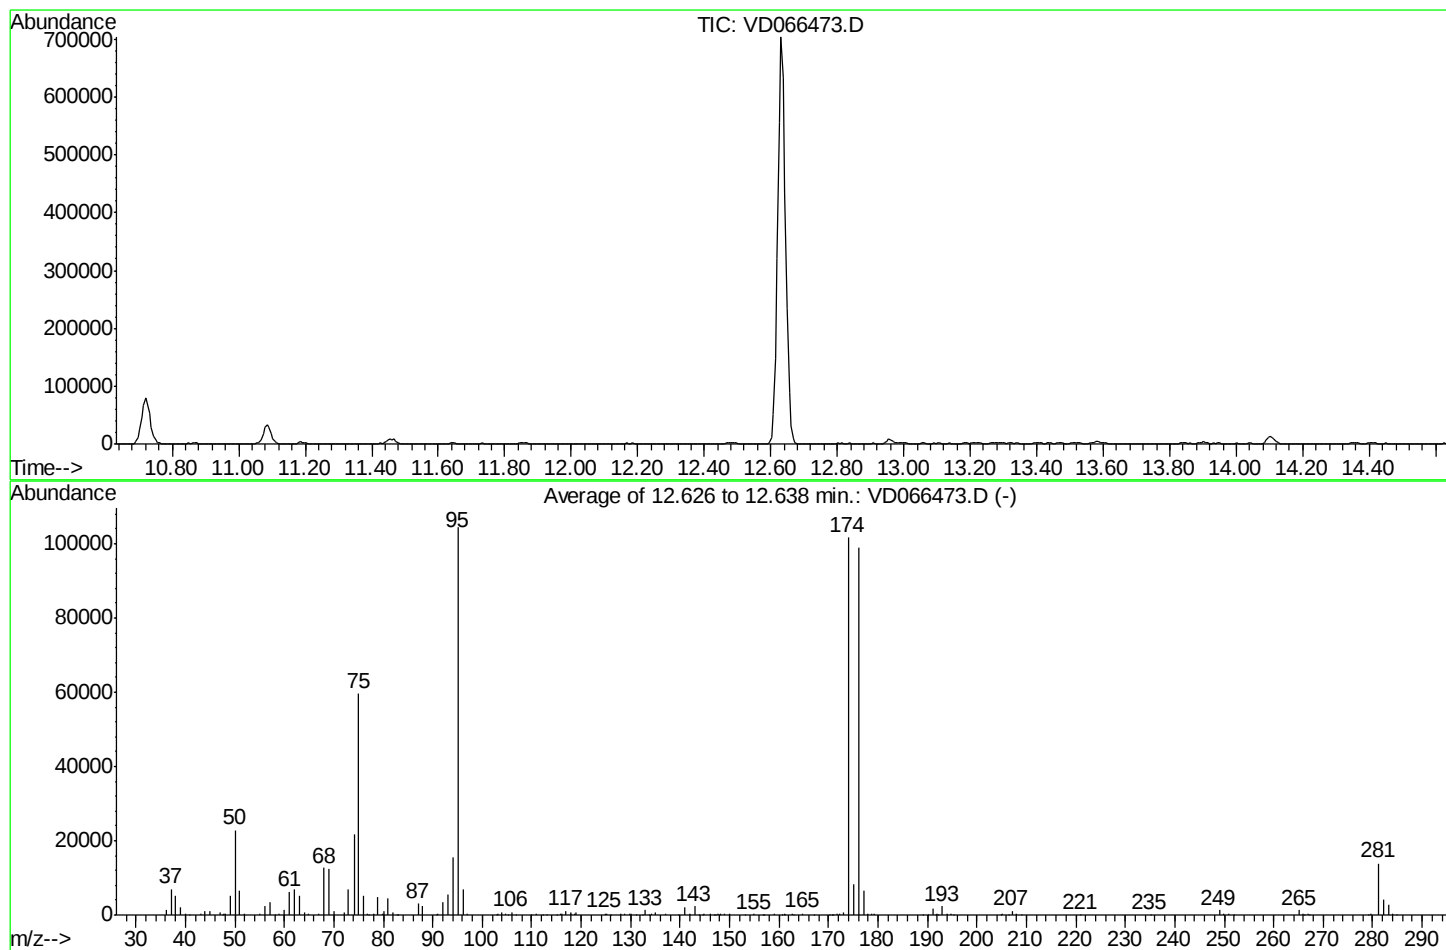

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	22821	PASS
75	95	30	60	57.0	59549	PASS
95	95	100	100	100.0	104408	PASS
96	95	5	9	6.5	6822	PASS
173	174	0.00	2	0.6	646	PASS
174	95	50	100	97.4	101690	PASS
175	174	5	9	8.1	8224	PASS
176	174	95	101	97.2	98837	PASS
177	176	5	9	6.8	6691	PASS