

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD090120\
 Data File : VD066499.D
 Acq On : 01 Sep 2020 16:39
 Operator : VA/SY
 Sample : L3851-07
 Misc : 7.49G/5.00ml/MSVOA D/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 20058

Quant Time: Sep 02 01:32:01 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082120S.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 21 13:36:12 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	165112	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.86	114	233166	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.64	117	211851	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	106588	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.33	65	90052	55.63	ug/l	0.00
Spiked Amount	50.000		Recovery	=	111.26%	
35) Dibromofluoromethane	7.91	113	72550	49.76	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.52%	
50) Toluene-d8	10.34	98	270402	50.69	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.38%	
62) 4-Bromofluorobenzene	12.63	95	91330	48.25	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.50%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD090120\
Data File : VD066499.D
Acq On : 01 Sep 2020 16:39
Operator : VA/SY
Sample : L3851-07
Misc : 7.49G/5.00ml/MSVOA D/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
20058

Quant Time: Sep 02 01:32:01 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D082120S.M
Quant Title : SW846 8260
QLast Update : Fri Aug 21 13:36:12 2020
Response via : Initial Calibration

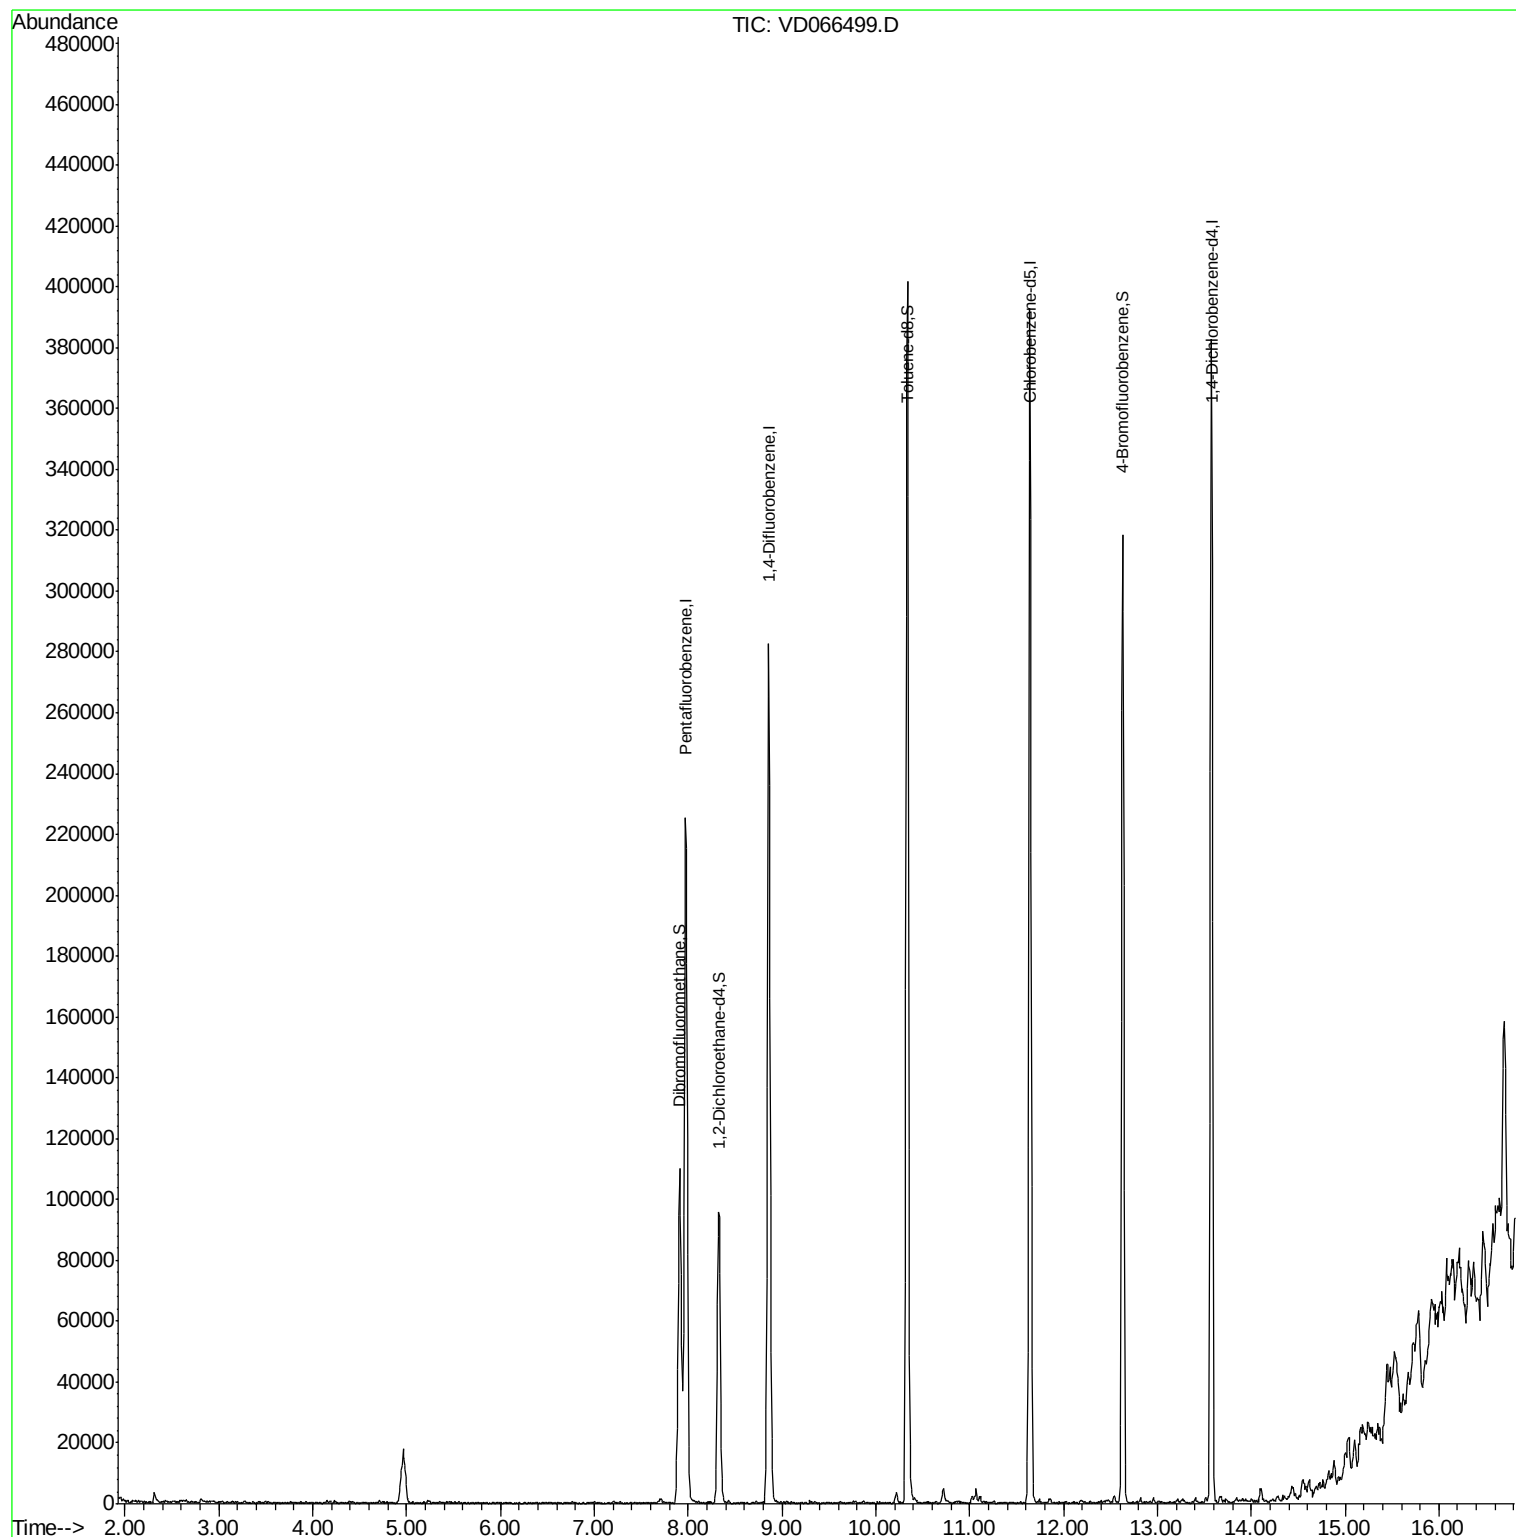

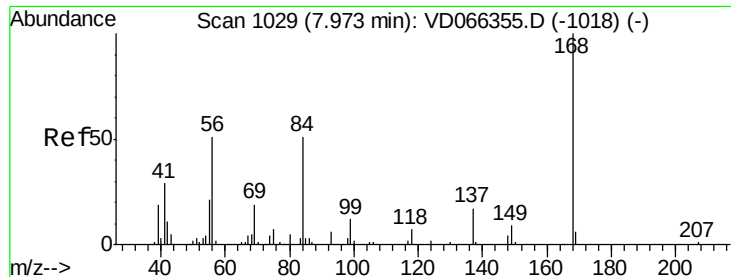

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1030

Delta R.T. 0.01 min

Lab File: VD066499.D

Acq: 01 Sep 2020 16:39

Instrument :

MSVOA_D

ClientSampleId :


20058

Tot Ion:168 Resp: 165112

Ion Ratio Lower Upper




168 100

99 59.9 45.4 68.0

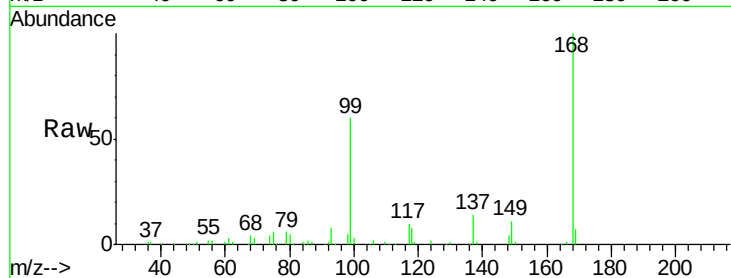

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

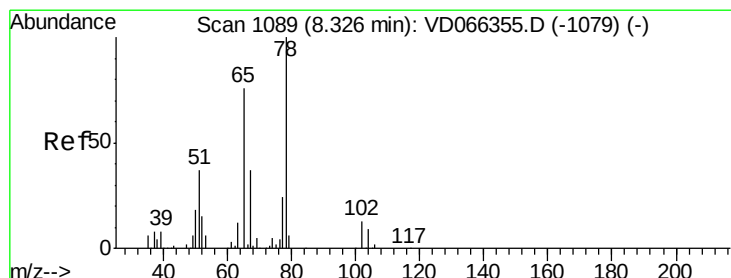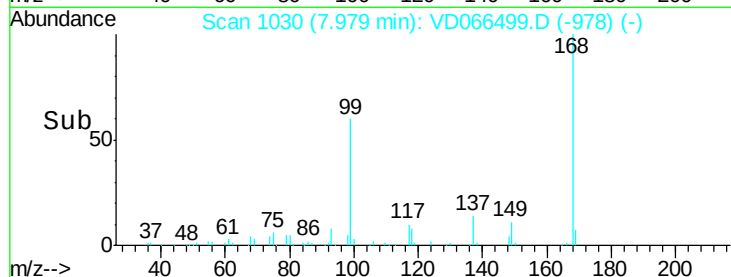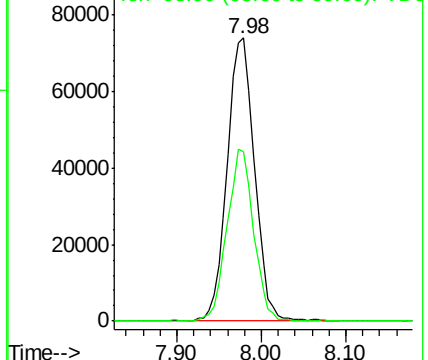

#33

1,2-Dichloroethane-d4

Concen: 55.631 ug/l

RT: 8.33 min Scan# 1089

Delta R.T. -0.00 min

Lab File: VD066499.D


Acq: 01 Sep 2020 16:39

Tgt Ion: 65 Resp: 90052

Ion Ratio Lower Upper



65 100


67 44.9 0.0 101.6

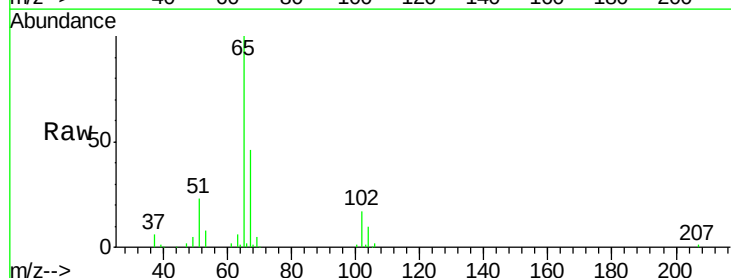

Abundance Ion 64.90 (64.60 to 65.60): VDC

Ion 66.90 (66.60 to 67.60): VDC

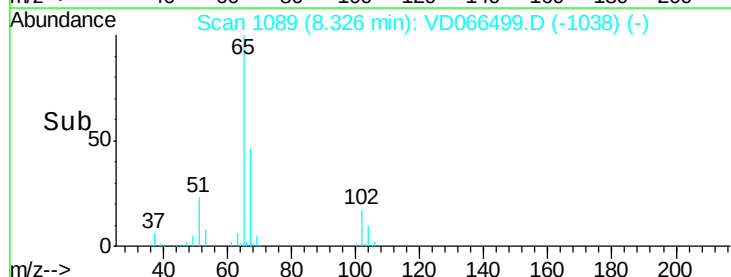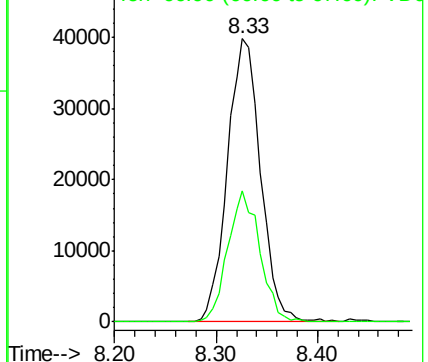


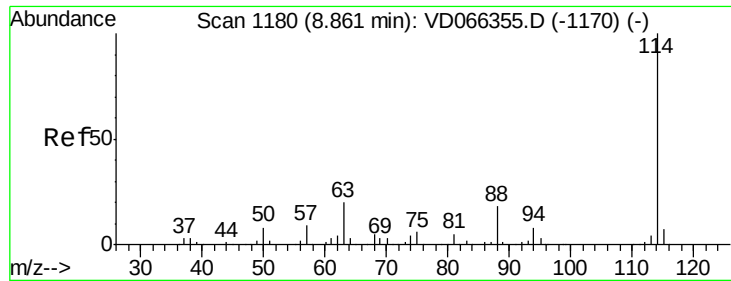




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.86 min Scan# 1180
 Delta R.T. -0.00 min
 Lab File: VD066499.D
 Acq: 01 Sep 2020 16:39

Instrument :
 MSVOA_D
 ClientSampleId :
 20058

Tot Ion:114 Resp: 233166
 Ion Ratio Lower Upper
 114 100
 63 17.7 0.0 40.8
 88 14.7 0.0 35.4

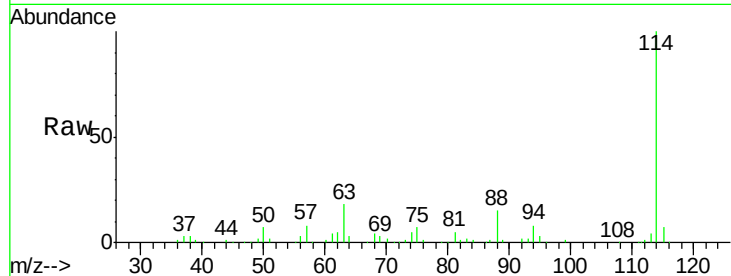


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): V
 Ion 87.90 (87.60 to 88.60): V

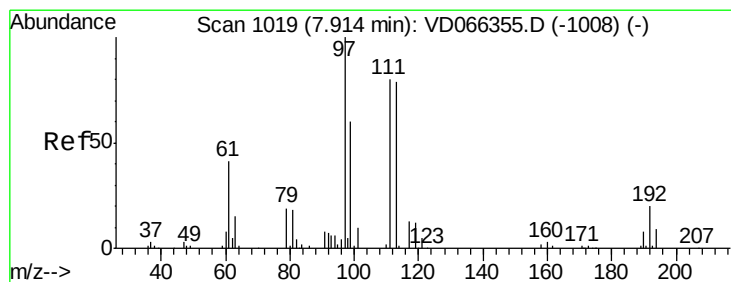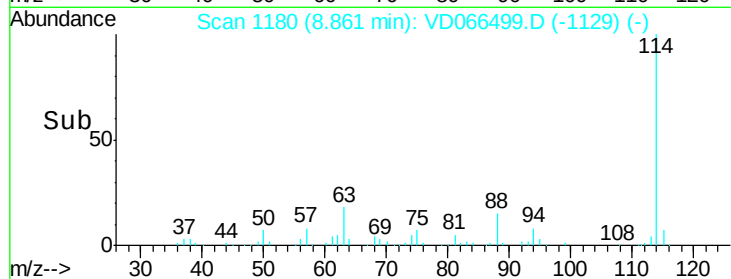
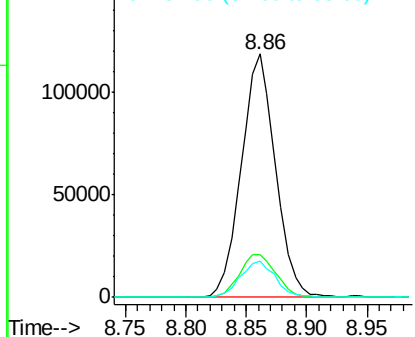



#35
 Dibromofluoromethane
 Concen: 49.760 ug/l
 RT: 7.91 min Scan# 1019
 Delta R.T. -0.00 min
 Lab File: VD066499.D
 Acq: 01 Sep 2020 16:39

Tgt Ion:113 Resp: 72550
 Ion Ratio Lower Upper
 113 100
 111 101.1 80.3 120.5
 192 24.1 19.0 28.6

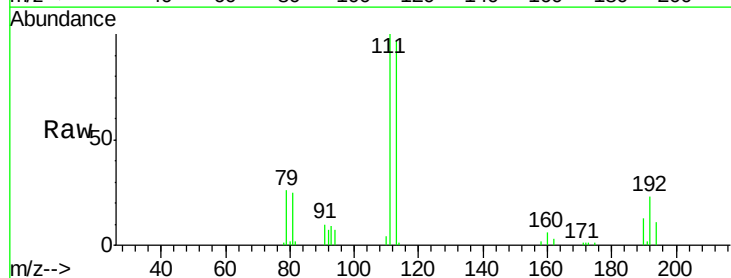

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V



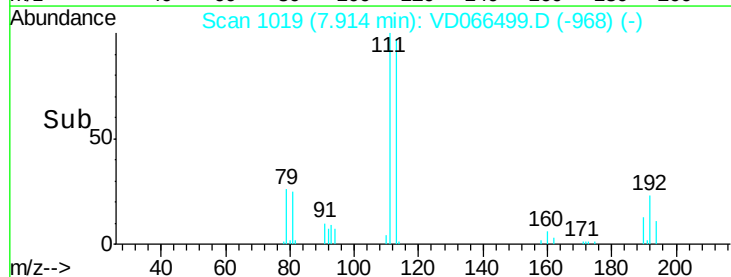
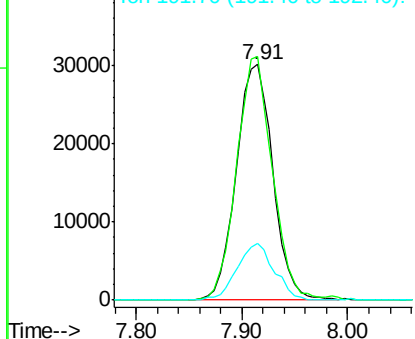


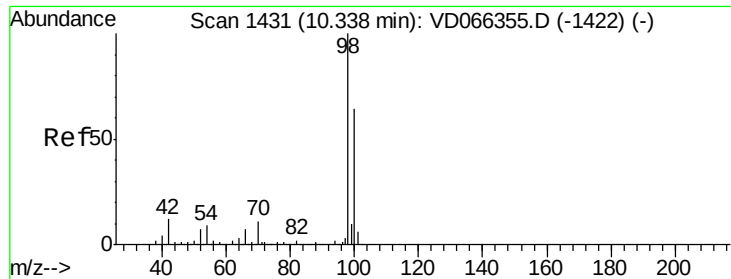

#50
Toluene-d8
Concen: 50.688 ug/l
RT: 10.34 min Scan# 1431
Delta R.T. -0.00 min
Lab File: VD066499.D
Acq: 01 Sep 2020 16:39




Instrument :
MSVOA_D
ClientSampleId :
20058


Tot Ion: 98 Resp: 270402
Ion Ratio Lower Upper
98 100
100 66.5 53.0 79.4

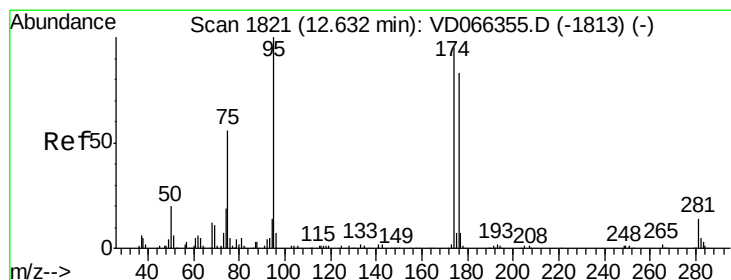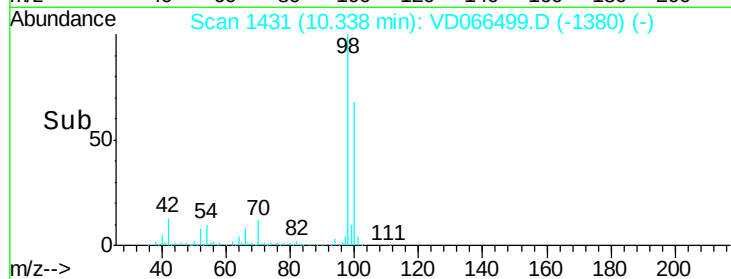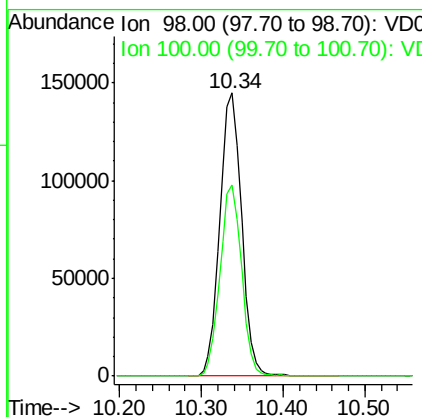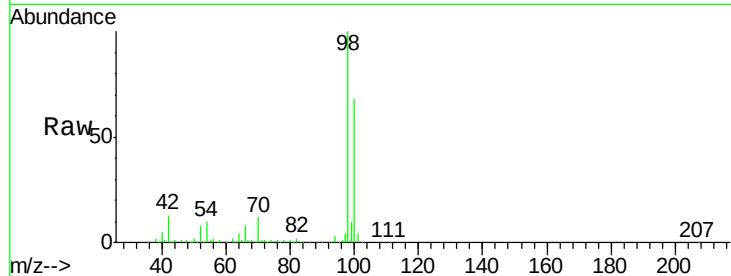

#62
4-Bromofluorobenzene
Concen: 48.247 ug/l
RT: 12.63 min Scan# 1821
Delta R.T. -0.00 min
Lab File: VD066499.D
Acq: 01 Sep 2020 16:39

Tgt Ion: 95 Resp: 91330
Ion Ratio Lower Upper
95 100
174 97.2 0.0 183.4
176 95.5 0.0 173.8


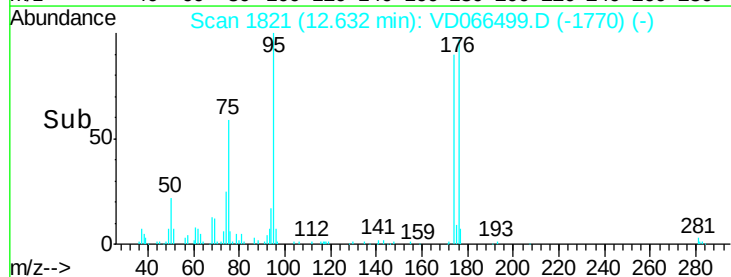
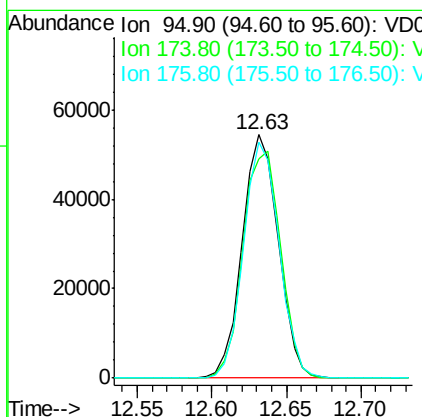
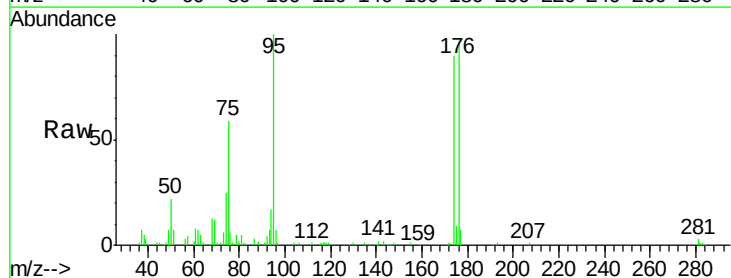


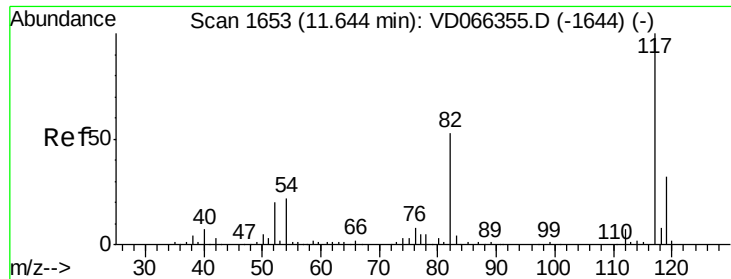

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.64 min Scan# 1653
Delta R.T. -0.00 min
Lab File: VD066499.D
Acq: 01 Sep 2020 16:39

Instrument :
MSVOA_D
ClientSampleId :
20058

Tot Ion:117 Resp: 211851
Ion Ratio Lower Upper
117 100
82 52.0 42.8 64.2
119 34.3 25.8 38.8

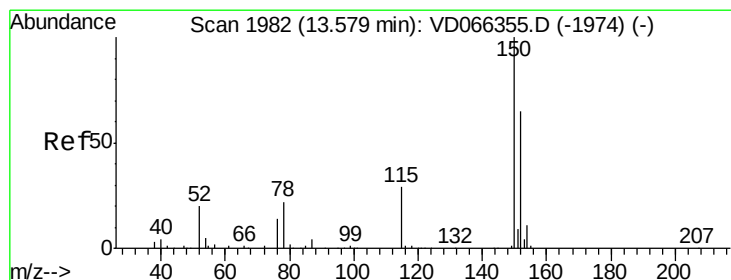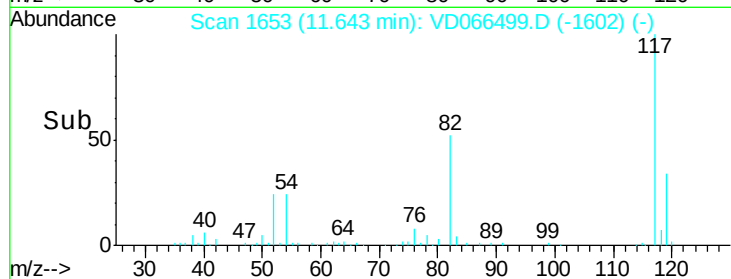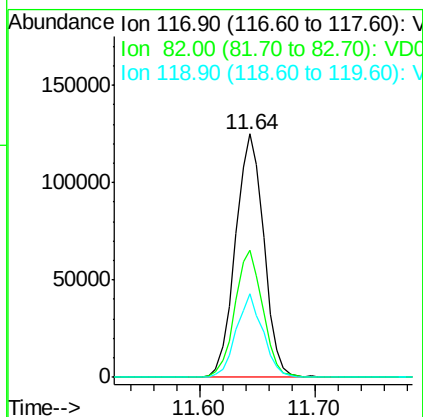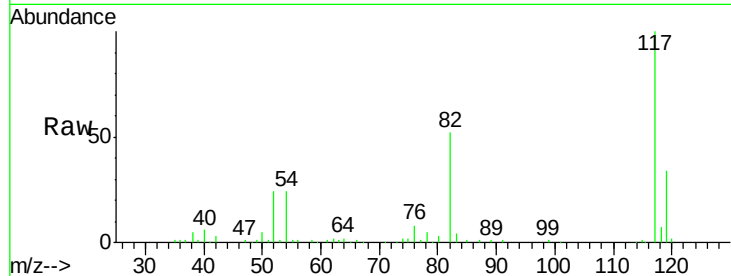

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.58 min Scan# 1982
Delta R.T. -0.00 min
Lab File: VD066499.D
Acq: 01 Sep 2020 16:39

Tgt Ion:152 Resp: 106588
Ion Ratio Lower Upper
152 100
115 55.5 28.3 85.0
150 154.4 0.0 343.2

