

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD090120\
 Data File : VD066499.D
 Acq On : 01 Sep 2020 16:39
 Operator : VA/SY
 Sample : L3851-07
 Misc : 7.49G/5.00ml/MSVOA D/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 20058

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082120S.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.961	506	517	530	rVB3	17918	54118	7.28%	1.183%
2	7.914	1008	1019	1024	rBV	109895	273115	36.72%	5.972%
3	7.973	1024	1029	1040	rVB	224668	481165	64.70%	10.521%
4	8.326	1079	1089	1100	rBV	95894	220017	29.58%	4.811%
5	8.861	1171	1180	1191	rBV	282669	567362	76.28%	12.405%
6	10.338	1423	1431	1442	rBV	401758	743741	100.00%	16.262%
7	10.720	1489	1496	1501	rBV2	4895	9775	1.31%	0.214%
8	11.643	1645	1653	1663	rBV	392808	659700	88.70%	14.424%
9	12.632	1813	1821	1832	rVB	318272	530415	71.32%	11.598%
10	13.579	1974	1982	1989	rBV	381853	634590	85.32%	13.875%
11	14.555	2142	2148	2151	rBV4	5626	11993	1.61%	0.262%
12	14.620	2155	2159	2165	rVB9	5717	11682	1.57%	0.255%
13	14.826	2187	2194	2197	rBV7	5950	10945	1.47%	0.239%
14	14.884	2200	2204	2209	rVB5	7954	13445	1.81%	0.294%
15	15.002	2218	2224	2226	rBV6	8232	13558	1.82%	0.296%
16	15.043	2226	2231	2234	rVB6	10029	17812	2.39%	0.389%
17	15.096	2236	2240	2245	rBV8	9358	16707	2.25%	0.365%
18	15.167	2247	2252	2254	rBV3	12261	20390	2.74%	0.446%
19	15.243	2263	2265	2268	rBV4	5640	7712	1.04%	0.169%
20	15.455	2291	2301	2302	rBV8	26309	59863	8.05%	1.309%
21	15.614	2326	2328	2332	rBV5	5903	7763	1.04%	0.170%
22	15.673	2334	2338	2341	rBV6	10206	17695	2.38%	0.387%
23	15.726	2344	2347	2351	rBV6	10144	21110	2.84%	0.462%
24	16.314	2445	2447	2451	rBV5	14904	20810	2.80%	0.455%
25	16.696	2507	2512	2518	rVB7	68662	148003	19.90%	3.236%


Sum of corrected areas: 4573486

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD090120\
Data File : VD066499.D
Acq On : 01 Sep 2020 16:39
Operator : VA/SY
Sample : L3851-07
Misc : 7.49G/5.00ml/MSVOA D/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
20058

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D082120S.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

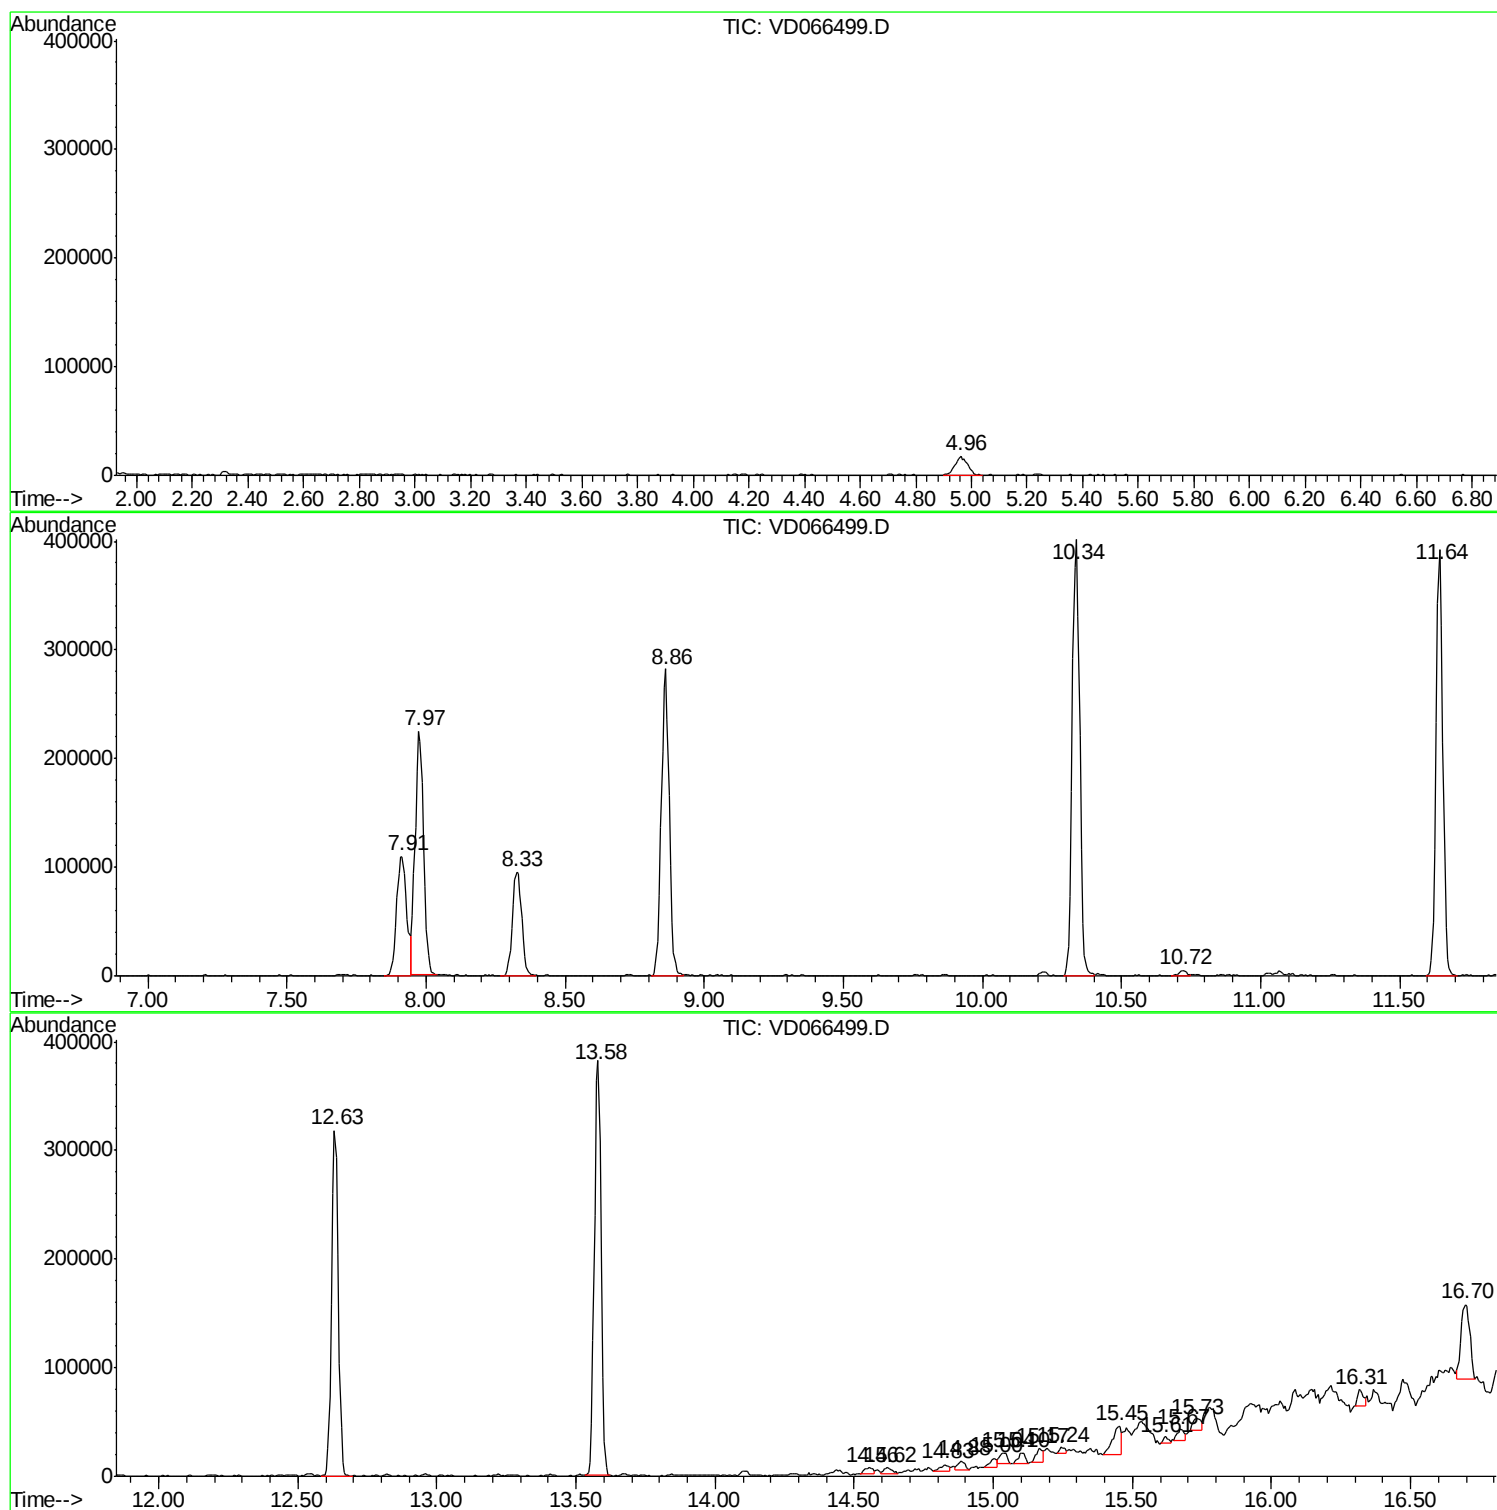

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD090120\
Data File : VD066499.D
Acq On : 01 Sep 2020 16:39
Operator : VA/SY
Sample : L3851-07
Misc : 7.49G/5.00ml/MSVOA D/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
20058










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D082120S.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown16.70 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.70	11.66 ug/l	148003	1,4-Dichlorobenzene-d4	13.58

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Cyclopentane, 1-methyl-1-(2-meth...	138	C10H18	074764-47-9	43
2		2(1H)-Naphthalenone, octahydro-4...	208	C14H24O	054594-42-2	41
3		Cyclohexene, 1,2-dimethyl-	110	C8H14	001674-10-8	38
4		Bicyclo[3.1.0]hexan-3-one, 4-met...	152	C10H16O	000471-15-8	38
5		2-Pyrimidinamine, 4,6-dimethyl-	123	C6H9N3	000767-15-7	35

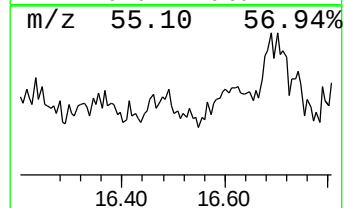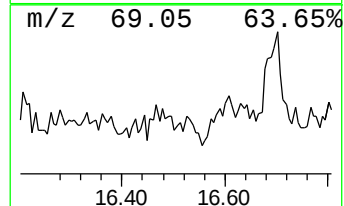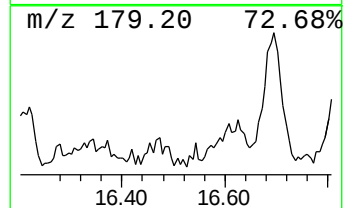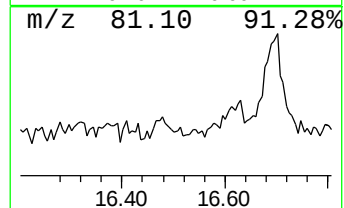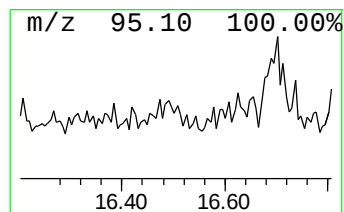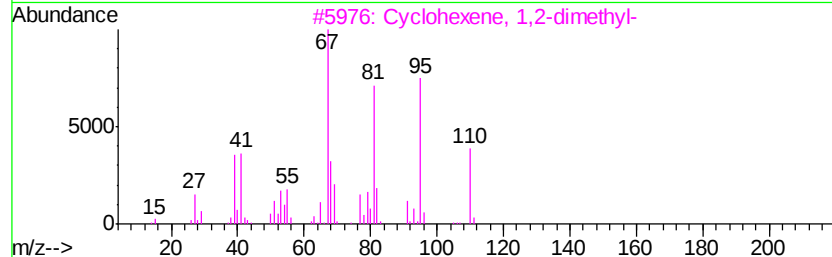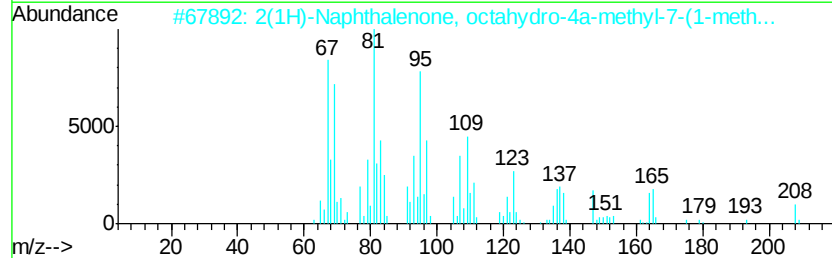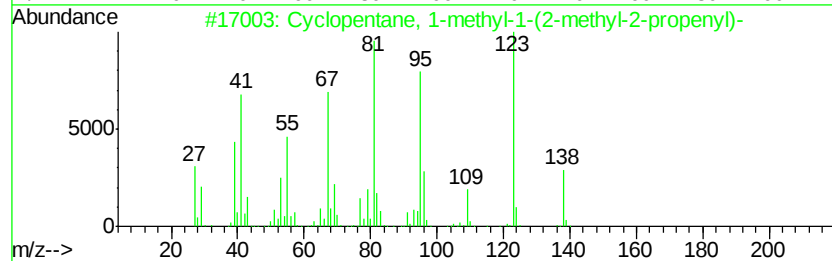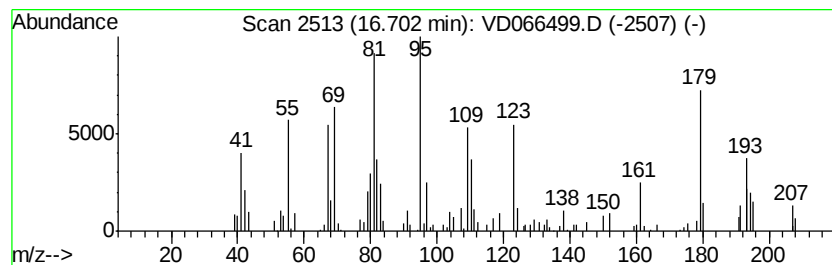

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_D\DATA\VD090120\
Data File : VD066499.D
Acq On : 01 Sep 2020 16:39
Operator : VA/SY
Sample : L3851-07
Misc : 7.49G/5.00ml/MSV0A_D/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSV0A_D
ClientSampleId :
20058

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_D\METHOD\82D082120S.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown16.70	16.70	11.7	ug/l	148003	4	13.58	634590	50.0