
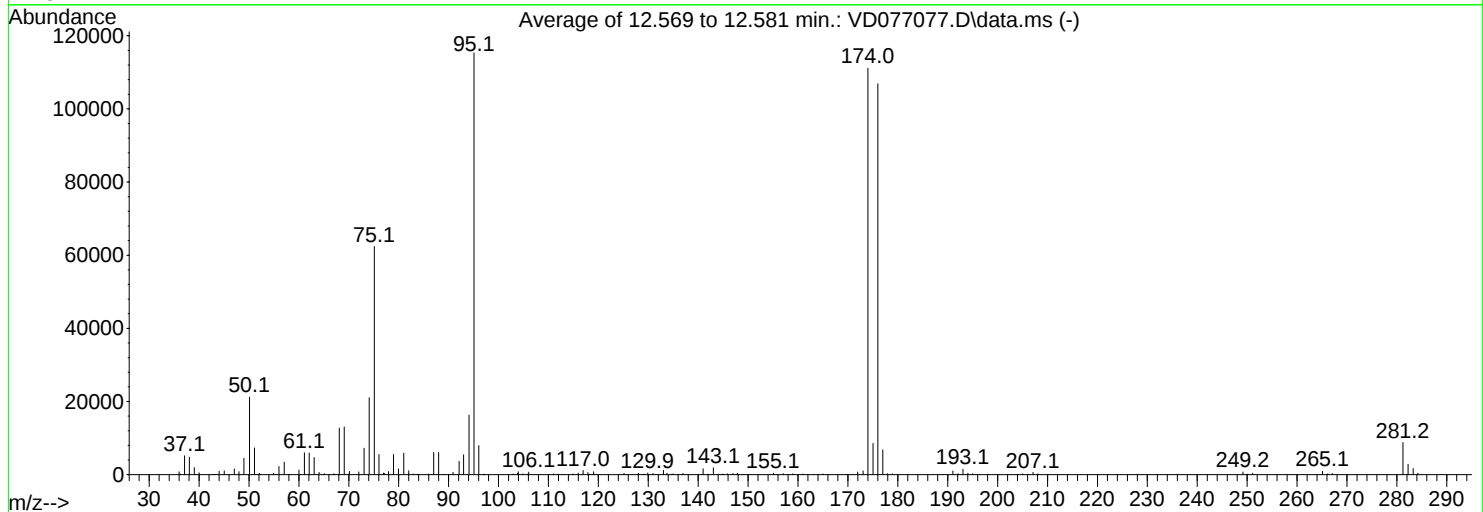


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD090123\
Data File : VD077077.D
Acq On : 01 Sep 2023 09:01
Operator : JC/SY
Sample : BFB159
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB159

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM090123SMA.M
Title : SFAM01.0
Last Update : Sat Sep 02 01:35:39 2023

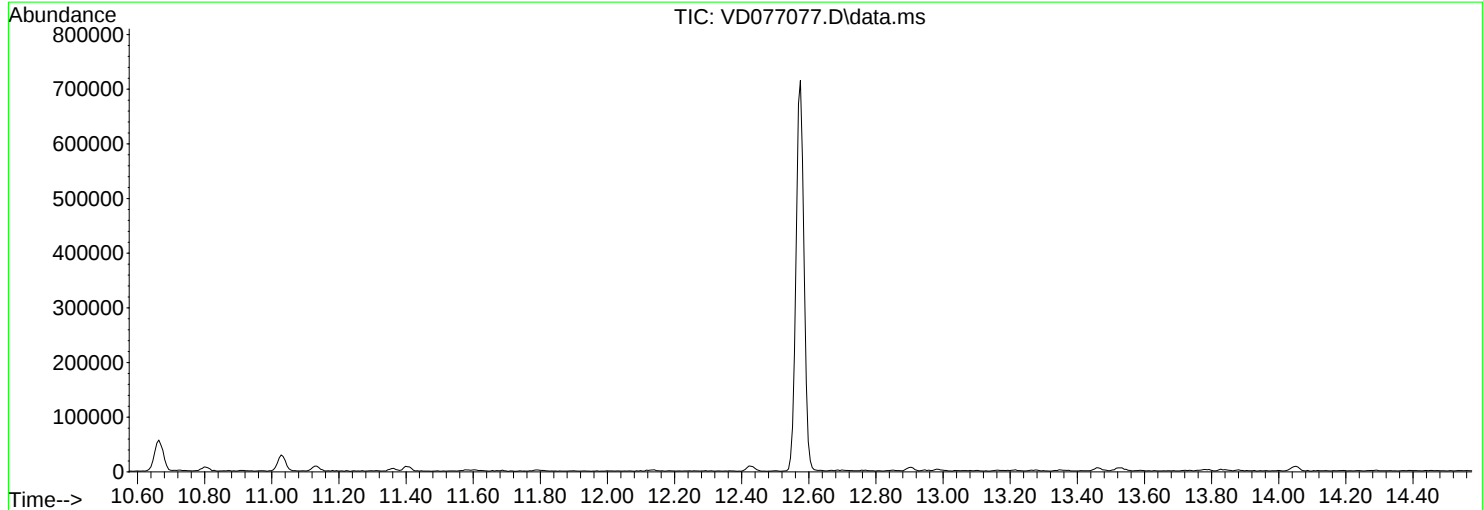

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.4	21168	PASS
75	95	30	80	54.1	62387	PASS
95	95	100	100	100.0	115331	PASS
96	95	5	9	6.9	7945	PASS
173	174	0.00	2	0.9	1012	PASS
174	95	50	120	96.4	111128	PASS
175	174	5	9	7.7	8513	PASS
176	174	95	105	96.2	106864	PASS
177	176	5	10	6.3	6764	PASS

m/z	Abundance
40.00	968.0
44.10	444.0

Instrument :
MSVOA_D
ClientSampleId :
BFB159

m/z	Abundance
36.00	1088.0
37.10	6489.0
38.10	5125.0
39.00	2103.0
40.00	1400.0
43.00	200.0
44.00	1431.0
45.00	925.0
47.10	1513.0
48.10	913.0
49.00	4639.0
50.10	22344.0
51.10	6927.0
52.10	293.0
54.90	760.0
56.00	2648.0
57.00	3434.0
60.00	1353.0
61.10	5285.0
62.10	5597.0
63.10	5040.0
64.00	793.0
64.90	262.0
66.90	395.0
68.10	13631.0
69.10	13658.0
70.20	805.0
72.00	852.0
73.00	6876.0
74.10	22048.0
75.10	65728.0
76.10	5730.0
77.00	939.0
78.00	1043.0
78.90	5726.0
79.90	1552.0
81.00	6596.0
82.10	1188.0
83.00	199.0
86.00	316.0
87.00	6168.0
88.00	6578.0
90.90	683.0
92.10	3927.0
93.00	5504.0
94.10	16784.0
95.10	121640.0
96.00	8203.0
97.00	332.0
102.80	318.0
103.80	1008.0
104.90	252.0
106.10	681.0
106.90	236.0
111.00	262.0
114.80	210.0
115.90	423.0
117.00	1024.0
117.90	723.0
119.00	771.0
125.00	381.0
126.00	153.0
127.90	441.0
129.00	196.0
129.90	500.0
130.90	408.0
133.10	739.0
133.70	244.0
135.00	396.0
136.90	396.0
141.00	1578.0
141.90	182.0
143.10	1948.0
144.10	229.0
144.90	342.0
146.90	430.0
147.80	552.0
155.00	244.0
157.00	354.0
159.00	462.0
161.00	252.0
163.20	192.0
165.20	169.0
172.00	709.0
173.00	1085.0
174.00	116568.0
175.00	8512.0
176.00	108432.0
177.00	6754.0
177.90	346.0
191.00	806.0
192.10	176.0

Instrument :
MSVOA_D
ClientSampleId :
BFB159

193.00	1199.0
194.10	509.0
195.10	199.0
207.10	525.0
208.10	159.0
249.20	570.0
251.20	258.0
265.10	854.0
266.10	274.0
267.10	286.0
281.20	6279.0
282.20	2282.0
283.20	1525.0
284.30	311.0

Instrument :
MSVOA_D
ClientSampleId :
BFB159

m/z	Abundance
36.00	1255.0
37.10	5170.0
38.00	5203.0
39.10	2395.0
40.00	1496.0
44.00	1530.0
45.00	1331.0
47.10	1816.0
47.90	770.0
49.00	5248.0
50.10	23008.0
51.10	8335.0
52.00	558.0
55.20	281.0
56.00	2029.0
57.10	4036.0
58.00	234.0
59.90	1470.0
61.10	7305.0
62.00	6639.0
63.00	5101.0
64.10	482.0
65.10	294.0
67.10	359.0
68.10	14421.0
69.10	14612.0
70.10	764.0
72.00	859.0
73.10	8311.0
74.10	22712.0
75.10	66576.0
76.00	6323.0
77.20	742.0
77.80	860.0
79.00	5847.0
80.00	1776.0
81.00	6645.0
81.90	1078.0
82.90	158.0
83.80	152.0
85.90	163.0
87.10	7592.0
88.00	5871.0
89.00	161.0
90.90	605.0
92.10	4319.0
93.00	5476.0
94.10	18240.0
95.10	127640.0
96.10	8667.0
97.20	453.0
103.00	220.0
104.00	1374.0
104.90	439.0
106.00	883.0
111.00	307.0
115.00	322.0
115.90	516.0
116.90	1186.0
117.90	587.0
119.00	735.0
125.20	460.0
128.10	581.0
129.20	360.0
130.00	454.0
131.00	245.0
133.10	1618.0
133.70	658.0
134.70	460.0
135.90	171.0
137.00	343.0
141.00	2147.0
142.10	160.0
143.00	2040.0
145.10	280.0
145.80	181.0
147.00	185.0
148.00	215.0
155.10	564.0
157.10	284.0
158.80	214.0
165.00	244.0
170.90	246.0
171.90	791.0
173.00	1054.0
174.00	119440.0
175.00	10037.0
176.00	117568.0
177.00	7602.0
178.00	487.0
178.90	309.0
191.10	1049.0

Instrument :
MSVOA_D
ClientSampleId :
BFB159

192.10	324.0
193.10	1698.0
194.10	389.0
195.10	184.0
205.00	408.0
207.10	762.0
208.20	154.0
249.20	1012.0
251.10	526.0
265.10	704.0
266.20	245.0
267.10	428.0
281.20	9586.0
282.30	3129.0
283.20	1580.0
284.20	309.0

Instrument :
MSVOA_D
ClientSampleId :
BFB159

m/z	Abundance
36.20	562.0
37.10	3866.0
38.10	3984.0
39.10	1330.0
40.00	1579.0
43.20	151.0
44.00	1076.0
45.10	956.0
47.00	1442.0
48.00	852.0
49.00	3542.0
50.10	18152.0
51.10	6705.0
52.00	198.0
54.90	373.0
56.00	1972.0
57.00	2777.0
60.10	987.0
61.10	5424.0
62.10	5481.0
63.10	3960.0
64.10	589.0
65.10	500.0
67.00	330.0
68.10	10178.0
69.10	10855.0
70.00	1016.0
72.00	489.0
73.10	6530.0
74.10	18336.0
75.10	54856.0
76.00	4517.0
76.90	324.0
77.20	306.0
78.00	649.0
79.00	5010.0
80.00	1365.0
81.00	4297.0
82.00	878.0
82.80	173.0
83.80	187.0
86.90	4419.0
88.00	5684.0
90.90	591.0
92.10	2659.0
93.00	5359.0
94.10	13810.0
95.10	96712.0
96.10	6966.0
103.10	235.0
103.90	955.0
105.80	460.0
106.10	492.0
110.10	167.0
111.90	364.0
112.90	203.0
114.90	224.0
116.00	402.0
117.00	1255.0
117.90	373.0
118.30	442.0
119.10	924.0
119.80	179.0
125.10	642.0
128.00	445.0
129.00	179.0
129.80	321.0
131.00	233.0
132.90	1184.0
133.80	315.0
135.00	316.0
136.90	299.0
141.00	1172.0
142.10	285.0
143.00	1680.0
144.00	152.0
144.70	244.0
145.90	466.0
147.10	328.0
147.90	648.0
149.00	194.0
150.10	297.0
155.00	351.0
157.00	188.0
161.00	242.0
165.00	151.0
171.90	619.0
173.10	898.0
174.00	97376.0
175.10	6989.0
176.00	94592.0
177.00	5936.0

Instrument :
MSVOA_D
ClientSampleId :
BFB159

179.00	367.0
189.00	213.0
191.00	1195.0
192.10	300.0
193.00	1594.0
194.00	322.0
194.90	379.0
205.00	307.0
207.10	531.0
208.10	327.0
249.10	634.0
250.10	350.0
251.00	415.0
265.10	1249.0
266.10	166.0
267.00	284.0
281.20	10584.0
282.20	3125.0
283.30	1840.0
284.10	518.0
285.00	193.0

Instrument :
MSVOA_D
ClientSampleId :
BFB159