



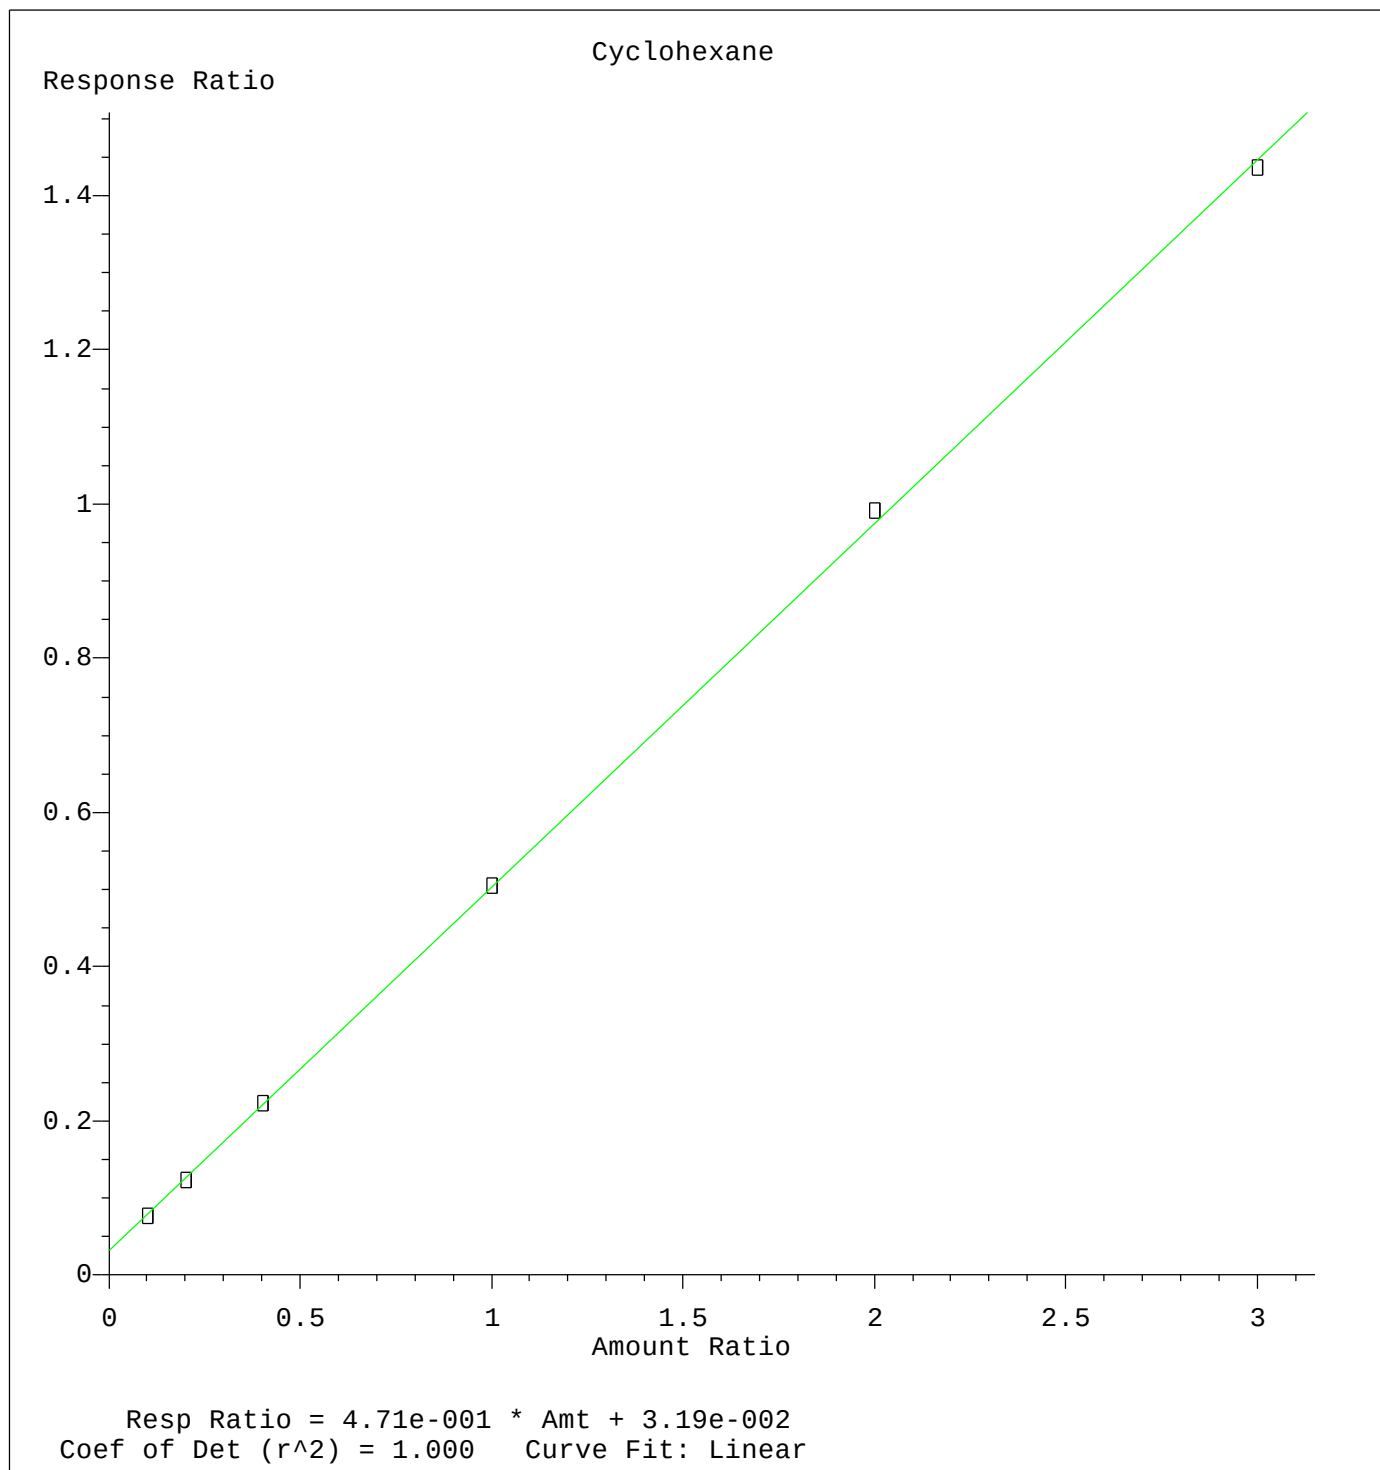

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D090220S.M
Calibration Table Last Updated: Wed Sep 02 15:08:44 2020


Methylene Chloride

Response Ratio

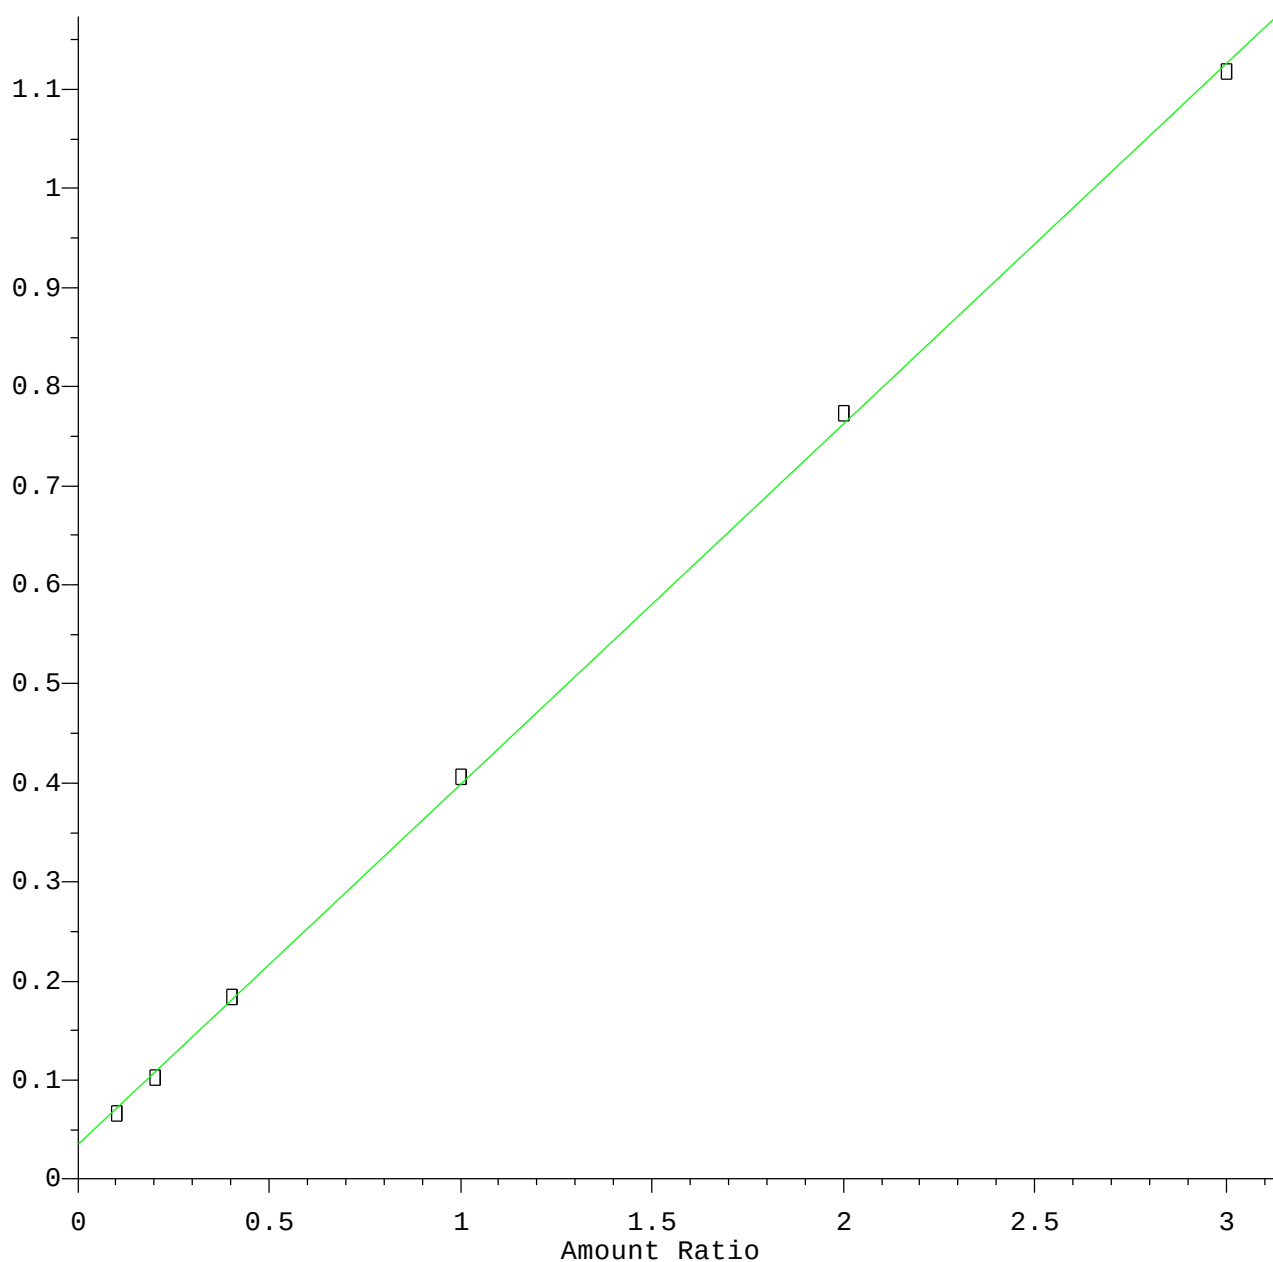

Resp Ratio = $3.64 \times 10^{-1} \times \text{Amt} + 3.46 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D090220S.M
Calibration Table Last Updated: Wed Sep 02 15:08:44 2020

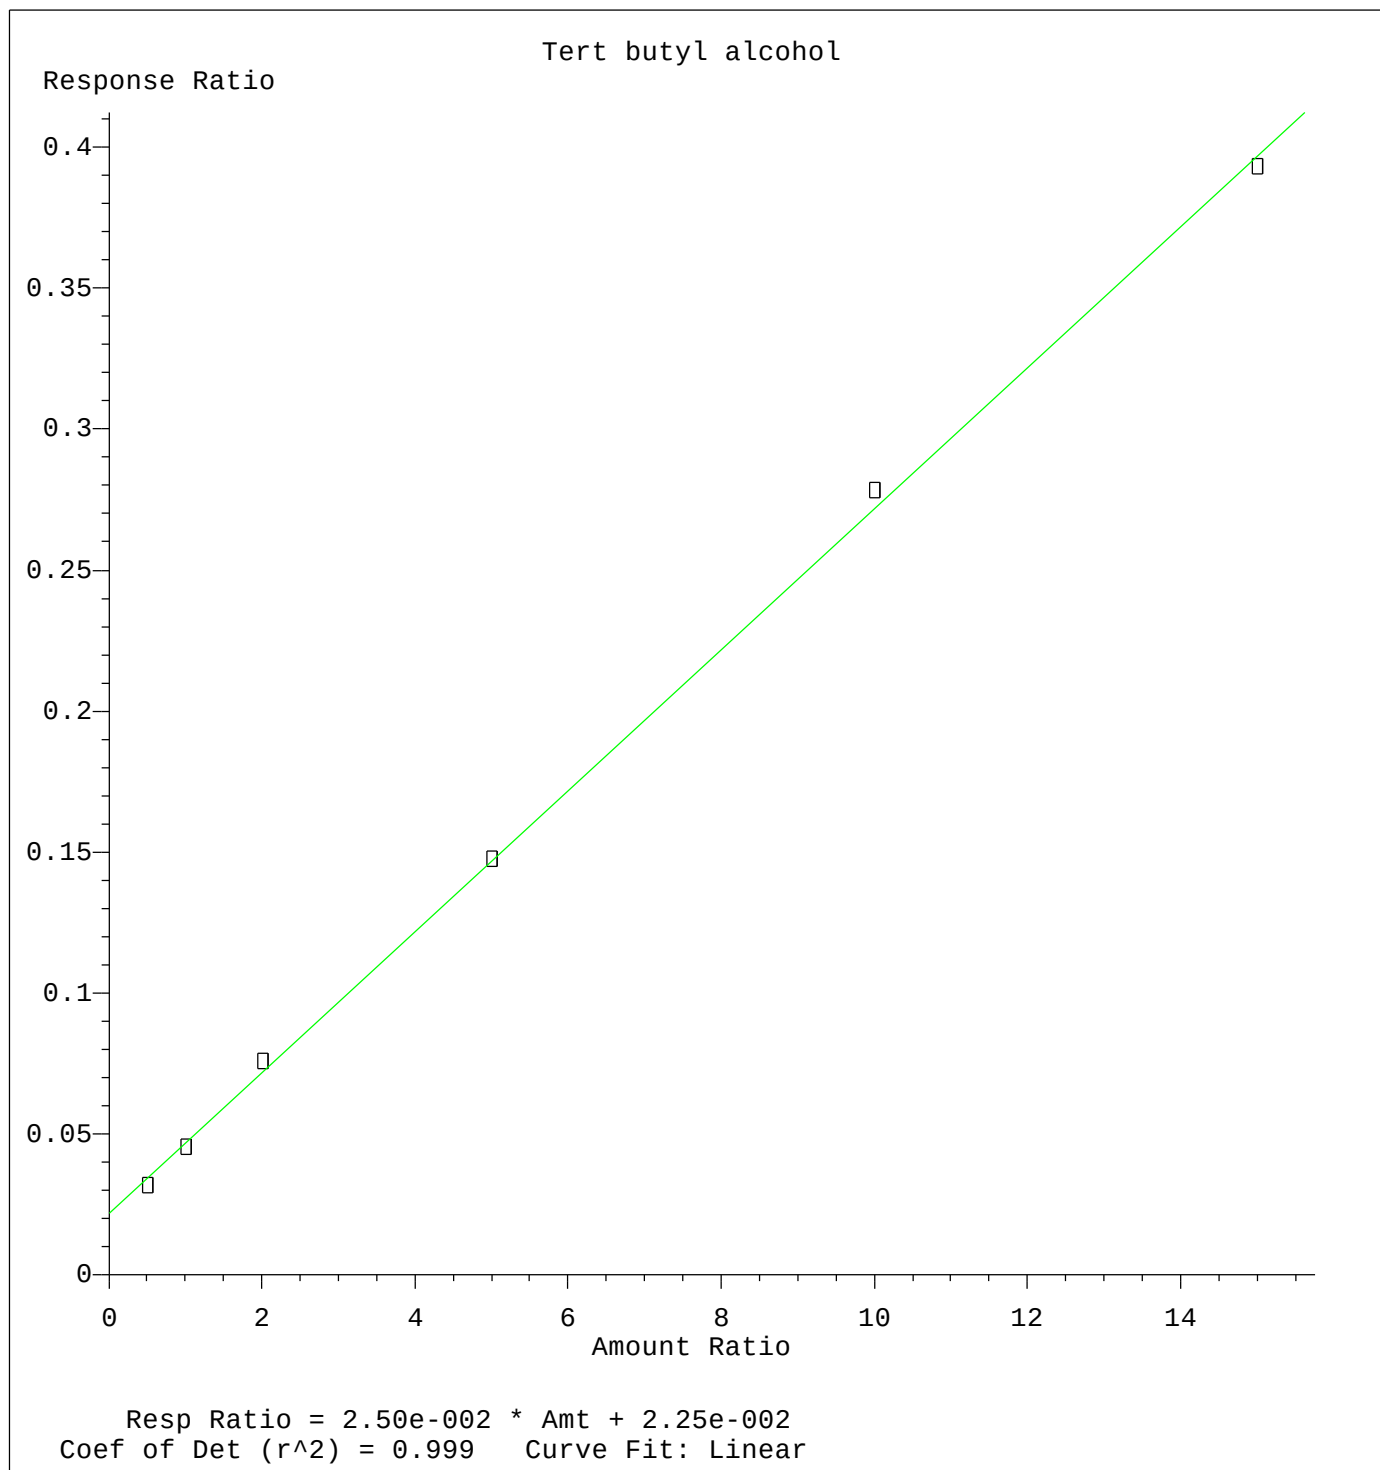

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D090220S.M
Calibration Table Last Updated: Wed Sep 02 15:08:44 2020