



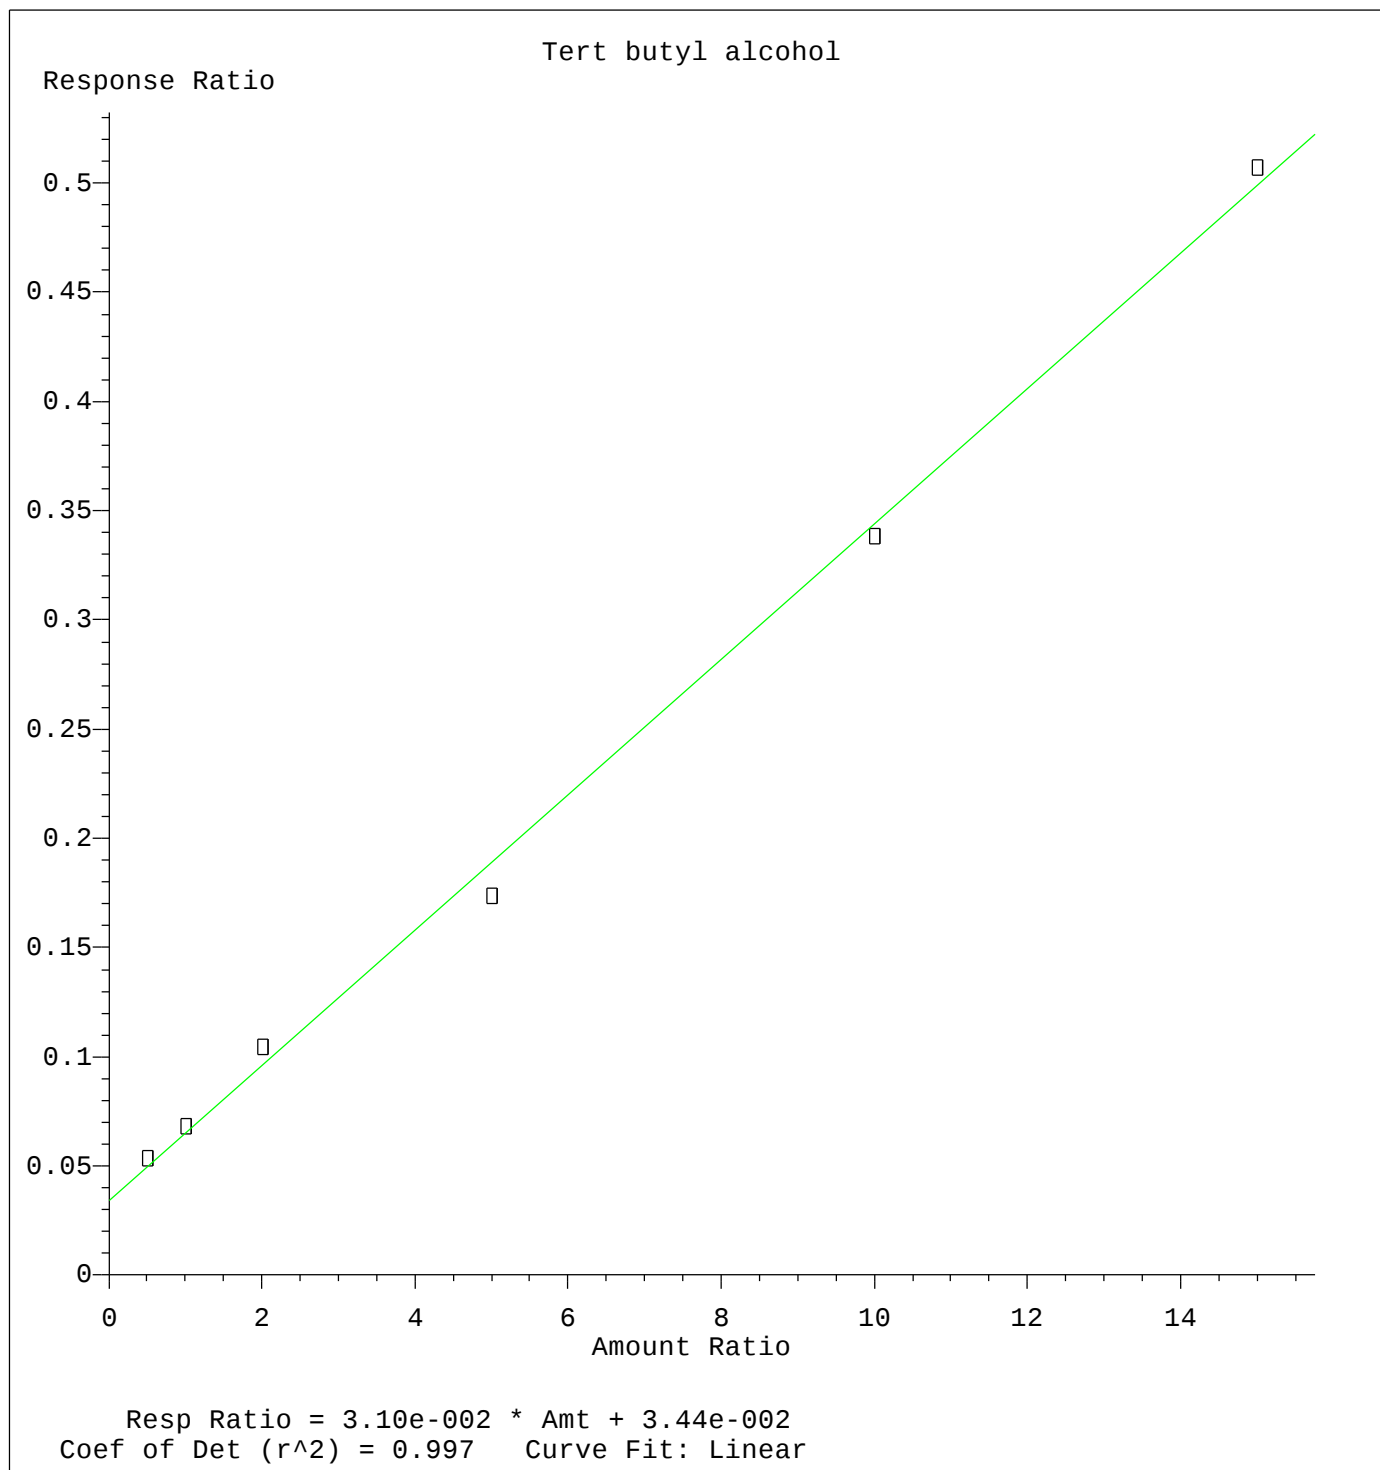

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D090320S.M
Calibration Table Last Updated: Fri Sep 04 01:57:04 2020

Methylene Chloride

Response Ratio

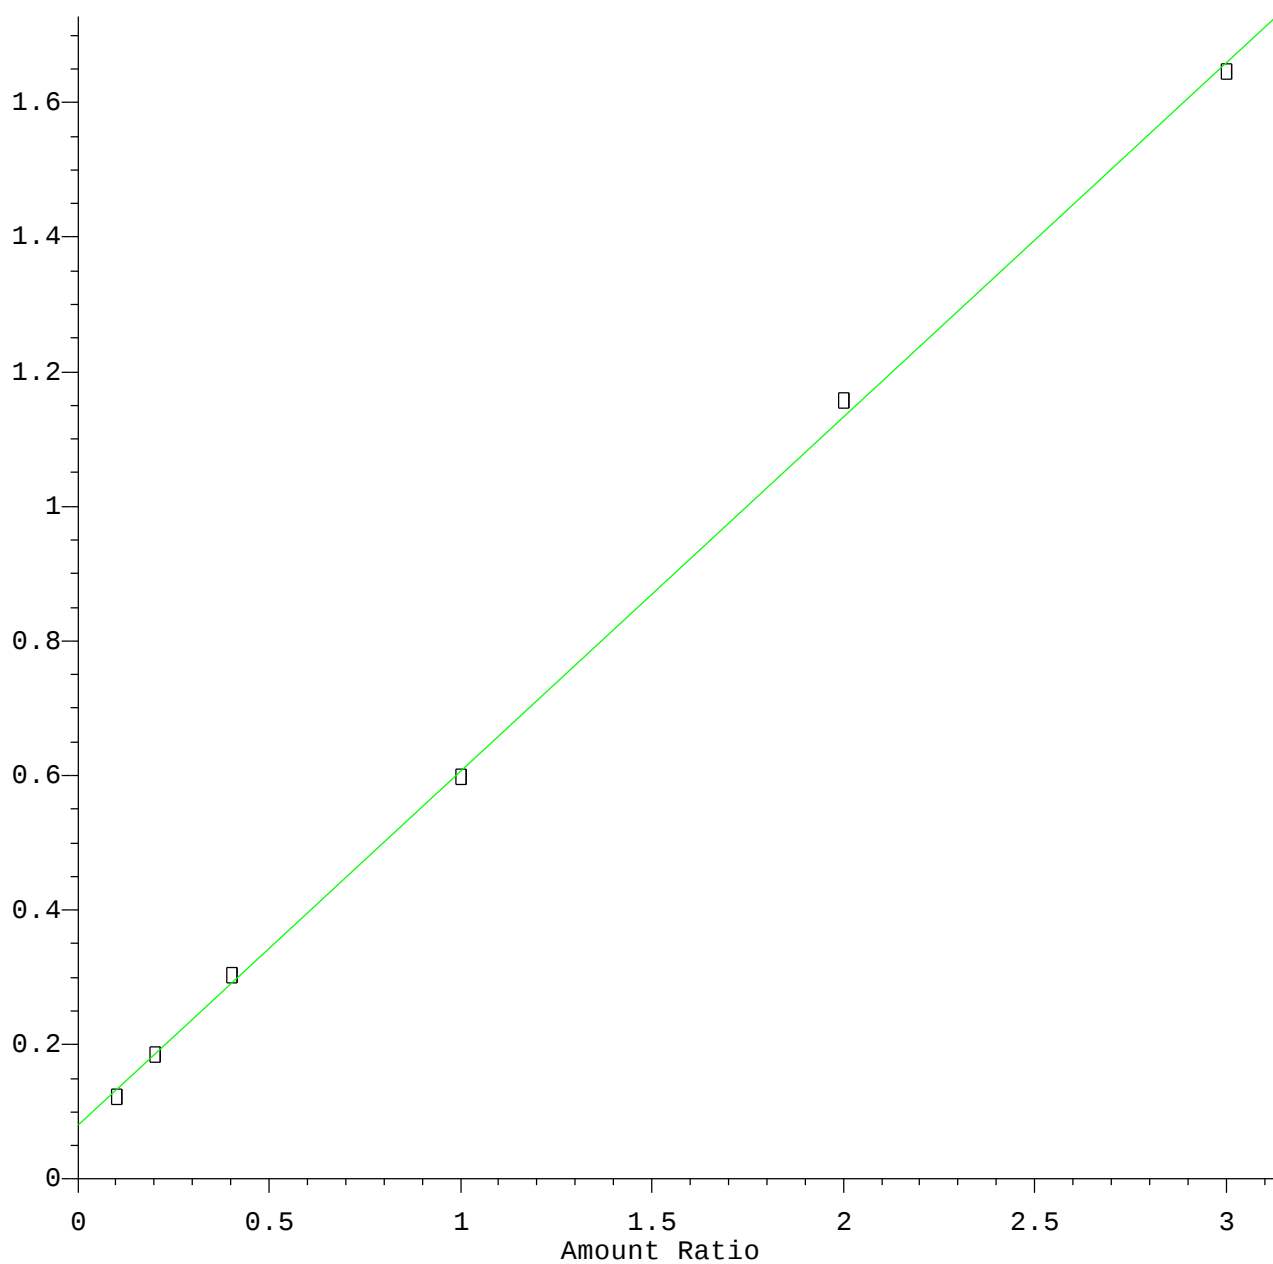


Resp Ratio = 5.26e-001 * Amt + 8.03e-002
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D090320S.M
Calibration Table Last Updated: Fri Sep 04 01:57:04 2020


Dichlorodifluoromethane

Response Ratio

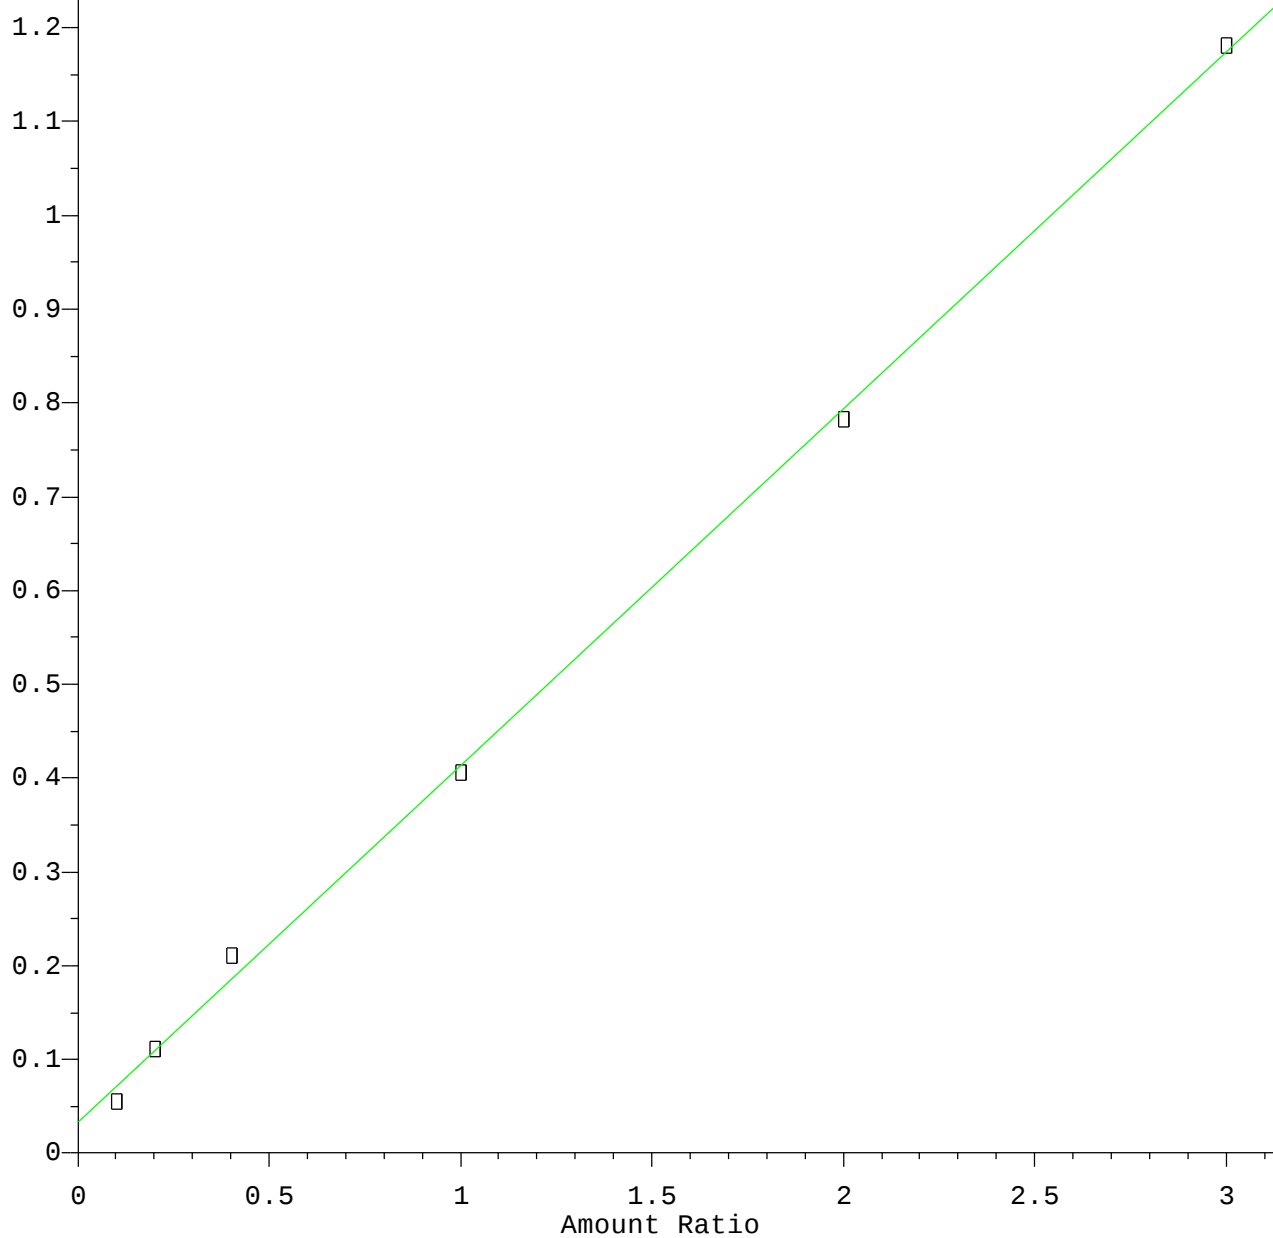


Resp Ratio = $3.80 \times 10^{-1} \times \text{Amt} + 3.26 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D090320S.M
Calibration Table Last Updated: Fri Sep 04 01:57:04 2020

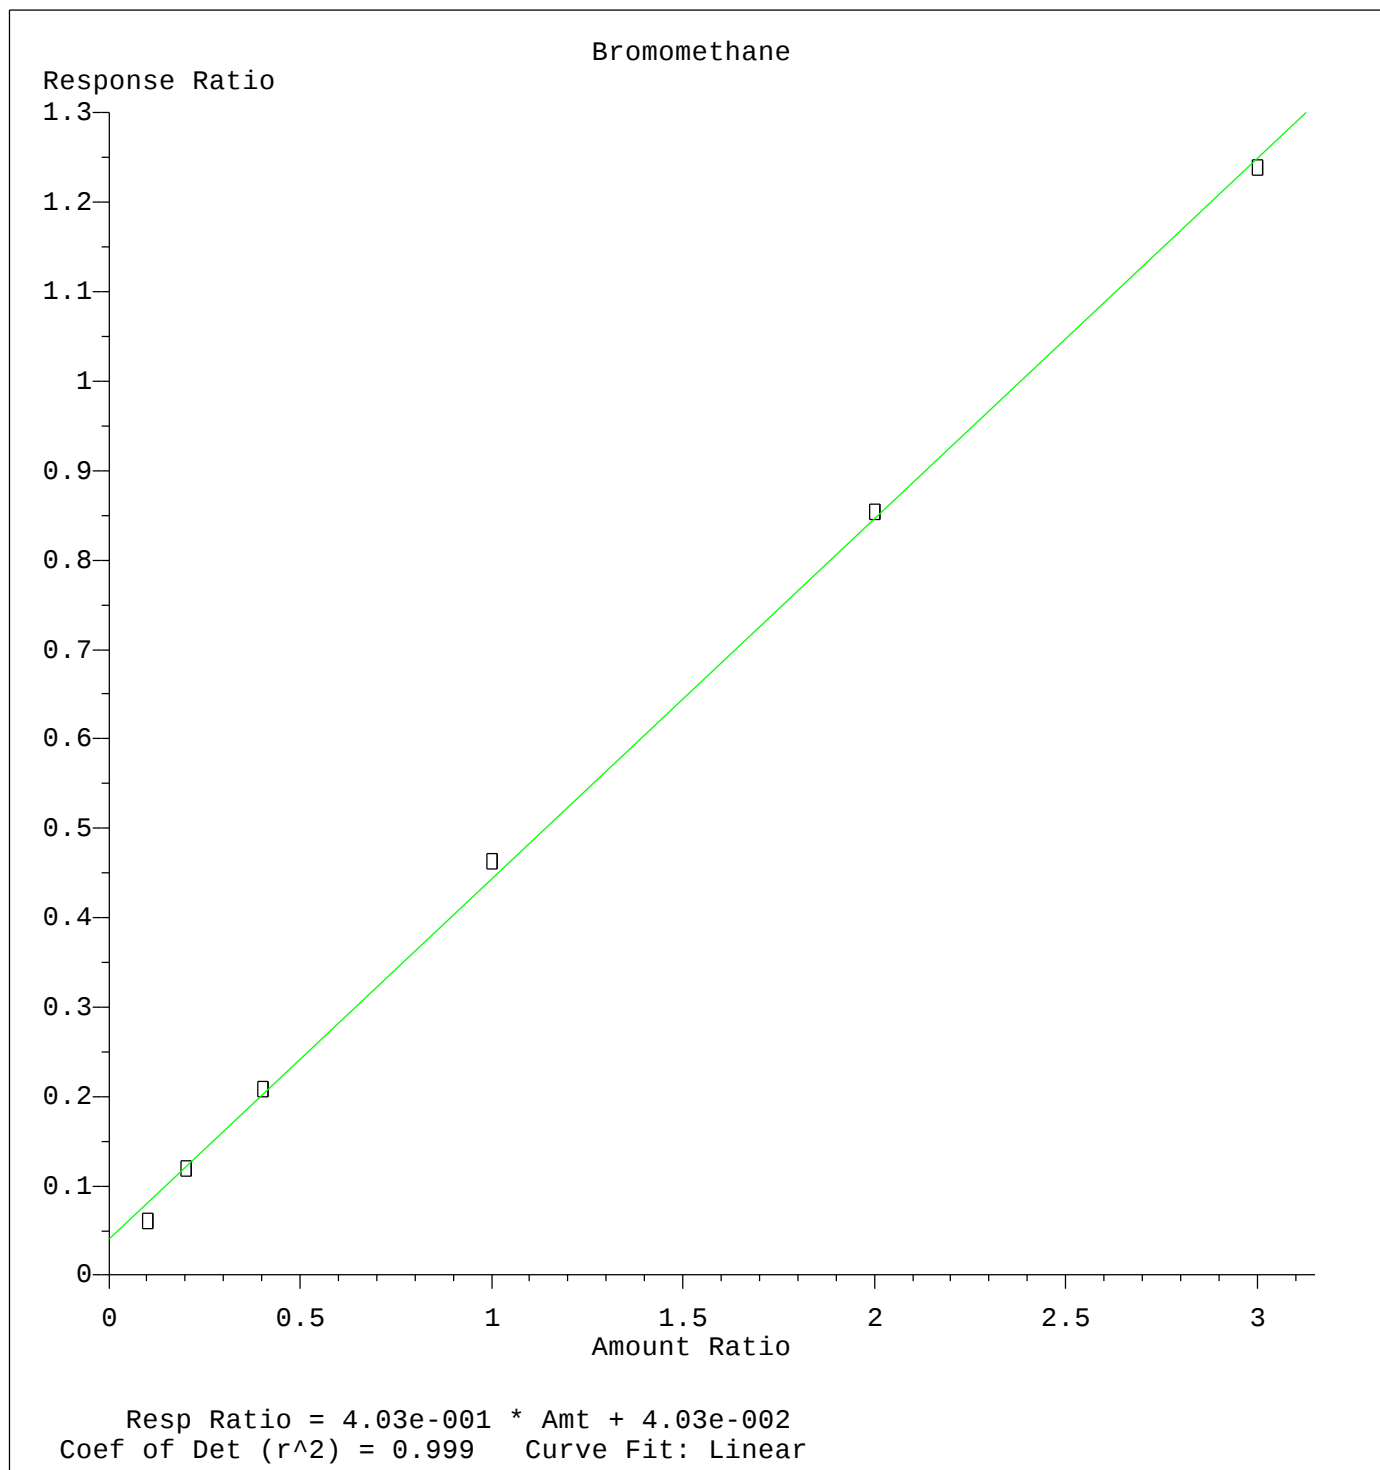

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D090320S.M
Calibration Table Last Updated: Fri Sep 04 01:57:04 2020

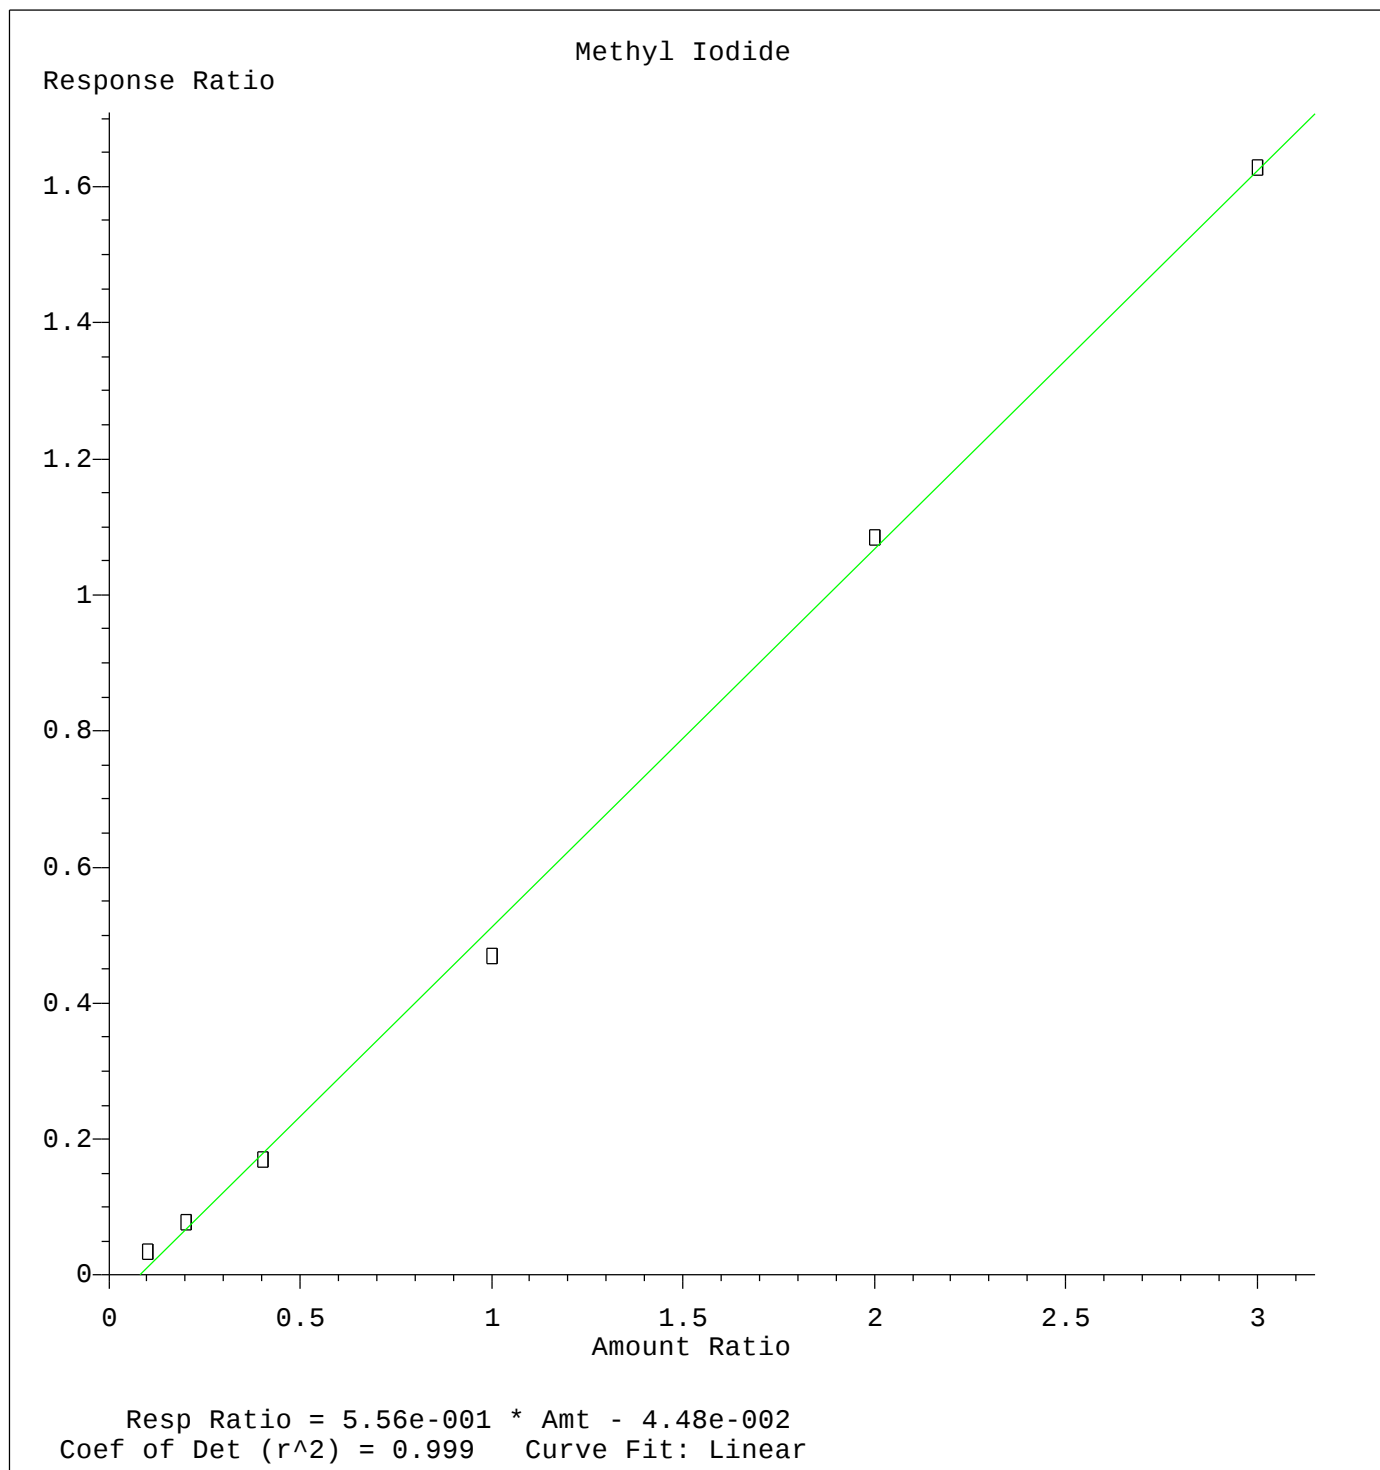

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D090320S.M
Calibration Table Last Updated: Fri Sep 04 01:57:04 2020