


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD090418\
Data File : VD059942.D
Acq On : 4 Sep 2018 12:11
Operator : JC/SY
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082218S.M
Title : SW846 8260
Last Update : Thu Aug 23 03:03:08 2018

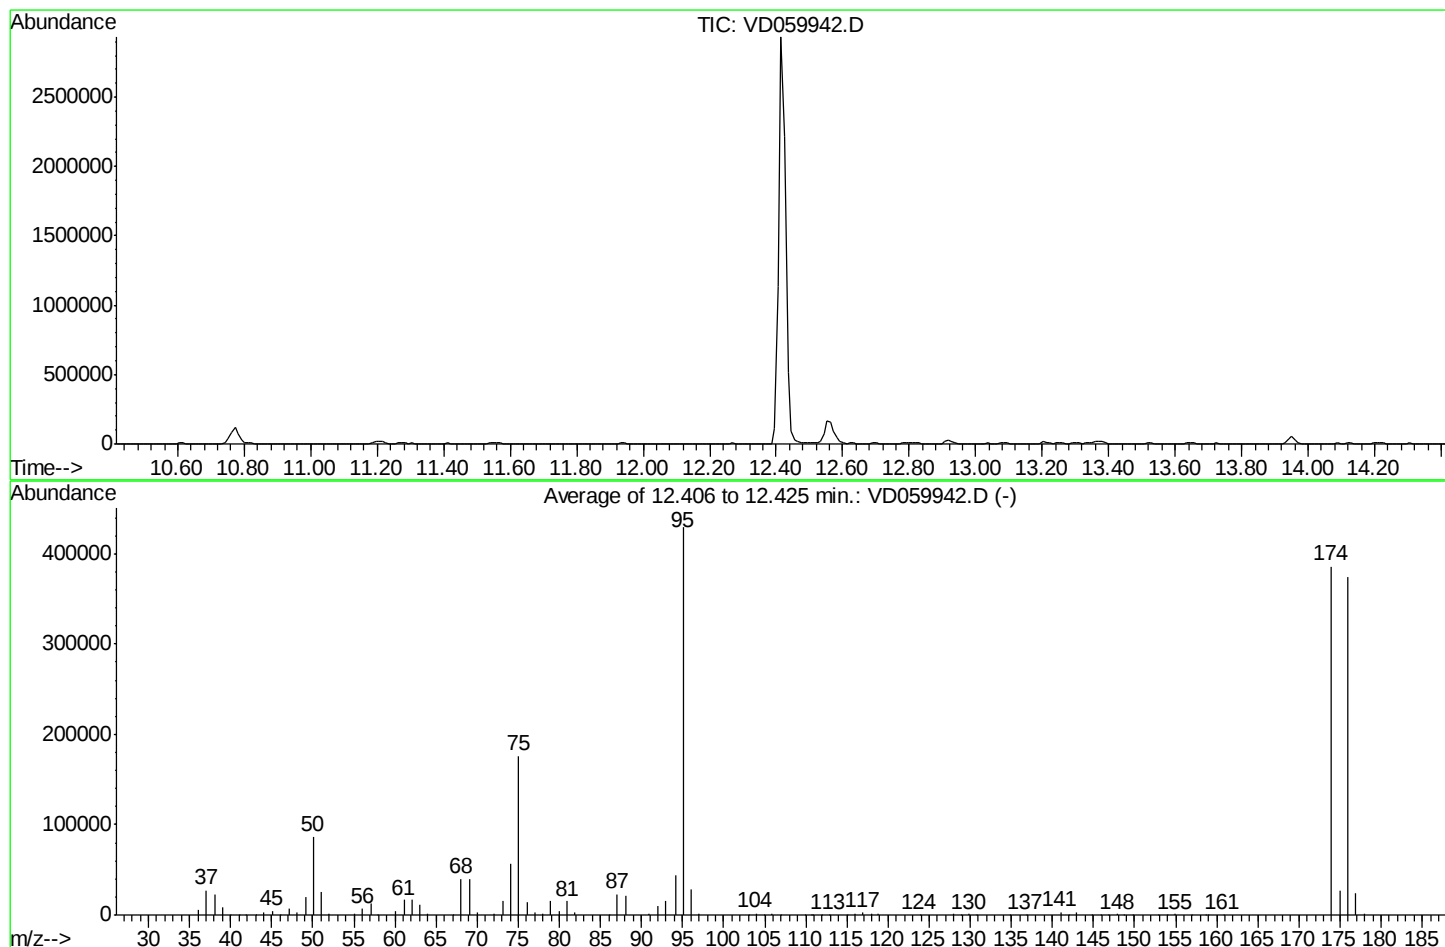

AutoFind: Scans 1238, 1239, 1240; Background Corrected with Scan 1233

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	86856	PASS
75	95	30	60	41.1	176426	PASS
95	95	100	100	100.0	429226	PASS
96	95	5	9	6.5	27906	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	89.9	385813	PASS
175	174	5	9	7.1	27227	PASS
176	174	95	101	97.1	374677	PASS
177	176	5	9	6.6	24622	PASS