

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD090518\
 Data File : VD059968.D
 Acq On : 5 Sep 2018 14:42
 Operator : JC/SY
 Sample : J4741-09
 Misc : 6.32g/5ml/MSVOA D/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 AOC10-02-A

Quant Time: Sep 05 16:07:52 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D082218S.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 23 03:03:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-6.41
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-7.45
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-11.29
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.38

System Monitoring Compounds		R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4		0.00	65	0	0.00	ug/l	
Spiked Amount	50.000			Recovery	=	0.00%	
35) Dibromofluoromethane		0.00	113	0	0.00	ug/l	
Spiked Amount	50.000			Recovery	=	0.00%	
50) Toluene-d8		0.00	98	0	0.00	ug/l	
Spiked Amount	50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene		0.00	95	0	0.00	ug/l	
Spiked Amount	50.000			Recovery	=	0.00%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD090518\
Data File : VD059968.D
Acq On : 5 Sep 2018 14:42
Operator : JC/SY
Sample : J4741-09
Misc : 6.32g/5ml/MSVOA D/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
AOC10-02-A

Quant Time: Sep 05 16:07:52 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D082218S.M
Quant Title : SW846 8260
QLast Update : Thu Aug 23 03:03:08 2018
Response via : Initial Calibration

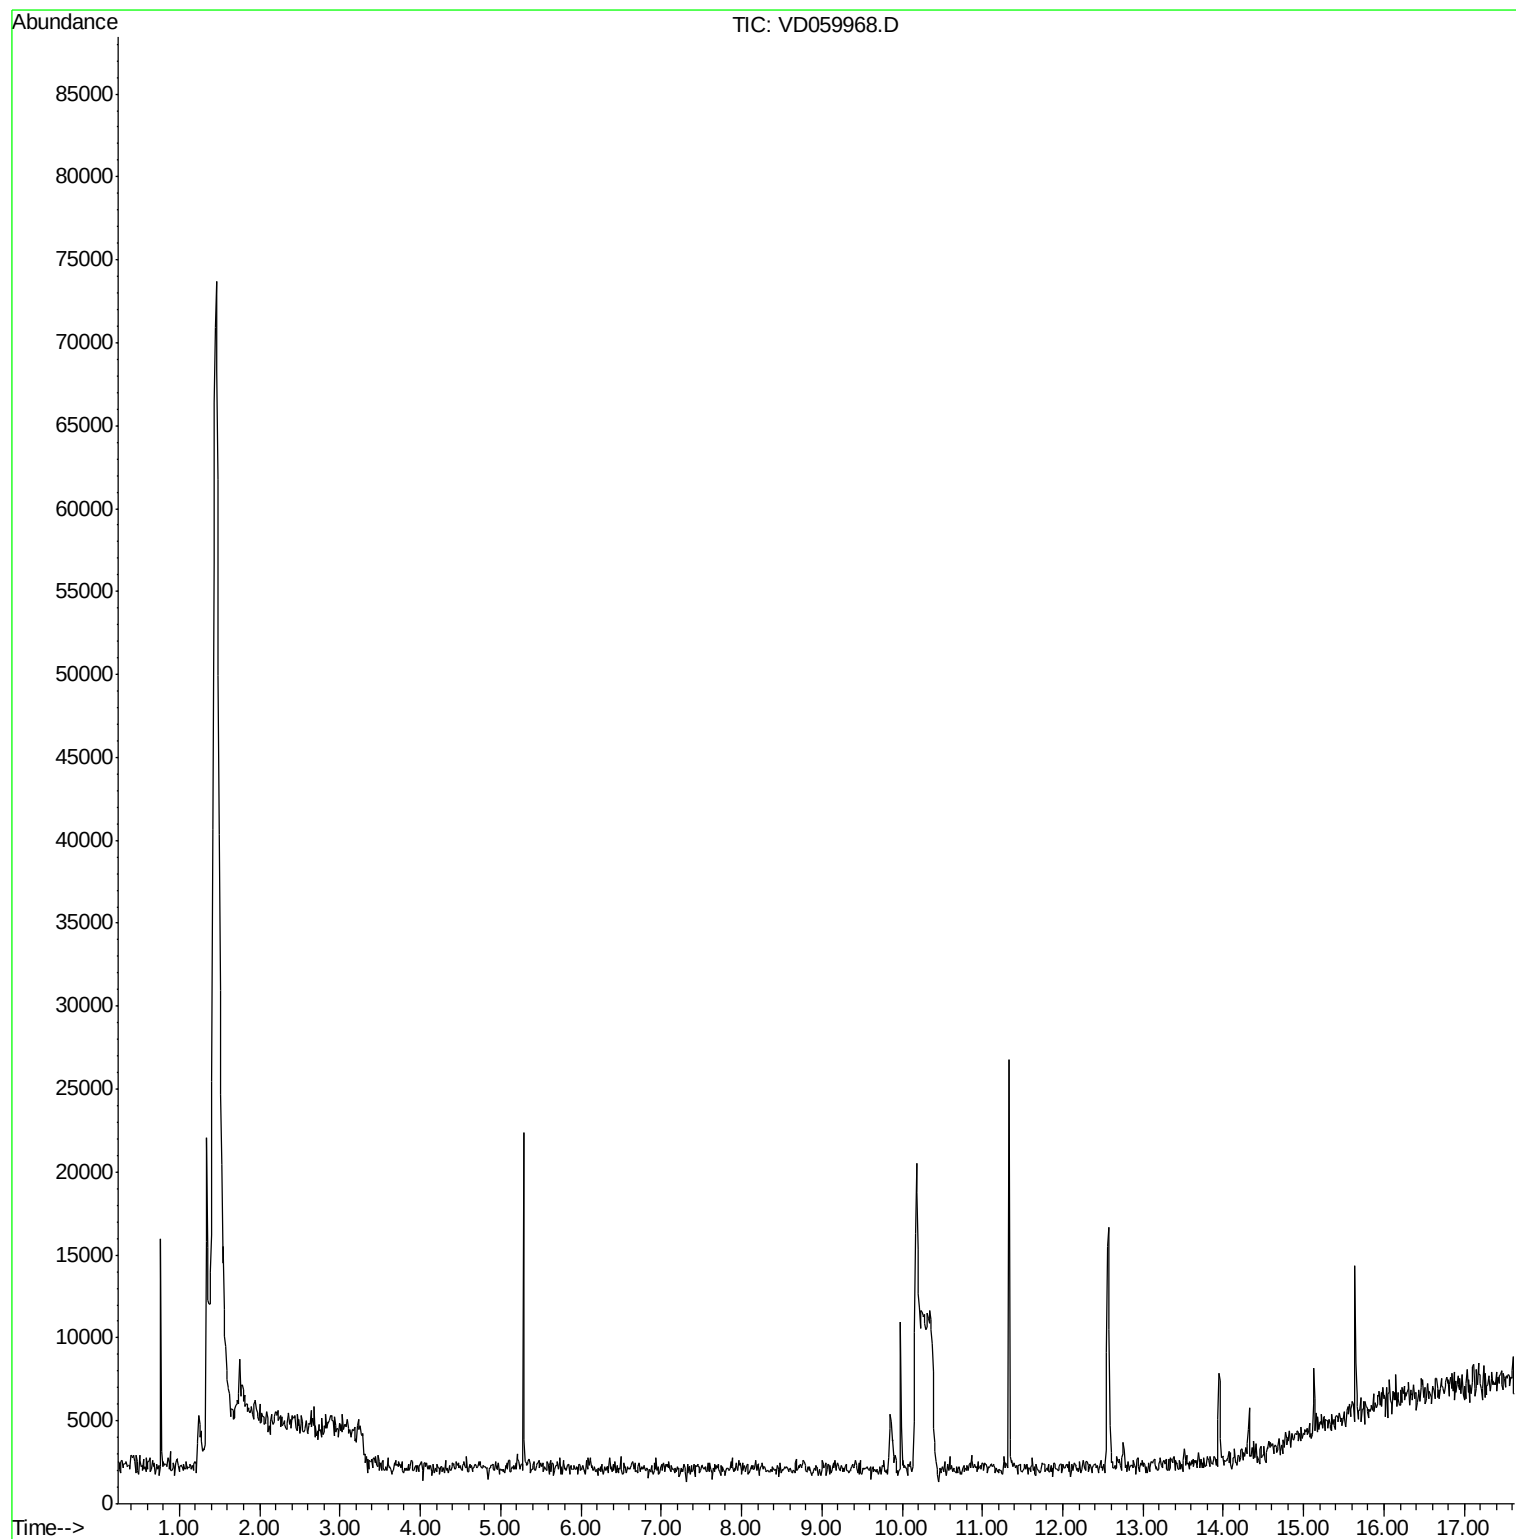


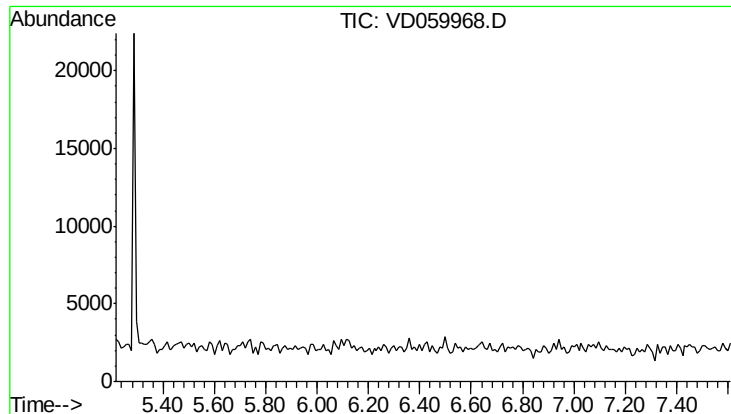


#1
Pentafluorobenzene
Concen: 0.00 ug/l
Expected RT: 6.41 min

Lab File: VD059968.D
Acq: 5 Sep 2018 14:42

Instrument :
MSVOA_D
ClientSampleId :
AOC10-02-A


Tot Ion: 168
Sig Exp Ratio
168 100
99 52.7

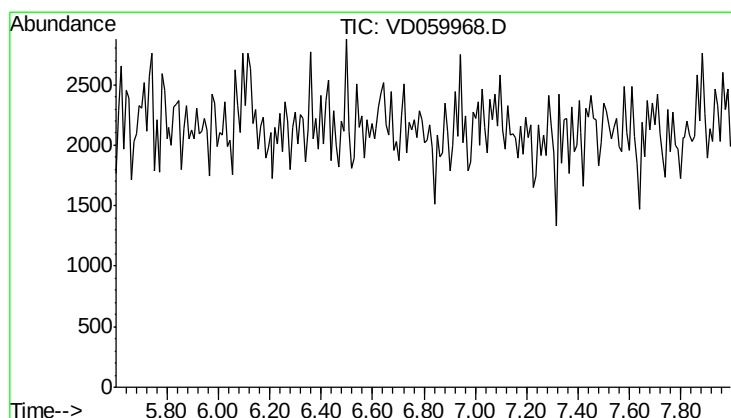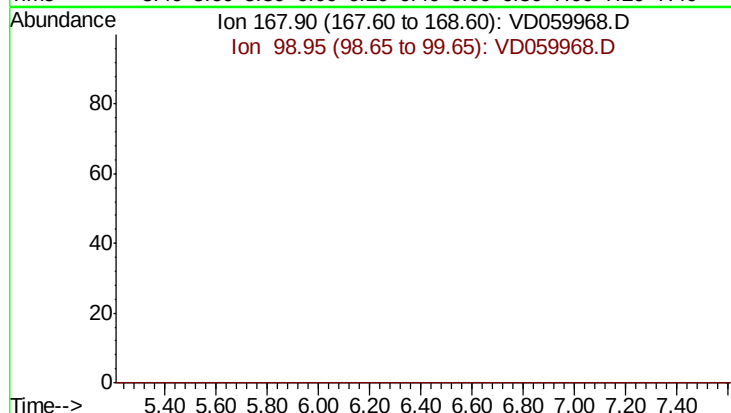


#33
1,2-Dichloroethane-d4
Concen: N.D. ug/l
Expected RT: 6.80 min

Lab File: VD059968.D
Acq: 5 Sep 2018 14:42

Tgt Ion: 65
Sig Exp Ratio
65 100
67 51.9


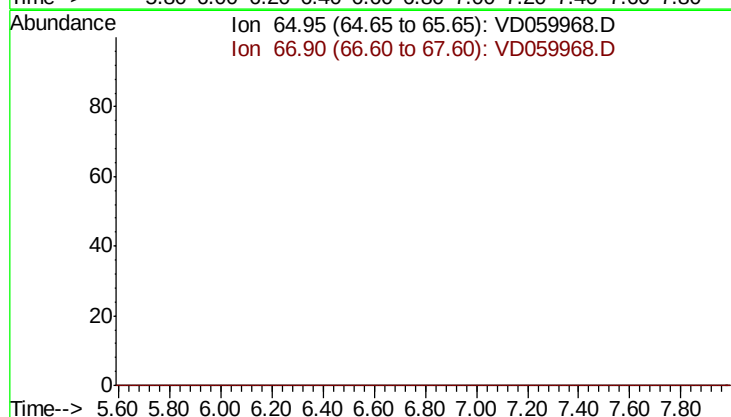


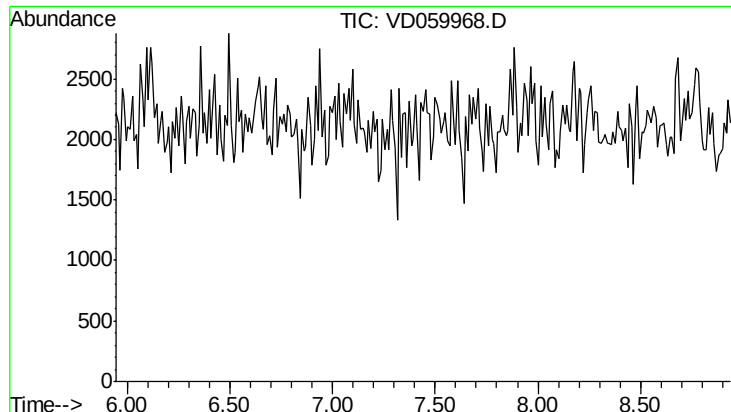

#34
 1,4-Difluorobenzene
 Concen: 0.00 ug/l
 Expected RT: 7.45 min
 Lab File: VD059968.D
 Acq: 5 Sep 2018 14:42


Instrument :
 MSVOA_D
 ClientSampleId :
 AOC10-02-A


Tot Ion	114
Sig	Exp Ratio
114	100
63	19.7
88	18.8

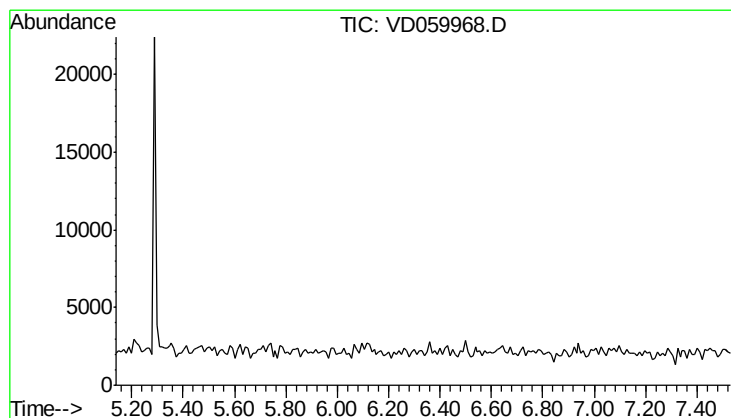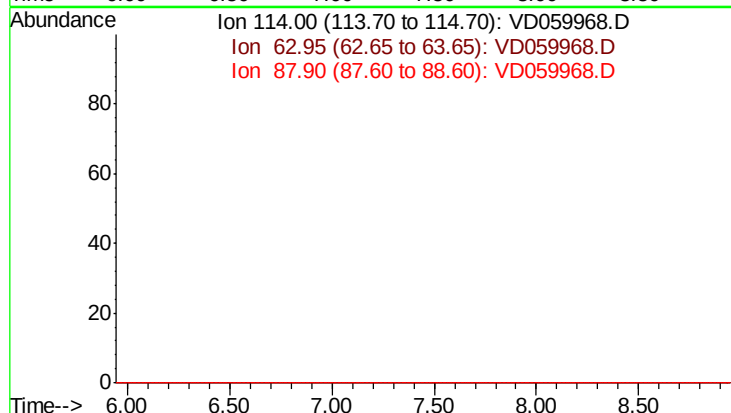

#35
 Dibromofluoromethane
 Concen: 0.00 ug/l
 Expected RT: 6.33 min
 Lab File: VD059968.D
 Acq: 5 Sep 2018 14:42

Tgt Ion	113
Sig	Exp Ratio
113	100
111	101.8
192	21.3

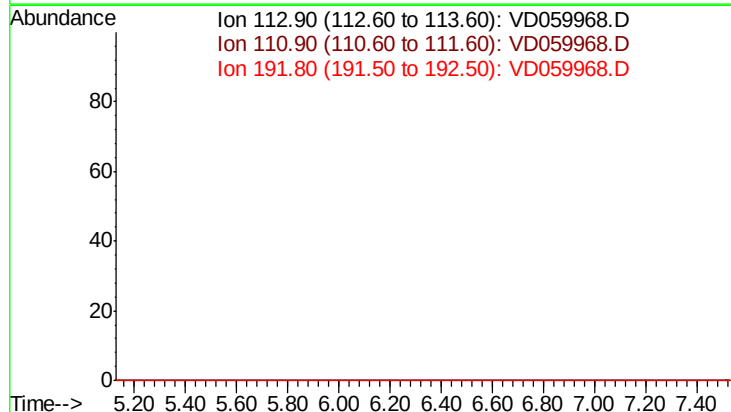


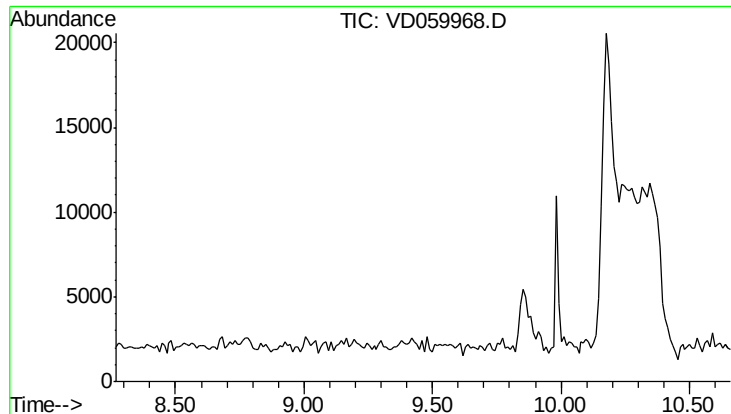


#50
Toluene-d8
Concen: N.D. ug/l
Expected RT: 9.46 min

Lab File: VD059968.D
Acq: 5 Sep 2018 14:42

Instrument :
MSVOA_D
ClientSampleId :
AOC10-02-A


Tot Ion: 98
Sig Exp Ratio
98 100
100 69.7

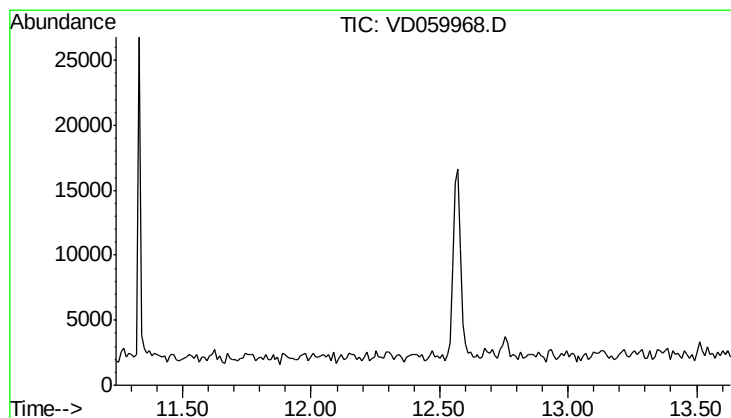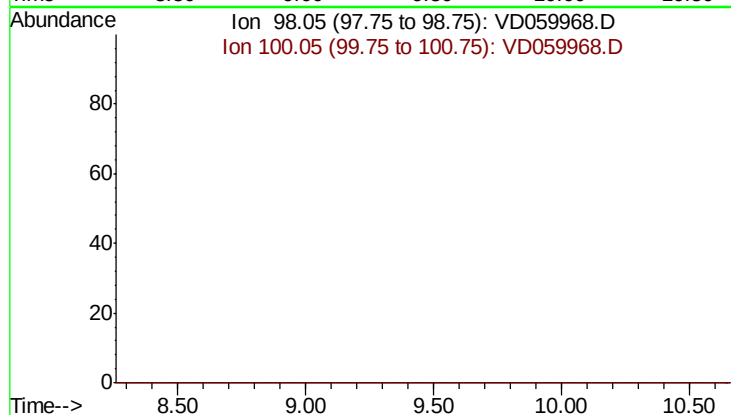


#62
4-Bromofluorobenzene
Concen: N.D. ug/l
Expected RT: 12.43 min

Lab File: VD059968.D
Acq: 5 Sep 2018 14:42

Tgt Ion: 95
Sig Exp Ratio
95 100
174 97.8
176 95.6


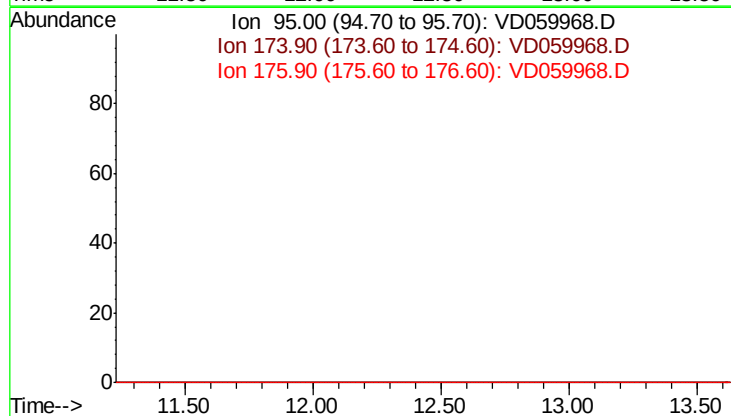


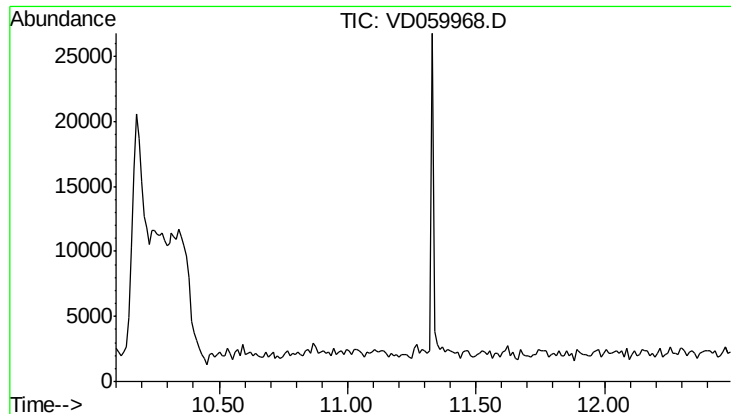

#63
 Chlorobenzene-d5
 Concen: 0.00 ug/l
 Expected RT: 11.29 min
 Lab File: VD059968.D
 Acq: 5 Sep 2018 14:42

Instrument :
 MSVOA_D
 ClientSampleId :
 AOC10-02-A

Tot Ion	117
Sig	Exp Ratio
117	100
82	50.1
119	33.4

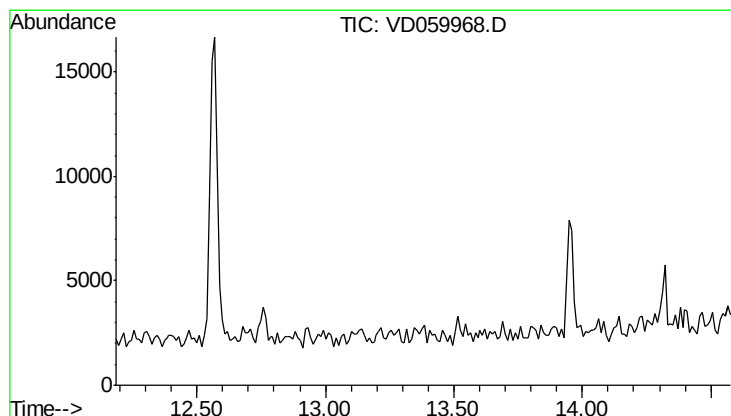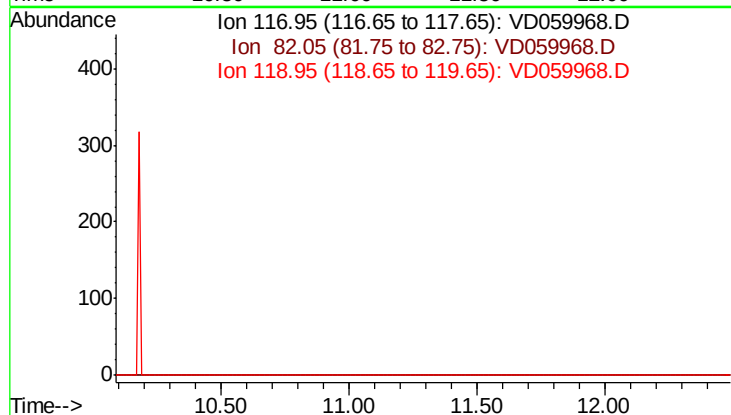

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.00 ug/l
 Expected RT: 13.38 min
 Lab File: VD059968.D
 Acq: 5 Sep 2018 14:42

Tgt Ion	152
Sig	Exp Ratio
152	100
115	51.3
150	155.1

