
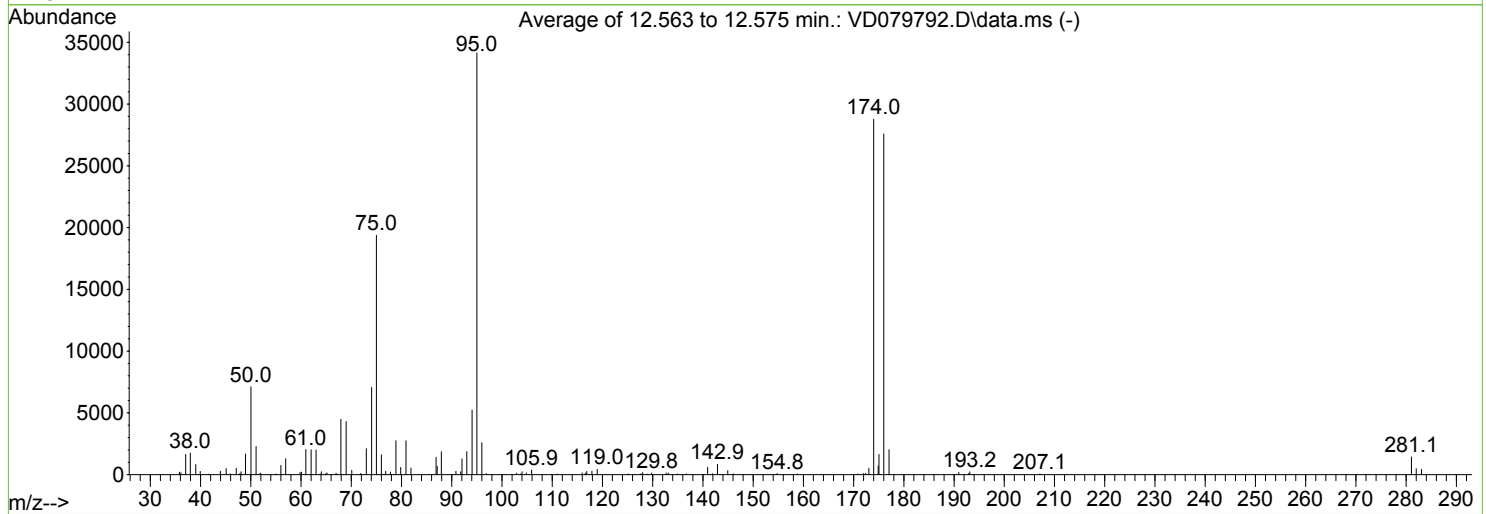


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD090624\
Data File : VD079792.D
Acq On : 06 Sep 2024 11:05
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D083024S.M
Title : SW846 8260
Last Update : Fri Aug 30 15:57:30 2024

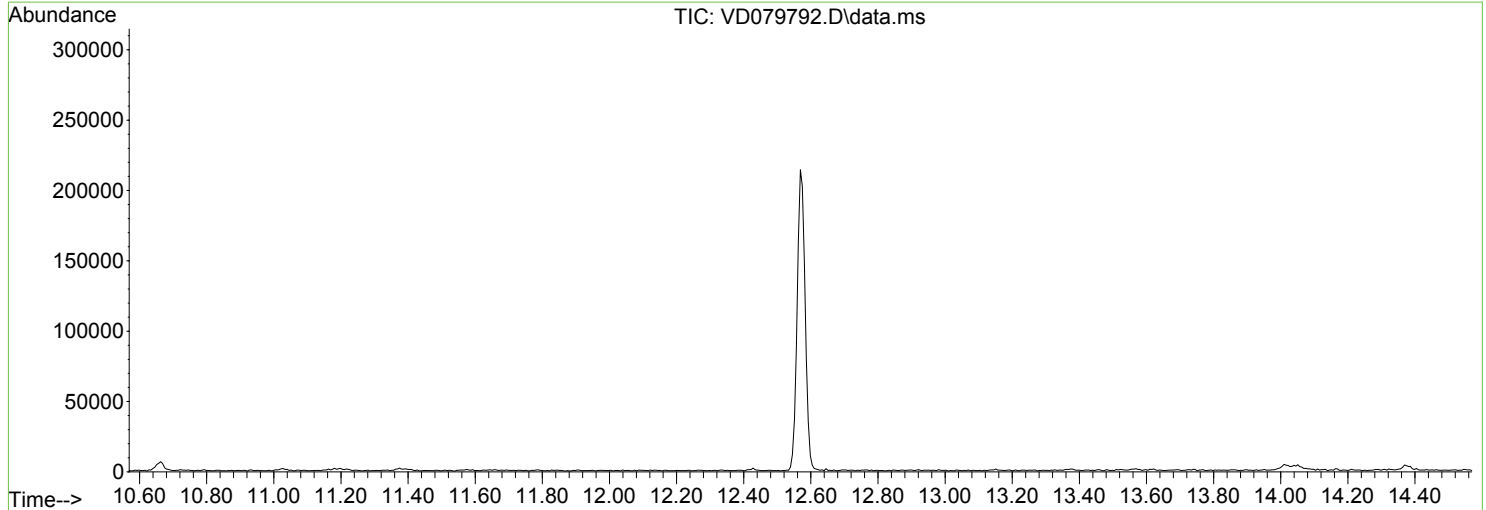

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	7108	PASS
75	95	30	60	56.8	19379	PASS
95	95	100	100	100.0	34144	PASS
96	95	5	9	7.6	2595	PASS
173	174	0.00	2	1.8	517	PASS
174	95	50	100	84.3	28773	PASS
175	174	5	9	5.7	1634	PASS
176	174	95	101	95.8	27568	PASS
177	176	5	9	7.3	2018	PASS