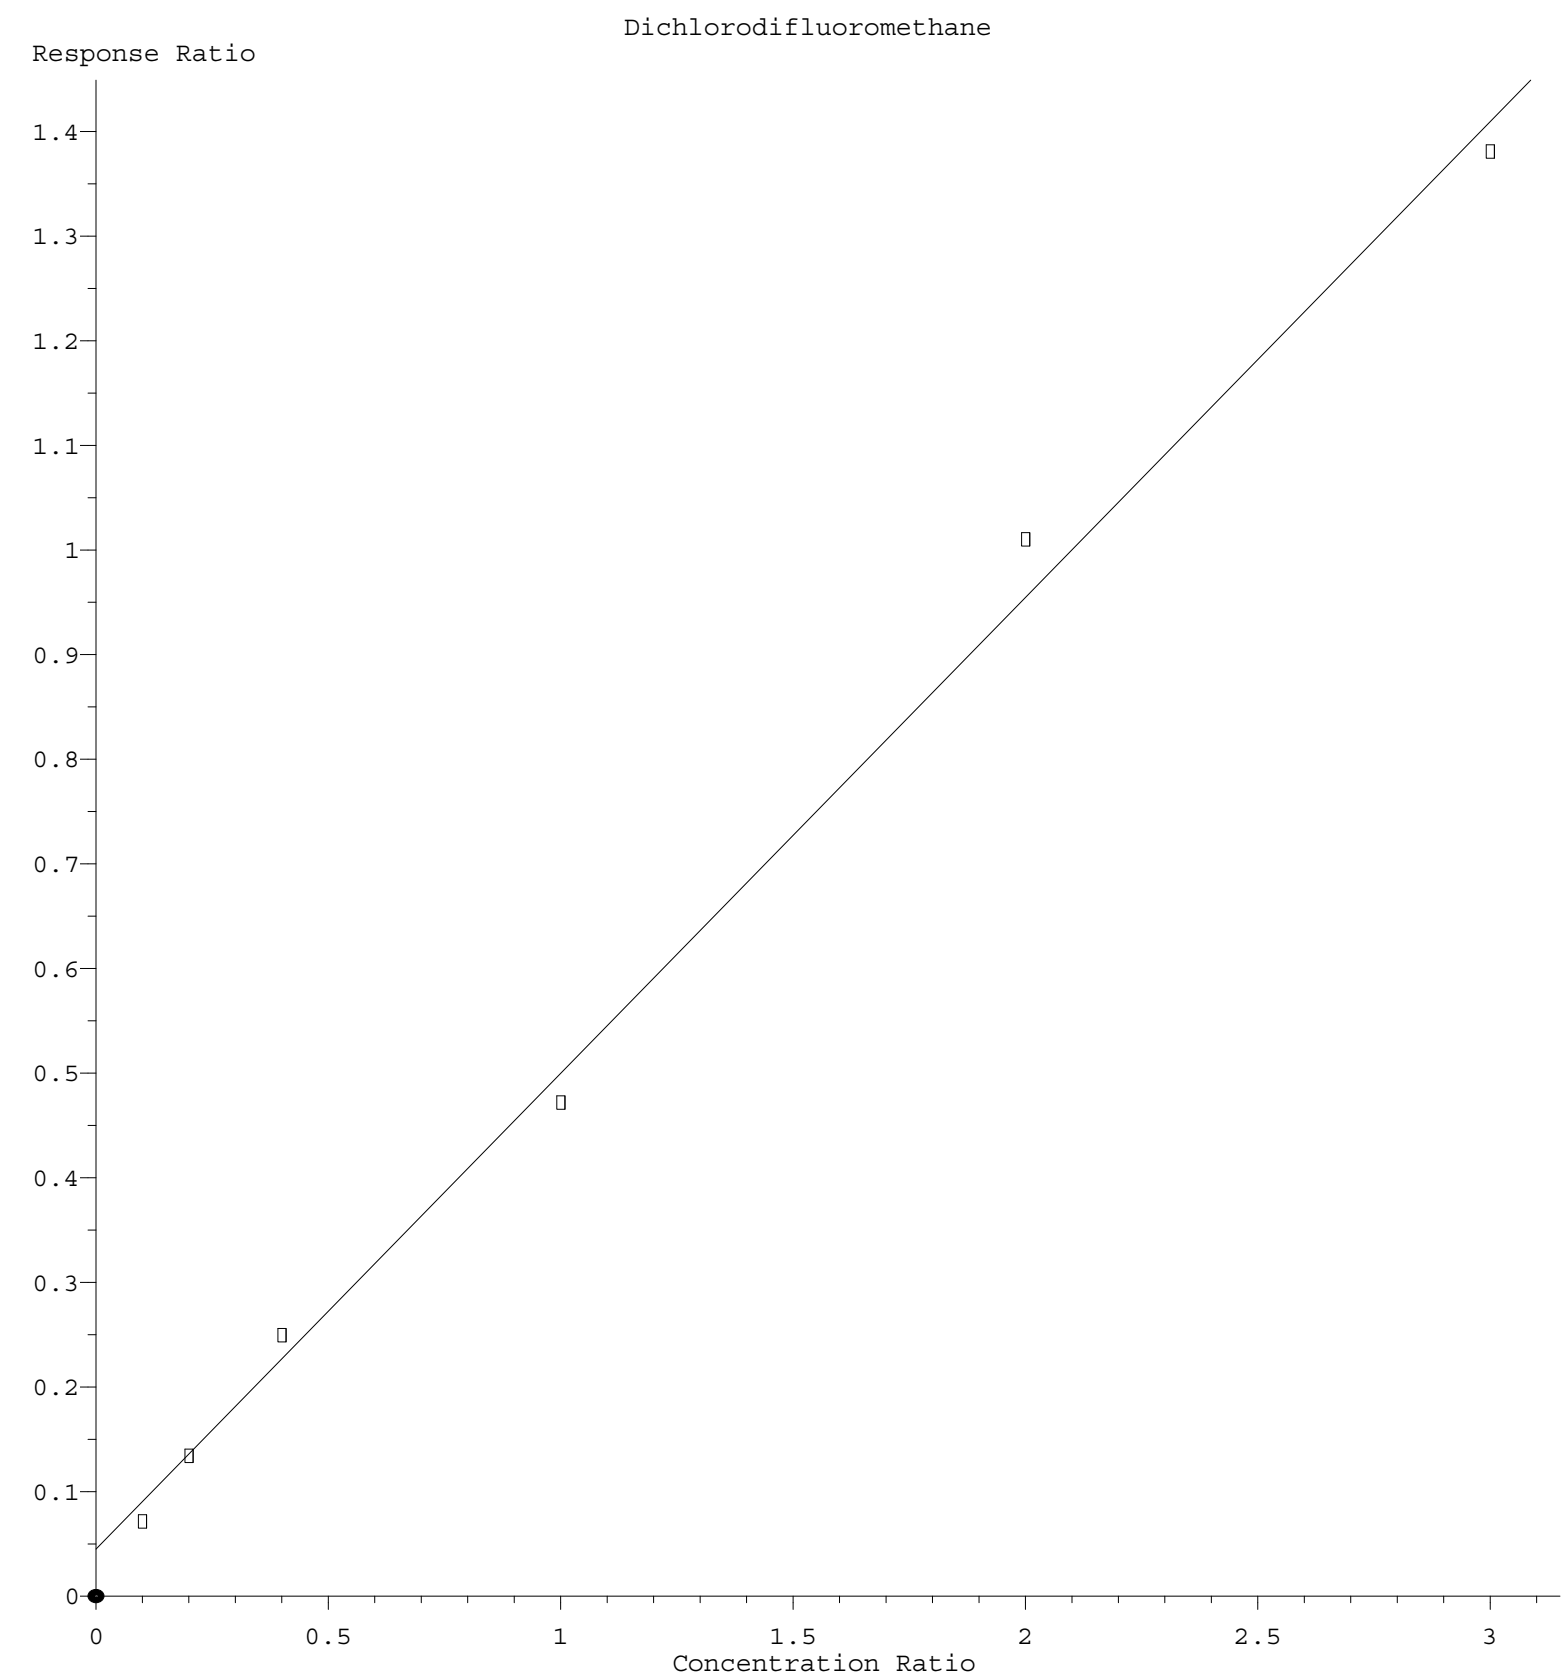

Response = 4.553e-001 * Amt + 4.454e-002
Coef of Det (r^2) = 0.996045 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D090821S.M
Calibration Table Last Updated: Thu Sep 09 03:07:09 2021

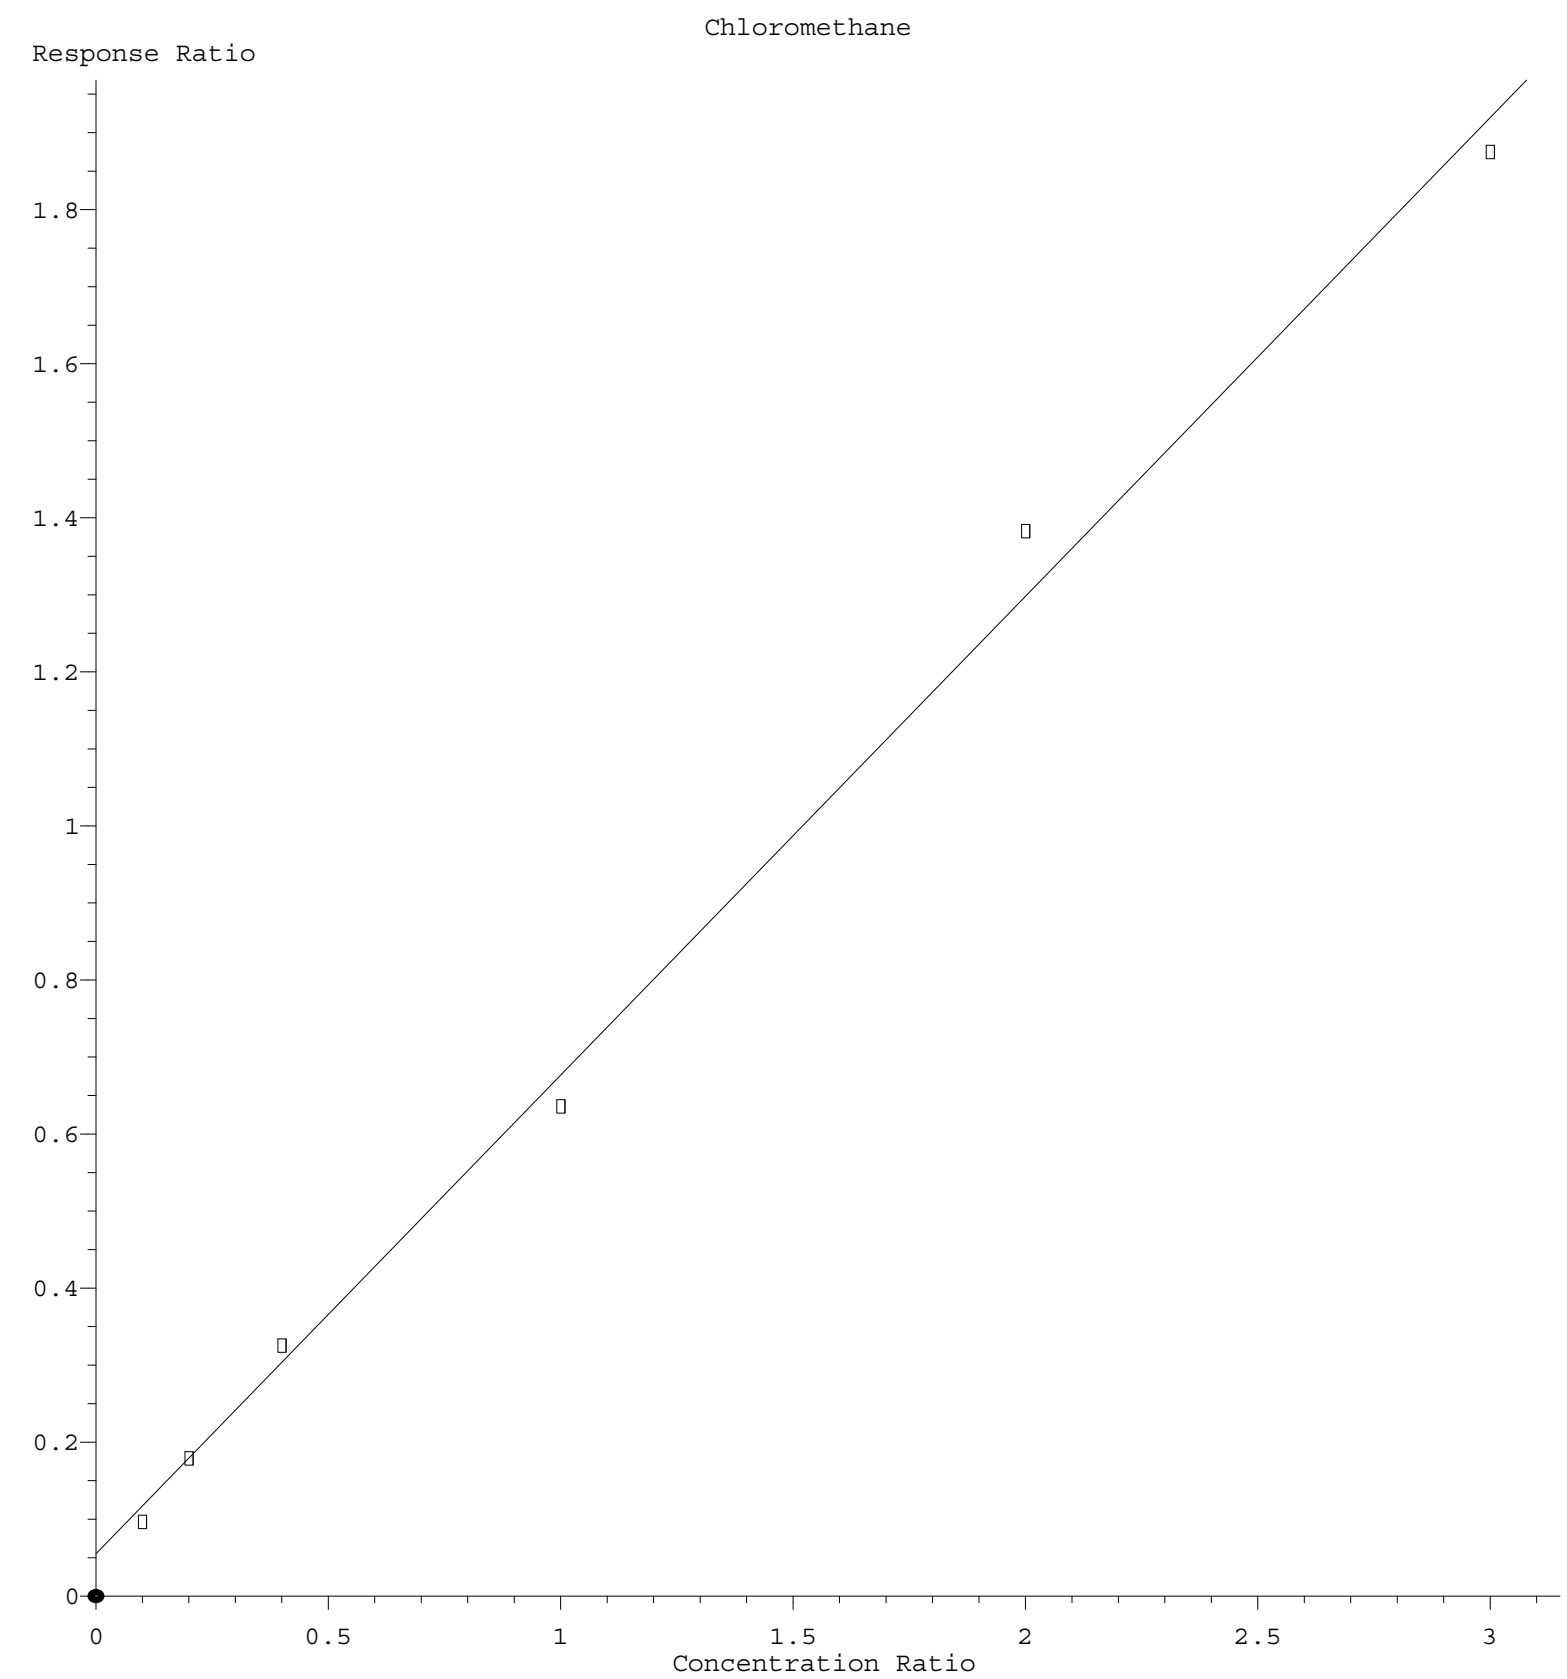

Response = 6.216e-001 * Amt + 5.474e-002
Coef of Det (r^2) = 0.995515 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D090821S.M
Calibration Table Last Updated: Thu Sep 09 03:07:09 2021

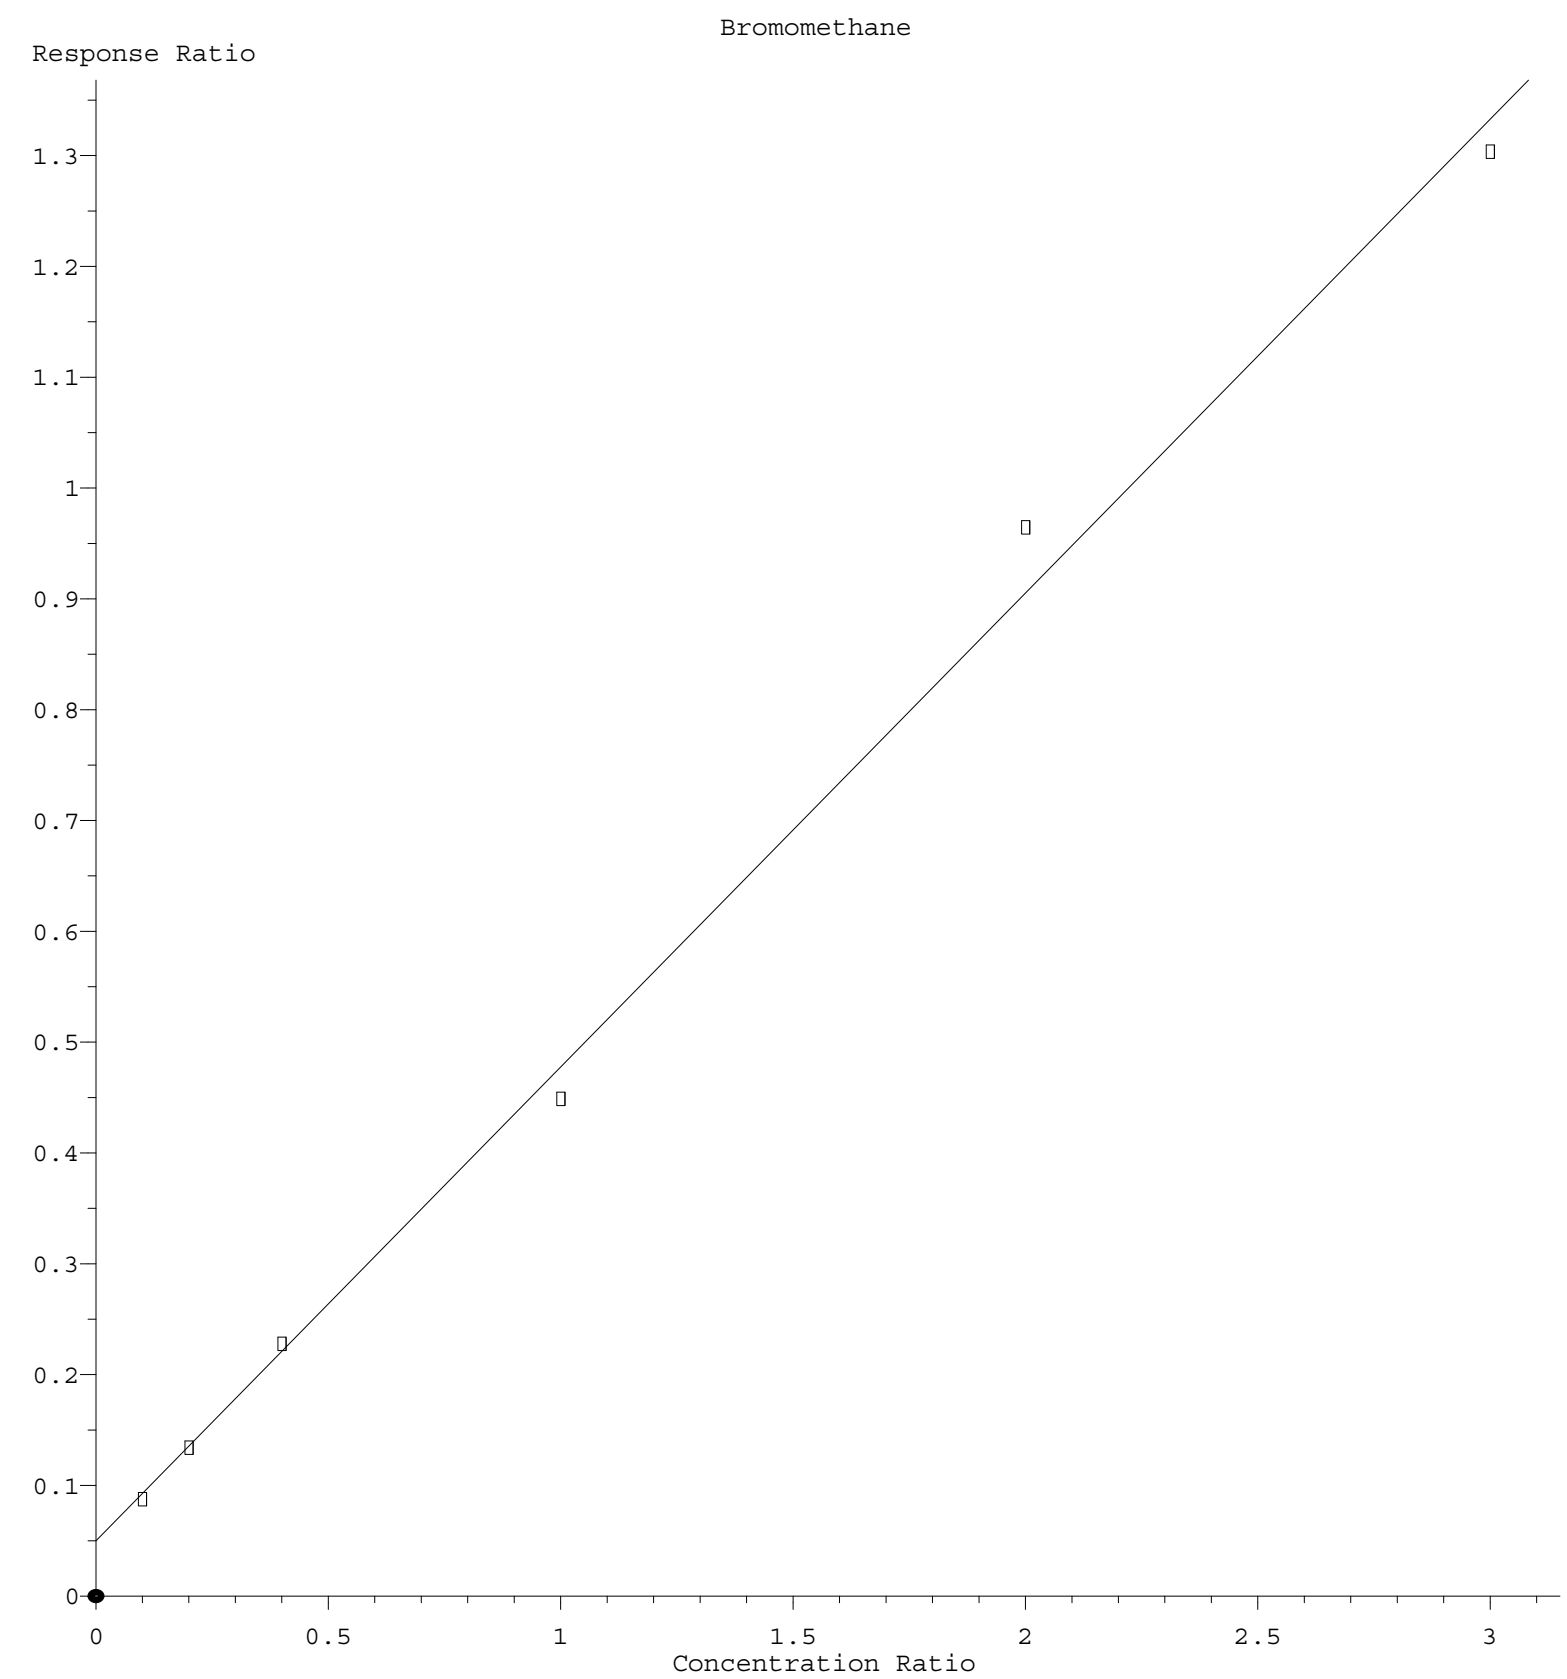

Response = 4.280e-001 * Amt + 4.973e-002
Coef of Det (r^2) = 0.995730 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D090821S.M
Calibration Table Last Updated: Thu Sep 09 03:07:09 2021

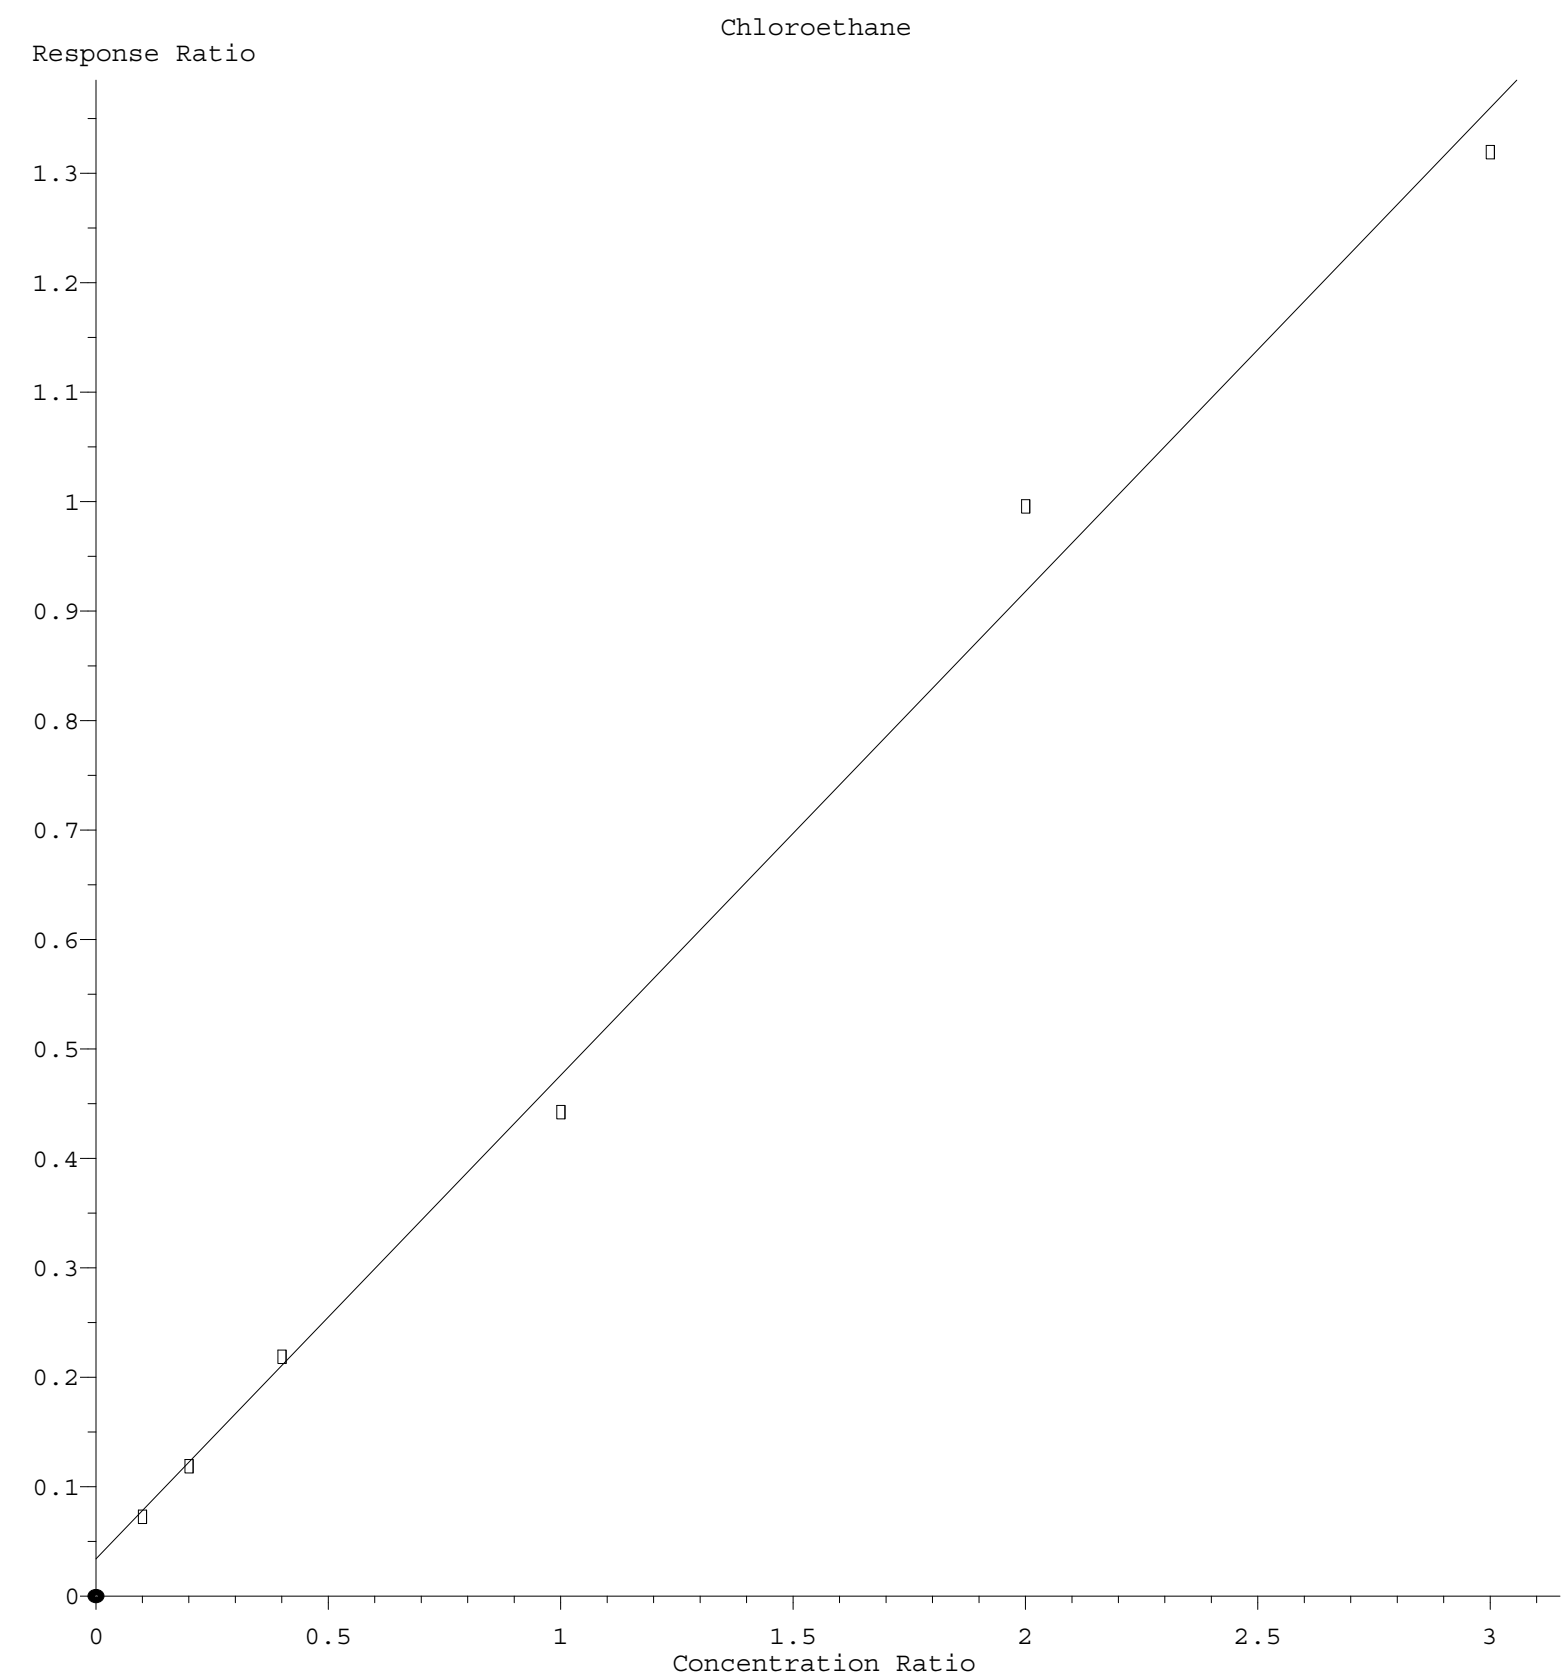

Response = 4.419e-001 * Amt + 3.435e-002
Coef of Det (r^2) = 0.993243 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D090821S.M
Calibration Table Last Updated: Thu Sep 09 03:07:09 2021

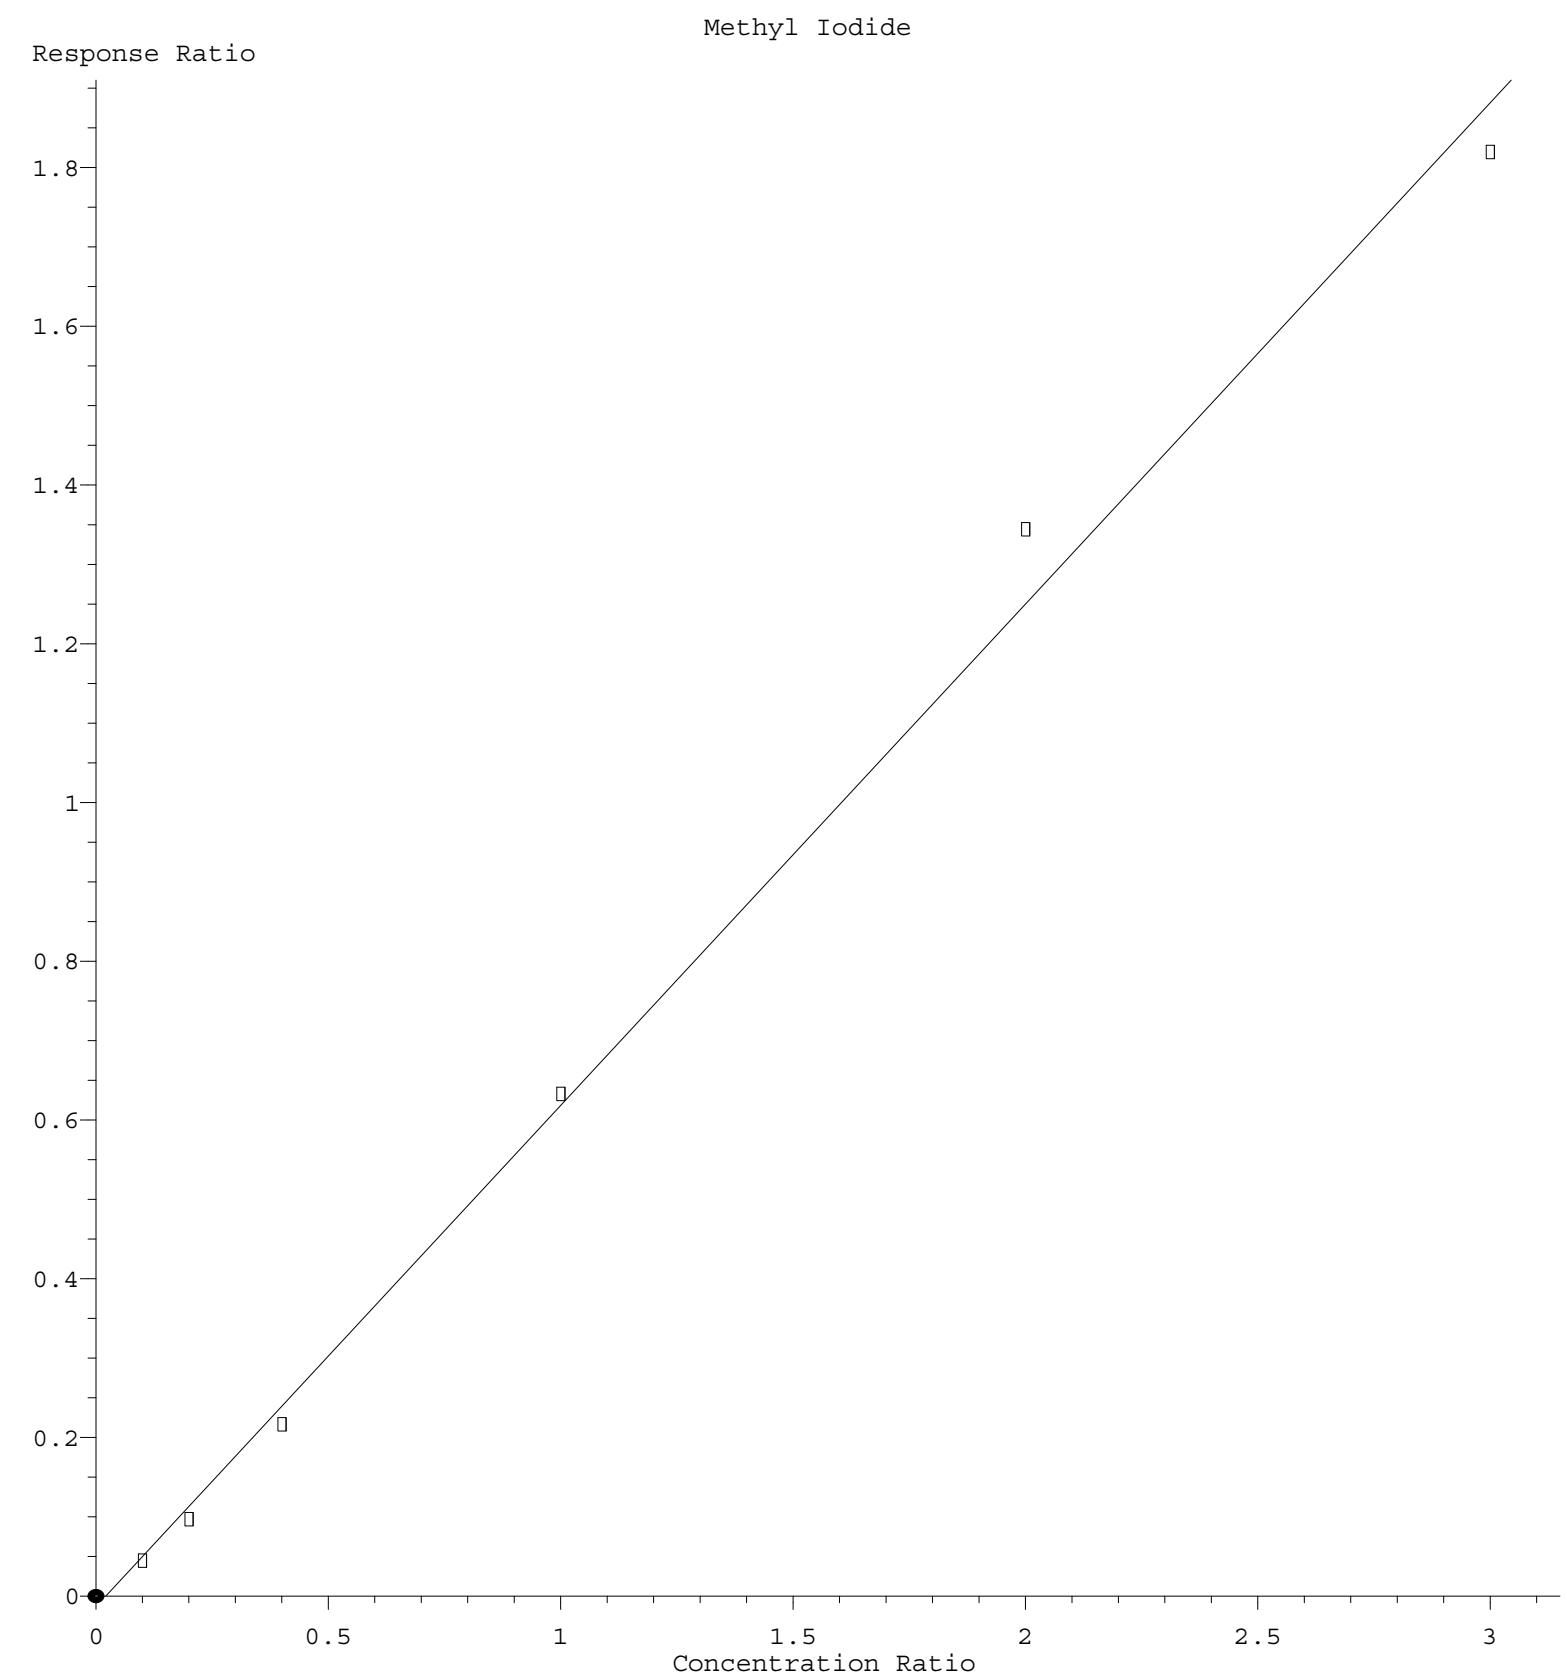

Response = 6.317e-001 * Amt - 1.300e-002
Coef of Det (r^2) = 0.994908 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D090821S.M
Calibration Table Last Updated: Thu Sep 09 03:07:09 2021

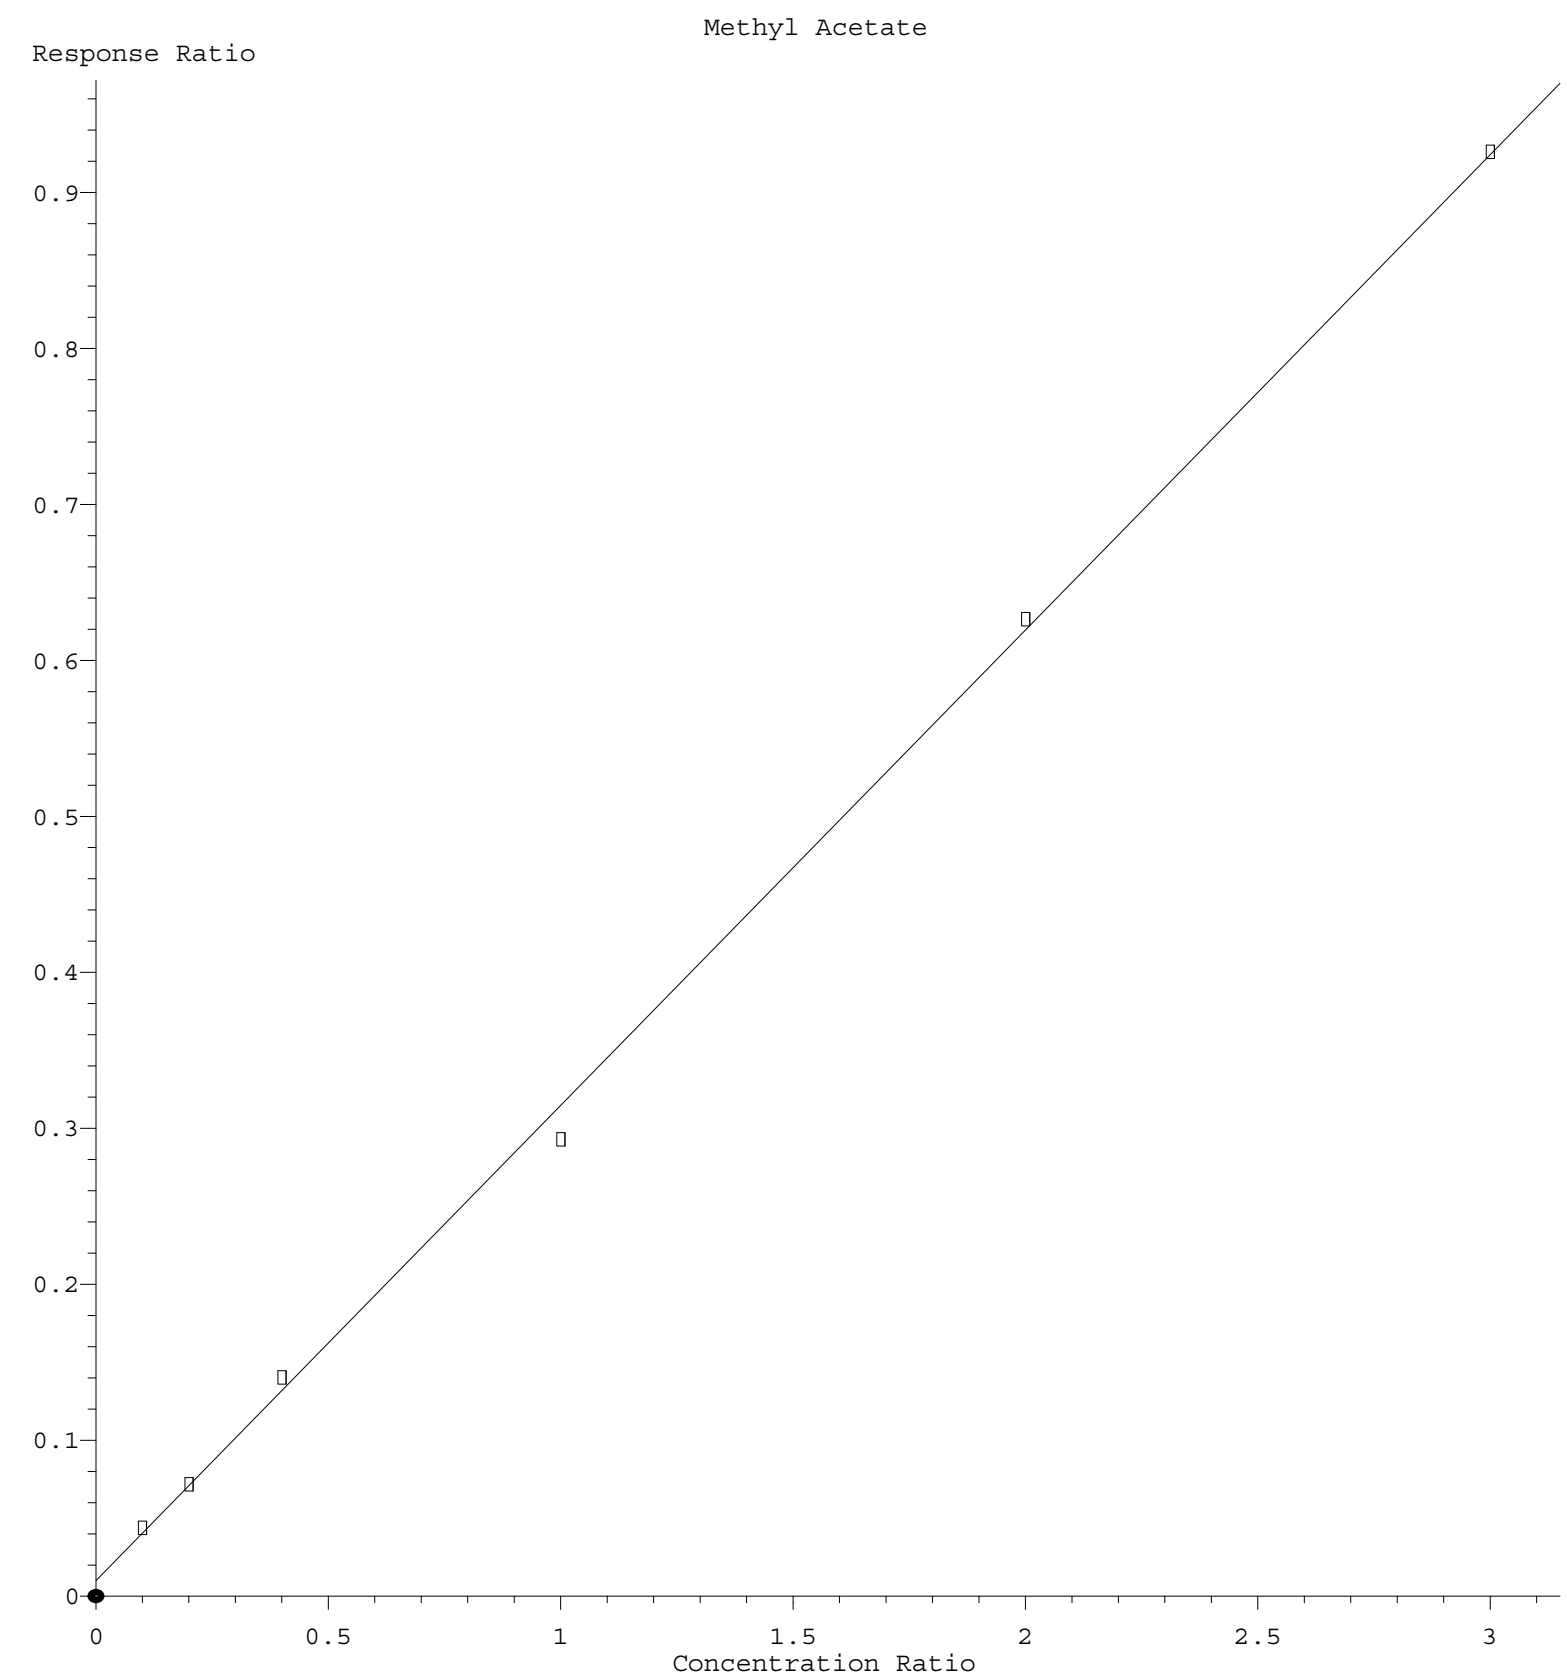

Response = 3.050e-001 * Amt + 9.529e-003
Coef of Det (r^2) = 0.999026 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D090821S.M
Calibration Table Last Updated: Thu Sep 09 03:07:09 2021

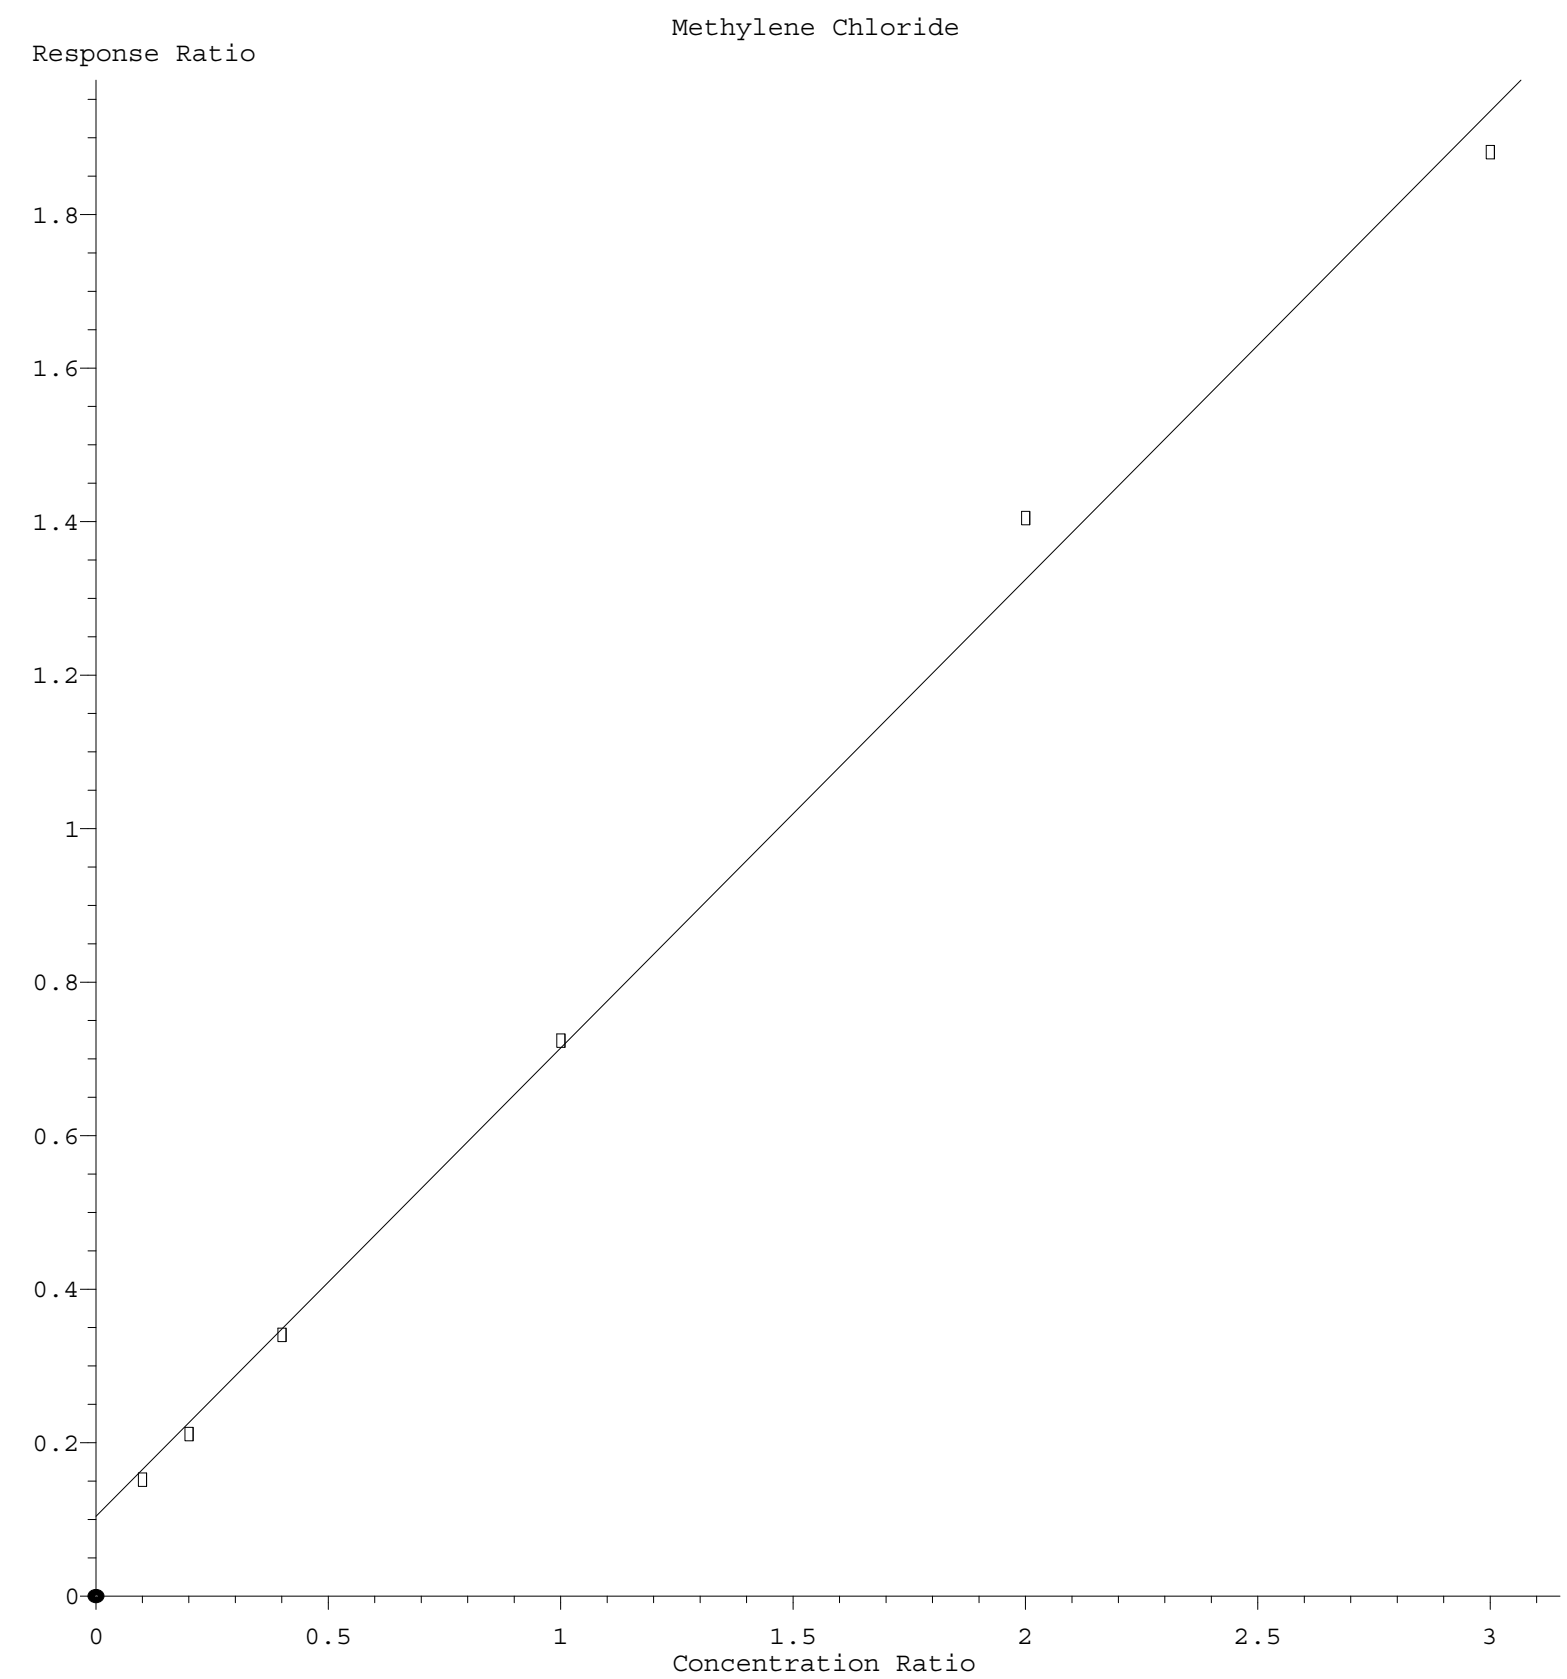

Response = 6.104e-001 * Amt + 1.038e-001
Coef of Det (r^2) = 0.996092 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D090821S.M
Calibration Table Last Updated: Thu Sep 09 03:07:09 2021