
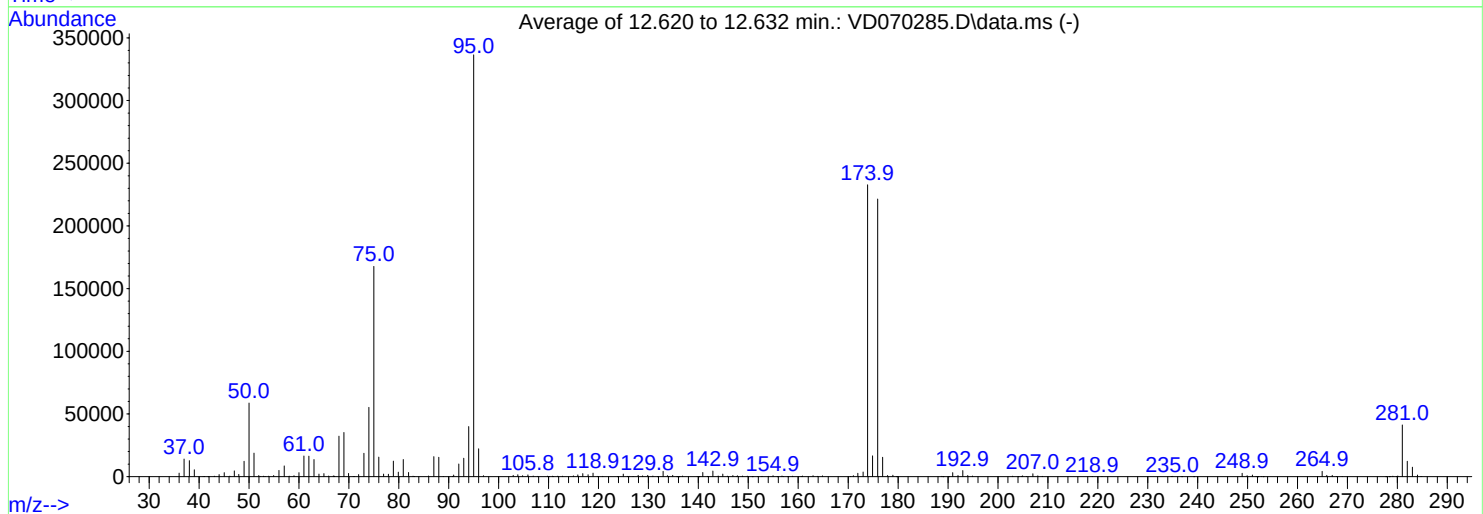


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD090821\
Data File : VD070285.D
Acq On : 08 Sep 2021 08:46
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D090821S.M
Title : SW846 8260
Last Update : Thu Sep 09 03:07:09 2021

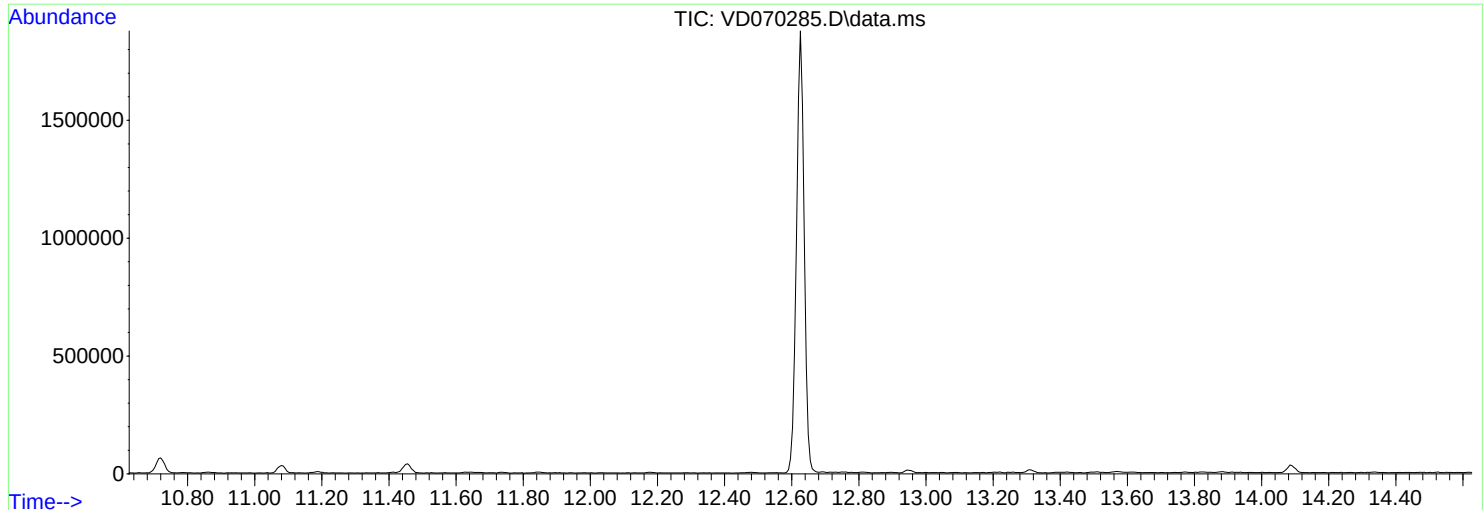

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	58736	PASS
75	95	30	60	49.8	167723	PASS
95	95	100	100	100.0	336469	PASS
96	95	5	9	6.6	22264	PASS
173	174	0.00	2	1.6	3671	PASS
174	95	50	100	69.2	232811	PASS
175	174	5	9	7.1	16558	PASS
176	174	95	101	95.1	221483	PASS
177	176	5	9	7.0	15459	PASS