


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD090920\
 Data File : VD066595.D
 Acq On : 09 Sep 2020 21:11
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D090320S.M
 Title : SW846 8260
 Last Update : Fri Sep 04 01:57:04 2020

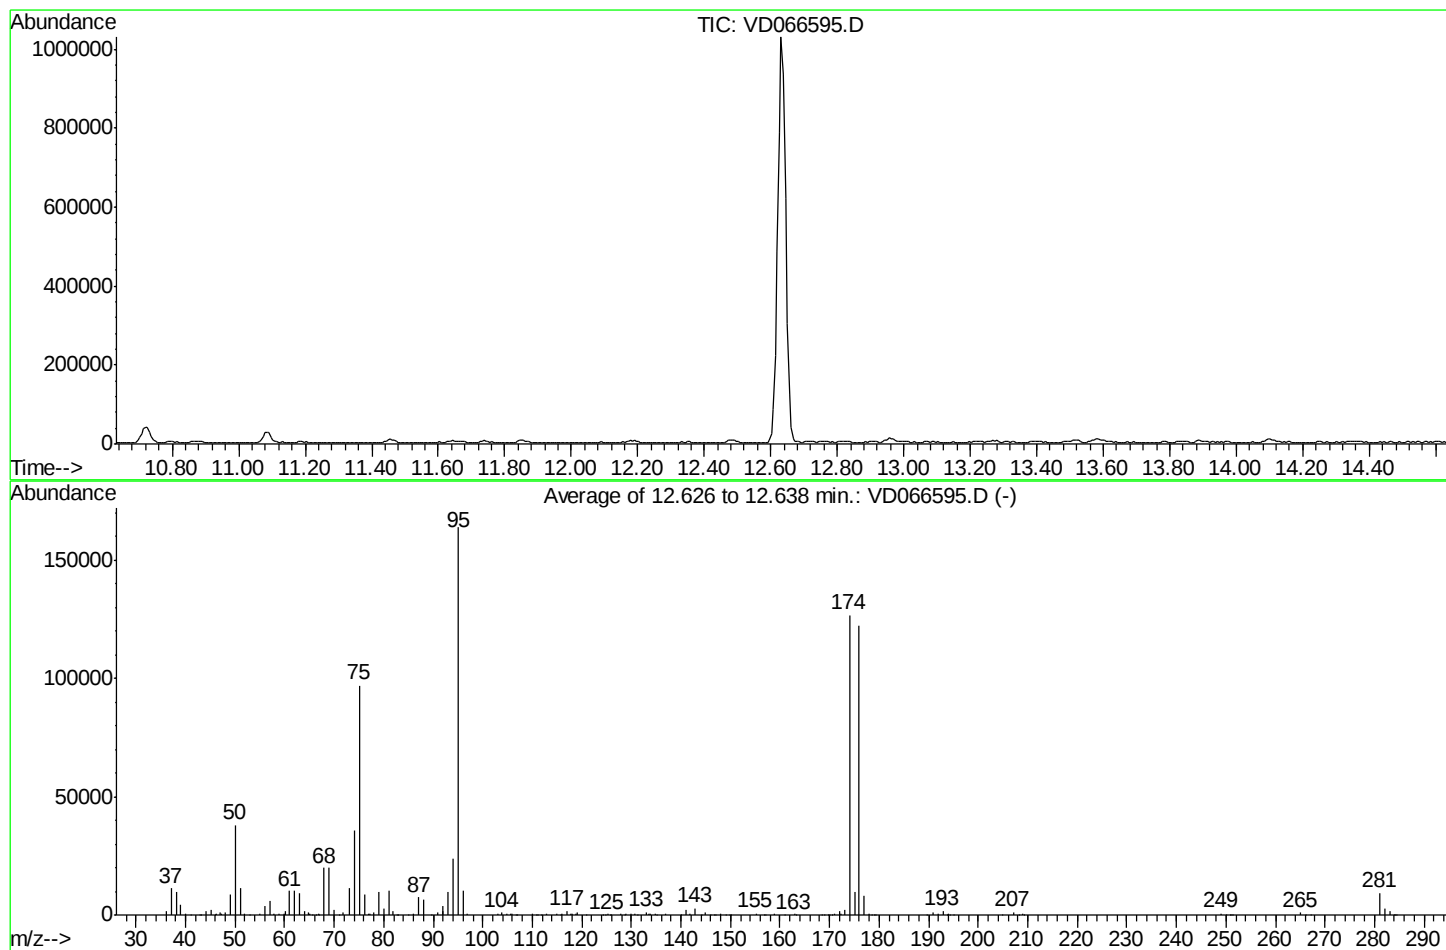

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	37994	PASS
75	95	30	60	59.2	96970	PASS
95	95	100	100	100.0	163840	PASS
96	95	5	9	6.3	10339	PASS
173	174	0.00	2	1.8	2315	PASS
174	95	50	100	77.3	126685	PASS
175	174	5	9	7.6	9582	PASS
176	174	95	101	96.7	122509	PASS
177	176	5	9	6.8	8353	PASS