


Dichlorodifluoromethane

Response Ratio

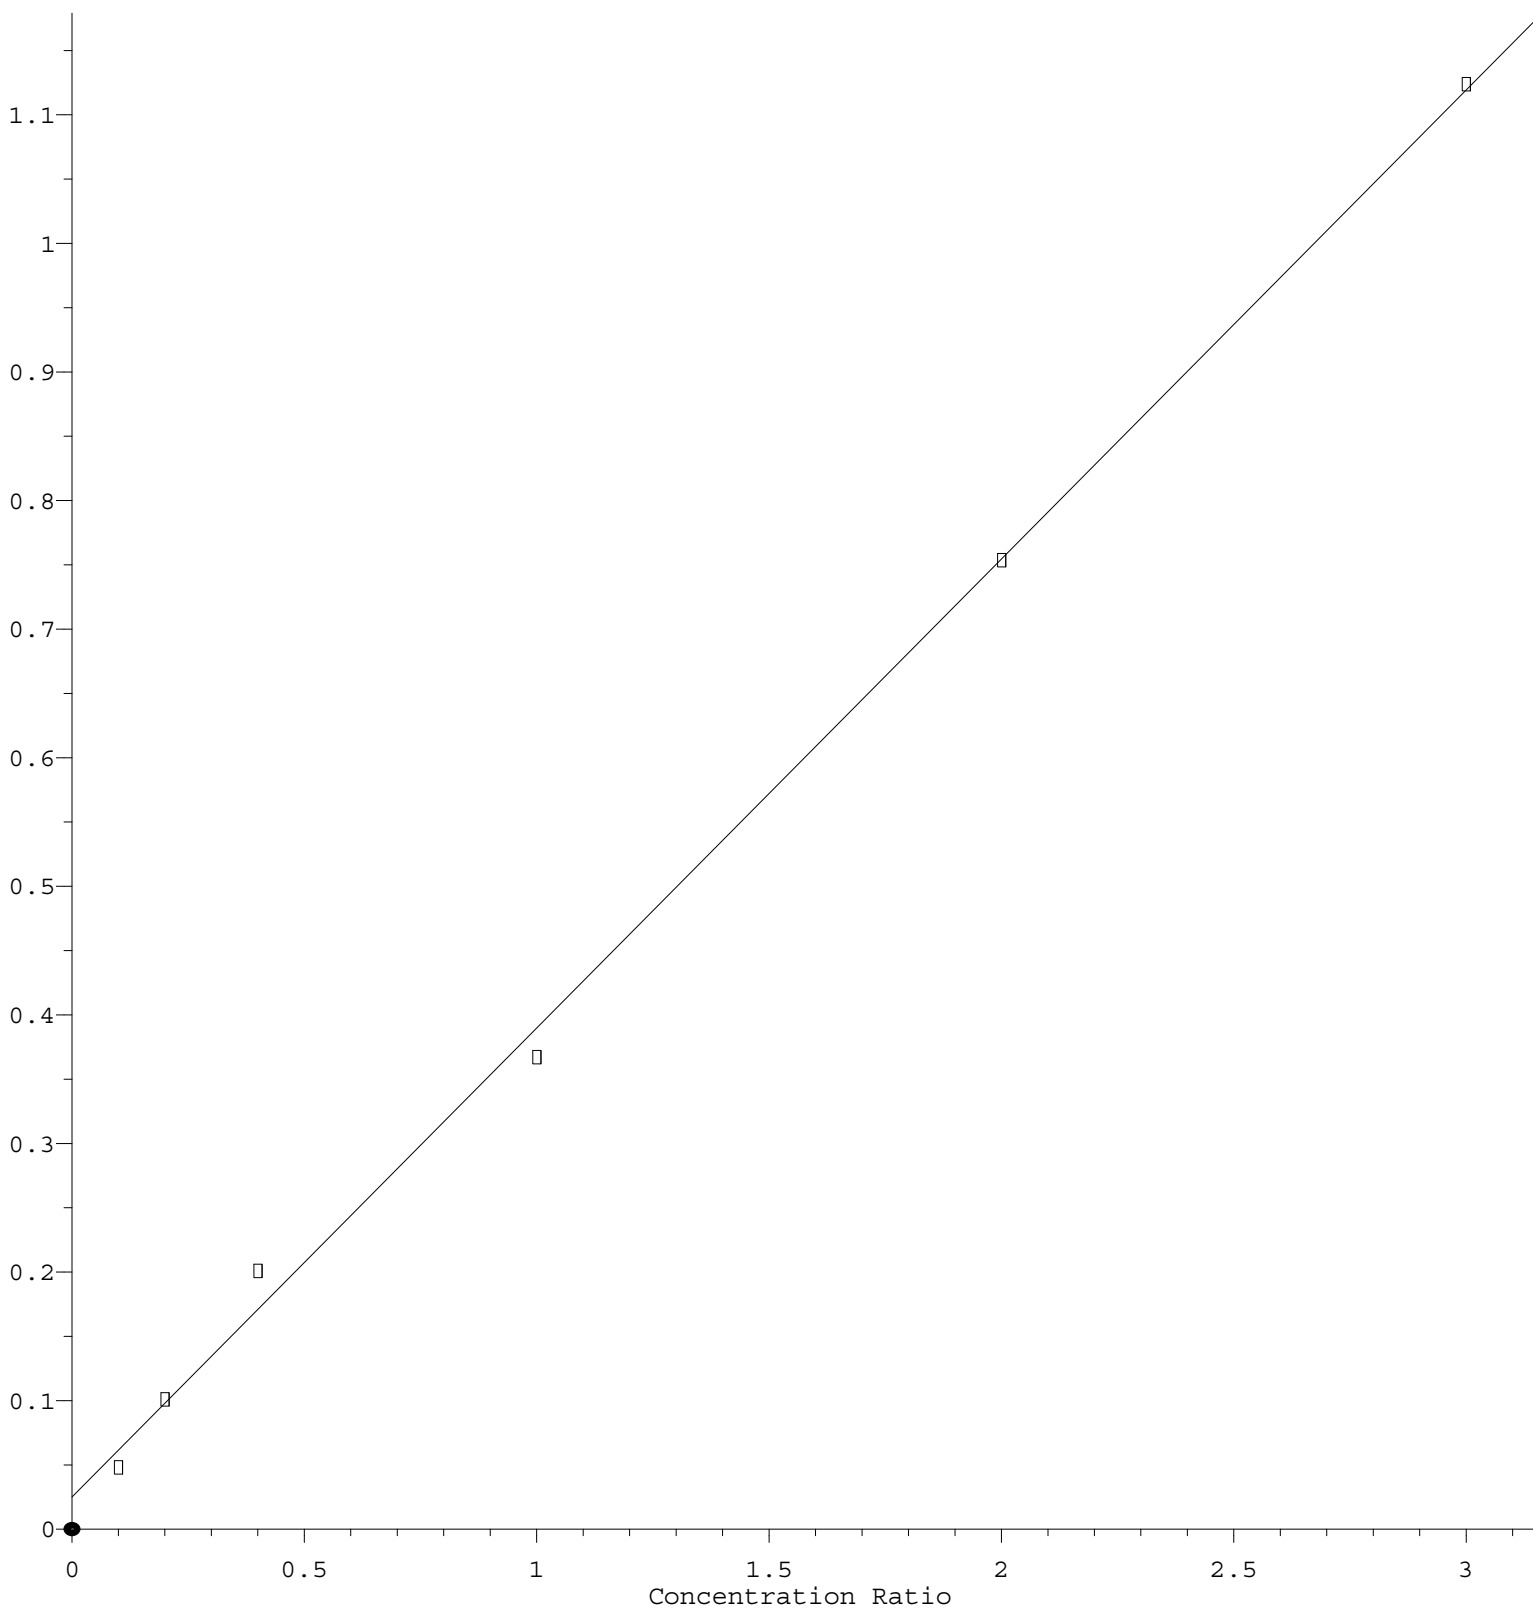

$$\text{Response} = 3.647\text{e-}001 * \text{Amt} + 2.514\text{e-}002$$


Coef of Det (r^2) = 0.998195 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D090922S.M

Calibration Table Last Updated: Sat Sep 10 04:45:19 2022

4-Bromofluorobenzene

Response Ratio

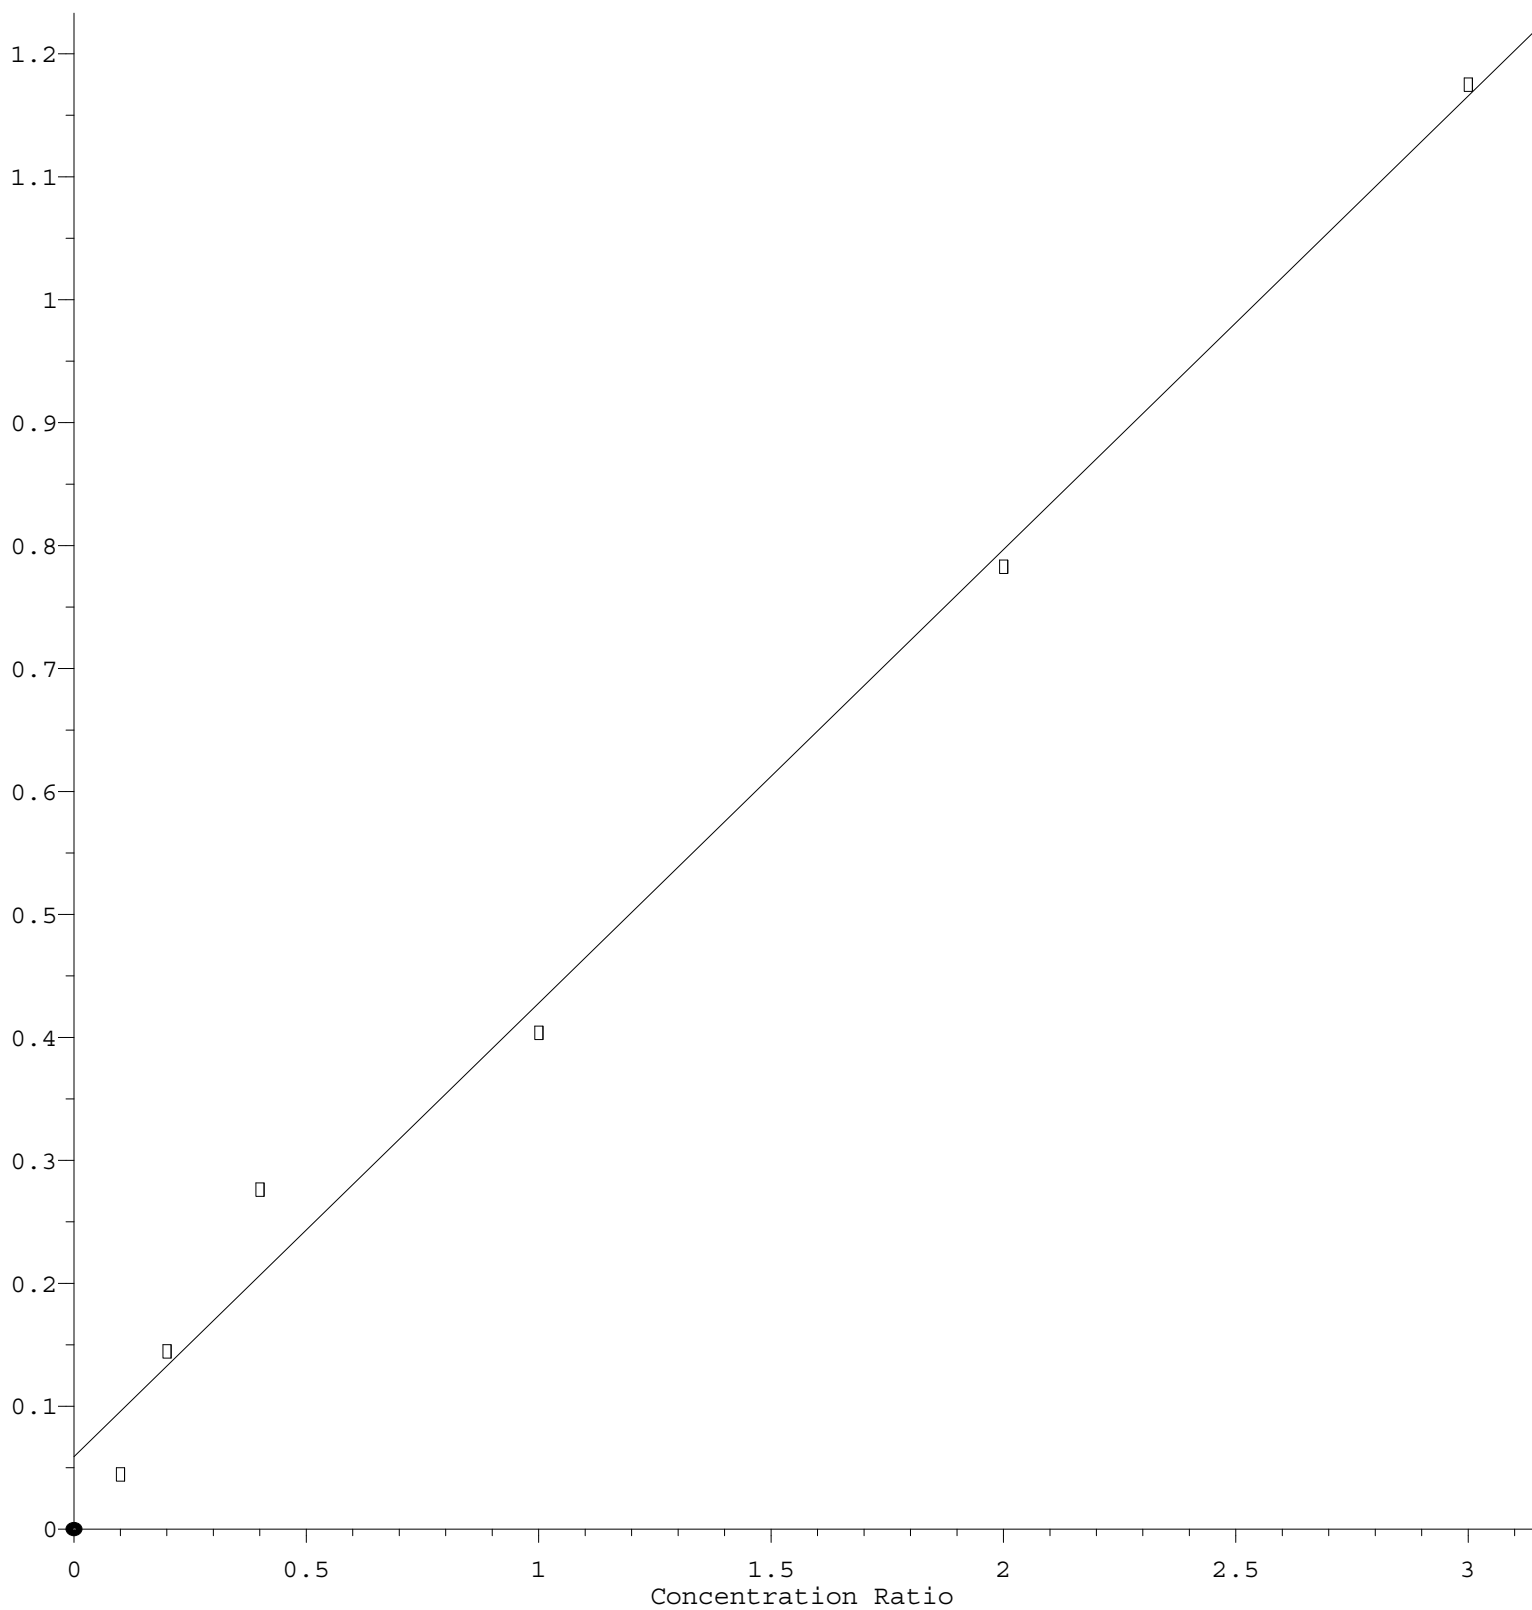

$$\text{Response} = 3.688\text{e-}001 * \text{Amt} + 5.926\text{e-}002$$


Coef of Det (r^2) = 0.990804 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D090922S.M

Calibration Table Last Updated: Sat Sep 10 04:45:19 2022

2-Chloroethyl Vinyl ether

Response Ratio

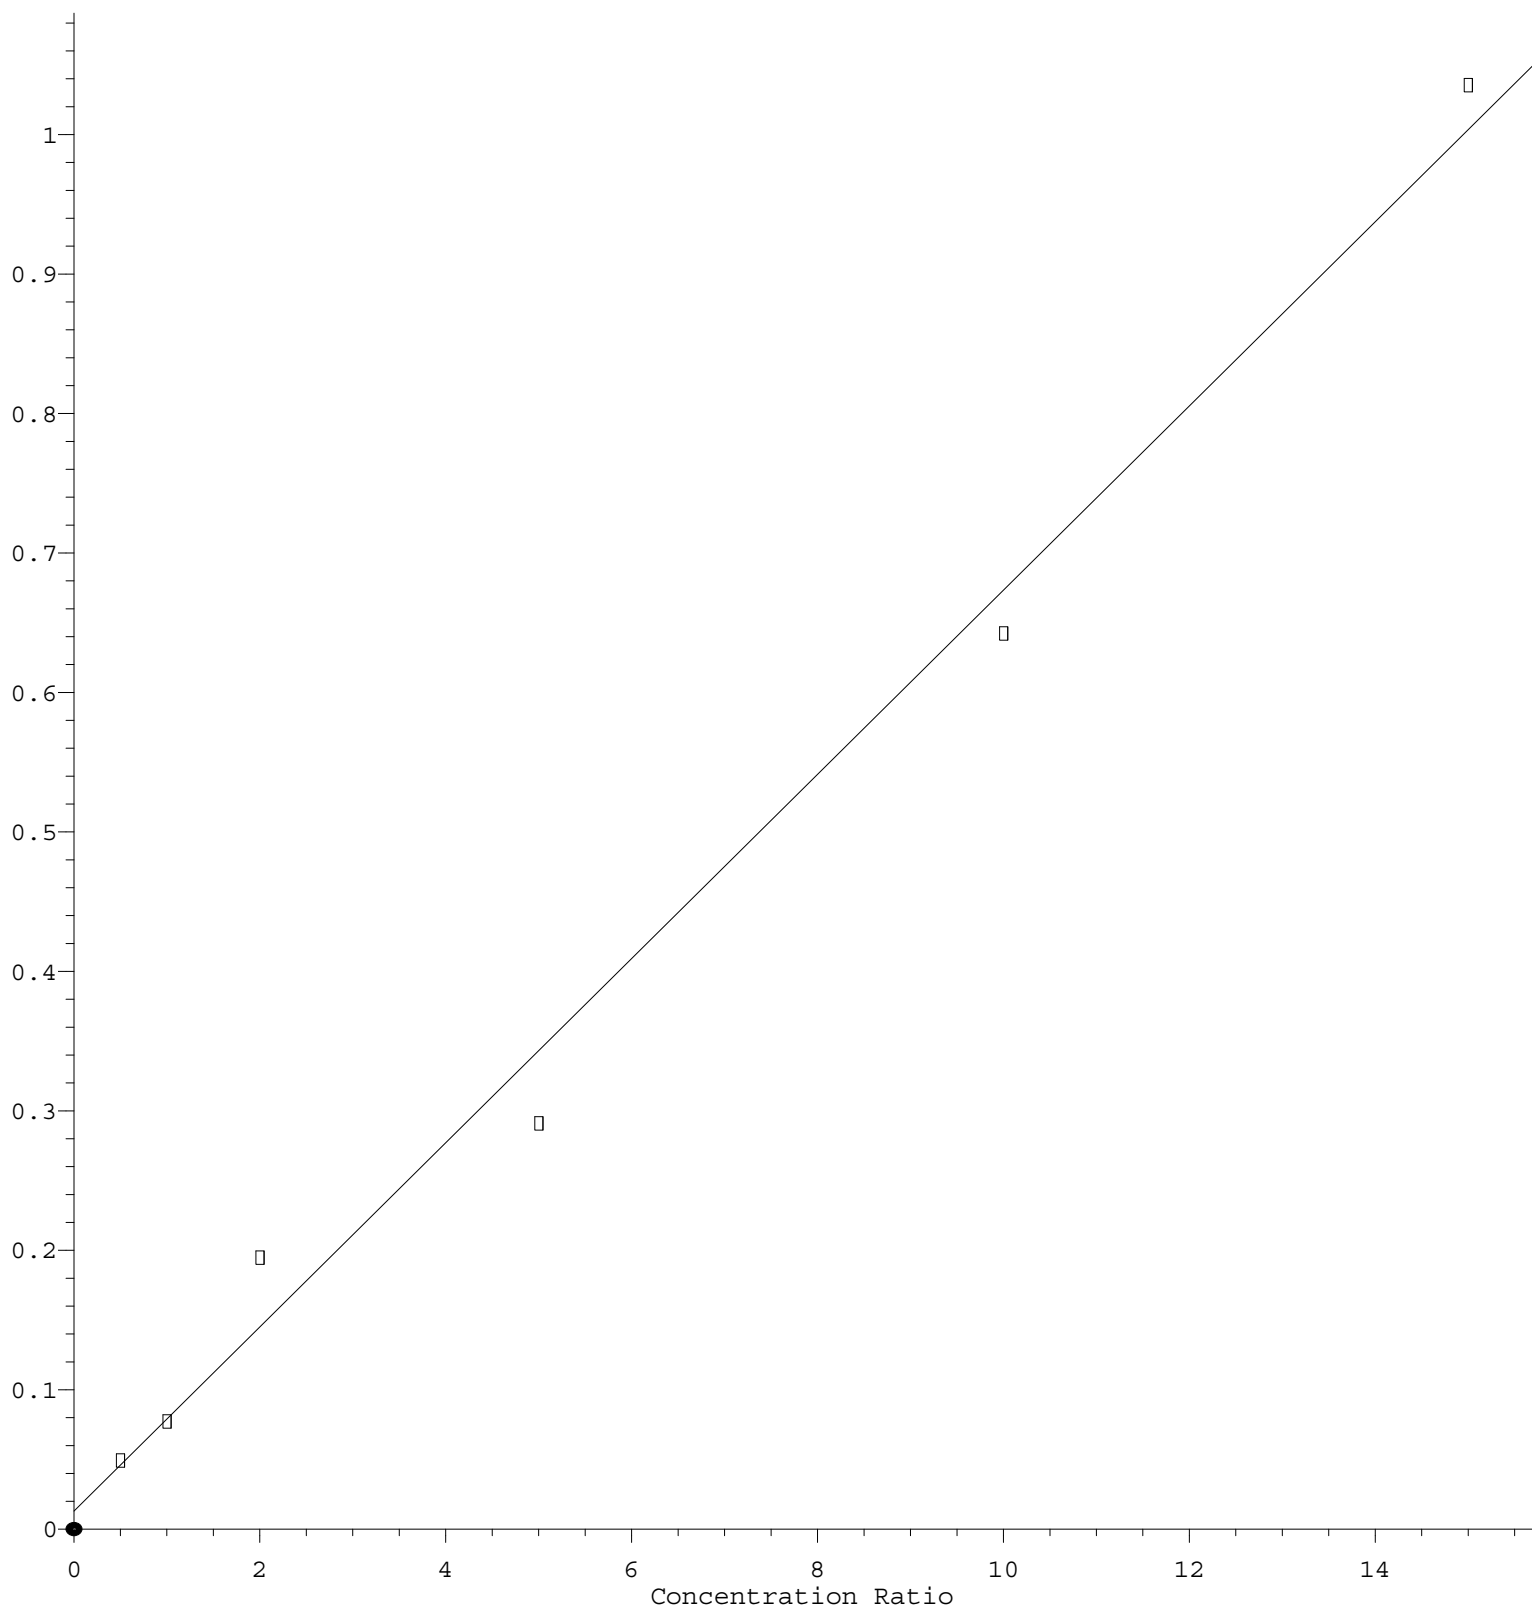

$$\text{Response} = 6.608\text{e-}002 * \text{Amt} + 1.265\text{e-}002$$


Coef of Det (r^2) = 0.990305 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D090922S.M

Calibration Table Last Updated: Sat Sep 10 04:45:19 2022

Dibromofluoromethane

Response Ratio

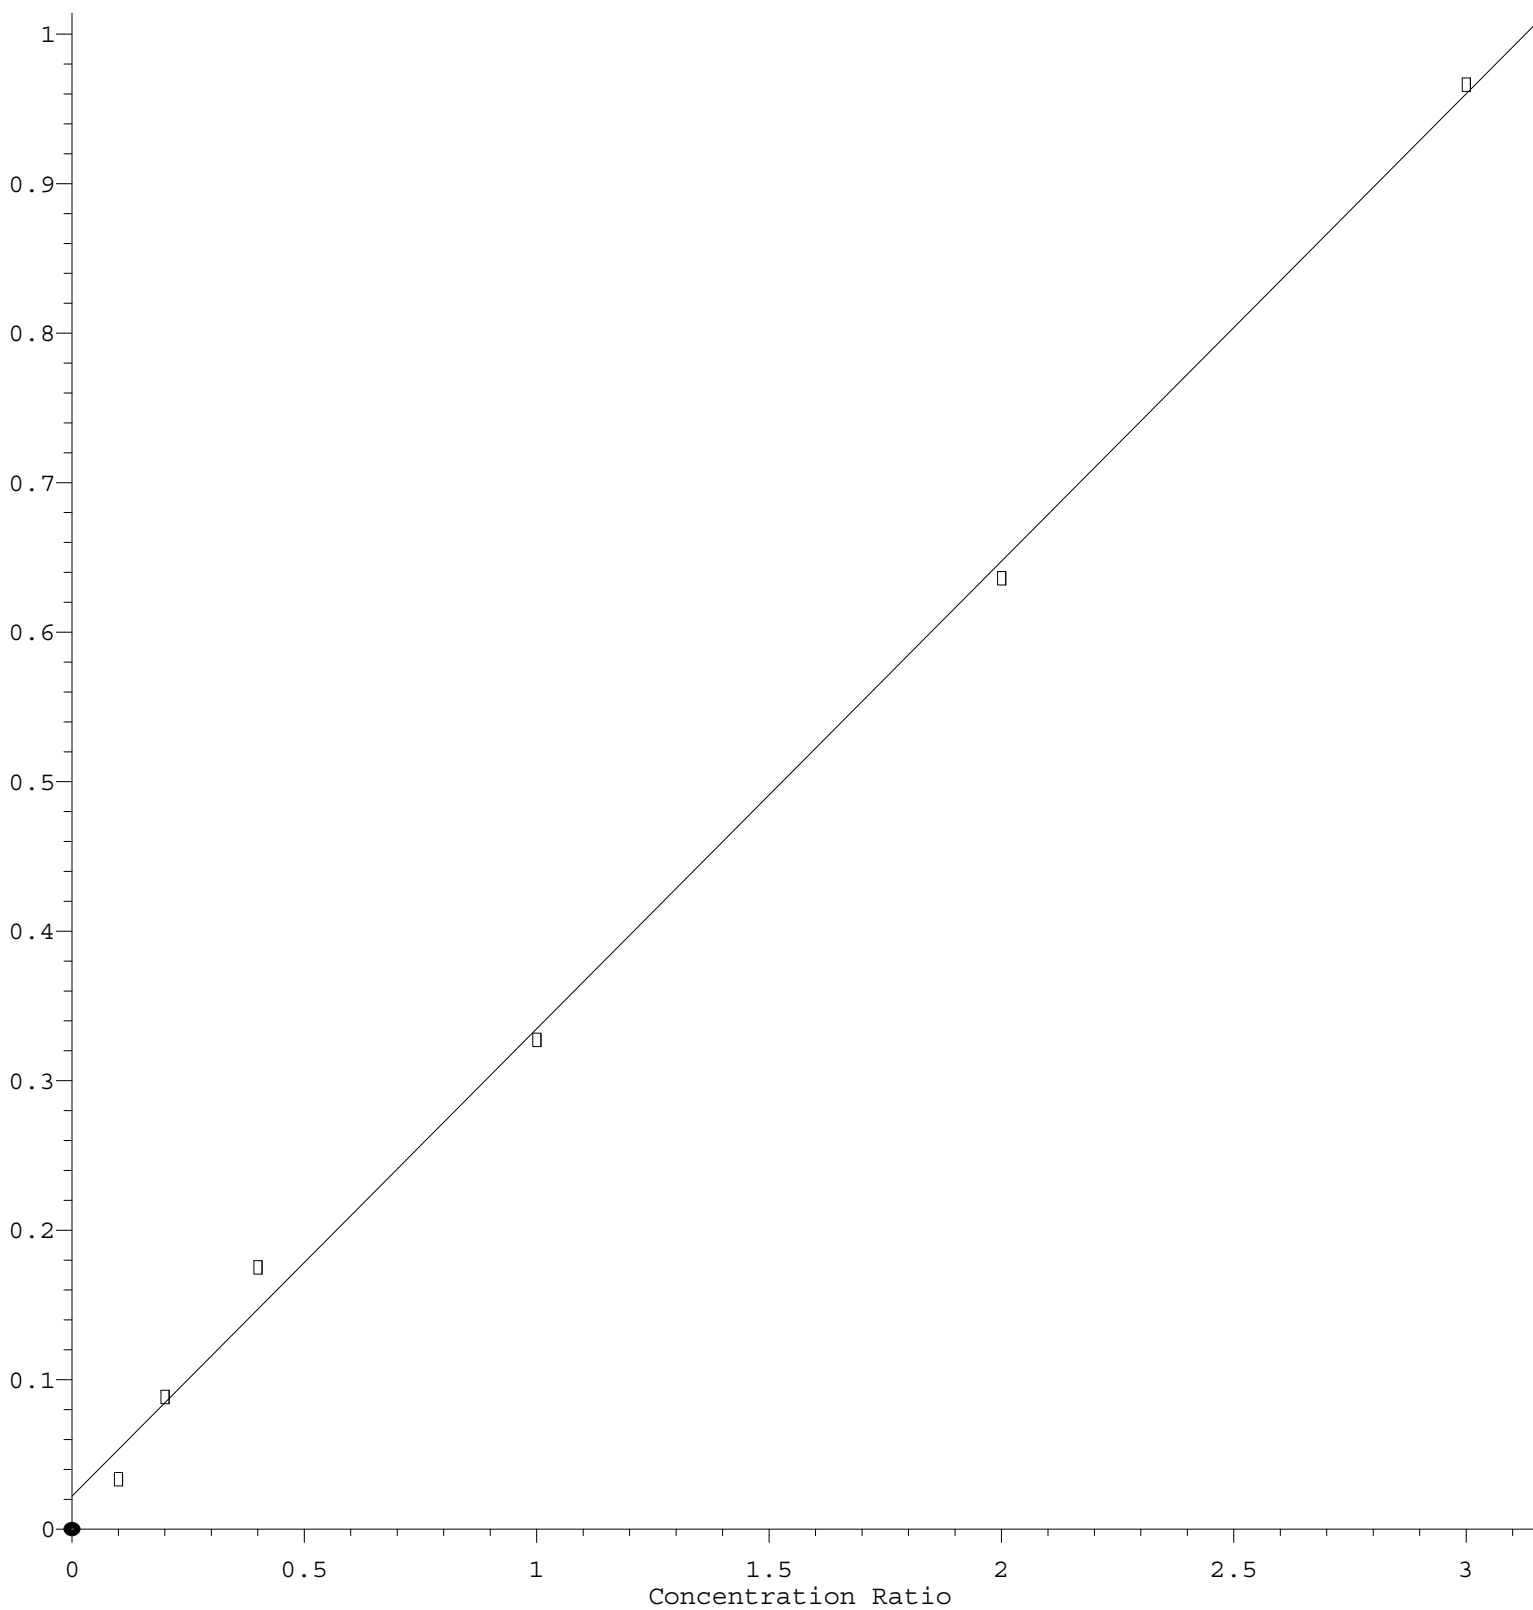

$$\text{Response} = 3.125\text{e-}001 * \text{Amt} + 2.207\text{e-}002$$


Coef of Det (r^2) = 0.997857 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D090922S.M

Calibration Table Last Updated: Sat Sep 10 04:45:19 2022

Methylene Chloride

Response Ratio

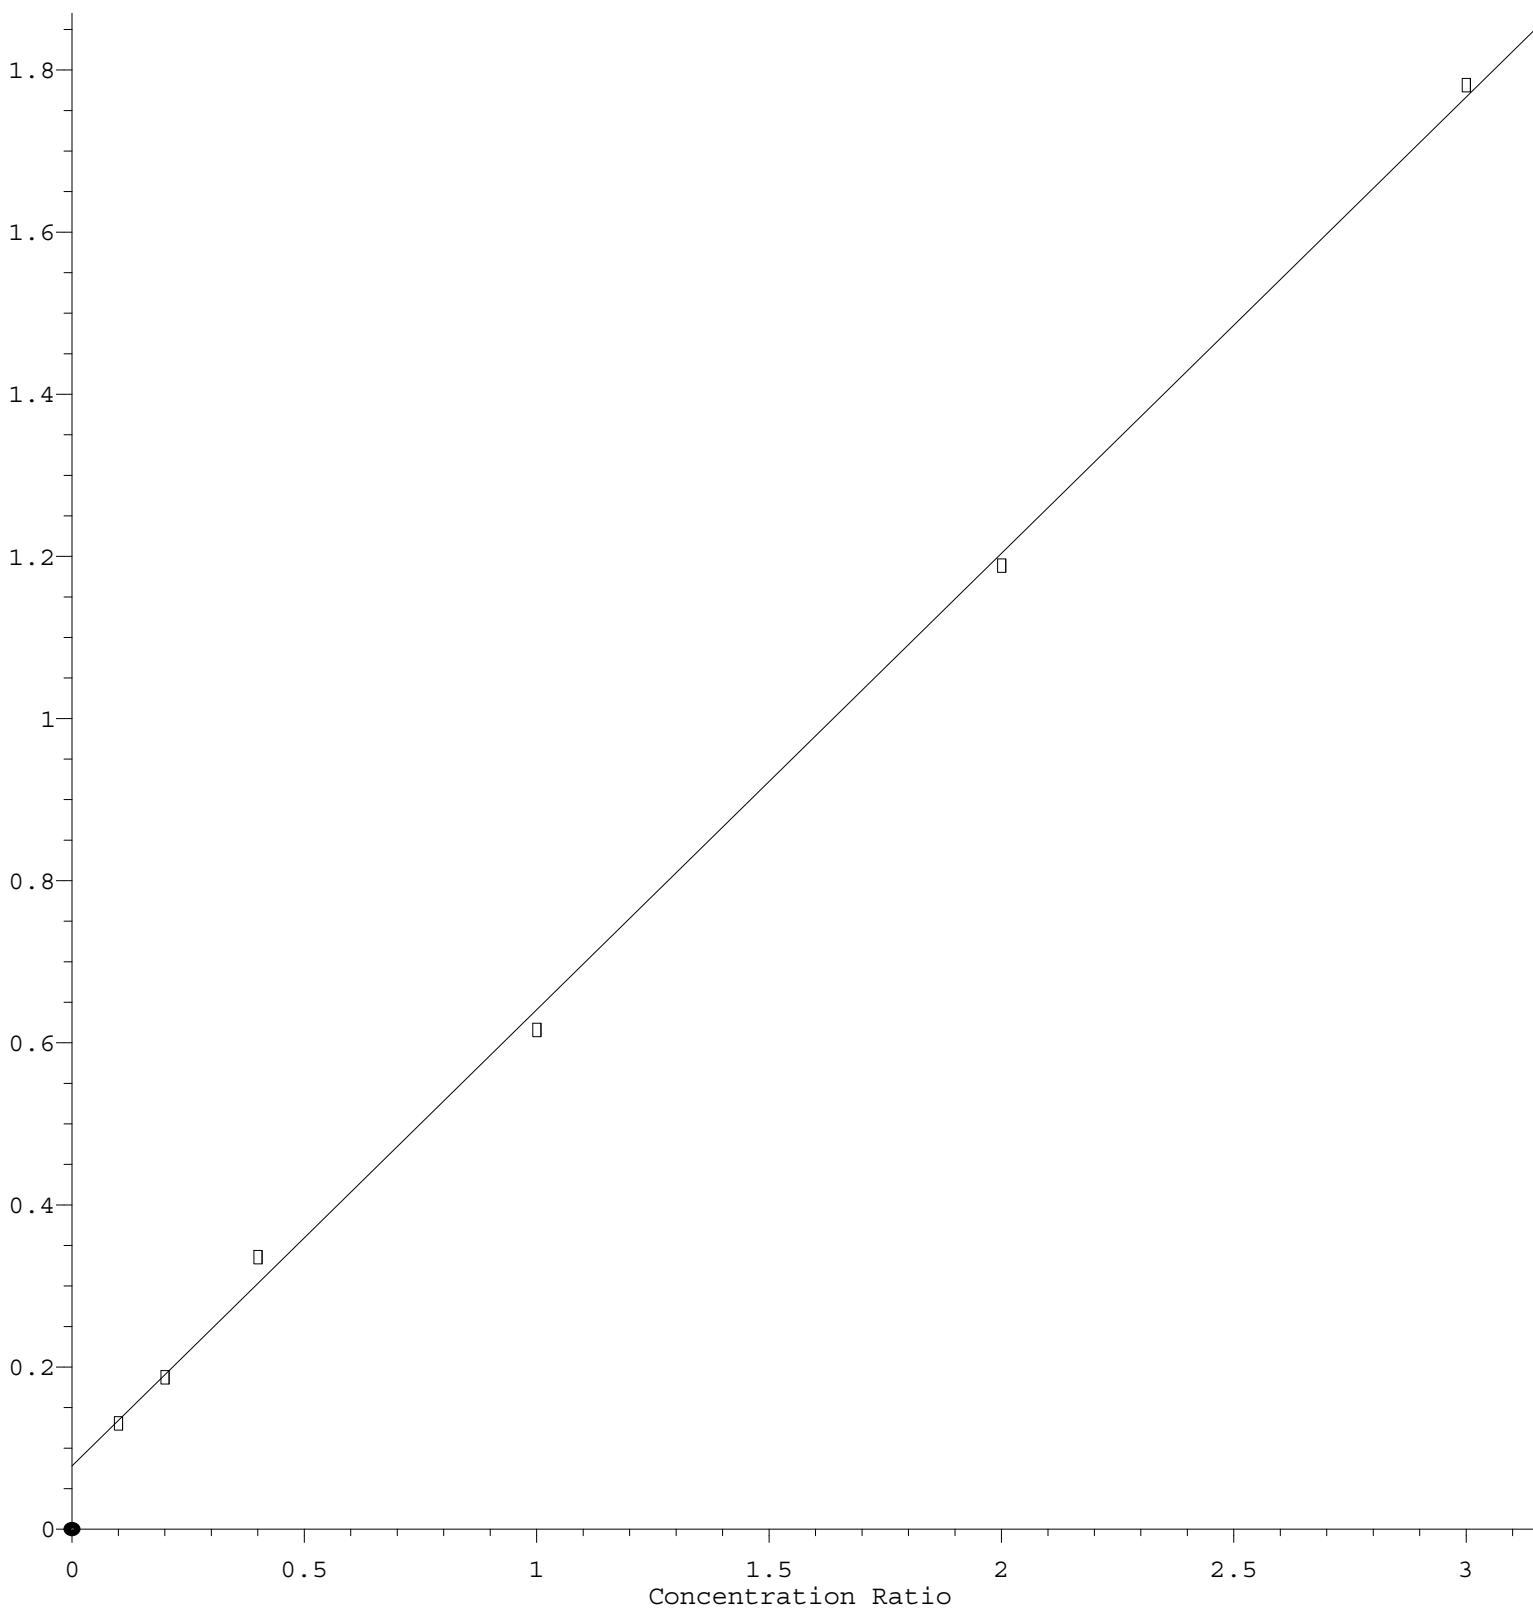

$$\text{Response} = 5.630\text{e-}001 * \text{Amt} + 7.783\text{e-}002$$

Coef of Det (r^2) = 0.998995 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D090922S.M

Calibration Table Last Updated: Sat Sep 10 04:45:19 2022